

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041224\
 Data File : VX041050.D
 Acq On : 12 Apr 2024 22:51
 Operator : JC/MD
 Sample : P2049-20
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MCORE7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
 Title : VOC Analysis

Signal : TIC: VX041050.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.252	24	27	29	rBV	3231	4172	0.41%	0.053%
2	1.368	42	46	57	rBV	133918	147624	14.49%	1.880%
3	1.666	91	95	111	rVB	89782	135735	13.32%	1.729%
4	2.306	194	200	208	rBV	220927	343132	33.68%	4.371%
5	2.380	208	212	217	rVB	3167	5560	0.55%	0.071%
6	2.538	231	238	240	rBV2	1283	2533	0.25%	0.032%
7	2.642	254	255	258	rVB2	221	218	0.02%	0.003%
8	2.672	258	260	262	rVB	207	154	0.02%	0.002%
9	2.703	262	265	269	rVB3	228	369	0.04%	0.005%
10	2.745	269	272	273	rBV	199	174	0.02%	0.002%
11	2.794	276	280	285	rVB3	595	1084	0.11%	0.014%
12	2.849	285	289	291	rBV2	199	238	0.02%	0.003%
13	2.898	295	297	298	rBV	188	146	0.01%	0.002%
14	2.946	299	305	316	rVB3	1707	3850	0.38%	0.049%
15	3.093	325	329	331	rBV2	373	502	0.05%	0.006%
16	3.190	342	345	348	rVV2	154	183	0.02%	0.002%
17	3.227	348	351	353	rVV	224	172	0.02%	0.002%
18	3.324	362	367	368	rVV2	158	166	0.02%	0.002%
19	3.367	372	374	378	rBV2	105	172	0.02%	0.002%
20	3.770	437	440	443	rBV2	98	145	0.01%	0.002%
21	3.806	443	446	447	rVB2	198	171	0.02%	0.002%
22	3.995	474	477	478	rBV2	175	154	0.02%	0.002%
23	4.452	542	552	570	rBV	73258	231626	22.74%	2.950%
24	4.928	628	630	633	rVB2	159	178	0.02%	0.002%
25	5.056	639	651	675	rVV	134199	415137	40.75%	5.288%
26	5.349	696	699	700	rBV2	186	177	0.02%	0.002%
27	5.477	717	720	721	rVV2	212	234	0.02%	0.003%
28	5.525	727	728	729	rVV	234	145	0.01%	0.002%
29	5.562	730	734	742	rVV2	760	1619	0.16%	0.021%
30	5.672	749	752	756	rVB3	317	439	0.04%	0.006%
31	5.855	779	782	785	rBV2	191	295	0.03%	0.004%
32	5.970	789	801	819	rBV2	344884	1018652	100.00%	12.975%
33	6.306	854	856	858	rBV2	228	170	0.02%	0.002%
34	6.470	881	883	885	rVV2	171	136	0.01%	0.002%
35	6.550	894	896	897	rVB	222	143	0.01%	0.002%
36	6.653	909	913	914	rBV	259	268	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041224\
 Data File : VX041050.D
 Acq On : 12 Apr 2024 22:51
 Operator : JC/MD
 Sample : P2049-20
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MCORE7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
 Title : VOC Analysis

37	6.763	922	931	946	rBV	238788	572739	56.23%	7.295%
38	7.123	984	990	999	rBV8	1675	4296	0.42%	0.055%
39	7.305	1012	1020	1043	rBV	201888	454410	44.61%	5.788%
40	7.562	1060	1062	1065	rVB	188	154	0.02%	0.002%
41	7.592	1065	1067	1068	rBV	175	139	0.01%	0.002%
42	7.714	1085	1087	1090	rVB2	129	136	0.01%	0.002%
43	7.769	1092	1096	1097	rBV	106	155	0.02%	0.002%
44	7.824	1102	1105	1107	rBV3	151	188	0.02%	0.002%
45	7.921	1119	1121	1124	rVB2	169	135	0.01%	0.002%
46	7.964	1126	1128	1131	rVB2	204	172	0.02%	0.002%
47	8.141	1155	1157	1160	rBV2	177	200	0.02%	0.003%
48	8.324	1181	1187	1200	rBV	134702	221660	21.76%	2.823%
49	8.458	1208	1209	1214	rVB2	357	233	0.02%	0.003%
50	8.513	1217	1218	1221	rVB3	384	343	0.03%	0.004%
51	8.543	1221	1223	1226	rBV2	178	179	0.02%	0.002%
52	8.574	1226	1228	1233	rVB2	506	665	0.07%	0.008%
53	8.647	1234	1240	1250	rBV	522647	826887	81.17%	10.533%
54	8.952	1284	1290	1304	rBV	97276	144465	14.18%	1.840%
55	9.153	1321	1323	1327	rVB2	192	249	0.02%	0.003%
56	9.275	1337	1343	1352	rVB	12832	20906	2.05%	0.266%
57	9.384	1356	1361	1382	rBV	323877	497196	48.81%	6.333%
58	9.671	1404	1408	1409	rBV3	212	239	0.02%	0.003%
59	9.945	1451	1453	1459	rVB2	187	313	0.03%	0.004%
60	10.000	1459	1462	1465	rBV	238	301	0.03%	0.004%
61	10.055	1465	1471	1491	rVV	502489	702560	68.97%	8.949%
62	10.189	1491	1493	1500	rVB3	598	1057	0.10%	0.013%
63	10.311	1510	1513	1517	rVV3	614	721	0.07%	0.009%
64	10.659	1565	1570	1572	rVB2	411	679	0.07%	0.009%
65	10.738	1581	1583	1590	rVB2	154	193	0.02%	0.002%
66	10.854	1599	1602	1605	rBV2	122	204	0.02%	0.003%
67	10.927	1611	1614	1615	rBV	153	164	0.02%	0.002%
68	10.963	1617	1620	1624	rVB2	495	702	0.07%	0.009%
69	11.091	1637	1641	1646	rVV4	621	932	0.09%	0.012%
70	11.189	1652	1657	1672	rVV	399454	515011	50.56%	6.560%
71	11.311	1672	1677	1683	rVB	21254	29259	2.87%	0.373%
72	11.427	1694	1696	1698	rVV	133	158	0.02%	0.002%
73	11.457	1698	1701	1704	rVB2	453	586	0.06%	0.007%
74	11.707	1740	1742	1745	rVB	259	231	0.02%	0.003%
75	11.756	1746	1750	1756	rVB3	491	750	0.07%	0.010%
76	11.975	1780	1786	1788	rBV2	3120	3774	0.37%	0.048%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041224\
 Data File : VX041050.D
 Acq On : 12 Apr 2024 22:51
 Operator : JC/MD
 Sample : P2049-20
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MCORE7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
 Title : VOC Analysis

77	12.018	1788	1793	1804	rBV	541927	705757	69.28%	8.990%
78	12.225	1822	1827	1835	rBV3	5356	11441	1.12%	0.146%
79	12.317	1837	1842	1857	rVB	627429	791187	77.67%	10.078%
80	12.628	1891	1893	1895	rBV2	219	244	0.02%	0.003%
81	12.762	1911	1915	1921	rVB	4545	5985	0.59%	0.076%
82	12.865	1928	1932	1937	rVB2	1079	1208	0.12%	0.015%
83	12.926	1940	1942	1943	rBV	244	160	0.02%	0.002%
84	13.097	1966	1970	1971	rBV2	169	249	0.02%	0.003%
85	13.115	1971	1973	1976	rVV	651	680	0.07%	0.009%
86	13.219	1986	1990	1992	rVB	198	180	0.02%	0.002%
87	13.280	1998	2000	2003	rBV	202	167	0.02%	0.002%
88	13.506	2034	2037	2038	rBV	148	159	0.02%	0.002%
89	13.524	2038	2040	2041	rVV2	178	172	0.02%	0.002%
90	13.560	2044	2046	2048	rVV2	110	145	0.01%	0.002%
91	13.591	2048	2051	2058	rVB	2730	3685	0.36%	0.047%
92	13.792	2080	2084	2086	rBV2	505	658	0.06%	0.008%
93	13.890	2098	2100	2103	rBV2	171	177	0.02%	0.002%
94	13.963	2109	2112	2116	rBV2	959	1044	0.10%	0.013%
95	14.054	2126	2127	2131	rBV	174	277	0.03%	0.004%
96	14.097	2133	2134	2135	rBV	210	151	0.01%	0.002%
97	14.127	2135	2139	2145	rVB	3290	4705	0.46%	0.060%
98	14.396	2179	2183	2186	rBV2	225	378	0.04%	0.005%
99	15.243	2319	2322	2323	rBV2	647	661	0.06%	0.008%
100	15.395	2342	2347	2352	rBV5	1228	1968	0.19%	0.025%

Sum of corrected areas: 7850652




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041224\
Data File : VX041050.D
Acq On : 12 Apr 2024 22:51
Operator : JC/MD
Sample : P2049-20
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MC0RE7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

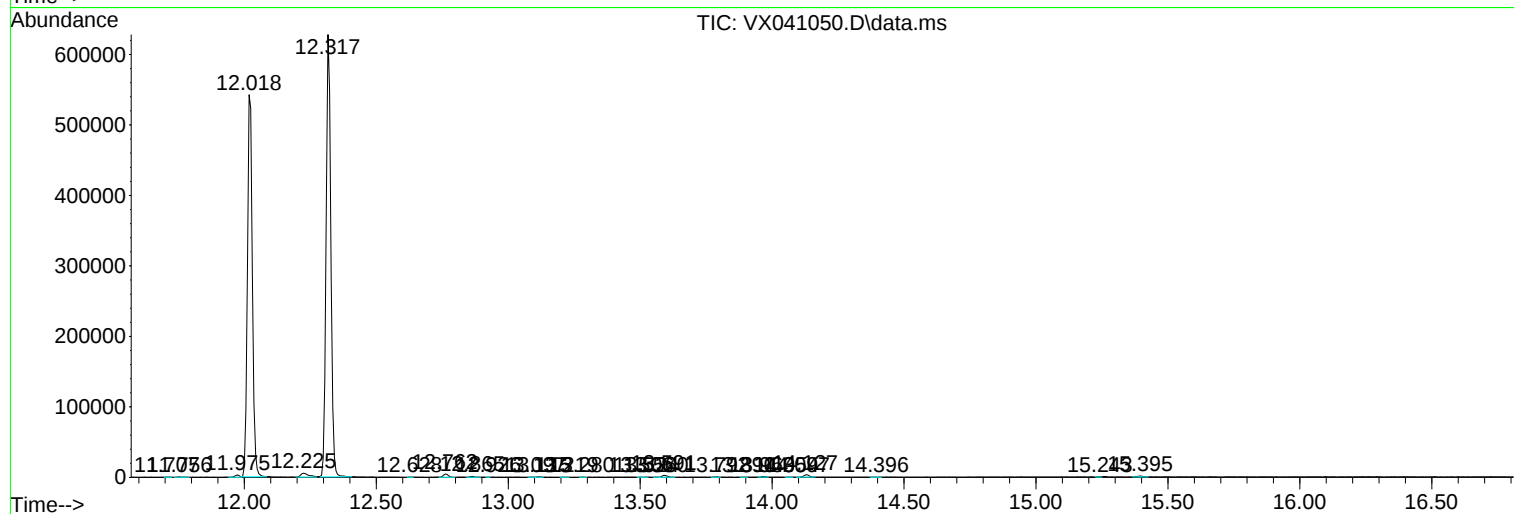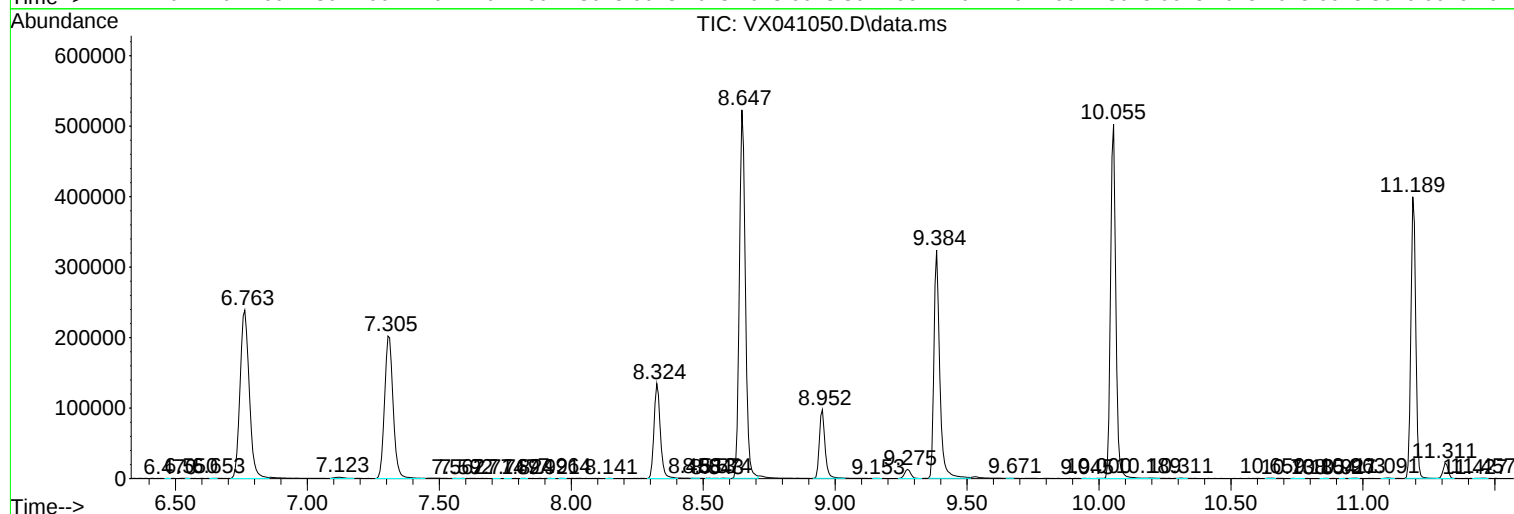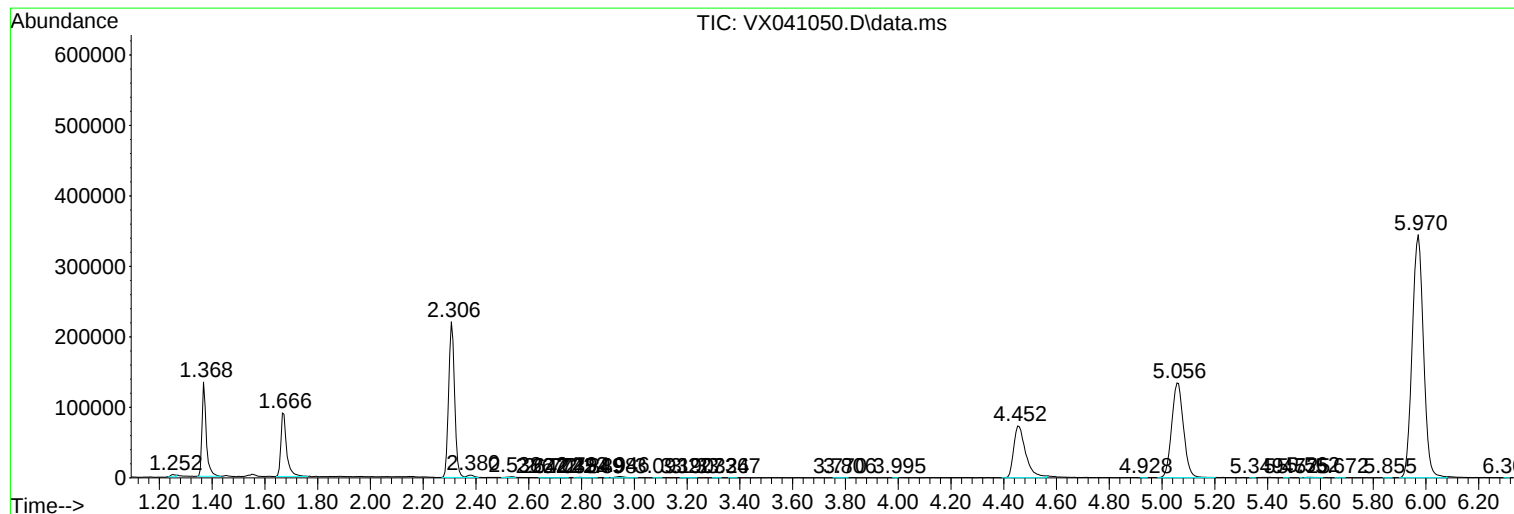

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041224\
Data File : VX041050.D
Acq On : 12 Apr 2024 22:51
Operator : JC/MD
Sample : P2049-20
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MC0RE7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM041024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041224\
Data File : VX041050.D
Acq On : 12 Apr 2024 22:51
Operator : JC/MD
Sample : P2049-20
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MC0RE7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------