

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041224\
 Data File : VX041052.D
 Acq On : 12 Apr 2024 23:37
 Operator : JC/MD
 Sample : P2098-02 100X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0RJ1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
 Title : VOC Analysis

Signal : TIC: VX041052.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.270	25	30	32	rBV4	1911	3018	0.29%	0.038%
2	1.368	42	46	59	rVB	134608	148399	14.24%	1.861%
3	1.666	91	95	110	rBV	90946	140943	13.52%	1.768%
4	2.306	194	200	209	rBV	224994	346836	33.28%	4.350%
5	2.465	224	226	227	rVV2	228	138	0.01%	0.002%
6	2.623	250	252	254	rBV	203	139	0.01%	0.002%
7	2.666	255	259	260	rVV2	123	139	0.01%	0.002%
8	2.721	266	268	269	rBV	248	157	0.02%	0.002%
9	2.788	275	279	286	rBV3	1180	2107	0.20%	0.026%
10	2.947	295	305	316	rBV	4680	10069	0.97%	0.126%
11	3.093	324	329	330	rBV	189	236	0.02%	0.003%
12	3.184	340	344	345	rBV2	192	214	0.02%	0.003%
13	3.203	345	347	350	rVV	123	175	0.02%	0.002%
14	3.233	350	352	355	rVV	228	216	0.02%	0.003%
15	3.294	358	362	365	rBV2	133	162	0.02%	0.002%
16	3.392	376	378	381	rBV2	95	122	0.01%	0.002%
17	3.465	389	390	395	rVB2	92	128	0.01%	0.002%
18	3.666	421	423	425	rVB2	169	131	0.01%	0.002%
19	3.696	425	428	429	rBV2	211	174	0.02%	0.002%
20	3.837	447	451	452	rBV2	110	120	0.01%	0.002%
21	4.129	498	499	502	rVB	144	125	0.01%	0.002%
22	4.160	502	504	506	rBV2	124	121	0.01%	0.002%
23	4.337	531	533	535	rBV	164	146	0.01%	0.002%
24	4.452	544	552	567	rBV	74831	230684	22.13%	2.893%
25	4.946	630	633	634	rBV3	176	173	0.02%	0.002%
26	5.056	638	651	669	rBV	137989	420068	40.31%	5.269%
27	5.300	689	691	693	rVB2	168	138	0.01%	0.002%
28	5.391	704	706	712	rVB2	583	787	0.08%	0.010%
29	5.458	716	717	722	rVB3	159	199	0.02%	0.002%
30	5.556	726	733	738	rBV4	575	1559	0.15%	0.020%
31	5.818	774	776	778	rBV2	210	204	0.02%	0.003%
32	5.970	789	801	820	rBV2	347359	1042205	100.00%	13.072%
33	6.287	852	853	856	rVB2	275	210	0.02%	0.003%
34	6.330	856	860	861	rBV3	192	273	0.03%	0.003%
35	6.458	879	881	883	rVV	173	124	0.01%	0.002%
36	6.543	891	895	896	rBV2	154	204	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041224\
 Data File : VX041052.D
 Acq On : 12 Apr 2024 23:37
 Operator : JC/MD
 Sample : P2098-02 100X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 CORJ1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
 Title : VOC Analysis

37	6.562	896	898	902	rVV3	141	181	0.02%	0.002%
38	6.763	921	931	958	rBV	243123	594527	57.05%	7.457%
39	7.117	984	989	991	rBV6	1184	2273	0.22%	0.029%
40	7.214	1002	1005	1009	rBV2	206	258	0.02%	0.003%
41	7.306	1009	1020	1039	rBV	209011	462930	44.42%	5.806%
42	7.714	1086	1087	1091	rBV	151	173	0.02%	0.002%
43	7.952	1124	1126	1127	rBV	241	176	0.02%	0.002%
44	8.104	1149	1151	1154	rBV2	182	281	0.03%	0.004%
45	8.324	1181	1187	1204	rBV	133227	225080	21.60%	2.823%
46	8.488	1213	1214	1216	rBV	195	157	0.02%	0.002%
47	8.507	1216	1217	1220	rVV2	238	204	0.02%	0.003%
48	8.537	1220	1222	1226	rVB2	246	226	0.02%	0.003%
49	8.580	1226	1229	1234	rBV3	373	399	0.04%	0.005%
50	8.647	1234	1240	1264	rBV	536455	844979	81.08%	10.598%
51	8.952	1284	1290	1305	rBV	97090	146308	14.04%	1.835%
52	9.147	1320	1322	1323	rVB2	228	126	0.01%	0.002%
53	9.159	1323	1324	1326	rBV	144	121	0.01%	0.002%
54	9.220	1332	1334	1338	rBV2	129	208	0.02%	0.003%
55	9.275	1338	1343	1348	rBV2	3428	5039	0.48%	0.063%
56	9.384	1355	1361	1381	rBV	329162	501562	48.13%	6.291%
57	9.695	1410	1412	1413	rBV	357	272	0.03%	0.003%
58	9.933	1449	1451	1453	rBV	168	132	0.01%	0.002%
59	10.055	1465	1471	1491	rBV	521717	739599	70.96%	9.277%
60	10.311	1510	1513	1516	rVB	560	596	0.06%	0.007%
61	10.622	1562	1564	1566	rBV2	210	173	0.02%	0.002%
62	10.646	1566	1568	1569	rBV	348	289	0.03%	0.004%
63	10.963	1618	1620	1624	rVB	338	357	0.03%	0.004%
64	11.091	1638	1641	1646	rVB2	615	804	0.08%	0.010%
65	11.189	1652	1657	1668	rBV	405166	523496	50.23%	6.566%
66	11.317	1673	1678	1683	rVB	5874	8177	0.78%	0.103%
67	11.451	1698	1700	1705	rBV2	417	462	0.04%	0.006%
68	11.561	1717	1718	1721	rBV2	173	157	0.02%	0.002%
69	11.707	1739	1742	1745	rBV2	256	302	0.03%	0.004%
70	11.756	1748	1750	1757	rVB3	394	534	0.05%	0.007%
71	11.908	1773	1775	1777	rBV2	106	130	0.01%	0.002%
72	11.975	1783	1786	1788	rBV	1480	1531	0.15%	0.019%
73	12.024	1788	1794	1805	rVV	547711	732908	70.32%	9.193%
74	12.201	1821	1823	1826	rVB2	267	267	0.03%	0.003%
75	12.317	1837	1842	1852	rBV	619257	797331	76.50%	10.001%
76	12.549	1879	1880	1883	rVB	237	152	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041224\
 Data File : VX041052.D
 Acq On : 12 Apr 2024 23:37
 Operator : JC/MD
 Sample : P2098-02 100X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0RJ1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
 Title : VOC Analysis

77	12.628	1891	1893	1895	rBV	168	129	0.01%	0.002%
78	12.762	1910	1915	1920	rVB	5637	7552	0.72%	0.095%
79	12.963	1947	1948	1952	rBV2	153	212	0.02%	0.003%
80	13.097	1967	1970	1971	rVV2	165	168	0.02%	0.002%
81	13.115	1971	1973	1980	rVV2	471	685	0.07%	0.009%
82	13.317	2004	2006	2010	rVB2	157	214	0.02%	0.003%
83	13.347	2010	2011	2014	rBV	157	124	0.01%	0.002%
84	13.414	2020	2022	2023	rBV2	189	143	0.01%	0.002%
85	13.493	2030	2035	2037	rVB2	167	288	0.03%	0.004%
86	13.567	2044	2047	2048	rBV	208	184	0.02%	0.002%
87	13.597	2048	2052	2057	rBV2	2270	2919	0.28%	0.037%
88	13.780	2079	2082	2083	rBV2	331	278	0.03%	0.003%
89	13.938	2106	2108	2109	rBV	157	125	0.01%	0.002%
90	13.963	2110	2112	2116	rVV2	695	859	0.08%	0.011%
91	14.030	2119	2123	2124	rVB2	199	205	0.02%	0.003%
92	14.134	2135	2140	2145	rVB	6887	9633	0.92%	0.121%
93	14.310	2167	2169	2170	rVB	341	197	0.02%	0.002%
94	14.329	2170	2172	2174	rBV2	281	297	0.03%	0.004%
95	14.469	2193	2195	2197	rVB	304	206	0.02%	0.003%
96	14.499	2197	2200	2202	rBV2	147	204	0.02%	0.003%
97	14.652	2223	2225	2227	rBV2	268	292	0.03%	0.004%
98	14.688	2229	2231	2232	rBV	242	166	0.02%	0.002%
99	15.389	2342	2346	2352	rVB3	2102	3587	0.34%	0.045%
100	15.505	2364	2365	2368	rBV2	349	320	0.03%	0.004%




Sum of corrected areas: 7972707

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041224\
Data File : VX041052.D
Acq On : 12 Apr 2024 23:37
Operator : JC/MD
Sample : P2098-02 100X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0RJ1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

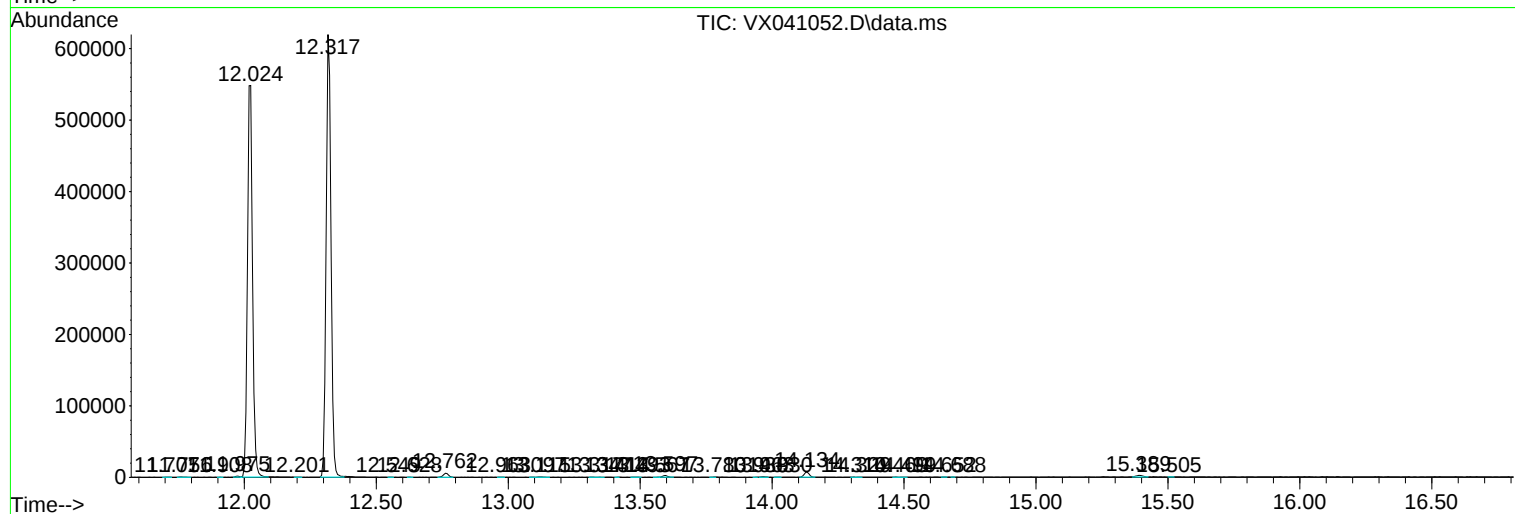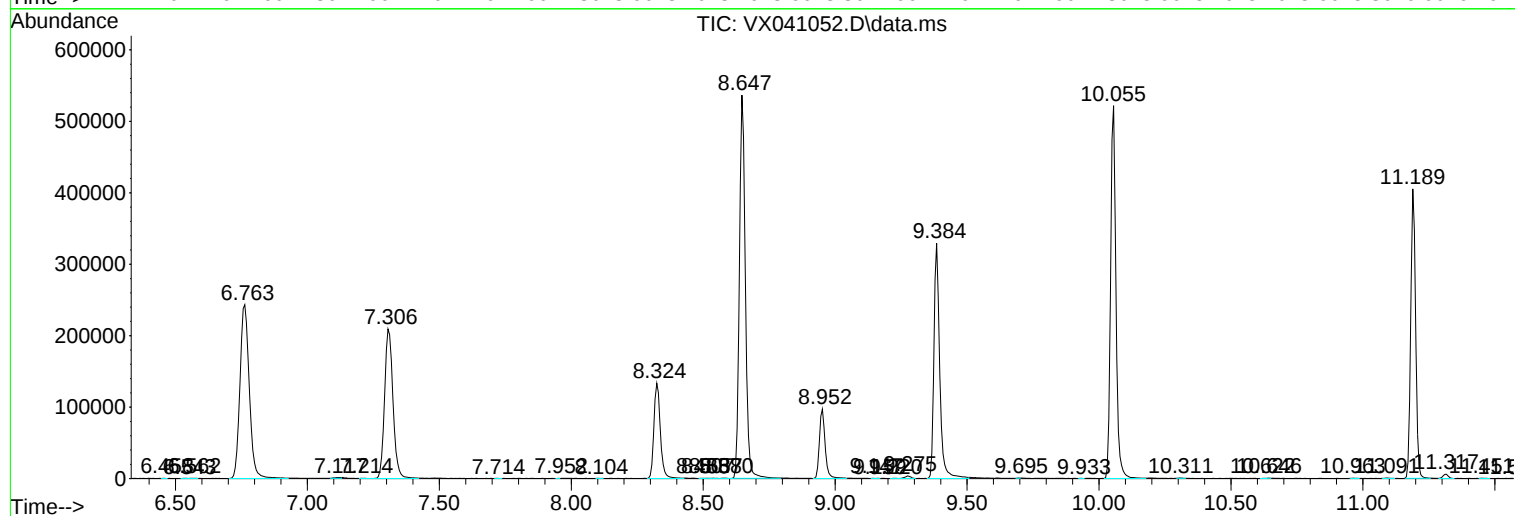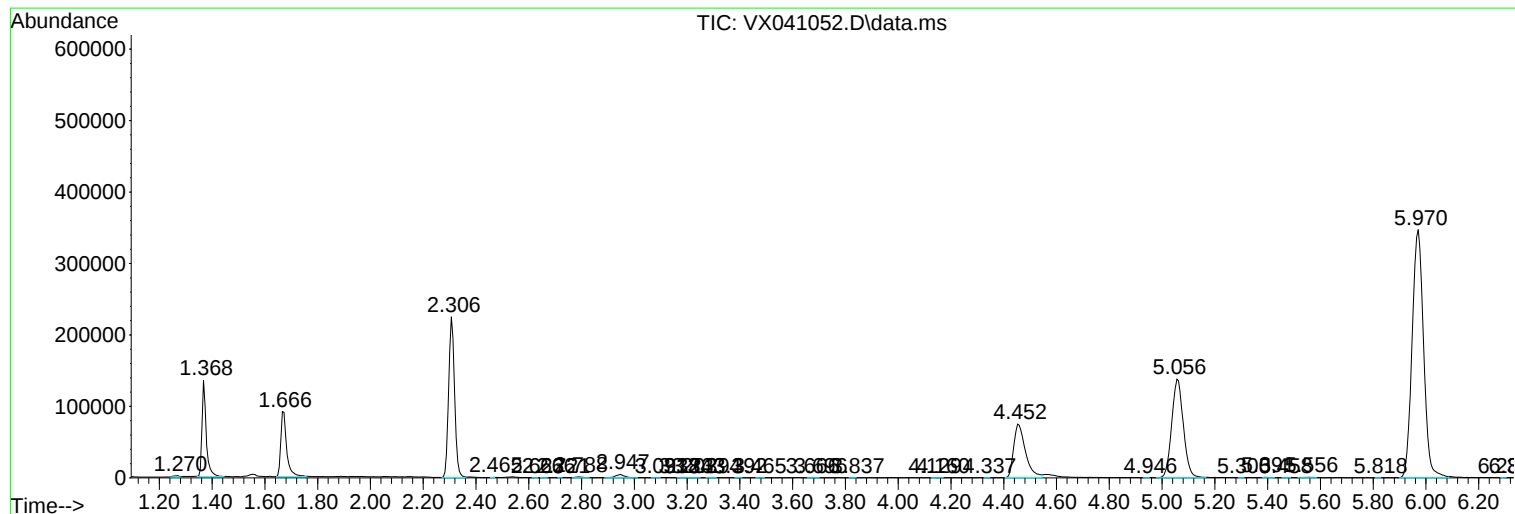

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041224\
Data File : VX041052.D
Acq On : 12 Apr 2024 23:37
Operator : JC/MD
Sample : P2098-02 100X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0RJ1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM041024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041224\
Data File : VX041052.D
Acq On : 12 Apr 2024 23:37
Operator : JC/MD
Sample : P2098-02 100X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0RJ1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc