

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041224\
 Data File : VX041053.D
 Acq On : 13 Apr 2024 00:00
 Operator : JC/MD
 Sample : P2098-03 100X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0RJ5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
 Title : VOC Analysis

Signal : TIC: VX041053.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.367	43	46	59	rBV	125149	141518	14.45%	1.820%
2	1.672	91	96	109	rBV	85031	133190	13.60%	1.713%
3	2.306	194	200	210	rBV	208219	324469	33.12%	4.174%
4	2.532	230	237	243	rBV3	1384	3082	0.31%	0.040%
5	2.702	263	265	268	rBV2	175	155	0.02%	0.002%
6	2.788	276	279	285	rVB3	828	1363	0.14%	0.018%
7	2.946	297	305	313	rBV	4994	10905	1.11%	0.140%
8	3.086	327	328	330	rBV	160	132	0.01%	0.002%
9	3.288	357	361	364	rVB2	119	172	0.02%	0.002%
10	3.428	381	384	385	rVB2	154	137	0.01%	0.002%
11	3.458	385	389	394	rVB2	131	242	0.02%	0.003%
12	3.495	394	395	400	rVB2	178	181	0.02%	0.002%
13	3.532	400	401	403	rBV	138	125	0.01%	0.002%
14	3.611	412	414	420	rVV	139	185	0.02%	0.002%
15	4.013	477	480	482	rVV2	161	182	0.02%	0.002%
16	4.031	482	483	486	rVV2	131	139	0.01%	0.002%
17	4.062	486	488	490	rVB	168	115	0.01%	0.001%
18	4.458	544	553	567	rBV	73517	226726	23.14%	2.916%
19	5.056	638	651	668	rBV	126037	392367	40.05%	5.047%
20	5.306	690	692	696	rVB3	296	363	0.04%	0.005%
21	5.513	725	726	728	rBV	206	161	0.02%	0.002%
22	5.562	732	734	736	rVB3	265	248	0.03%	0.003%
23	5.677	750	753	757	rBV2	211	282	0.03%	0.004%
24	5.970	789	801	809	rBV2	330396	979600	100.00%	12.601%
25	6.482	883	885	886	rBV	215	120	0.01%	0.002%
26	6.555	895	897	898	rVV	300	219	0.02%	0.003%
27	6.598	901	904	906	rVB2	155	126	0.01%	0.002%
28	6.763	918	931	947	rBV	225739	544031	55.54%	6.998%
29	7.122	985	990	1001	rVB5	1597	3815	0.39%	0.049%
30	7.202	1001	1003	1008	rVB2	118	179	0.02%	0.002%
31	7.305	1012	1020	1035	rBV	192668	430844	43.98%	5.542%
32	7.958	1126	1127	1130	rVB2	177	123	0.01%	0.002%
33	8.061	1140	1144	1147	rBV2	126	226	0.02%	0.003%
34	8.104	1150	1151	1156	rVB2	170	157	0.02%	0.002%
35	8.323	1181	1187	1206	rBV	127251	209878	21.42%	2.700%
36	8.500	1214	1216	1217	rBV2	226	161	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041224\
 Data File : VX041053.D
 Acq On : 13 Apr 2024 00:00
 Operator : JC/MD
 Sample : P2098-03 100X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0RJ5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
 Title : VOC Analysis

37	8.549	1221	1224	1225	rVB	183	129	0.01%	0.002%
38	8.585	1227	1230	1234	rBV2	370	415	0.04%	0.005%
39	8.646	1234	1240	1258	rBV	497121	796714	81.33%	10.248%
40	8.951	1284	1290	1299	rBV	91674	137952	14.08%	1.775%
41	9.067	1307	1309	1310	rVB	229	113	0.01%	0.001%
42	9.274	1339	1343	1348	rVV2	987	1228	0.13%	0.016%
43	9.384	1356	1361	1382	rBV	327949	491314	50.15%	6.320%
44	9.604	1395	1397	1398	rBV2	302	178	0.02%	0.002%
45	9.646	1403	1404	1406	rVB2	212	135	0.01%	0.002%
46	9.695	1409	1412	1418	rVB3	848	1190	0.12%	0.015%
47	9.780	1424	1426	1427	rBV	195	129	0.01%	0.002%
48	9.866	1438	1440	1446	rVB2	172	232	0.02%	0.003%
49	9.927	1448	1450	1451	rBV	226	155	0.02%	0.002%
50	9.969	1455	1457	1459	rVB	178	119	0.01%	0.002%
51	10.055	1465	1471	1492	rBV2	489367	827761	84.50%	10.648%
52	10.189	1492	1493	1499	rVB3	542	838	0.09%	0.011%
53	10.311	1510	1513	1520	rVB3	461	759	0.08%	0.010%
54	10.408	1526	1529	1531	rVB2	142	142	0.01%	0.002%
55	10.433	1531	1533	1535	rBV2	122	117	0.01%	0.002%
56	10.646	1565	1568	1571	rBV3	446	548	0.06%	0.007%
57	10.823	1593	1597	1599	rVB2	205	195	0.02%	0.003%
58	10.908	1608	1611	1612	rBV	166	126	0.01%	0.002%
59	10.920	1612	1613	1617	rVV2	142	133	0.01%	0.002%
60	10.963	1617	1620	1628	rVV3	386	663	0.07%	0.009%
61	11.030	1628	1631	1634	rVV	176	152	0.02%	0.002%
62	11.061	1634	1636	1639	rVV2	125	157	0.02%	0.002%
63	11.091	1639	1641	1648	rVV3	505	673	0.07%	0.009%
64	11.189	1652	1657	1671	rVV	391546	511859	52.25%	6.584%
65	11.317	1673	1678	1682	rVV	1888	2833	0.29%	0.036%
66	11.463	1698	1702	1706	rVB4	397	523	0.05%	0.007%
67	11.506	1706	1709	1712	rBV2	127	202	0.02%	0.003%
68	11.609	1725	1726	1730	rVB	181	114	0.01%	0.001%
69	11.664	1730	1735	1736	rBV2	87	118	0.01%	0.002%
70	11.713	1740	1743	1748	rVV	240	350	0.04%	0.005%
71	11.756	1748	1750	1754	rVB2	525	513	0.05%	0.007%
72	11.859	1765	1767	1770	rBV	223	151	0.02%	0.002%
73	11.969	1780	1785	1788	rBV2	2362	3004	0.31%	0.039%
74	12.024	1788	1794	1808	rVV	535472	747146	76.27%	9.611%
75	12.268	1832	1834	1837	rBV	240	145	0.01%	0.002%
76	12.317	1837	1842	1857	rVV	607335	814705	83.17%	10.480%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041224\
 Data File : VX041053.D
 Acq On : 13 Apr 2024 00:00
 Operator : JC/MD
 Sample : P2098-03 100X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0RJ5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM041024WMA.M
 Title : VOC Analysis

77	12.536	1876	1878	1881	rVB2	267	184	0.02%	0.002%
78	12.725	1906	1909	1911	rVB3	173	158	0.02%	0.002%
79	12.762	1911	1915	1920	rBV	4168	5423	0.55%	0.070%
80	12.877	1932	1934	1935	rVV	234	116	0.01%	0.001%
81	12.920	1939	1941	1944	rVV2	161	137	0.01%	0.002%
82	13.115	1970	1973	1976	rBV3	638	721	0.07%	0.009%
83	13.493	2034	2035	2039	rVB	188	160	0.02%	0.002%
84	13.524	2039	2040	2044	rBV2	137	139	0.01%	0.002%
85	13.591	2048	2051	2059	rVB2	2662	4154	0.42%	0.053%
86	13.694	2066	2068	2069	rBV	153	116	0.01%	0.001%
87	13.743	2075	2076	2079	rBV	163	112	0.01%	0.001%
88	13.774	2079	2081	2082	rBV	251	195	0.02%	0.003%
89	13.786	2082	2083	2084	rBV	290	144	0.01%	0.002%
90	13.859	2093	2095	2097	rBV2	182	175	0.02%	0.002%
91	13.920	2104	2105	2107	rBV	171	118	0.01%	0.002%
92	13.944	2107	2109	2110	rVV	228	176	0.02%	0.002%
93	13.969	2110	2113	2116	rVV3	564	655	0.07%	0.008%
94	14.091	2132	2133	2134	rBV	230	147	0.02%	0.002%
95	14.133	2135	2140	2144	rVV	4948	6390	0.65%	0.082%
96	14.408	2183	2185	2189	rVB	168	132	0.01%	0.002%
97	14.505	2199	2201	2203	rBV2	202	136	0.01%	0.002%
98	14.688	2230	2231	2233	rBV	197	145	0.01%	0.002%
99	15.389	2342	2346	2354	rVB5	2392	4134	0.42%	0.053%
100	15.633	2384	2386	2387	rBV2	352	250	0.03%	0.003%




Sum of corrected areas: 7774065

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041224\
Data File : VX041053.D
Acq On : 13 Apr 2024 00:00
Operator : JC/MD
Sample : P2098-03 100X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0RJ5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

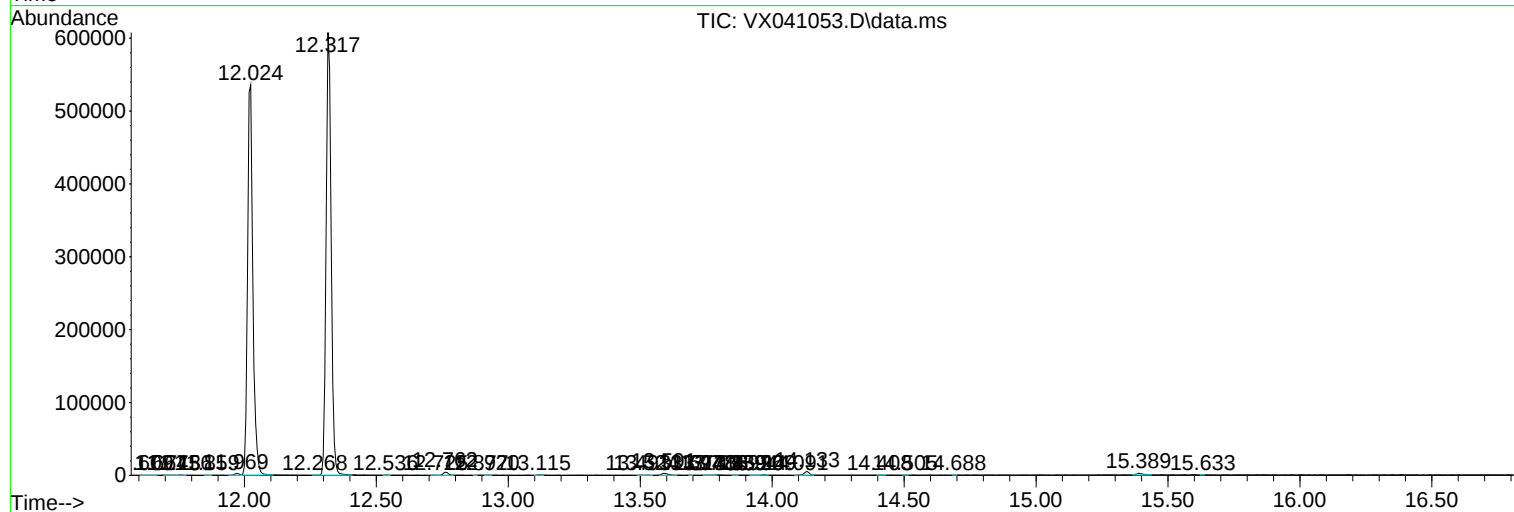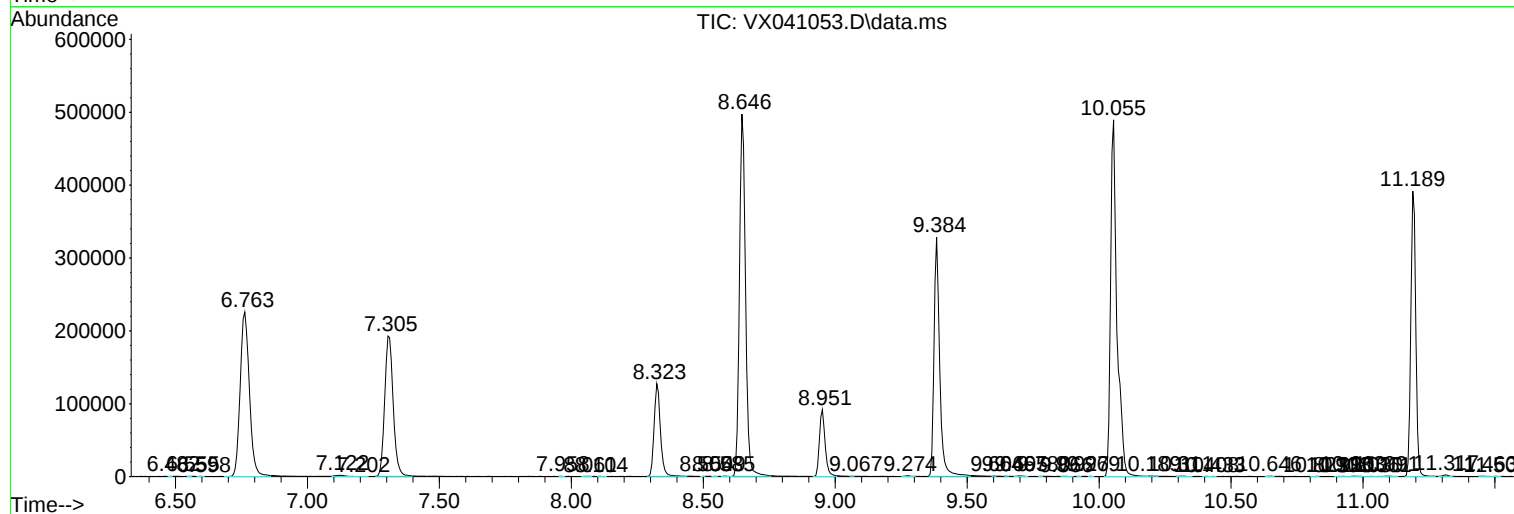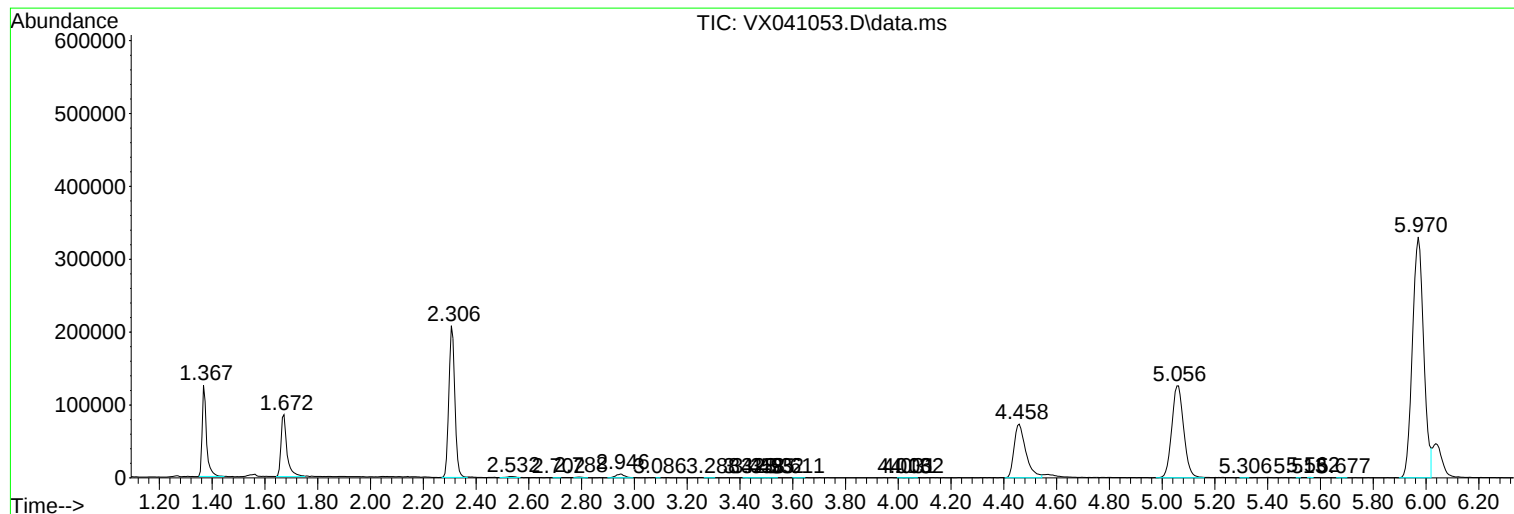

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041224\
Data File : VX041053.D
Acq On : 13 Apr 2024 00:00
Operator : JC/MD
Sample : P2098-03 100X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0RJ5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM041024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041224\
Data File : VX041053.D
Acq On : 13 Apr 2024 00:00
Operator : JC/MD
Sample : P2098-03 100X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0RJ5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------