

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041224\
 Data File : VX041054.D
 Acq On : 13 Apr 2024 00:23
 Operator : JC/MD
 Sample : P2098-04 100X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MC0R55

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M

Title : VOC Analysis

Signal : TIC: VX041054.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	42	46	57	rBV	130022	140671	1.47%	0.503%
2	1.666	91	95	112	rVB	88952	135668	1.42%	0.485%
3	2.306	194	200	209	rBV	211478	328190	3.43%	1.174%
4	2.532	230	237	246	rBV3	1946	4222	0.04%	0.015%
5	2.654	254	257	258	rBV2	144	168	0.00%	0.001%
6	2.709	264	266	269	rVB2	174	151	0.00%	0.001%
7	2.788	274	279	285	rVV3	865	1600	0.02%	0.006%
8	2.947	296	305	316	rVB	6563	15300	0.16%	0.055%
9	3.020	316	317	320	rBV2	146	109	0.00%	0.000%
10	3.099	326	330	334	rVB3	288	346	0.00%	0.001%
11	3.142	334	337	339	rBV2	160	174	0.00%	0.001%
12	3.245	352	354	355	rVB	183	114	0.00%	0.000%
13	3.349	368	371	372	rBV2	161	150	0.00%	0.001%
14	3.367	372	374	377	rVB2	118	130	0.00%	0.000%
15	3.404	377	380	382	rBV2	151	182	0.00%	0.001%
16	3.629	415	417	418	rVB	191	116	0.00%	0.000%
17	3.648	418	420	421	rBV2	170	154	0.00%	0.001%
18	3.727	431	433	439	rBV2	149	307	0.00%	0.001%
19	3.892	459	460	464	rBV2	115	143	0.00%	0.001%
20	3.983	472	475	477	rBV2	106	120	0.00%	0.000%
21	4.263	519	521	522	rVB	175	105	0.00%	0.000%
22	4.300	522	527	532	rBV4	580	1225	0.01%	0.004%
23	4.459	544	553	567	rBV2	68563	226785	2.37%	0.811%
24	4.922	628	629	633	rVB2	281	264	0.00%	0.001%
25	5.056	639	651	669	rBV	127790	400174	4.19%	1.432%
26	5.300	689	691	695	rVB	154	179	0.00%	0.001%
27	5.330	695	696	699	rBV2	103	111	0.00%	0.000%
28	5.397	702	707	710	rBV2	381	829	0.01%	0.003%
29	5.458	713	717	718	rBV3	443	573	0.01%	0.002%
30	5.562	727	734	735	rBV2	407	715	0.01%	0.003%
31	5.970	789	801	804	rBV2	338643	869169	9.09%	3.110%
32	6.038	806	812	845	rVB	2622666	6880717	71.99%	24.621%
33	6.470	881	883	888	rBB2	198	217	0.00%	0.001%
34	6.763	922	931	949	rVV	225622	543550	5.69%	1.945%
35	7.123	983	990	1001	rVB7	1860	4630	0.05%	0.017%
36	7.306	1012	1020	1042	rBV	192558	433243	4.53%	1.550%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041224\
 Data File : VX041054.D
 Acq On : 13 Apr 2024 00:23
 Operator : JC/MD
 Sample : P2098-04 100X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MC0R55

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
 Title : VOC Analysis

37	7.568	1060	1063	1064	rBV2	119	146	0.00%	0.001%
38	7.818	1102	1104	1107	rBV2	172	171	0.00%	0.001%
39	7.848	1107	1109	1112	rVB2	118	109	0.00%	0.000%
40	7.940	1123	1124	1127	rBV	140	129	0.00%	0.000%
41	8.025	1137	1138	1145	rVB2	155	238	0.00%	0.001%
42	8.074	1145	1146	1148	rBV2	169	112	0.00%	0.000%
43	8.116	1150	1153	1155	rVB2	89	117	0.00%	0.000%
44	8.208	1166	1168	1172	rBV2	91	140	0.00%	0.001%
45	8.251	1172	1175	1178	rBV2	136	214	0.00%	0.001%
46	8.324	1181	1187	1200	rBV	127932	209694	2.19%	0.750%
47	8.464	1208	1210	1214	rVB	302	282	0.00%	0.001%
48	8.580	1224	1229	1234	rBV2	437	868	0.01%	0.003%
49	8.647	1234	1240	1266	rVV	507123	802052	8.39%	2.870%
50	8.952	1285	1290	1302	rBV	90575	138383	1.45%	0.495%
51	9.275	1338	1343	1347	rBV5	1125	1538	0.02%	0.006%
52	9.384	1356	1361	1386	rBV2	312431	485294	5.08%	1.736%
53	9.708	1410	1414	1418	rVB3	619	961	0.01%	0.003%
54	9.756	1421	1422	1426	rBV2	203	174	0.00%	0.001%
55	9.823	1432	1433	1435	rBV	196	200	0.00%	0.001%
56	9.897	1442	1445	1448	rVB2	148	178	0.00%	0.001%
57	10.079	1465	1475	1503	rBV	6701047	9558338	100.00%	34.202%
58	10.531	1547	1549	1552	rBV	221	301	0.00%	0.001%
59	10.921	1607	1613	1614	rBV2	197	289	0.00%	0.001%
60	10.963	1617	1620	1623	rBV2	439	570	0.01%	0.002%
61	11.091	1637	1641	1646	rVB4	744	965	0.01%	0.003%
62	11.189	1652	1657	1672	rBV	390611	501972	5.25%	1.796%
63	11.311	1674	1677	1683	rVB	2139	2907	0.03%	0.010%
64	11.366	1683	1686	1689	rBV2	454	557	0.01%	0.002%
65	11.457	1698	1701	1706	rBV2	448	571	0.01%	0.002%
66	11.524	1711	1712	1715	rBV	129	122	0.00%	0.000%
67	11.707	1739	1742	1746	rVB2	293	368	0.00%	0.001%
68	11.756	1746	1750	1755	rBV3	405	597	0.01%	0.002%
69	11.829	1760	1762	1766	rBV2	111	159	0.00%	0.001%
70	11.884	1770	1771	1774	rBV2	140	120	0.00%	0.000%
71	11.933	1777	1779	1780	rVB	198	118	0.00%	0.000%
72	11.969	1780	1785	1789	rBV	91868	112558	1.18%	0.403%
73	12.036	1789	1796	1808	rVB2	2333826	3603727	37.70%	12.895%
74	12.329	1837	1844	1856	rBV2	1397072	2394182	25.05%	8.567%
75	12.683	1901	1902	1905	rBV	142	121	0.00%	0.000%
76	12.762	1909	1915	1920	rBV2	4717	6583	0.07%	0.024%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041224\
 Data File : VX041054.D
 Acq On : 13 Apr 2024 00:23
 Operator : JC/MD
 Sample : P2098-04 100X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MC0R55

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
 Title : VOC Analysis

77	12.859	1930	1931	1934	rVB2	135	128	0.00%	0.000%
78	12.927	1939	1942	1946	rVV2	236	336	0.00%	0.001%
79	12.975	1948	1950	1951	rVV2	198	117	0.00%	0.000%
80	12.994	1951	1953	1956	rVB2	151	157	0.00%	0.001%
81	13.067	1962	1965	1966	rBV2	152	177	0.00%	0.001%
82	13.085	1966	1968	1969	rVV	195	131	0.00%	0.000%
83	13.122	1969	1974	1977	rVV3	573	726	0.01%	0.003%
84	13.372	2012	2015	2017	rBV2	137	182	0.00%	0.001%
85	13.481	2031	2033	2036	rBV2	156	155	0.00%	0.001%
86	13.591	2046	2051	2059	rBV	81158	108653	1.14%	0.389%
87	13.780	2079	2082	2087	rBV2	690	947	0.01%	0.003%
88	13.817	2087	2088	2091	rVB	251	142	0.00%	0.001%
89	13.853	2093	2094	2097	rBV	228	219	0.00%	0.001%
90	13.896	2099	2101	2105	rVV3	185	236	0.00%	0.001%
91	13.963	2108	2112	2120	rVB2	4138	5514	0.06%	0.020%
92	14.134	2135	2140	2146	rVB	5153	6922	0.07%	0.025%
93	14.201	2149	2151	2153	rVB2	249	223	0.00%	0.001%
94	14.225	2153	2155	2160	rBV3	190	391	0.00%	0.001%
95	14.268	2160	2162	2165	rBV2	190	215	0.00%	0.001%
96	14.701	2231	2233	2235	rBV2	270	198	0.00%	0.001%
97	14.737	2238	2239	2244	rBV3	339	497	0.01%	0.002%
98	14.835	2254	2255	2258	rBV	392	274	0.00%	0.001%
99	15.389	2343	2346	2352	rVB2	2266	3266	0.03%	0.012%
100	16.609	2544	2546	2549	rBV3	392	309	0.00%	0.001%




Sum of corrected areas: 27946741

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041224\
Data File : VX041054.D
Acq On : 13 Apr 2024 00:23
Operator : JC/MD
Sample : P2098-04 100X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MC0R55

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

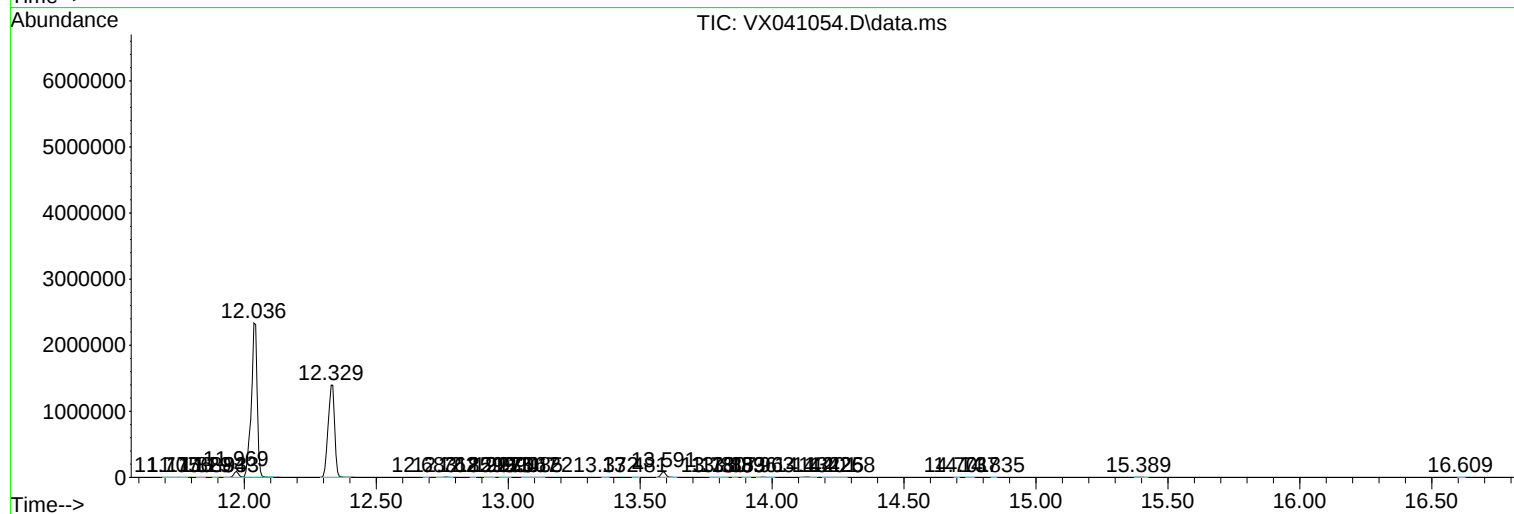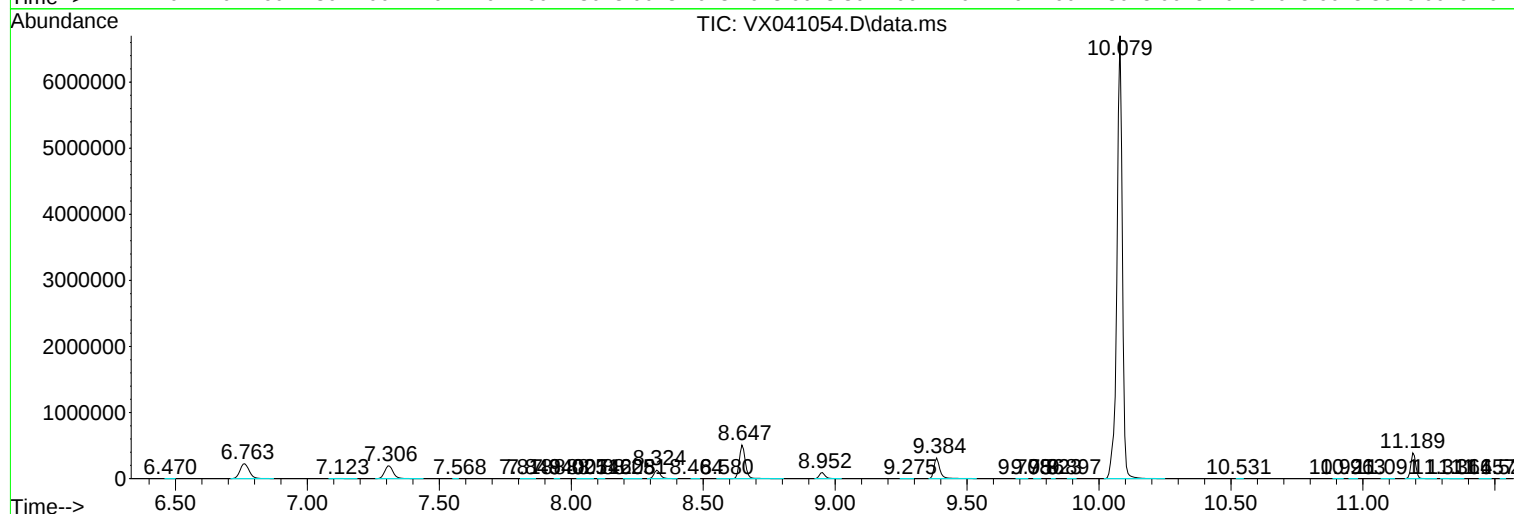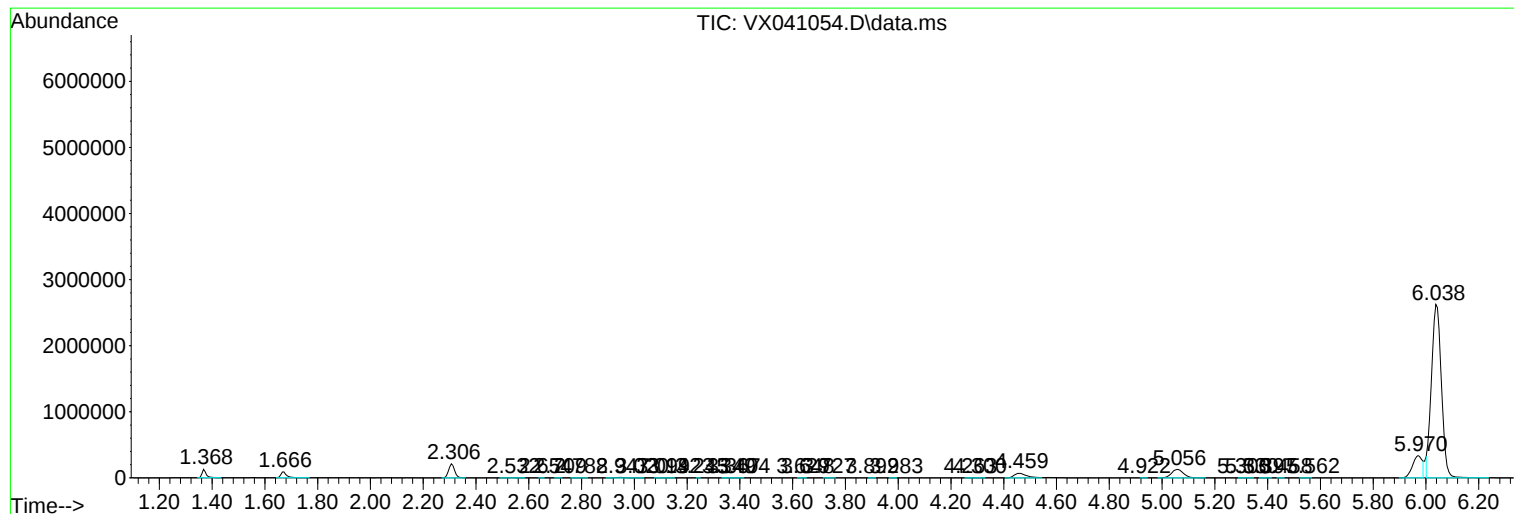

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041224\
Data File : VX041054.D
Acq On : 13 Apr 2024 00:23
Operator : JC/MD
Sample : P2098-04 100X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MC0R55

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM041024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041224\
Data File : VX041054.D
Acq On : 13 Apr 2024 00:23
Operator : JC/MD
Sample : P2098-04 100X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MC0R55

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
