

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041224\
 Data File : VX041057.D
 Acq On : 13 Apr 2024 01:32
 Operator : JC/MD
 Sample : P2098-09 100X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MCORA1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
 Title : VOC Analysis

Signal : TIC: VX041057.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	43	46	58	rVB	117882	129451	14.05%	1.841%
2	1.673	91	96	109	rBV	83041	127562	13.84%	1.814%
3	2.307	194	200	210	rBV	190405	292779	31.77%	4.164%
4	2.611	248	250	251	rBV2	167	124	0.01%	0.002%
5	2.630	251	253	256	rVB2	198	189	0.02%	0.003%
6	2.697	263	264	266	rVV2	217	174	0.02%	0.002%
7	2.739	269	271	275	rVB2	199	236	0.03%	0.003%
8	2.794	275	280	285	rBV3	1236	2386	0.26%	0.034%
9	2.947	298	305	315	rVV	5103	11486	1.25%	0.163%
10	3.203	346	347	352	rBV2	119	172	0.02%	0.002%
11	3.410	379	381	384	rBV2	144	165	0.02%	0.002%
12	3.526	398	400	403	rVB2	197	191	0.02%	0.003%
13	3.562	403	406	407	rBV2	113	119	0.01%	0.002%
14	3.709	424	430	431	rBV	229	199	0.02%	0.003%
15	3.892	459	460	463	rBV	153	114	0.01%	0.002%
16	3.928	465	466	470	rVB	152	157	0.02%	0.002%
17	3.971	471	473	476	rBV	140	134	0.01%	0.002%
18	4.306	526	528	529	rBV2	154	116	0.01%	0.002%
19	4.459	544	553	565	rBV	70297	213309	23.14%	3.034%
20	4.885	621	623	625	rBV2	178	110	0.01%	0.002%
21	4.965	634	636	638	rVB	192	138	0.01%	0.002%
22	5.056	638	651	669	rBV	121576	376370	40.84%	5.353%
23	5.373	701	703	705	rBV2	260	280	0.03%	0.004%
24	5.483	720	721	724	rBV2	148	133	0.01%	0.002%
25	5.550	729	732	733	rBV2	270	308	0.03%	0.004%
26	5.769	767	768	771	rVB	182	130	0.01%	0.002%
27	5.971	789	801	822	rBV2	306138	921652	100.00%	13.109%
28	6.385	865	869	871	rBV2	143	177	0.02%	0.003%
29	6.440	876	878	880	rBV	123	115	0.01%	0.002%
30	6.544	893	895	901	rVB3	313	385	0.04%	0.005%
31	6.690	917	919	920	rBV2	153	122	0.01%	0.002%
32	6.763	922	931	942	rBV	209449	502034	54.47%	7.141%
33	7.117	984	989	997	rVB5	1572	3723	0.40%	0.053%
34	7.306	1011	1020	1035	rBV	185494	411398	44.64%	5.851%
35	7.586	1062	1066	1068	rVB2	178	167	0.02%	0.002%
36	7.708	1084	1086	1087	rVB	242	134	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041224\
 Data File : VX041057.D
 Acq On : 13 Apr 2024 01:32
 Operator : JC/MD
 Sample : P2098-09 100X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MCORA1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
 Title : VOC Analysis

37	7.726	1087	1089	1092	rBV2	181	260	0.03%	0.004%
38	8.269	1175	1178	1180	rBV2	113	146	0.02%	0.002%
39	8.324	1181	1187	1203	rVV	118798	195692	21.23%	2.783%
40	8.580	1226	1229	1234	rBV	470	704	0.08%	0.010%
41	8.647	1234	1240	1260	rVV	457519	725267	78.69%	10.316%
42	8.952	1284	1290	1300	rBV	84822	128868	13.98%	1.833%
43	9.147	1321	1322	1326	rVB2	247	213	0.02%	0.003%
44	9.208	1328	1332	1336	rVB2	187	233	0.03%	0.003%
45	9.275	1339	1343	1347	rBV2	870	1203	0.13%	0.017%
46	9.385	1355	1361	1375	rBV	306094	465840	50.54%	6.626%
47	9.702	1408	1413	1420	rVB3	963	1774	0.19%	0.025%
48	9.848	1435	1437	1439	rVB2	157	140	0.02%	0.002%
49	9.872	1439	1441	1443	rBV	128	118	0.01%	0.002%
50	10.055	1465	1471	1488	rBV	452411	630691	68.43%	8.970%
51	10.311	1509	1513	1516	rBV2	369	460	0.05%	0.007%
52	10.372	1521	1523	1524	rVB	188	112	0.01%	0.002%
53	10.403	1524	1528	1530	rBV	123	181	0.02%	0.003%
54	10.482	1539	1541	1543	rVB2	168	126	0.01%	0.002%
55	10.579	1555	1557	1559	rVB2	139	135	0.01%	0.002%
56	10.604	1559	1561	1562	rBV	227	165	0.02%	0.002%
57	10.647	1566	1568	1570	rVV	201	172	0.02%	0.002%
58	10.768	1586	1588	1589	rBV2	170	105	0.01%	0.001%
59	10.817	1592	1596	1597	rBV2	106	113	0.01%	0.002%
60	10.927	1611	1614	1617	rVB2	176	161	0.02%	0.002%
61	10.970	1617	1621	1625	rBV3	323	467	0.05%	0.007%
62	11.061	1634	1636	1638	rBV	106	112	0.01%	0.002%
63	11.098	1639	1642	1646	rVV3	494	793	0.09%	0.011%
64	11.189	1652	1657	1669	rVV	387203	495199	53.73%	7.043%
65	11.311	1673	1677	1682	rVV	1989	2873	0.31%	0.041%
66	11.366	1684	1686	1689	rVB2	183	146	0.02%	0.002%
67	11.457	1698	1701	1706	rVB3	440	465	0.05%	0.007%
68	11.713	1741	1743	1746	rVB2	302	246	0.03%	0.003%
69	11.756	1746	1750	1751	rBV2	274	353	0.04%	0.005%
70	11.841	1759	1764	1765	rBV2	149	224	0.02%	0.003%
71	11.890	1769	1772	1773	rBV2	179	156	0.02%	0.002%
72	11.921	1773	1777	1778	rBV2	116	123	0.01%	0.002%
73	11.969	1782	1785	1788	rBV2	935	1114	0.12%	0.016%
74	12.018	1788	1793	1803	rBV	481873	631265	68.49%	8.979%
75	12.219	1825	1826	1831	rVB2	167	107	0.01%	0.002%
76	12.317	1837	1842	1853	rBV	562422	717621	77.86%	10.207%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041224\
 Data File : VX041057.D
 Acq On : 13 Apr 2024 01:32
 Operator : JC/MD
 Sample : P2098-09 100X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MCORA1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM041024WMA.M
 Title : VOC Analysis

77	12.512	1872	1874	1877	rBB2	160	139	0.02%	0.002%
78	12.591	1885	1887	1889	rBV2	186	240	0.03%	0.003%
79	12.762	1911	1915	1920	rBV3	5199	7724	0.84%	0.110%
80	12.914	1938	1940	1942	rBV	196	197	0.02%	0.003%
81	12.951	1944	1946	1948	rBV2	142	168	0.02%	0.002%
82	13.122	1970	1974	1977	rVB	388	417	0.05%	0.006%
83	13.439	2025	2026	2029	rVB	224	144	0.02%	0.002%
84	13.469	2029	2031	2033	rVB	128	113	0.01%	0.002%
85	13.597	2048	2052	2057	rVB3	1467	1947	0.21%	0.028%
86	13.676	2061	2065	2066	rBV	150	180	0.02%	0.003%
87	13.725	2071	2073	2075	rBV2	124	115	0.01%	0.002%
88	13.792	2079	2084	2086	rBV2	419	628	0.07%	0.009%
89	13.859	2093	2095	2097	rBV2	107	117	0.01%	0.002%
90	13.884	2097	2099	2101	rVB2	237	189	0.02%	0.003%
91	13.902	2101	2102	2104	rBV2	154	141	0.02%	0.002%
92	13.969	2110	2113	2115	rBV3	454	579	0.06%	0.008%
93	14.006	2118	2119	2121	rBV2	174	112	0.01%	0.002%
94	14.067	2127	2129	2132	rBB2	166	165	0.02%	0.002%
95	14.128	2135	2139	2145	rVB	7462	10464	1.14%	0.149%
96	14.396	2181	2183	2184	rBV	235	140	0.02%	0.002%
97	14.591	2213	2215	2216	rBV2	224	158	0.02%	0.002%
98	14.609	2216	2218	2219	rBV	283	212	0.02%	0.003%
99	15.048	2287	2290	2293	rBV3	316	412	0.04%	0.006%
100	15.390	2341	2346	2355	rBV2	3209	5458	0.59%	0.078%




Sum of corrected areas: 7030741

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041224\
Data File : VX041057.D
Acq On : 13 Apr 2024 01:32
Operator : JC/MD
Sample : P2098-09 100X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MCORA1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

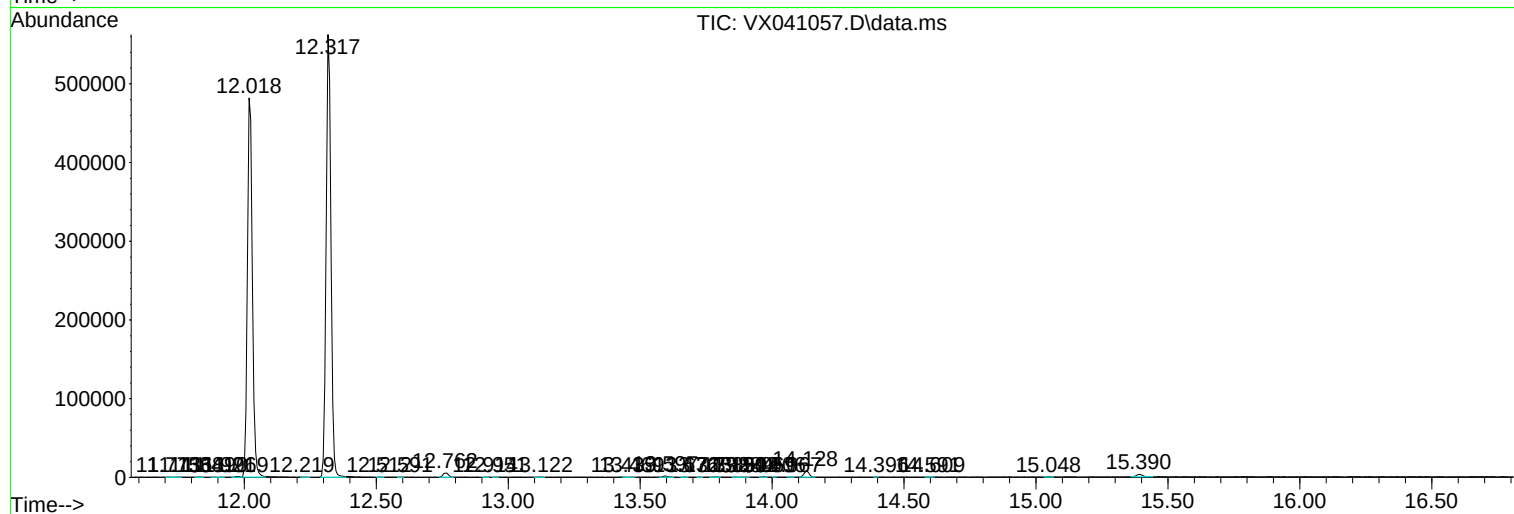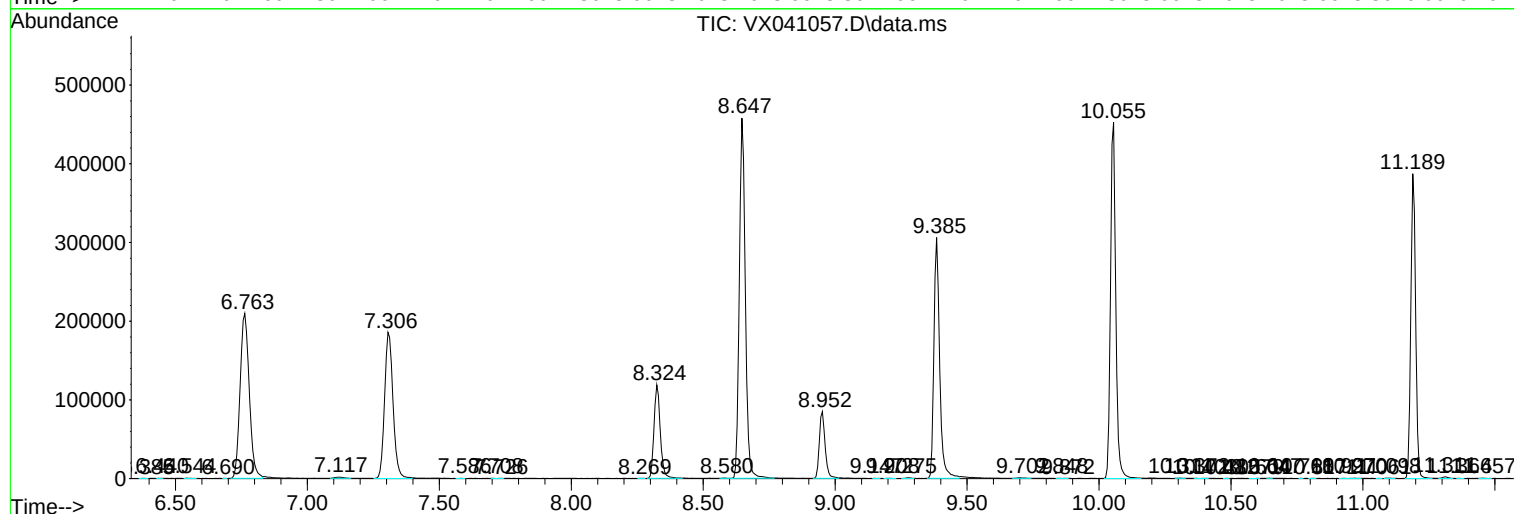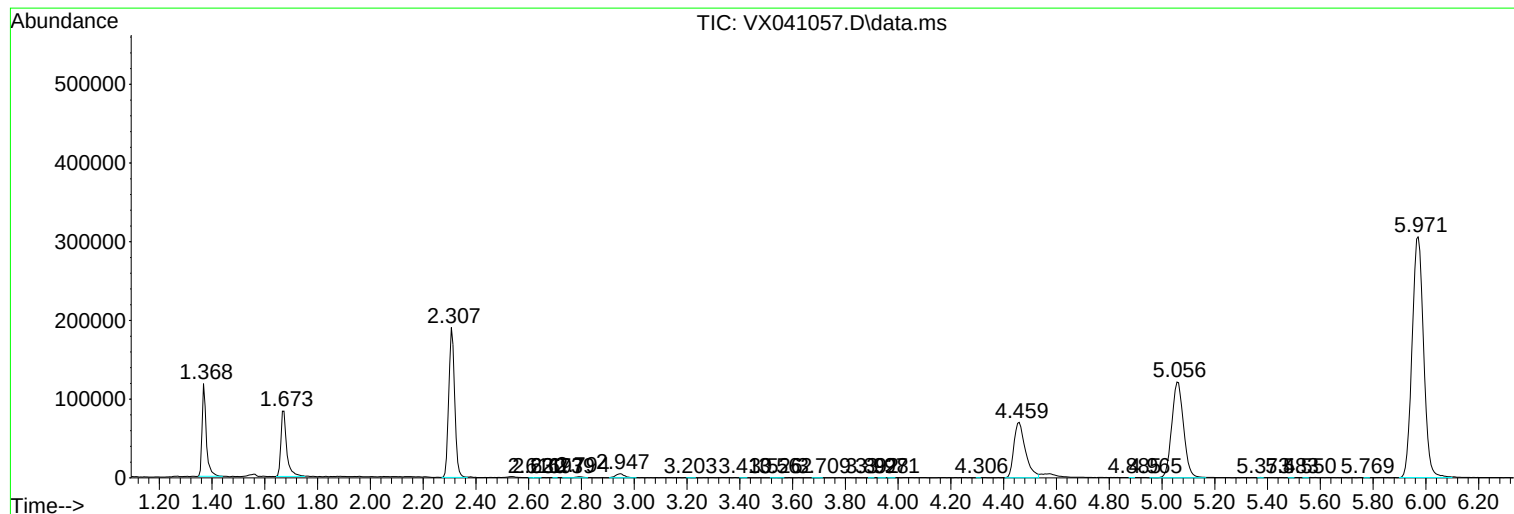

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041224\
Data File : VX041057.D
Acq On : 13 Apr 2024 01:32
Operator : JC/MD
Sample : P2098-09 100X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MC0RA1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM041024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041224\
Data File : VX041057.D
Acq On : 13 Apr 2024 01:32
Operator : JC/MD
Sample : P2098-09 100X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MC0RA1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
