

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041224\
 Data File : VX041058.D
 Acq On : 13 Apr 2024 01:55
 Operator : JC/MD
 Sample : P2098-10 100X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MC0RA2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
 Title : VOC Analysis

Signal : TIC: VX041058.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	42	46	61	rVB	132360	144976	14.45%	1.878%
2	1.666	91	95	115	rVB	92666	139334	13.89%	1.805%
3	2.306	194	200	217	rVB	215300	334102	33.31%	4.328%
4	2.788	274	279	286	rVB4	1144	2127	0.21%	0.028%
5	2.867	291	292	297	rVB	116	119	0.01%	0.002%
6	2.947	297	305	314	rVB	3742	8659	0.86%	0.112%
7	3.020	314	317	319	rBV	161	169	0.02%	0.002%
8	3.117	325	333	341	rVB3	2085	4866	0.49%	0.063%
9	3.184	341	344	346	rBV2	173	177	0.02%	0.002%
10	3.282	357	360	361	rBV	250	134	0.01%	0.002%
11	3.410	380	381	384	rVV2	150	156	0.02%	0.002%
12	3.611	411	414	416	rVV3	123	163	0.02%	0.002%
13	3.770	438	440	443	rVB2	144	152	0.02%	0.002%
14	3.812	443	447	449	rBV2	112	156	0.02%	0.002%
15	3.873	454	457	459	rBV2	152	179	0.02%	0.002%
16	3.953	466	470	472	rVB2	138	171	0.02%	0.002%
17	4.245	515	518	520	rVV	184	163	0.02%	0.002%
18	4.459	544	553	568	rBV	75379	235442	23.47%	3.050%
19	4.958	633	635	636	rBV2	207	131	0.01%	0.002%
20	5.056	639	651	668	rVV	131632	405959	40.47%	5.259%
21	5.282	686	688	691	rVB2	165	175	0.02%	0.002%
22	5.312	691	693	695	rVB	146	112	0.01%	0.001%
23	5.336	695	697	701	rBV2	194	253	0.03%	0.003%
24	5.391	701	706	710	rBV4	338	686	0.07%	0.009%
25	5.513	722	726	728	rBV2	152	206	0.02%	0.003%
26	5.532	728	729	730	rBV	193	114	0.01%	0.001%
27	5.550	730	732	734	rBV2	279	256	0.03%	0.003%
28	5.970	788	801	816	rBV2	334421	1003110	100.00%	12.995%
29	6.287	852	853	856	rBV	183	151	0.02%	0.002%
30	6.458	879	881	885	rVB	211	283	0.03%	0.004%
31	6.495	885	887	889	rBV2	173	199	0.02%	0.003%
32	6.519	889	891	894	rVV2	135	180	0.02%	0.002%
33	6.550	894	896	899	rVB3	271	192	0.02%	0.002%
34	6.580	899	901	903	rBV	136	115	0.01%	0.001%
35	6.763	921	931	949	rBV	221295	544486	54.28%	7.054%
36	7.123	982	990	997	rVB6	1636	4232	0.42%	0.055%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041224\
 Data File : VX041058.D
 Acq On : 13 Apr 2024 01:55
 Operator : JC/MD
 Sample : P2098-10 100X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MCORA2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
 Title : VOC Analysis

37	7.178	997	999	1002	rVB2	149	150	0.01%	0.002%
38	7.306	1011	1020	1037	rBV	202417	448299	44.69%	5.807%
39	7.495	1046	1051	1058	rVB2	642	1295	0.13%	0.017%
40	7.549	1058	1060	1063	rBV2	100	145	0.01%	0.002%
41	7.629	1071	1073	1076	rBV2	133	162	0.02%	0.002%
42	7.745	1090	1092	1094	rVB	128	108	0.01%	0.001%
43	7.854	1107	1110	1115	rBV2	183	383	0.04%	0.005%
44	7.958	1124	1127	1129	rBV2	191	259	0.03%	0.003%
45	8.165	1159	1161	1163	rVB	200	127	0.01%	0.002%
46	8.196	1163	1166	1169	rBV2	113	196	0.02%	0.003%
47	8.324	1181	1187	1202	rBV	130344	214991	21.43%	2.785%
48	8.574	1226	1228	1231	rBV2	317	251	0.03%	0.003%
49	8.647	1234	1240	1257	rBV	524449	823727	82.12%	10.671%
50	8.872	1276	1277	1279	rBV2	227	127	0.01%	0.002%
51	8.952	1284	1290	1301	rBV	90407	141304	14.09%	1.831%
52	9.122	1317	1318	1320	rBV	165	122	0.01%	0.002%
53	9.281	1339	1344	1349	rVB3	1074	1472	0.15%	0.019%
54	9.384	1355	1361	1380	rBV	339051	516057	51.45%	6.685%
55	9.616	1398	1399	1401	rBV2	313	153	0.02%	0.002%
56	9.701	1409	1413	1419	rBV3	599	1063	0.11%	0.014%
57	9.781	1424	1426	1427	rBV2	173	115	0.01%	0.001%
58	9.945	1452	1453	1457	rBV	81	114	0.01%	0.001%
59	10.055	1465	1471	1487	rBV	479596	684619	68.25%	8.869%
60	10.201	1491	1495	1499	rVB2	464	707	0.07%	0.009%
61	10.305	1509	1512	1516	rVB2	501	670	0.07%	0.009%
62	10.525	1546	1548	1551	rVB2	161	127	0.01%	0.002%
63	10.592	1558	1559	1562	rVB	220	129	0.01%	0.002%
64	10.640	1564	1567	1570	rBV2	361	462	0.05%	0.006%
65	10.872	1601	1605	1606	rBV2	136	147	0.01%	0.002%
66	10.970	1616	1621	1623	rVV3	316	454	0.05%	0.006%
67	11.024	1627	1630	1633	rVB2	104	134	0.01%	0.002%
68	11.098	1637	1642	1646	rBV3	597	797	0.08%	0.010%
69	11.189	1652	1657	1669	rVV	415261	531941	53.03%	6.891%
70	11.317	1673	1678	1681	rVB	2293	3098	0.31%	0.040%
71	11.390	1686	1690	1691	rBV2	121	112	0.01%	0.001%
72	11.457	1698	1701	1704	rBV2	443	598	0.06%	0.008%
73	11.707	1740	1742	1746	rBV2	274	292	0.03%	0.004%
74	11.762	1747	1751	1753	rVV	349	398	0.04%	0.005%
75	11.975	1783	1786	1788	rBV2	933	1125	0.11%	0.015%
76	12.018	1788	1793	1804	rBV	530397	689858	68.77%	8.937%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041224\
 Data File : VX041058.D
 Acq On : 13 Apr 2024 01:55
 Operator : JC/MD
 Sample : P2098-10 100X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MC0RA2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM041024WMA.M
 Title : VOC Analysis

77	12.256	1828	1832	1833	rBV2	245	237	0.02%	0.003%
78	12.317	1837	1842	1856	rBV	622454	796333	79.39%	10.316%
79	12.591	1886	1887	1889	rBV2	231	160	0.02%	0.002%
80	12.652	1893	1897	1898	rBV2	135	147	0.01%	0.002%
81	12.762	1910	1915	1921	rVB2	5080	6533	0.65%	0.085%
82	12.878	1931	1934	1935	rBV2	108	107	0.01%	0.001%
83	12.927	1941	1942	1945	rBV2	195	224	0.02%	0.003%
84	13.000	1951	1954	1955	rVB2	143	112	0.01%	0.001%
85	13.116	1971	1973	1974	rBV	436	342	0.03%	0.004%
86	13.195	1983	1986	1988	rBV2	154	149	0.01%	0.002%
87	13.335	2007	2009	2013	rVB2	162	208	0.02%	0.003%
88	13.390	2013	2018	2019	rBV2	195	295	0.03%	0.004%
89	13.445	2024	2027	2029	rVB2	159	172	0.02%	0.002%
90	13.475	2029	2032	2033	rBV2	168	170	0.02%	0.002%
91	13.597	2048	2052	2060	rVB2	1470	2137	0.21%	0.028%
92	13.658	2060	2062	2065	rBV2	169	128	0.01%	0.002%
93	13.719	2070	2072	2073	rVB2	163	112	0.01%	0.001%
94	13.786	2079	2083	2085	rBV2	232	370	0.04%	0.005%
95	13.847	2091	2093	2095	rVB	151	117	0.01%	0.002%
96	13.963	2110	2112	2116	rVB2	500	641	0.06%	0.008%
97	14.042	2123	2125	2131	rBV3	253	431	0.04%	0.006%
98	14.134	2135	2140	2145	rVB	5803	7991	0.80%	0.104%
99	14.591	2212	2215	2216	rBV	336	342	0.03%	0.004%
100	15.389	2343	2346	2351	rVB2	2318	3499	0.35%	0.045%



Sum of corrected areas: 7719330

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041224\
Data File : VX041058.D
Acq On : 13 Apr 2024 01:55
Operator : JC/MD
Sample : P2098-10 100X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MC0RA2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

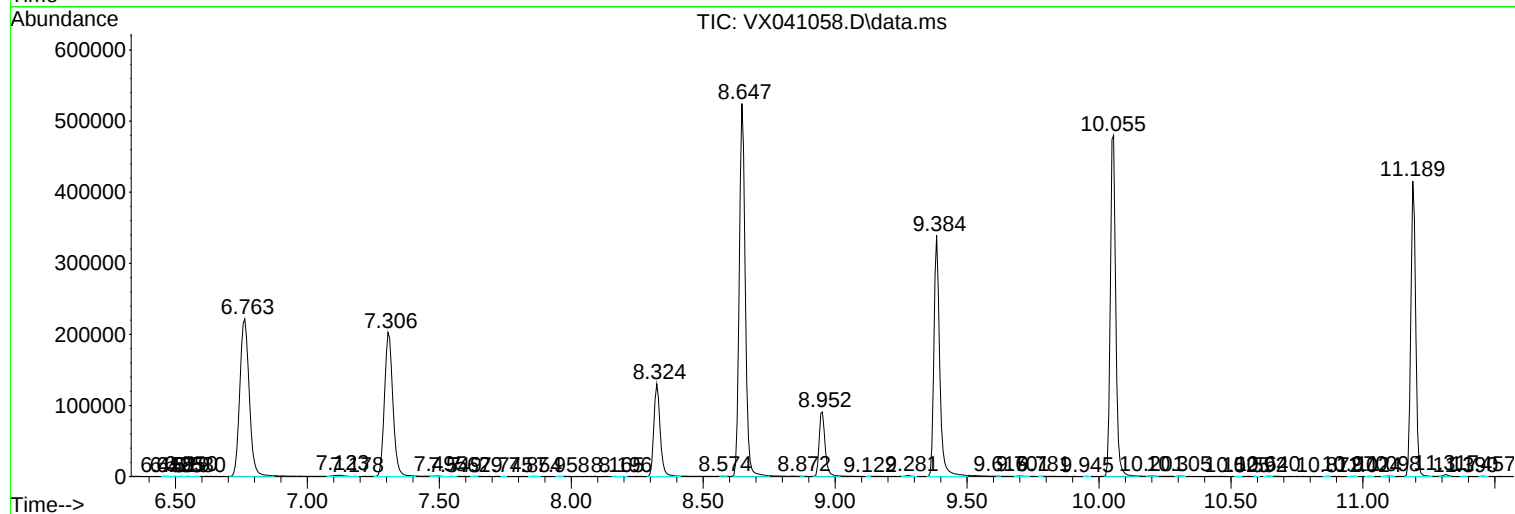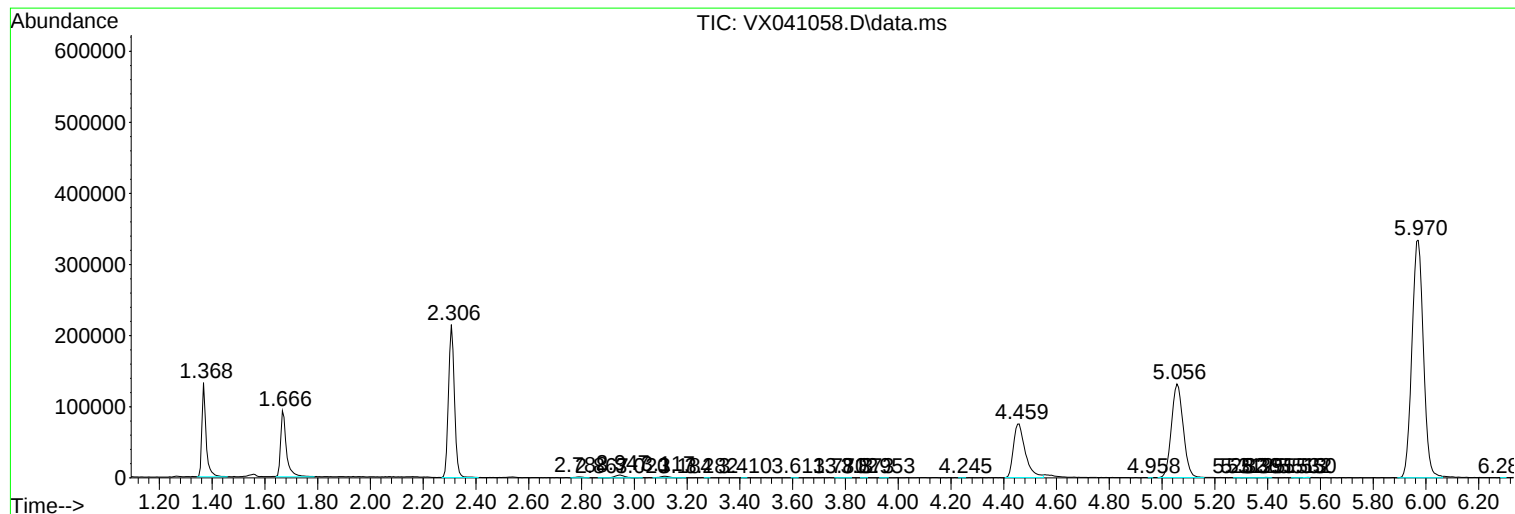

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041224\
Data File : VX041058.D
Acq On : 13 Apr 2024 01:55
Operator : JC/MD
Sample : P2098-10 100X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MC0RA2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM041024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041224\
Data File : VX041058.D
Acq On : 13 Apr 2024 01:55
Operator : JC/MD
Sample : P2098-10 100X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MC0RA2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------