

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041224\
 Data File : VX041062.D
 Acq On : 13 Apr 2024 03:27
 Operator : JC/MD
 Sample : P2098-14 100X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MC0RA9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
 Title : VOC Analysis

Signal : TIC: VX041062.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	43	46	61	rVB	113417	130255	14.24%	1.881%
2	1.673	91	96	112	rBV	85125	126169	13.80%	1.822%
3	2.307	194	200	211	rBV	190427	297700	32.55%	4.299%
4	2.471	223	227	230	rBV2	375	331	0.04%	0.005%
5	2.526	230	236	246	rVV3	1068	2829	0.31%	0.041%
6	2.624	249	252	253	rVB2	167	148	0.02%	0.002%
7	2.709	264	266	267	rVB	319	179	0.02%	0.003%
8	2.794	274	280	286	rBV4	1076	2024	0.22%	0.029%
9	2.941	298	304	316	rVB2	3006	6649	0.73%	0.096%
10	3.075	323	326	327	rBV2	104	110	0.01%	0.002%
11	3.087	327	328	330	rVV	191	136	0.01%	0.002%
12	3.117	330	333	339	rVB2	211	392	0.04%	0.006%
13	3.239	351	353	355	rBV2	146	131	0.01%	0.002%
14	3.294	360	362	364	rBV2	192	114	0.01%	0.002%
15	3.331	366	368	371	rBV2	171	170	0.02%	0.002%
16	3.441	384	386	388	rBV	169	154	0.02%	0.002%
17	3.550	398	404	407	rBV2	134	288	0.03%	0.004%
18	3.605	410	413	415	rVB2	126	126	0.01%	0.002%
19	3.642	415	419	420	rBV2	150	171	0.02%	0.002%
20	3.916	463	464	470	rVB2	108	125	0.01%	0.002%
21	4.196	508	510	512	rBV	94	132	0.01%	0.002%
22	4.239	515	517	519	rBV2	126	148	0.02%	0.002%
23	4.459	543	553	567	rBV	65616	205025	22.42%	2.960%
24	4.849	616	617	619	rVB2	204	128	0.01%	0.002%
25	4.885	621	623	624	rBV	173	130	0.01%	0.002%
26	5.056	638	651	670	rBV	120232	371274	40.60%	5.361%
27	5.233	678	680	683	rVB	213	159	0.02%	0.002%
28	5.300	686	691	693	rBV2	121	207	0.02%	0.003%
29	5.397	704	707	709	rBV	301	435	0.05%	0.006%
30	5.477	717	720	721	rBV2	138	118	0.01%	0.002%
31	5.495	721	723	726	rVB	196	127	0.01%	0.002%
32	5.757	763	766	769	rBB2	110	122	0.01%	0.002%
33	5.782	769	770	773	rBV2	146	129	0.01%	0.002%
34	5.971	789	801	819	rBV2	304166	914454	100.00%	13.204%
35	6.300	854	855	857	rVB	190	112	0.01%	0.002%
36	6.568	896	899	901	rBV2	189	212	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041224\
 Data File : VX041062.D
 Acq On : 13 Apr 2024 03:27
 Operator : JC/MD
 Sample : P2098-14 100X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MC0RA9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
 Title : VOC Analysis

37	6.763	922	931	951	rVV	192056	470213	51.42%	6.790%
38	7.117	983	989	996	rVB5	1757	4429	0.48%	0.064%
39	7.306	1012	1020	1040	rBV	182019	405626	44.36%	5.857%
40	7.671	1078	1080	1083	rVV2	210	254	0.03%	0.004%
41	7.702	1083	1085	1086	rVV2	153	118	0.01%	0.002%
42	7.720	1086	1088	1090	rVB2	204	150	0.02%	0.002%
43	7.854	1109	1110	1113	rBV2	138	116	0.01%	0.002%
44	7.946	1122	1125	1126	rBV	140	138	0.02%	0.002%
45	7.958	1126	1127	1130	rVV	207	176	0.02%	0.003%
46	8.324	1181	1187	1201	rBV	115775	193360	21.14%	2.792%
47	8.458	1207	1209	1211	rBV	395	329	0.04%	0.005%
48	8.513	1216	1218	1219	rVB2	221	109	0.01%	0.002%
49	8.647	1234	1240	1264	rBV	484598	741275	81.06%	10.704%
50	8.952	1284	1290	1304	rBV	83914	128725	14.08%	1.859%
51	9.275	1337	1343	1348	rBV	1220	1753	0.19%	0.025%
52	9.336	1351	1353	1355	rBV2	127	131	0.01%	0.002%
53	9.385	1355	1361	1383	rBV	290769	449149	49.12%	6.486%
54	9.702	1409	1413	1420	rBV3	994	1694	0.19%	0.024%
55	9.872	1439	1441	1444	rVV2	200	200	0.02%	0.003%
56	9.915	1446	1448	1451	rBV2	123	144	0.02%	0.002%
57	10.013	1462	1464	1465	rBV	188	185	0.02%	0.003%
58	10.055	1465	1471	1486	rBV	418735	589720	64.49%	8.515%
59	10.305	1510	1512	1517	rVB4	393	546	0.06%	0.008%
60	10.366	1520	1522	1525	rVB	172	137	0.01%	0.002%
61	10.470	1537	1539	1542	rBV2	99	123	0.01%	0.002%
62	10.616	1561	1563	1565	rVB	175	110	0.01%	0.002%
63	10.659	1565	1570	1571	rBV2	307	440	0.05%	0.006%
64	10.701	1575	1577	1581	rVB	198	250	0.03%	0.004%
65	10.756	1584	1586	1587	rBV2	141	118	0.01%	0.002%
66	10.829	1595	1598	1600	rBV2	196	224	0.02%	0.003%
67	10.860	1600	1603	1605	rBV2	129	161	0.02%	0.002%
68	10.970	1618	1621	1623	rBV2	389	443	0.05%	0.006%
69	11.092	1638	1641	1645	rVB3	435	620	0.07%	0.009%
70	11.189	1652	1657	1670	rVV	386480	487935	53.36%	7.046%
71	11.311	1673	1677	1683	rVB	2508	3391	0.37%	0.049%
72	11.396	1688	1691	1693	rBV2	211	167	0.02%	0.002%
73	11.457	1696	1701	1703	rBV2	259	318	0.03%	0.005%
74	11.506	1706	1709	1712	rBV2	145	214	0.02%	0.003%
75	11.707	1740	1742	1745	rBV	253	219	0.02%	0.003%
76	11.756	1748	1750	1754	rVV3	303	387	0.04%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041224\
 Data File : VX041062.D
 Acq On : 13 Apr 2024 03:27
 Operator : JC/MD
 Sample : P2098-14 100X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MC0RA9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
 Title : VOC Analysis

77	11.915	1774	1776	1779	rBV	127	174	0.02%	0.003%
78	11.969	1781	1785	1788	rBV3	1063	1484	0.16%	0.021%
79	12.018	1788	1793	1812	rVV	467532	607393	66.42%	8.771%
80	12.317	1837	1842	1852	rBV	587131	742675	81.22%	10.724%
81	12.518	1873	1875	1879	rVB2	219	232	0.03%	0.003%
82	12.555	1879	1881	1883	rBV2	130	137	0.01%	0.002%
83	12.573	1883	1884	1886	rVB2	225	125	0.01%	0.002%
84	12.689	1902	1903	1905	rBV	160	135	0.01%	0.002%
85	12.762	1910	1915	1921	rVB2	4597	5935	0.65%	0.086%
86	12.933	1941	1943	1946	rVB2	155	139	0.02%	0.002%
87	13.122	1971	1974	1977	rVB2	351	396	0.04%	0.006%
88	13.158	1977	1980	1981	rBV	148	142	0.02%	0.002%
89	13.268	1995	1998	2003	rBV2	155	268	0.03%	0.004%
90	13.384	2016	2017	2020	rVB	147	113	0.01%	0.002%
91	13.414	2020	2022	2025	rBV2	124	119	0.01%	0.002%
92	13.506	2033	2037	2040	rBV2	112	148	0.02%	0.002%
93	13.536	2040	2042	2043	rBV	159	117	0.01%	0.002%
94	13.591	2047	2051	2057	rVV	2357	3045	0.33%	0.044%
95	13.786	2081	2083	2085	rVB2	358	300	0.03%	0.004%
96	13.963	2109	2112	2122	rBV4	678	939	0.10%	0.014%
97	14.134	2132	2140	2145	rBV	7735	10807	1.18%	0.156%
98	14.207	2149	2152	2154	rBV2	240	274	0.03%	0.004%
99	14.347	2173	2175	2176	rBV	258	147	0.02%	0.002%
100	15.390	2343	2346	2352	rVB2	3615	5222	0.57%	0.075%




Sum of corrected areas: 6925376

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041224\
Data File : VX041062.D
Acq On : 13 Apr 2024 03:27
Operator : JC/MD
Sample : P2098-14 100X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 50 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MC0RA9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

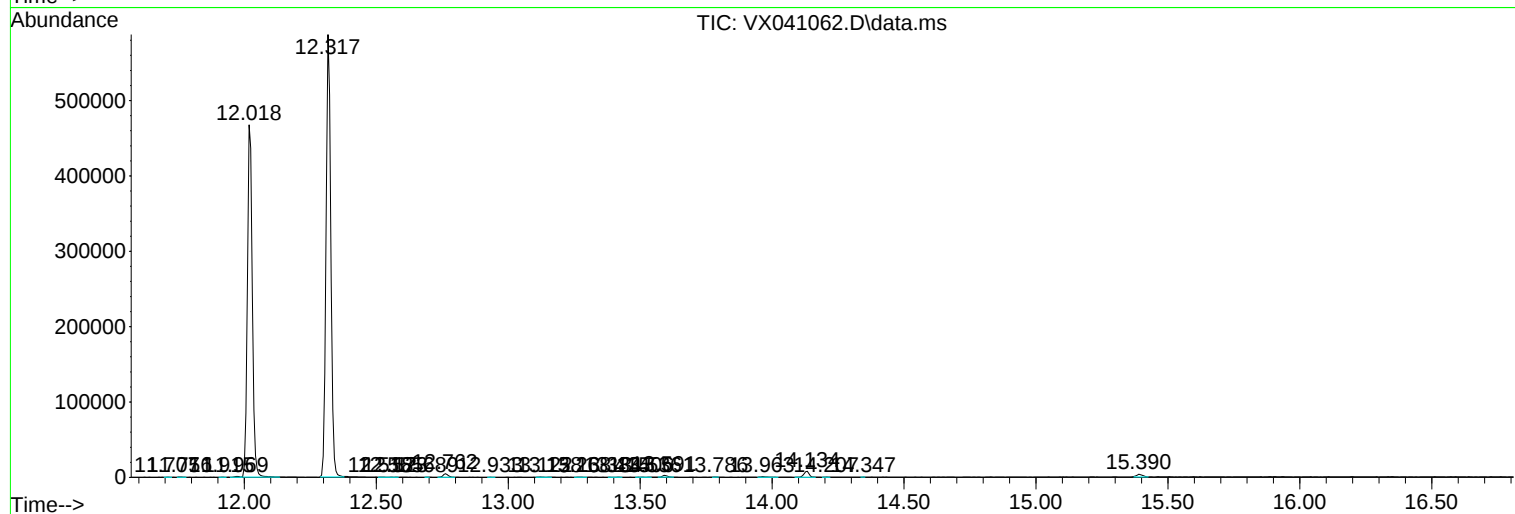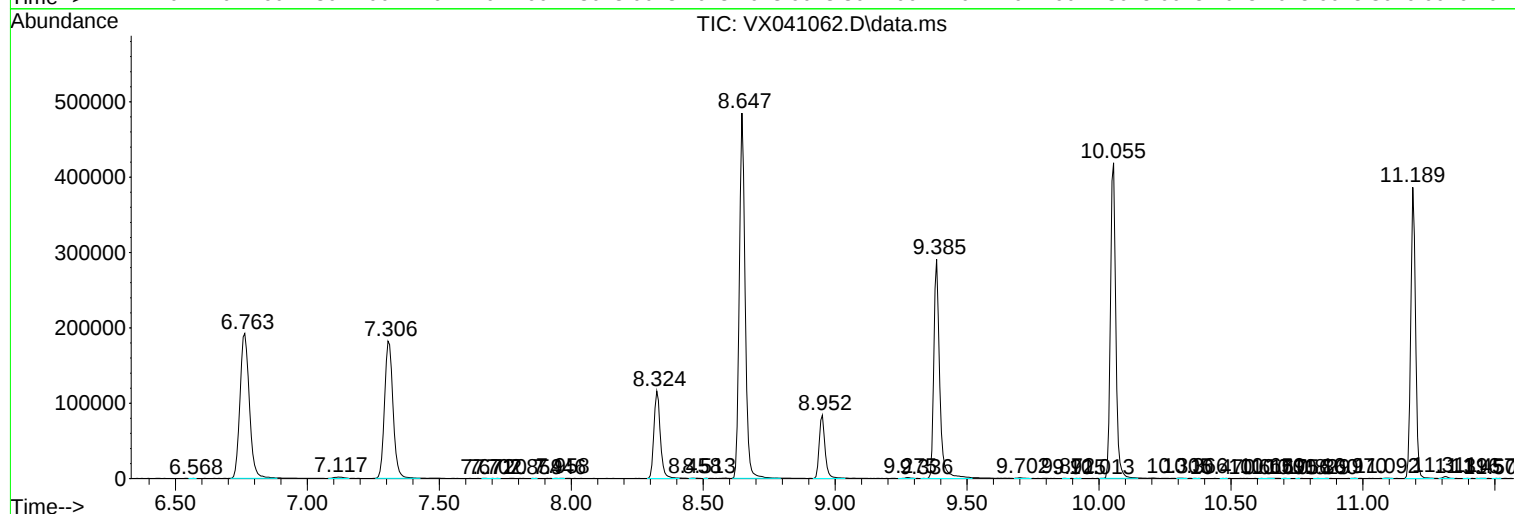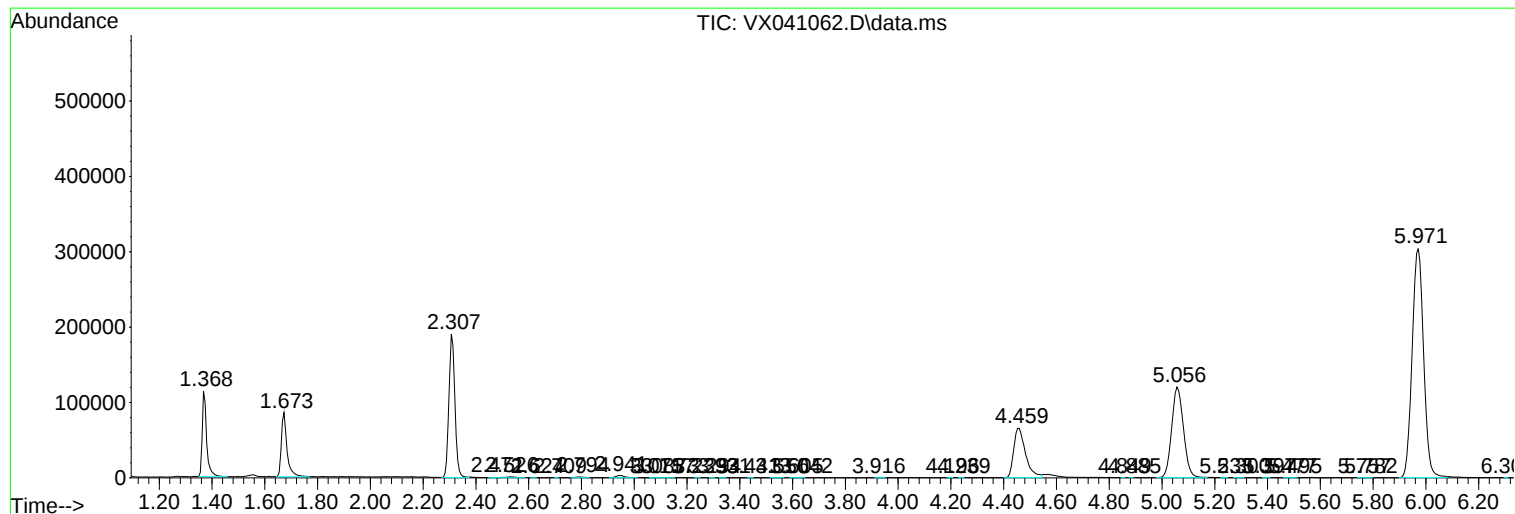

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041224\
Data File : VX041062.D
Acq On : 13 Apr 2024 03:27
Operator : JC/MD
Sample : P2098-14 100X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 50 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MC0RA9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM041024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041224\
Data File : VX041062.D
Acq On : 13 Apr 2024 03:27
Operator : JC/MD
Sample : P2098-14 100X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 50 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MC0RA9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------