

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041224\
 Data File : VX041063.D
 Acq On : 13 Apr 2024 03:50
 Operator : JC/MD
 Sample : P2098-15 100X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MCORD9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
 Title : VOC Analysis

Signal : TIC: VX041063.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.367	43	46	59	rVB	118472	135463	11.31%	1.687%
2	1.672	91	96	112	rBV	89891	130259	10.88%	1.623%
3	2.306	194	200	211	rBV	199873	311032	25.97%	3.874%
4	2.465	223	226	231	rBV2	387	591	0.05%	0.007%
5	2.526	231	236	237	rBV3	634	1022	0.09%	0.013%
6	2.593	245	247	248	rBV	209	128	0.01%	0.002%
7	2.654	253	257	260	rBV2	187	223	0.02%	0.003%
8	2.788	274	279	288	rBV3	1117	2442	0.20%	0.030%
9	2.946	296	305	313	rBV2	2400	5794	0.48%	0.072%
10	3.221	348	350	353	rBV2	104	128	0.01%	0.002%
11	3.446	385	387	391	rBV2	88	121	0.01%	0.002%
12	3.739	433	435	440	rVB2	93	151	0.01%	0.002%
13	3.879	456	458	459	rBV	195	119	0.01%	0.001%
14	4.025	479	482	483	rBV2	141	139	0.01%	0.002%
15	4.105	494	495	498	rVV	165	155	0.01%	0.002%
16	4.263	520	521	524	rBV2	167	151	0.01%	0.002%
17	4.324	529	531	533	rBV2	145	124	0.01%	0.002%
18	4.373	537	539	544	rVB2	200	278	0.02%	0.003%
19	4.452	544	552	568	rBV	66587	206226	17.22%	2.569%
20	4.879	620	622	623	rBV	223	191	0.02%	0.002%
21	4.958	632	635	638	rVB2	155	187	0.02%	0.002%
22	5.056	638	651	669	rBV	124721	381024	31.82%	4.746%
23	5.281	687	688	691	rBV2	197	134	0.01%	0.002%
24	5.385	702	705	706	rBV	271	283	0.02%	0.004%
25	5.464	713	718	720	rBV	289	328	0.03%	0.004%
26	5.556	728	733	737	rBV2	311	686	0.06%	0.009%
27	5.818	774	776	779	rBV2	140	151	0.01%	0.002%
28	5.970	789	801	822	rBV2	310816	943781	78.81%	11.756%
29	6.257	847	848	854	rVB3	231	367	0.03%	0.005%
30	6.366	863	866	867	rBV	180	176	0.01%	0.002%
31	6.452	878	880	881	rBV	158	120	0.01%	0.001%
32	6.555	895	897	899	rVB	195	122	0.01%	0.002%
33	6.763	921	931	950	rBV	208010	503184	42.02%	6.268%
34	7.110	984	988	997	rVB3	1706	4027	0.34%	0.050%
35	7.305	1012	1020	1038	rBV	189340	416653	34.79%	5.190%
36	7.464	1043	1046	1047	rBV3	137	151	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041224\
 Data File : VX041063.D
 Acq On : 13 Apr 2024 03:50
 Operator : JC/MD
 Sample : P2098-15 100X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MC0RD9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
 Title : VOC Analysis

37	7.482	1047	1049	1052	rVB2	553	579	0.05%	0.007%
38	7.671	1078	1080	1084	rVB2	187	229	0.02%	0.003%
39	7.781	1096	1098	1102	rVB	140	135	0.01%	0.002%
40	7.927	1121	1122	1125	rBV	130	135	0.01%	0.002%
41	7.951	1125	1126	1128	rVV	172	153	0.01%	0.002%
42	8.323	1181	1187	1201	rBV	118568	195230	16.30%	2.432%
43	8.646	1234	1240	1263	rBV	491019	773686	64.61%	9.637%
44	8.951	1284	1290	1305	rBV	83914	130998	10.94%	1.632%
45	9.274	1338	1343	1347	rVB2	1070	1499	0.13%	0.019%
46	9.384	1356	1361	1385	rBV	294063	448039	37.41%	5.581%
47	9.695	1411	1412	1417	rVB2	409	495	0.04%	0.006%
48	9.927	1448	1450	1453	rBV2	227	252	0.02%	0.003%
49	9.975	1457	1458	1461	rBV2	133	133	0.01%	0.002%
50	10.055	1465	1471	1491	rVV2	448249	789848	65.96%	9.838%
51	10.189	1491	1493	1495	rBV2	332	337	0.03%	0.004%
52	10.311	1509	1513	1516	rBV4	339	522	0.04%	0.007%
53	10.366	1520	1522	1524	rVB2	203	163	0.01%	0.002%
54	10.640	1564	1567	1572	rVV2	337	433	0.04%	0.005%
55	10.677	1572	1573	1576	rVV	147	149	0.01%	0.002%
56	10.731	1580	1582	1584	rBV	189	176	0.01%	0.002%
57	10.829	1596	1598	1603	rVB	146	157	0.01%	0.002%
58	10.969	1617	1621	1624	rVB2	397	510	0.04%	0.006%
59	11.024	1628	1630	1631	rBV2	164	130	0.01%	0.002%
60	11.103	1638	1643	1644	rBV4	309	455	0.04%	0.006%
61	11.189	1652	1657	1668	rBV	389707	491539	41.05%	6.123%
62	11.311	1674	1677	1683	rVB	2313	3005	0.25%	0.037%
63	11.408	1690	1693	1696	rVB2	170	165	0.01%	0.002%
64	11.463	1696	1702	1704	rBV3	315	494	0.04%	0.006%
65	11.518	1708	1711	1713	rBV2	133	118	0.01%	0.001%
66	11.561	1716	1718	1721	rBV2	151	225	0.02%	0.003%
67	11.707	1740	1742	1744	rVB	233	170	0.01%	0.002%
68	11.756	1747	1750	1755	rVB2	289	432	0.04%	0.005%
69	11.817	1759	1760	1764	rBV2	138	128	0.01%	0.002%
70	11.853	1764	1766	1768	rVB	215	172	0.01%	0.002%
71	11.884	1768	1771	1774	rVB2	153	186	0.02%	0.002%
72	11.932	1777	1779	1781	rBV	166	134	0.01%	0.002%
73	11.969	1781	1785	1789	rBV	13401	17812	1.49%	0.222%
74	12.024	1789	1794	1804	rVB	510772	722943	60.37%	9.005%
75	12.128	1810	1811	1819	rVB3	477	420	0.04%	0.005%
76	12.195	1821	1822	1823	rBV	232	153	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041224\
 Data File : VX041063.D
 Acq On : 13 Apr 2024 03:50
 Operator : JC/MD
 Sample : P2098-15 100X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MC0RD9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM041024WMA.M
 Title : VOC Analysis

77	12.323	1837	1843	1863	rVV2	703102	1197551	100.00%	14.917%
78	12.475	1866	1868	1869	rBV2	268	157	0.01%	0.002%
79	12.530	1875	1877	1880	rBV2	225	270	0.02%	0.003%
80	12.634	1892	1894	1895	rBV2	150	124	0.01%	0.002%
81	12.762	1911	1915	1920	rVV	5378	7059	0.59%	0.088%
82	12.926	1940	1942	1950	rVB2	499	684	0.06%	0.009%
83	13.072	1962	1966	1970	rBV3	312	610	0.05%	0.008%
84	13.115	1970	1973	1977	rBV2	430	671	0.06%	0.008%
85	13.207	1986	1988	1991	rVB2	178	165	0.01%	0.002%
86	13.286	1996	2001	2002	rBV2	162	195	0.02%	0.002%
87	13.414	2020	2022	2023	rBV	150	129	0.01%	0.002%
88	13.585	2045	2050	2061	rBV	106904	141306	11.80%	1.760%
89	13.835	2087	2091	2092	rBV	132	139	0.01%	0.002%
90	13.963	2107	2112	2118	rBV	22650	28367	2.37%	0.353%
91	14.030	2121	2123	2127	rVB3	155	167	0.01%	0.002%
92	14.084	2130	2132	2134	rBV2	138	134	0.01%	0.002%
93	14.133	2134	2140	2146	rBV	7381	10439	0.87%	0.130%
94	14.225	2153	2155	2156	rBV	232	172	0.01%	0.002%
95	14.261	2159	2161	2162	rVV	252	183	0.02%	0.002%
96	14.401	2183	2184	2187	rVB2	206	146	0.01%	0.002%
97	14.432	2187	2189	2190	rBV2	218	161	0.01%	0.002%
98	14.786	2244	2247	2251	rBV3	708	1053	0.09%	0.013%
99	15.249	2320	2323	2331	rBV2	2653	4082	0.34%	0.051%
100	15.395	2341	2347	2353	rBV3	3342	5659	0.47%	0.070%




Sum of corrected areas: 8028273

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041224\
Data File : VX041063.D
Acq On : 13 Apr 2024 03:50
Operator : JC/MD
Sample : P2098-15 100X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 51 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MCCORD9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

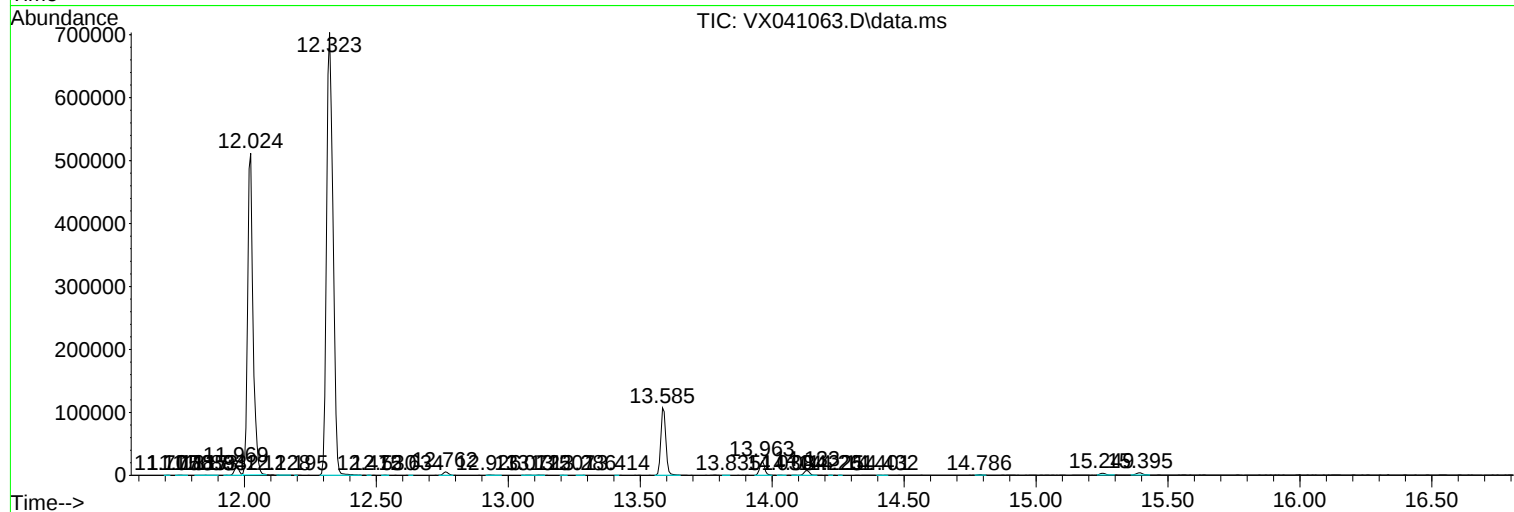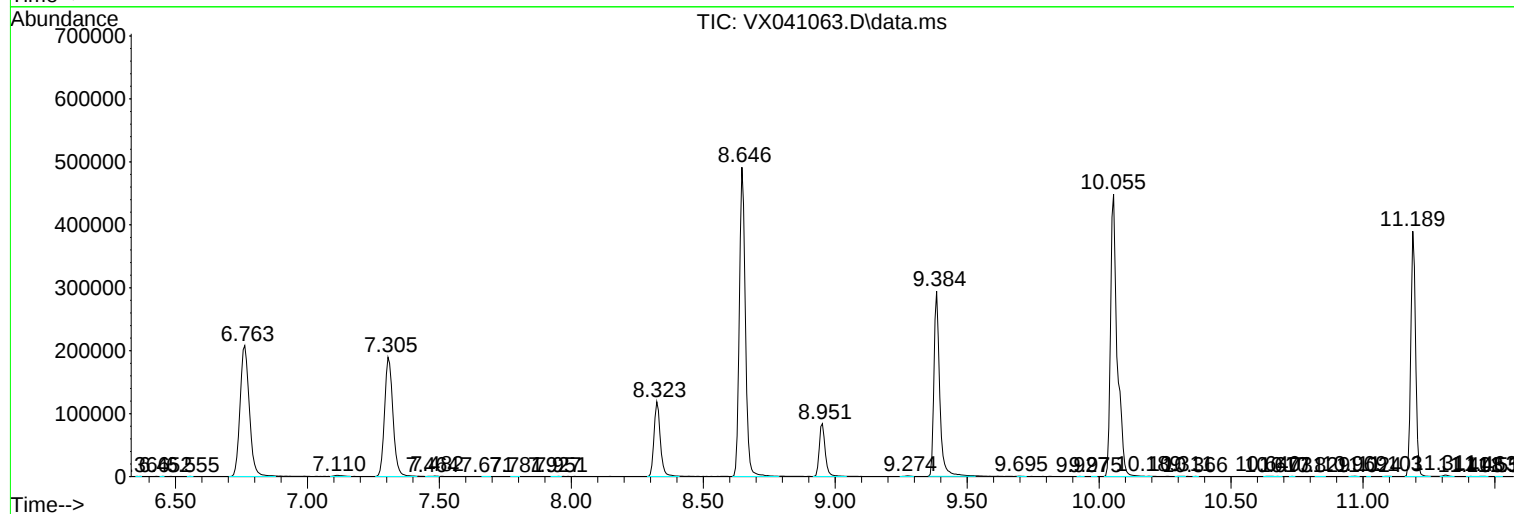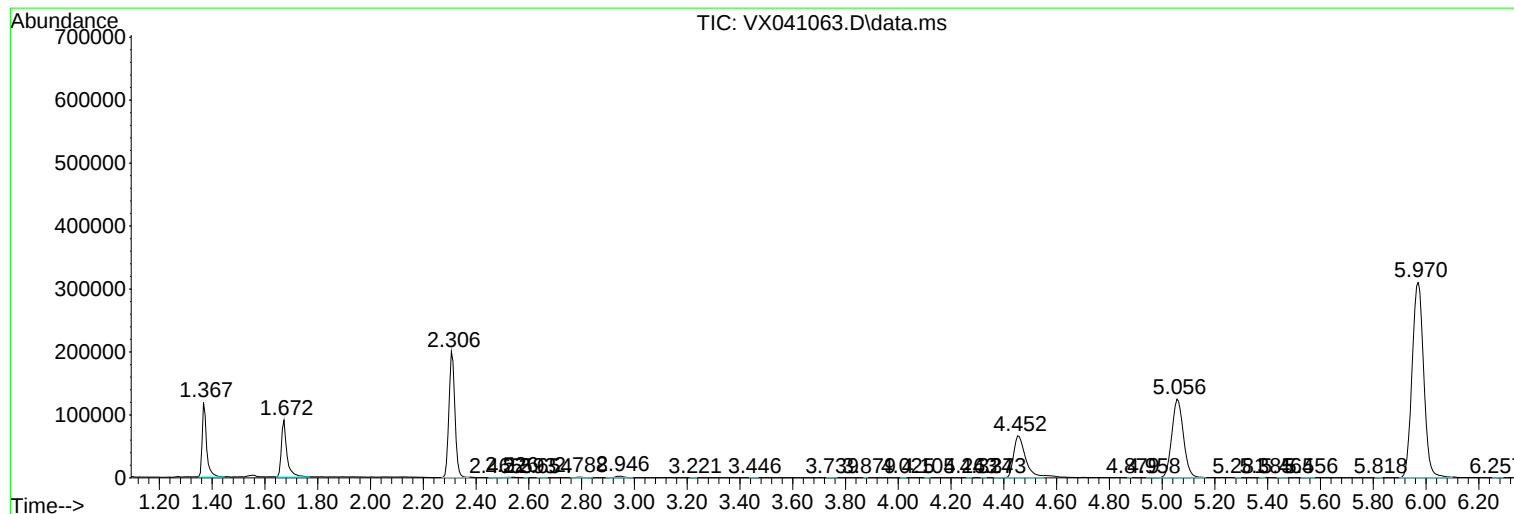

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041224\
Data File : VX041063.D
Acq On : 13 Apr 2024 03:50
Operator : JC/MD
Sample : P2098-15 100X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 51 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MC0RD9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM041024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041224\
Data File : VX041063.D
Acq On : 13 Apr 2024 03:50
Operator : JC/MD
Sample : P2098-15 100X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 51 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MC0RD9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc