
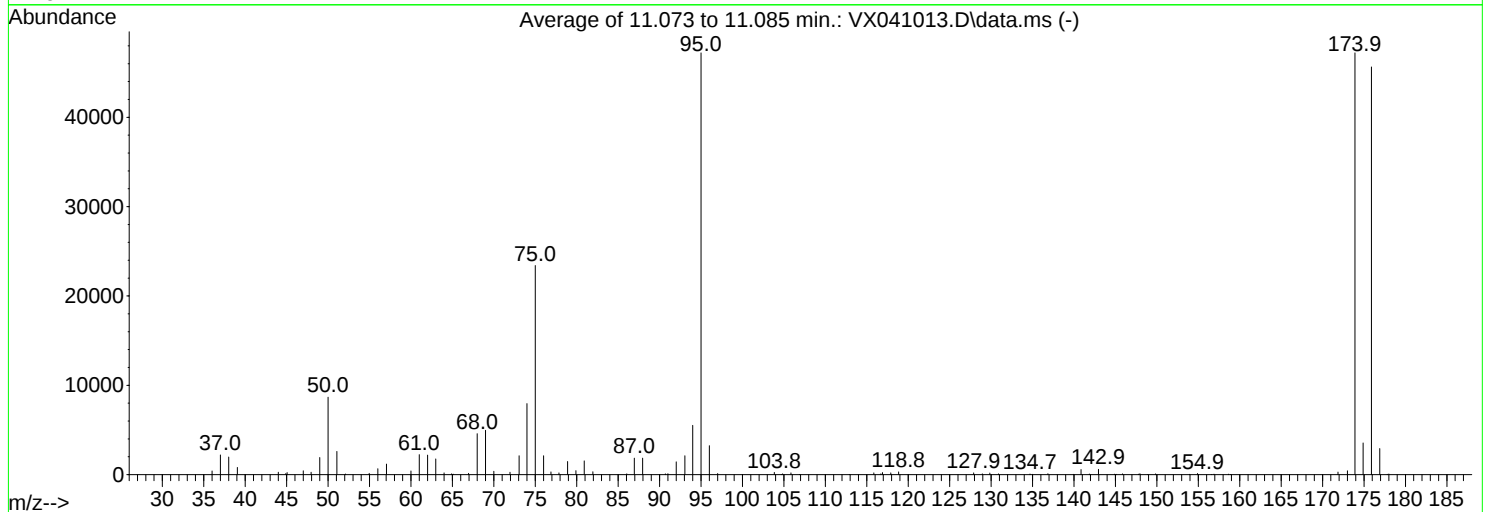


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041224\
Data File : VX041013.D
Acq On : 12 Apr 2024 08:20
Operator : JC/MD
Sample : BFB671
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB671

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
Title : VOC Analysis
Last Update : Sat Apr 13 04:06:48 2024

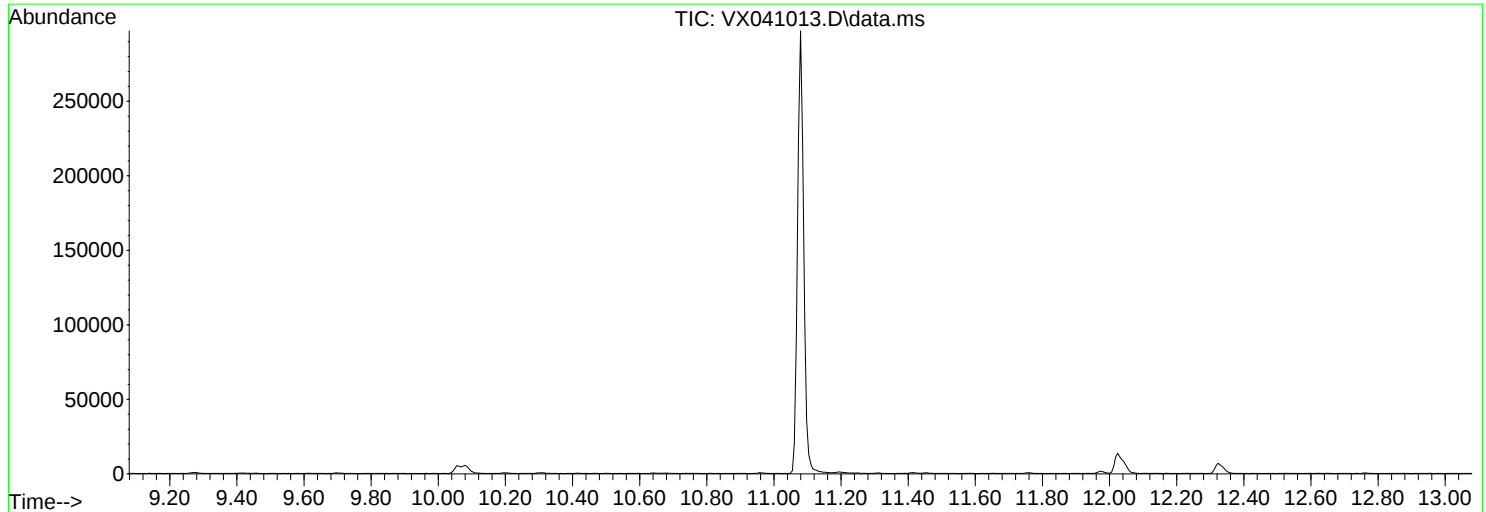

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1633

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.4	8664	PASS
75	95	30	80	49.6	23400	PASS
95	95	100	100	100.0	47203	PASS
96	95	5	9	6.9	3244	PASS
173	174	0.00	2	0.9	427	PASS
174	95	50	120	100.0	47213	PASS
175	174	5	9	7.5	3548	PASS
176	174	95	101	96.6	45629	PASS
177	176	5	9	6.4	2921	PASS

Scan 1633 (11.043 min): VX041013.D\data.ms
BFB671

m/z	Abundance
40.00	186.0
44.00	145.0

Instrument :
MSVOA_X
ClientSampleId :
BFB671

m/z	Abundance
36.00	488.0
37.00	2457.0
38.00	2117.0
39.00	856.0
40.00	166.0
44.00	445.0
44.90	394.0
47.10	459.0
47.90	305.0
49.00	1986.0
50.00	8619.0
51.10	2663.0
52.10	51.0
55.00	164.0
56.00	732.0
57.00	1160.0
60.00	478.0
61.00	2245.0
62.00	2232.0
63.00	1680.0
64.00	299.0
64.90	127.0
67.00	131.0
68.00	4297.0
69.00	4620.0
70.00	325.0
71.90	269.0
73.00	1940.0
74.00	8106.0
75.00	22936.0
76.00	2093.0
76.90	320.0
77.80	187.0
78.90	1420.0
79.90	543.0
80.90	1563.0
82.00	379.0
86.00	79.0
87.00	1814.0
88.00	1902.0
91.00	180.0
92.00	1193.0
93.00	1926.0
94.00	5168.0
95.00	44608.0
96.00	3134.0
97.10	135.0
103.80	269.0
104.70	65.0
104.90	61.0
105.90	162.0
115.80	165.0
116.70	290.0
117.80	192.0
118.80	320.0
127.90	173.0
128.90	82.0
129.90	149.0
131.00	82.0
135.00	86.0
136.80	102.0
139.90	52.0
140.80	573.0
141.90	114.0
143.00	451.0
144.90	75.0
145.80	82.0
147.80	180.0
149.80	57.0
153.90	59.0
154.90	144.0
157.00	76.0
158.60	57.0
171.90	280.0
173.90	38912.0
174.90	2801.0
175.90	37096.0
176.90	2362.0
177.80	118.0

Instrument :
MSVOA_X
ClientSampleId :
BFB671

m/z	Abundance
36.00	453.0
37.00	2580.0
38.00	2342.0
39.10	899.0
40.10	260.0
44.00	539.0
45.10	429.0
46.90	519.0
48.00	361.0
49.00	2408.0
50.00	10084.0
51.00	3091.0
52.10	92.0
54.90	163.0
56.00	736.0
57.00	1478.0
60.00	513.0
61.00	2656.0
62.00	2274.0
63.00	2175.0
64.00	138.0
64.90	143.0
66.90	172.0
68.00	5593.0
69.00	5901.0
70.10	402.0
72.00	245.0
73.00	2616.0
74.00	9434.0
75.00	27992.0
76.00	2702.0
77.00	384.0
77.90	283.0
78.90	1722.0
79.90	441.0
80.90	1889.0
82.00	339.0
86.10	115.0
87.00	2291.0
88.00	2207.0
90.70	252.0
92.00	1755.0
93.10	2440.0
94.00	6702.0
95.00	57040.0
96.00	3814.0
96.90	202.0
103.80	262.0
104.90	104.0
105.80	270.0
106.90	81.0
112.90	50.0
115.90	243.0
116.90	400.0
117.90	214.0
118.90	313.0
127.90	230.0
129.00	85.0
129.80	190.0
130.80	134.0
134.70	120.0
136.80	137.0
140.00	72.0
140.80	568.0
141.80	121.0
143.00	740.0
145.10	87.0
145.80	109.0
148.00	127.0
149.90	115.0
154.00	51.0
154.90	129.0
156.80	107.0
158.70	85.0
171.80	356.0
173.00	790.0
173.90	56288.0
174.90	4290.0
175.90	55168.0
176.90	3730.0
178.00	135.0

Instrument :
MSVOA_X
ClientSampleId :
BFB671

m/z	Abundance
36.00	293.0
37.10	1596.0
38.00	1451.0
39.00	645.0
40.10	173.0
44.10	285.0
45.00	290.0
47.00	318.0
48.00	151.0
49.00	1371.0
50.00	7290.0
51.00	2037.0
52.10	77.0
55.00	103.0
56.00	539.0
57.10	890.0
60.00	242.0
61.00	1820.0
62.00	2042.0
63.00	1402.0
64.00	160.0
65.10	146.0
67.00	116.0
68.00	3877.0
69.00	4341.0
69.90	380.0
71.90	293.0
73.10	1796.0
74.00	6296.0
75.00	19272.0
76.00	1528.0
76.80	209.0
77.90	152.0
78.90	1249.0
79.90	380.0
80.90	1145.0
81.80	271.0
86.10	62.0
86.90	1425.0
87.90	1417.0
91.00	139.0
92.00	1335.0
93.00	1997.0
94.00	4672.0
95.00	39960.0
96.00	2783.0
96.90	60.0
103.90	216.0
104.80	89.0
105.90	182.0
115.80	187.0
116.90	284.0
118.00	211.0
118.90	290.0
127.90	175.0
128.90	93.0
129.90	225.0
130.80	62.0
134.70	84.0
136.90	112.0
140.90	585.0
142.80	585.0
144.90	95.0
145.90	85.0
147.90	203.0
148.90	59.0
149.90	88.0
154.90	94.0
156.60	64.0
158.90	70.0
171.80	219.0
173.00	490.0
173.90	46440.0
174.90	3554.0
175.90	44624.0
176.90	2670.0
178.00	68.0

Instrument :
MSVOA_X
ClientSampleId :
BFB671