


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX041320\
Data File : VX015641.D
Acq On : 13 Apr 2020 12:29
Operator : JC/SP
Sample : BFB
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X032720W.M
Title : SW846 8260
Last Update : Fri Mar 27 09:35:51 2020

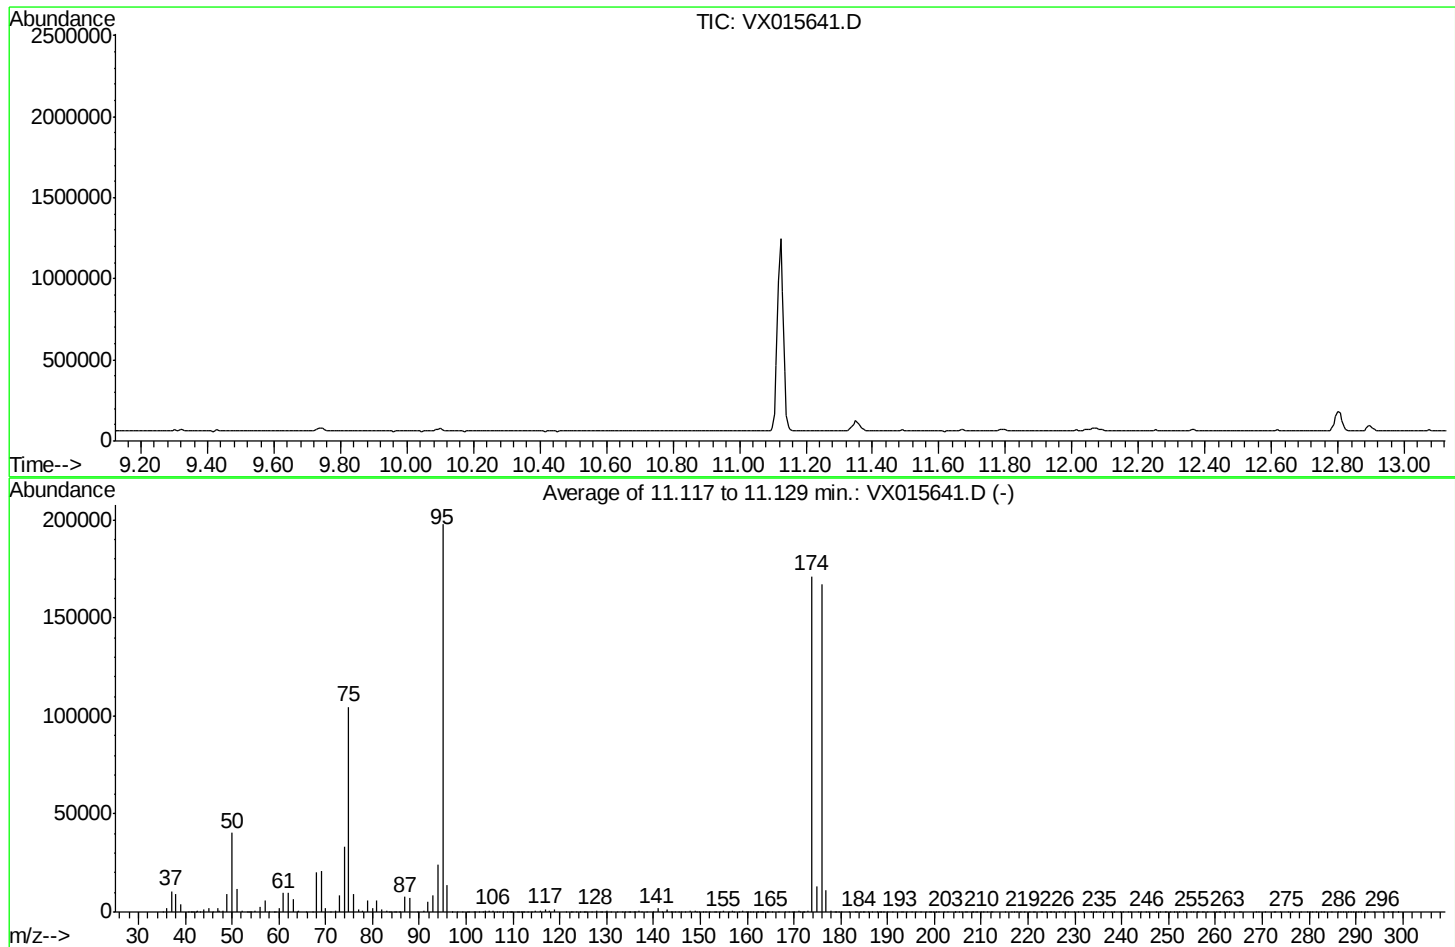

AutoFind: Scans 1678, 1679, 1680; Background Corrected with Scan 1671

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.4	40312	PASS
75	95	30	60	52.9	104666	PASS
95	95	100	100	100.0	197857	PASS
96	95	5	9	6.9	13570	PASS
173	174	0.00	2	0.4	629	PASS
174	95	50	100	86.6	171434	PASS
175	174	5	9	7.7	13168	PASS
176	174	95	101	97.7	167537	PASS
177	176	5	9	6.5	10918	PASS