

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041322\
 Data File : VX028092.D
 Acq On : 13 Apr 2022 16:00
 Operator : JC/MD
 Sample : IBLK
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 IBLK

Quant Time: Apr 14 04:06:29 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X041222W.M
 Quant Title : SW846 8260
 QLast Update : Tue Apr 12 22:07:23 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.556	168	243450	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	411974	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	376705	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	174566	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	154249	46.702	ug/l	0.00
Spiked Amount	50.000	Range	61 - 141	Recovery	=	93.400%
35) Dibromofluoromethane	5.391	113	134012	49.642	ug/l	0.00
Spiked Amount	50.000	Range	69 - 133	Recovery	=	99.280%
50) Toluene-d8	8.653	98	497981	49.461	ug/l	0.00
Spiked Amount	50.000	Range	65 - 126	Recovery	=	98.920%
62) 4-Bromofluorobenzene	11.079	95	163024	43.367	ug/l	0.00
Spiked Amount	50.000	Range	58 - 135	Recovery	=	86.740%


Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041322\
Data File : VX028092.D
Acq On : 13 Apr 2022 16:00
Operator : JC/MD
Sample : IBLK
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
IBLK

Quant Time: Apr 14 04:06:29 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X041222W.M
Quant Title : SW846 8260
QLast Update : Tue Apr 12 22:07:23 2022
Response via : Initial Calibration




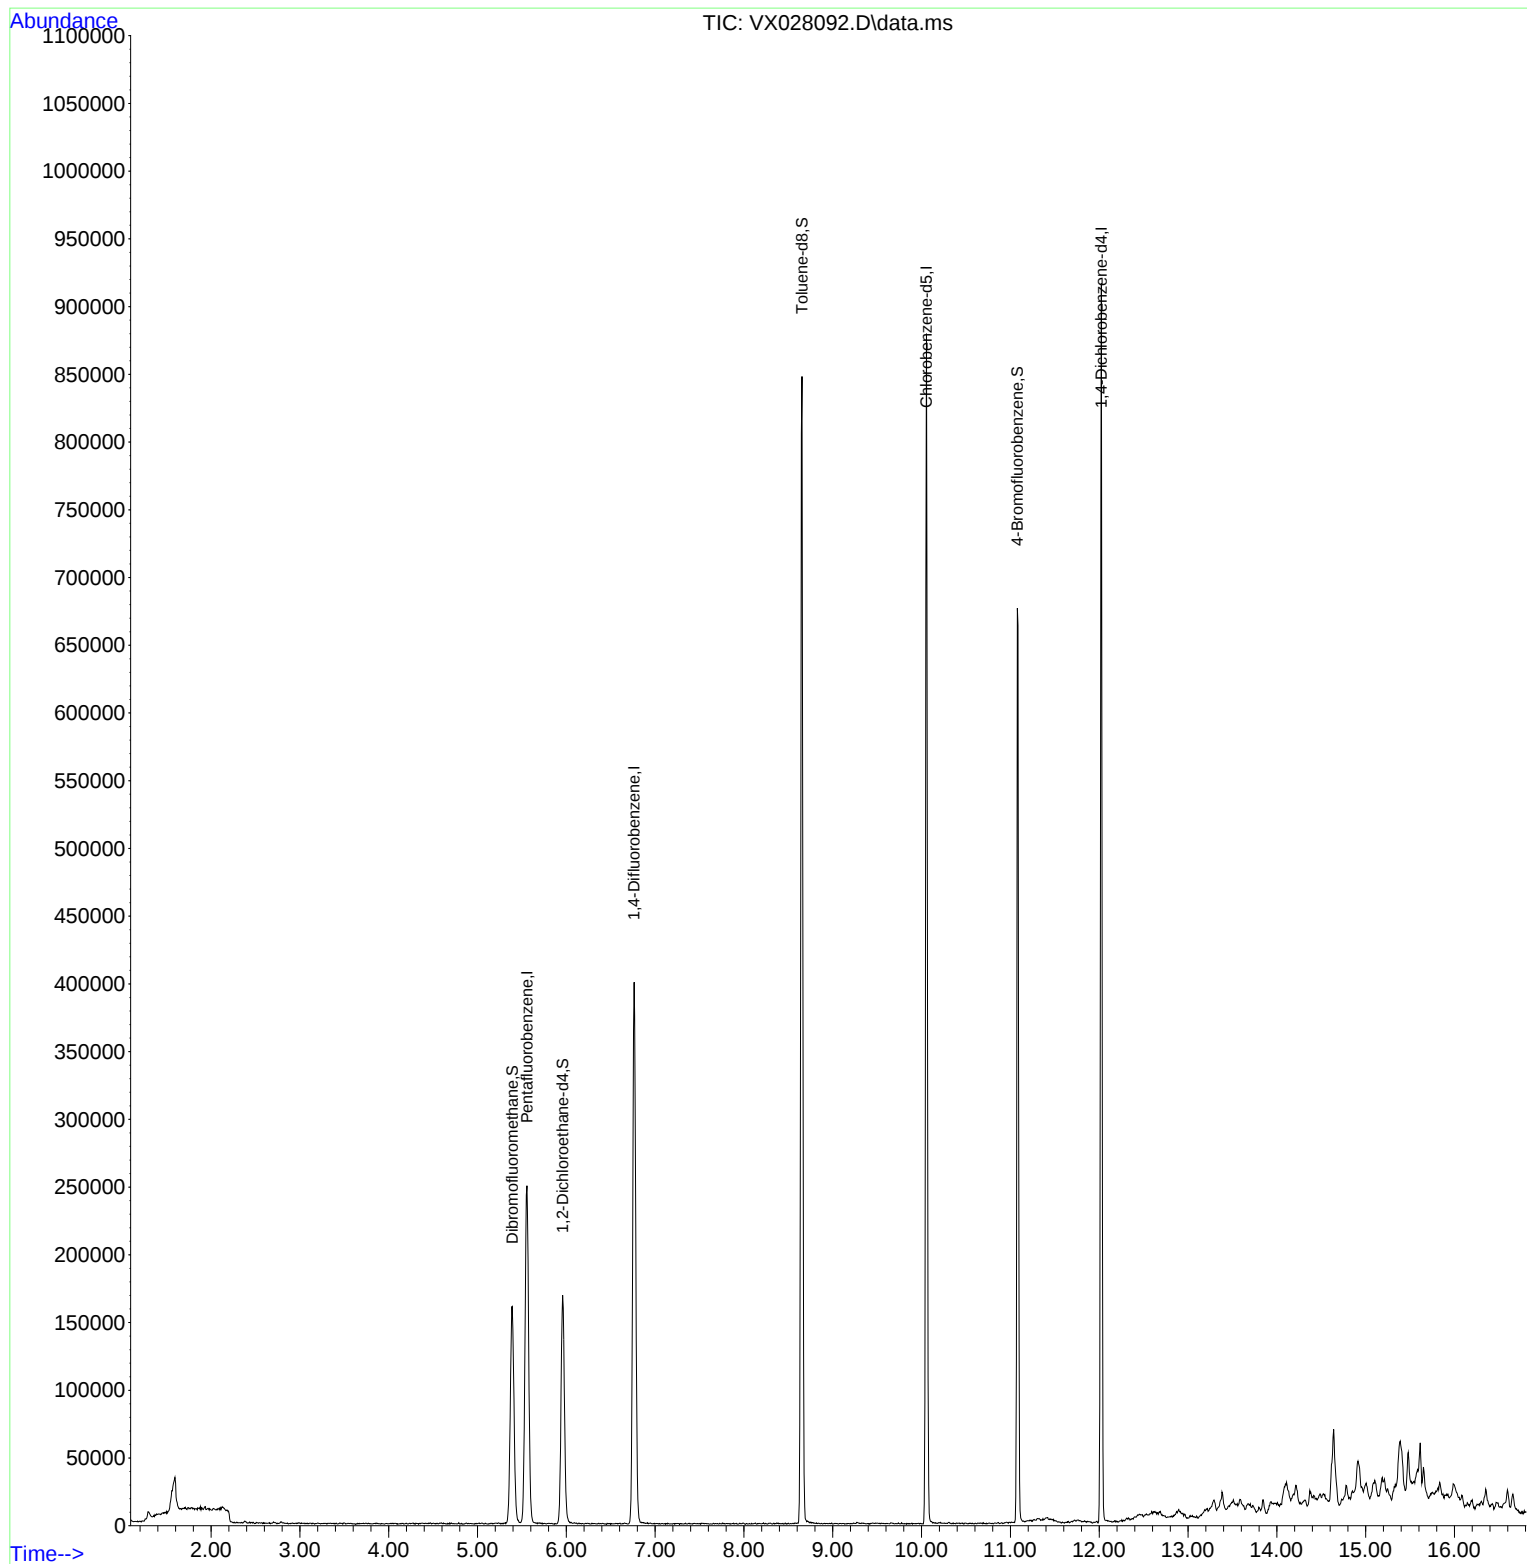




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.556 min Scan# 733
Delta R.T. -0.000 min
Lab File: VX028092.D
Acq: 13 Apr 2022 16:00




Instrument :
MSVOA_X
ClientSampleId :
IBLK


Tgt Ion:168 Resp: 243450
Ion Ratio Lower Upper
168 100
99 55.0 41.7 62.5

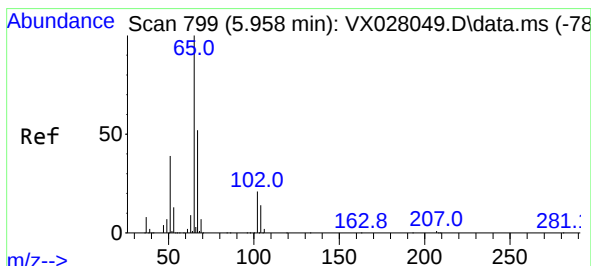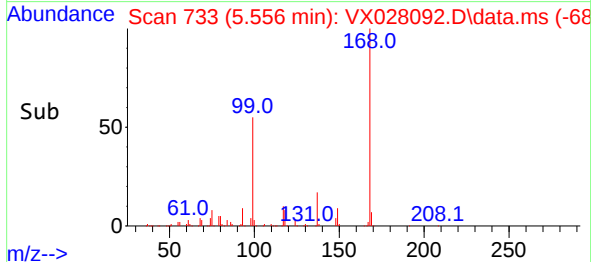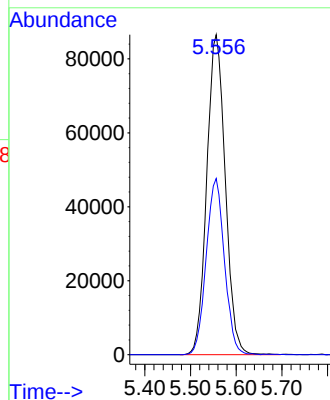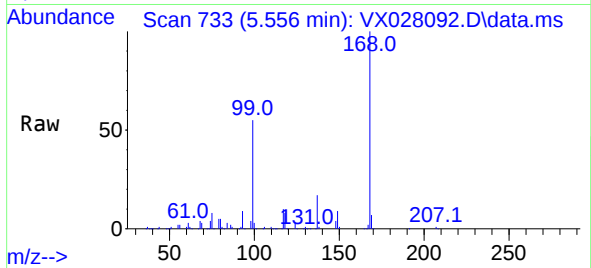

#33
1,2-Dichloroethane-d4
Concen: 46.702 ug/l
RT: 5.958 min Scan# 799
Delta R.T. 0.000 min
Lab File: VX028092.D
Acq: 13 Apr 2022 16:00

Tgt Ion: 65 Resp: 154249
Ion Ratio Lower Upper
65 100
67 52.5 0.0 107.4


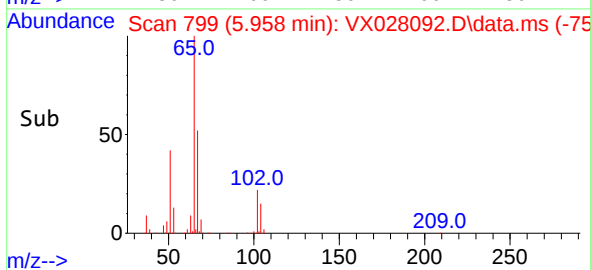
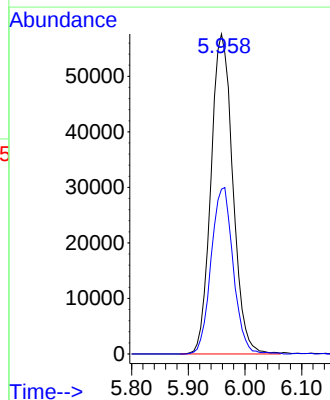
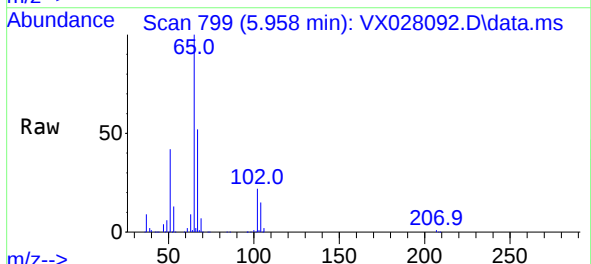


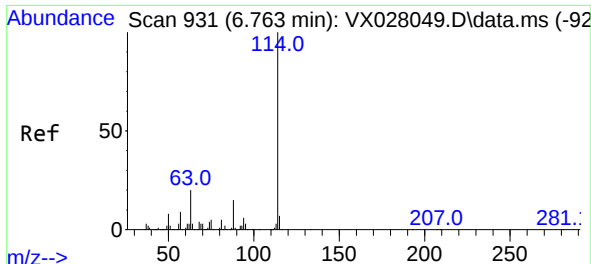

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.763 min Scan# 91
Delta R.T. 0.000 min
Lab File: VX028092.D
Acq: 13 Apr 2022 16:00




Instrument :
MSVOA_X
ClientSampleId :
IBLK


Tgt Ion:114 Resp: 411974
Ion Ratio Lower Upper
114 100
63 19.6 0.0 36.8
88 14.7 0.0 32.4

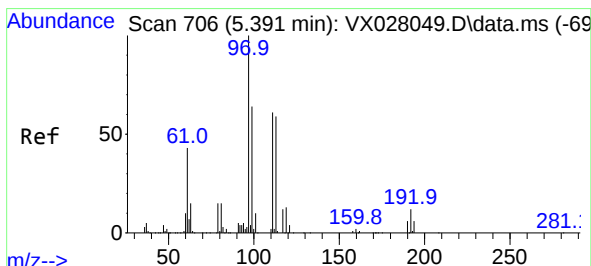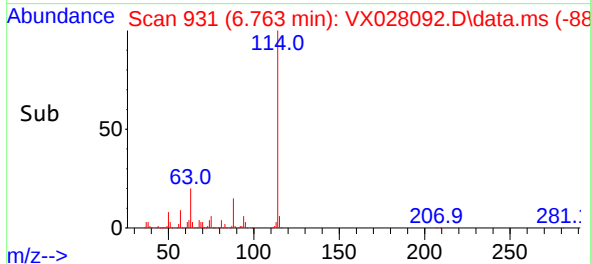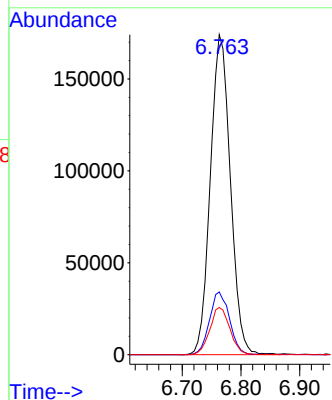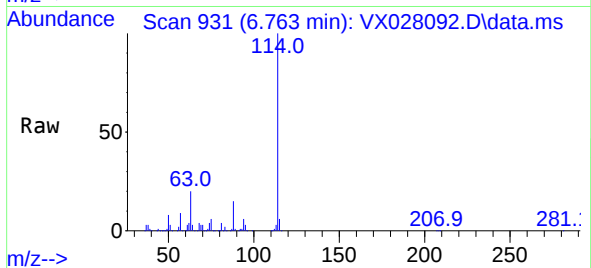

#35
Dibromofluoromethane
Concen: 49.642 ug/l
RT: 5.391 min Scan# 706
Delta R.T. 0.000 min
Lab File: VX028092.D
Acq: 13 Apr 2022 16:00

Tgt Ion:113 Resp: 134012
Ion Ratio Lower Upper
113 100
111 102.7 82.8 124.2
192 19.7 16.9 25.3


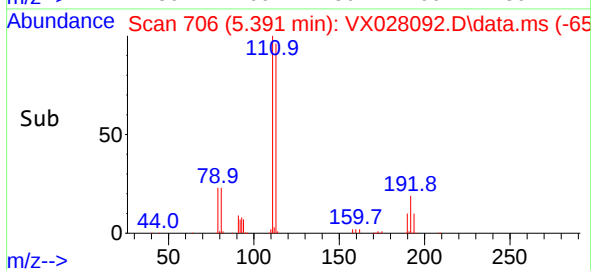
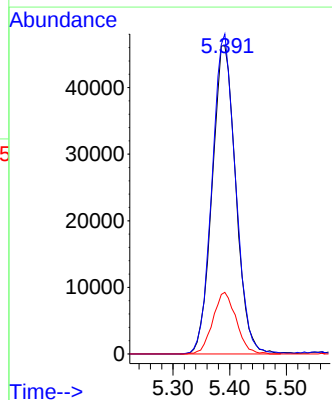
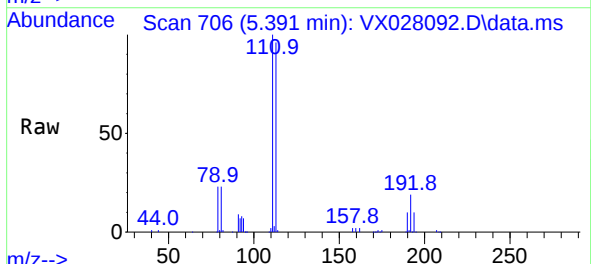


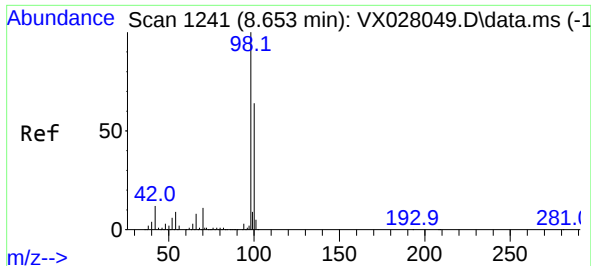

#50
Toluene-d8
Concen: 49.461 ug/l
RT: 8.653 min Scan# 11
Delta R.T. -0.000 min
Lab File: VX028092.D
Acq: 13 Apr 2022 16:00




Instrument :
MSVOA_X
ClientSampleId :
IBLK


Tgt Ion: 98 Resp: 497981
Ion Ratio Lower Upper
98 100
100 65.1 52.6 78.8

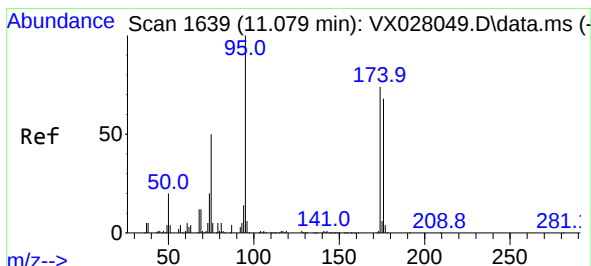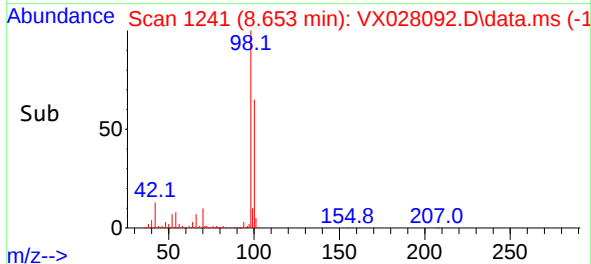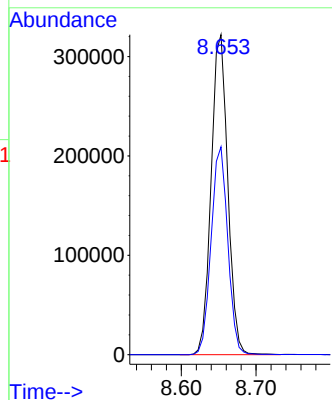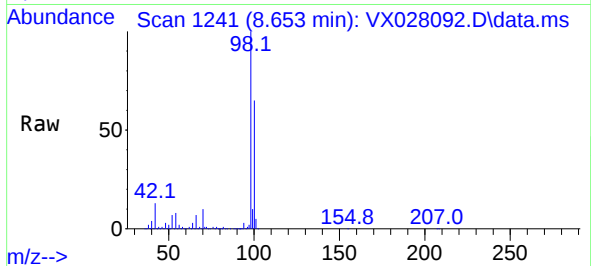

#62
4-Bromofluorobenzene
Concen: 43.367 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.000 min
Lab File: VX028092.D
Acq: 13 Apr 2022 16:00

Tgt Ion: 95 Resp: 163024
Ion Ratio Lower Upper
95 100
174 87.9 0.0 163.0
176 84.7 0.0 155.0


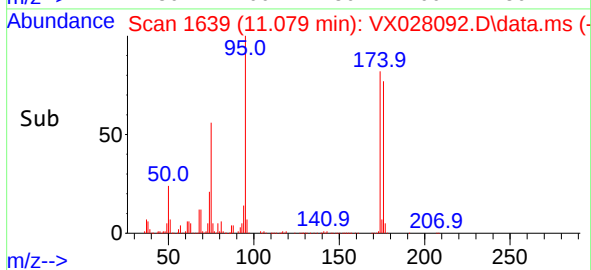
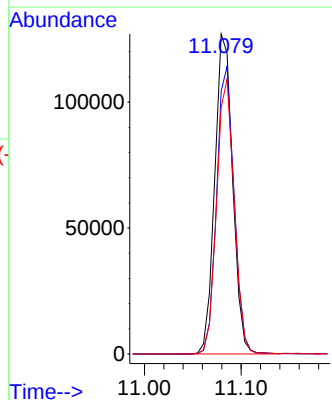
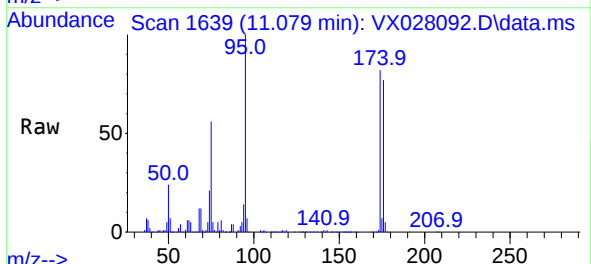


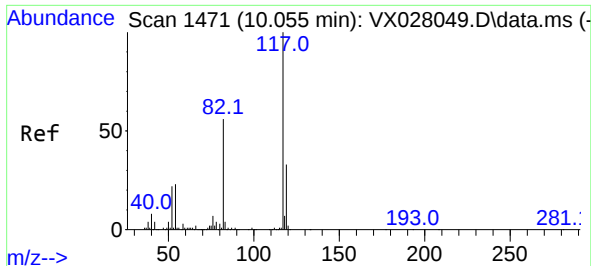

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX028092.D
Acq: 13 Apr 2022 16:00

Instrument :
MSVOA_X
ClientSampleId :
IBLK

Tgt Ion:117 Resp: 376705
Ion Ratio Lower Upper
117 100
82 53.4 41.8 62.8
119 32.4 24.8 37.2

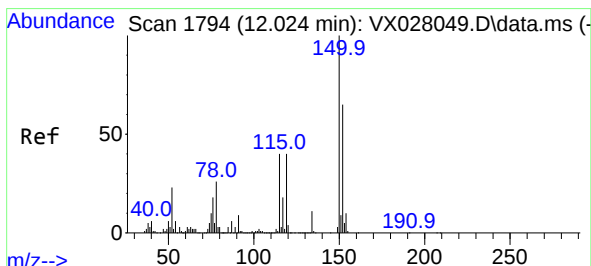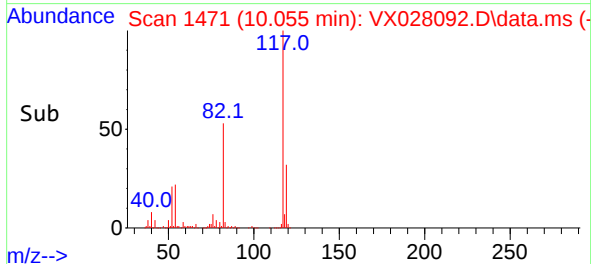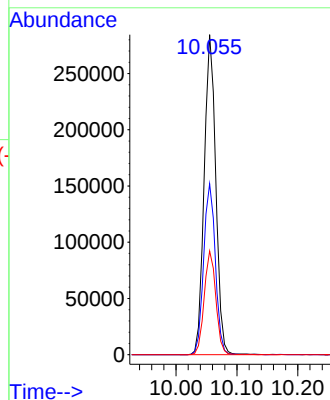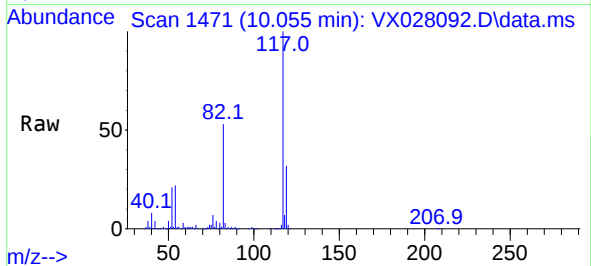

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. 0.000 min
Lab File: VX028092.D
Acq: 13 Apr 2022 16:00

Tgt Ion:152 Resp: 174566
Ion Ratio Lower Upper
152 100
115 57.8 37.5 112.7
150 158.3 0.0 338.2

