

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041323\
 Data File : VX035051.D
 Acq On : 12 Apr 2023 17:24
 Operator : JC/MD
 Sample : IBLK
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 IBLK

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032923W.M
 Title : SW846 8260

Signal : TIC: VX035051.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.385	692	705	721	rBV	152365	453747	30.28%	4.509%
2	5.549	721	732	751	rVB	290760	837535	55.89%	8.322%
3	5.958	787	799	819	rBV	187072	502015	33.50%	4.988%
4	6.763	921	931	947	rBV	461144	1094334	73.03%	10.873%
5	8.646	1234	1240	1250	rBV	947253	1498564	100.00%	14.890%
6	10.055	1465	1471	1482	rVB	963128	1294791	86.40%	12.865%
7	10.305	1504	1512	1518	rBV5	6784	15960	1.07%	0.159%
8	10.963	1615	1620	1624	rBV	35594	44665	2.98%	0.444%
9	11.079	1634	1639	1649	rBV	795890	1047970	69.93%	10.413%
10	11.475	1701	1704	1712	rVB	29815	40427	2.70%	0.402%
11	11.634	1723	1730	1735	rBV4	22267	36388	2.43%	0.362%
12	11.719	1740	1744	1746	rVV3	12351	17372	1.16%	0.173%
13	11.756	1746	1750	1760	rVB2	16161	32058	2.14%	0.319%
14	12.024	1789	1794	1800	rBV	1025764	1284498	85.72%	12.763%
15	12.268	1827	1834	1838	rVV2	18957	35661	2.38%	0.354%
16	12.316	1838	1842	1849	rVB3	28654	49595	3.31%	0.493%
17	12.426	1855	1860	1864	rBV	57473	65825	4.39%	0.654%
18	12.463	1864	1866	1872	rVB3	13945	21011	1.40%	0.209%
19	12.536	1874	1878	1879	rBV	13059	16257	1.08%	0.162%
20	12.725	1905	1909	1914	rVB3	15733	26376	1.76%	0.262%
21	12.902	1932	1938	1939	rBV5	13875	25854	1.73%	0.257%
22	12.963	1946	1948	1954	rVB2	21681	33922	2.26%	0.337%
23	13.042	1955	1961	1964	rBV4	20944	38480	2.57%	0.382%
24	13.164	1975	1981	1985	rVB4	21178	38926	2.60%	0.387%
25	13.213	1986	1989	1992	rBV2	15577	18671	1.25%	0.186%
26	13.268	1992	1998	2000	rBV3	41668	64445	4.30%	0.640%
27	13.292	2000	2002	2007	rVB4	26279	37557	2.51%	0.373%
28	13.383	2012	2017	2020	rVV2	12263	21976	1.47%	0.218%
29	13.420	2020	2023	2032	rVB8	19463	48247	3.22%	0.479%
30	13.505	2032	2037	2040	rBV4	15425	23883	1.59%	0.237%
31	13.542	2040	2043	2046	rBV2	16094	20629	1.38%	0.205%
32	13.585	2046	2050	2055	rBV3	23008	37679	2.51%	0.374%
33	13.670	2060	2064	2068	rVV2	13117	21336	1.42%	0.212%
34	13.853	2088	2094	2099	rVB5	32195	66767	4.46%	0.663%
35	13.926	2099	2106	2111	rBV4	31447	64628	4.31%	0.642%
36	14.036	2121	2124	2127	rVB3	21702	25693	1.71%	0.255%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041323\
Data File : VX035051.D
Acq On : 12 Apr 2023 17:24
Operator : JC/MD
Sample : IBLK
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
IBLK

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032923W.M
Title : SW846 8260

37	14.078	2127	2131	2134	rBV2	25355	33473	2.23%	0.333%
38	14.231	2149	2156	2163	rVB3	63638	115859	7.73%	1.151%
39	14.322	2167	2171	2176	rBV4	16376	22609	1.51%	0.225%
40	14.371	2176	2179	2184	rBV	25045	29443	1.96%	0.293%
41	14.420	2184	2187	2193	rVB6	11461	17778	1.19%	0.177%
42	14.481	2193	2197	2207	rBV6	40871	76540	5.11%	0.761%
43	14.615	2215	2219	2221	rBV	61906	81672	5.45%	0.812%
44	14.670	2226	2228	2233	rVB3	33068	43069	2.87%	0.428%
45	14.731	2234	2238	2239	rBV4	13676	16286	1.09%	0.162%
46	14.755	2239	2242	2244	rVV2	24086	27117	1.81%	0.269%
47	14.786	2244	2247	2250	rVV4	18076	27394	1.83%	0.272%
48	14.816	2250	2252	2255	rVV2	16839	23594	1.57%	0.234%
49	14.847	2255	2257	2263	rVV4	21063	26636	1.78%	0.265%
50	14.901	2263	2266	2273	rVB3	19693	33955	2.27%	0.337%
51	15.048	2285	2290	2294	rBV6	11094	20950	1.40%	0.208%
52	15.182	2307	2312	2315	rBV	40223	62893	4.20%	0.625%
53	15.377	2339	2344	2348	rBV3	25413	40412	2.70%	0.402%
54	15.487	2357	2362	2367	rBV2	45706	79626	5.31%	0.791%
55	15.615	2378	2383	2386	rBV4	32359	55235	3.69%	0.549%
56	15.651	2386	2389	2397	rVB4	22214	42208	2.82%	0.419%
57	15.840	2416	2420	2424	rBV7	9925	16561	1.11%	0.165%
58	16.023	2448	2450	2455	rVB5	11195	15881	1.06%	0.158%
59	16.090	2456	2461	2467	rBV2	18842	39248	2.62%	0.390%
60	16.377	2500	2508	2514	rBV3	47988	92215	6.15%	0.916%
61	16.596	2541	2544	2549	rVB5	12754	19839	1.32%	0.197%




Sum of corrected areas: 10064235

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041323\
Data File : VX035051.D
Acq On : 12 Apr 2023 17:24
Operator : JC/MD
Sample : IBLK
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
IBLK

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032923W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

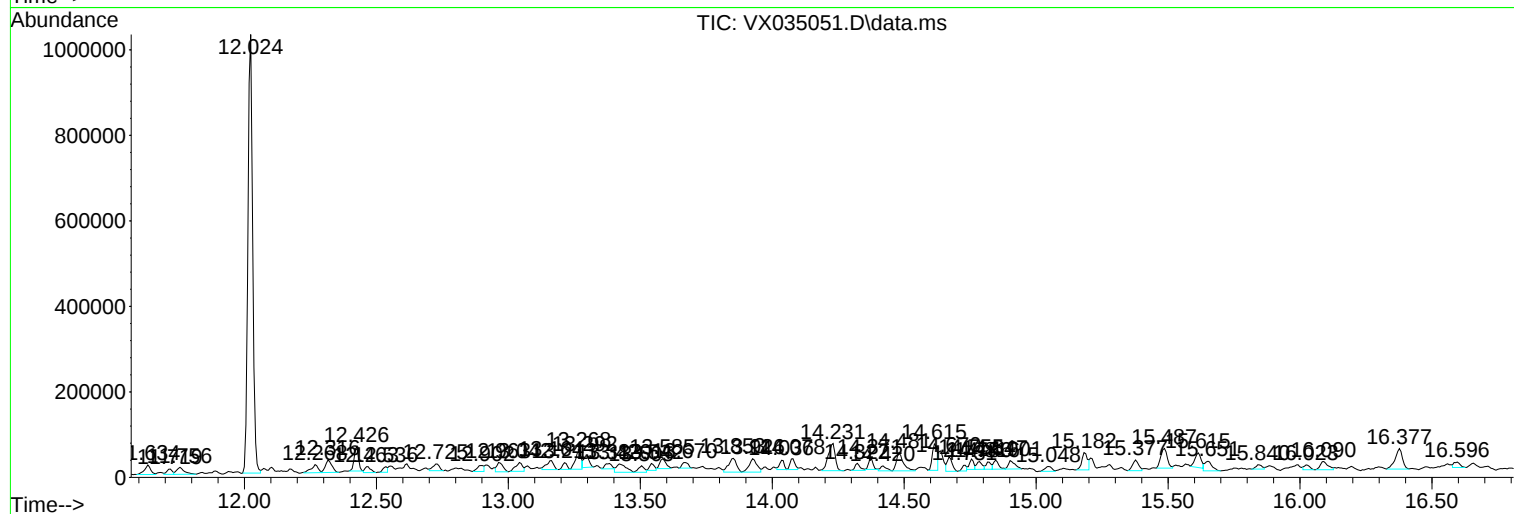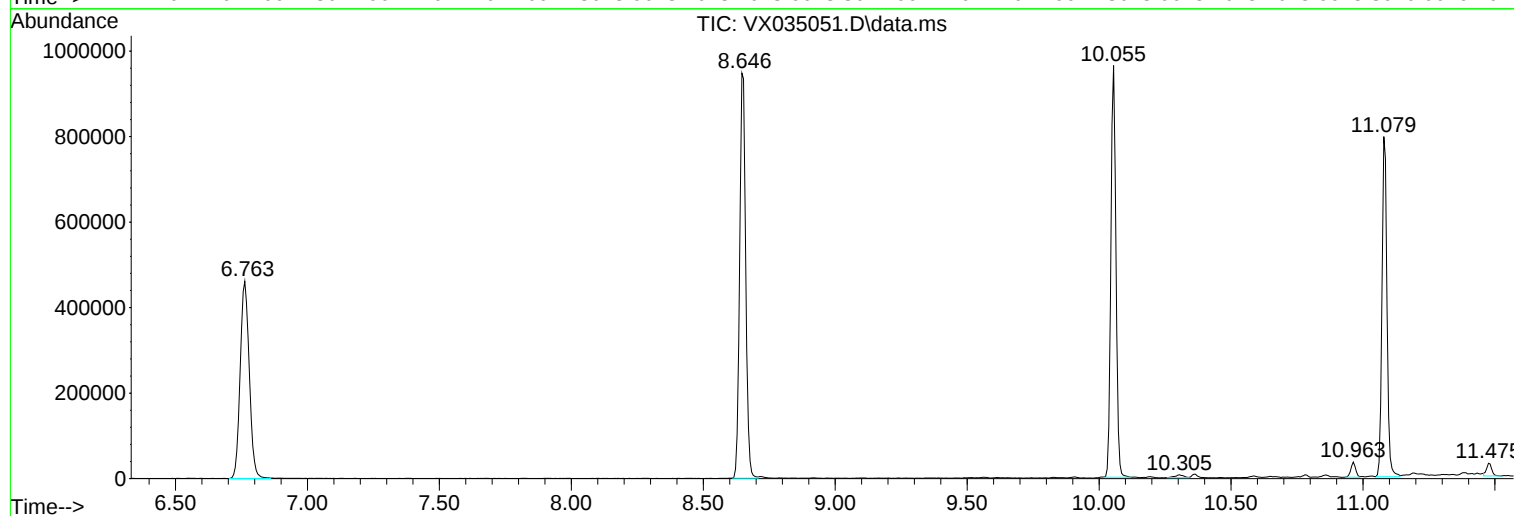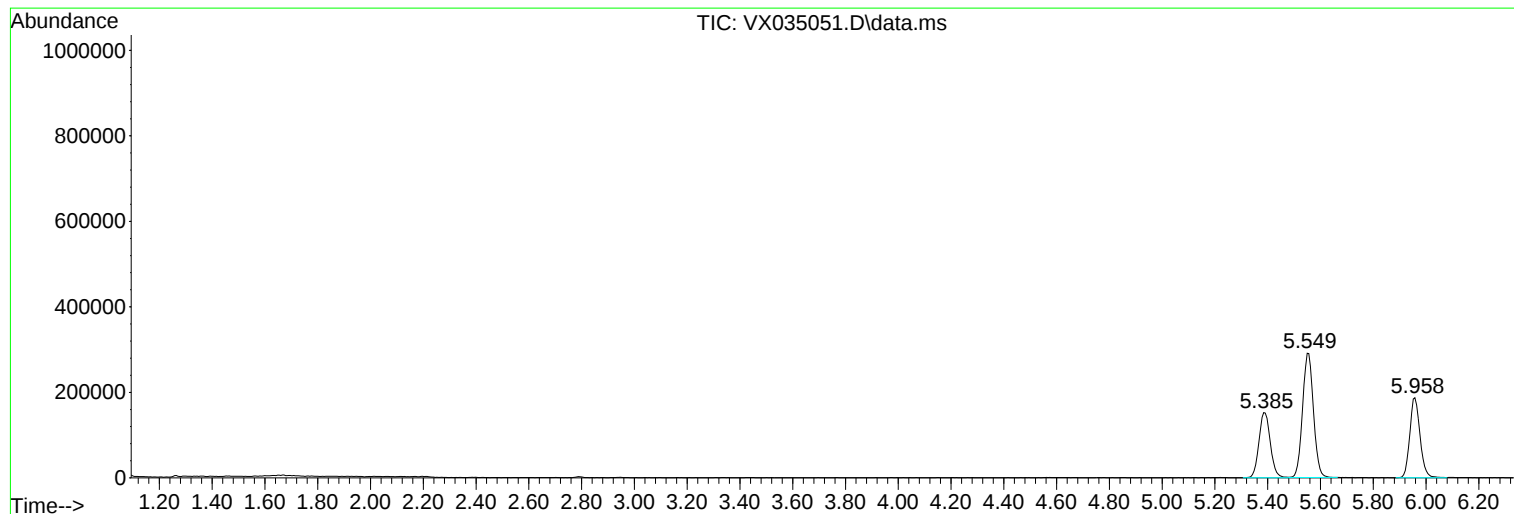

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041323\
Data File : VX035051.D
Acq On : 12 Apr 2023 17:24
Operator : JC/MD
Sample : IBLK
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
IBLK

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032923W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041323\
Data File : VX035051.D
Acq On : 12 Apr 2023 17:24
Operator : JC/MD
Sample : IBLK
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
IBLK

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032923W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------