
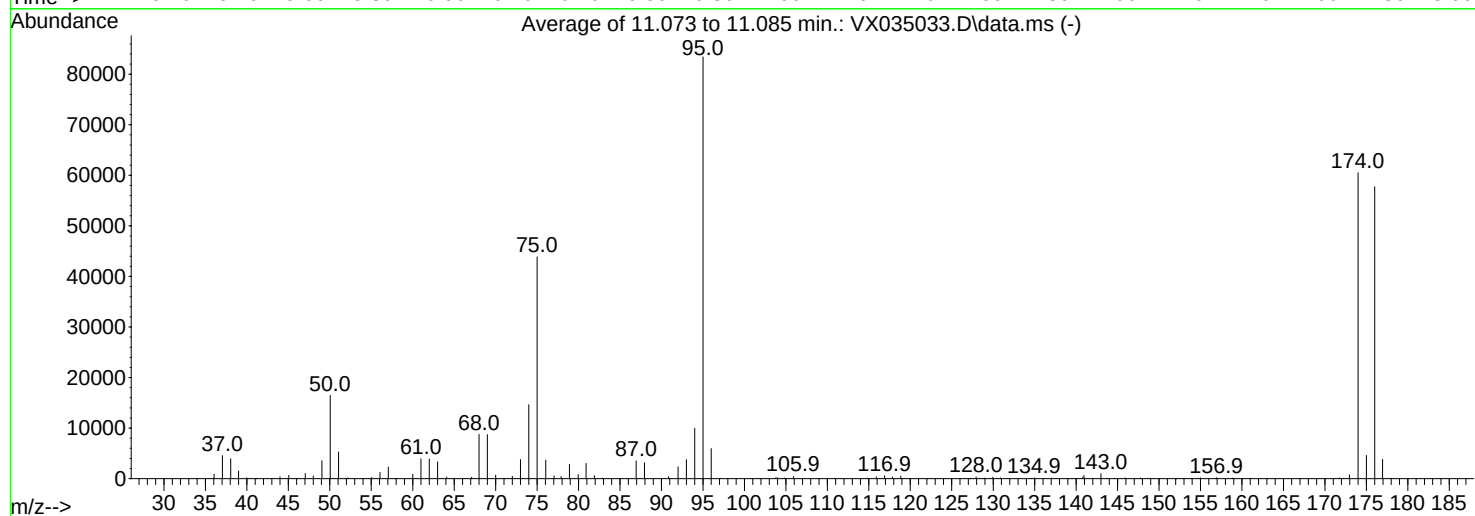


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041323\
Data File : VX035033.D
Acq On : 12 Apr 2023 08:00
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032923W.M
Title : SW846 8260
Last Update : Sat Apr 01 01:50:18 2023

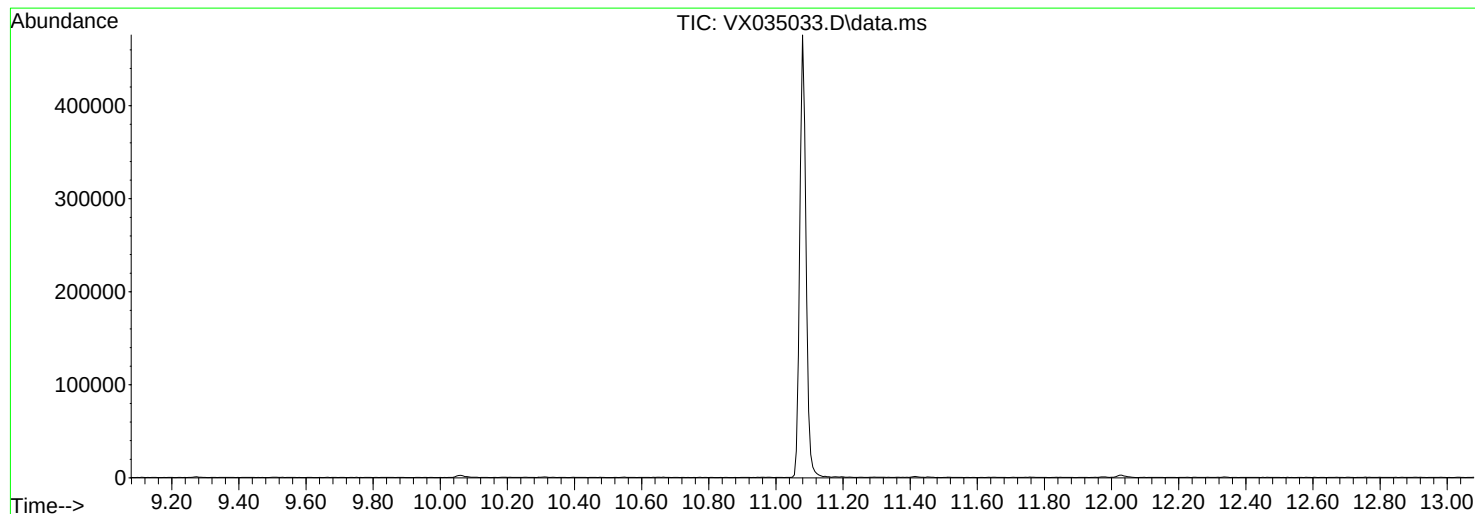

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.7	16450	PASS
75	95	30	60	52.6	43859	PASS
95	95	100	100	100.0	83435	PASS
96	95	5	9	7.1	5965	PASS
173	174	0.00	2	1.2	750	PASS
174	95	50	100	72.5	60528	PASS
175	174	5	9	7.6	4584	PASS
176	174	95	101	95.4	57728	PASS
177	176	5	9	6.6	3813	PASS