

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041422\
 Data File : VX028116.D
 Acq On : 14 Apr 2022 18:45
 Operator : JC/MD
 Sample : N2403-06DL 50X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MW-46DL

Quant Time: Apr 15 03:17:18 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X041222W.M
 Quant Title : SW846 8260
 QLast Update : Tue Apr 12 22:07:23 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) Pentafluorobenzene	5.556	168	215776	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	372666	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	354130	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	171225	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	136621	46.670	ug/l	0.00
Spiked Amount	50.000	Range	61 - 141	Recovery	=	93.340%
35) Dibromofluoromethane	5.391	113	120113	49.187	ug/l	0.00
Spiked Amount	50.000	Range	69 - 133	Recovery	=	98.380%
50) Toluene-d8	8.653	98	454021	49.851	ug/l	0.00
Spiked Amount	50.000	Range	65 - 126	Recovery	=	99.700%
62) 4-Bromofluorobenzene	11.085	95	156187	45.930	ug/l	0.00
Spiked Amount	50.000	Range	58 - 135	Recovery	=	91.860%
Target Compounds						
					Qvalue	
5) Bromomethane	1.617	94	768	Below Cal	#	65
6) Chloroethane	1.672	64	157	2.667	ug/l	100
11) Tert butyl alcohol	2.958	59	625	0.920	ug/l	# 72
13) Acrolein	2.209	56	450	Below Cal	#	1
15) Acrylonitrile	3.099	53	480	0.341	ug/l	# 27
16) Acetone	2.379	43	1979	1.623	ug/l	# 75
18) Methyl Acetate	2.708	43	668	0.205	ug/l	# 75
20) Methylene Chloride	2.788	84	492	0.203	ug/l	# 81
25) 2-Butanone	4.586	43	1112	0.527	ug/l	# 44
31) Cyclohexane	5.476	56	14343	3.563	ug/l	92
36) 1,1-Dichloropropene	5.549	75	16488	4.424	ug/l	# 50
38) Carbon Tetrachloride	5.556	117	20518	5.157	ug/l	# 16
39) Methylcyclohexane	7.384	83	10890	2.472	ug/l	# 91
48) Methyl methacrylate	7.653	41	1191	0.361	ug/l	# 88
52) Toluene	8.720	92	9601	1.328	ug/l	100
55) 1,1,2-Trichloroethane	9.098	97	647	0.221	ug/l	# 16
67) Ethyl Benzene	10.195	91	307287	22.583	ug/l	98
68) m/p-Xylenes	10.305	106	325400	57.270	ug/l	96
69) o-Xylene	10.646	106	105925	19.178	ug/l	99
70) Styrene	10.646	104	5380	5.152	ug/l	# 1
73) Isopropylbenzene	10.963	105	19877	1.634	ug/l	99
76) 1,2,3-Trichloropropane	11.079	75	86983	22.819	ug/l	# 38
78) n-propylbenzene	11.305	91	51687	3.656	ug/l	99
79) 2-Chlorotoluene	11.378	91	26754	3.121	ug/l	# 40
80) 1,3,5-Trimethylbenzene	11.451	105	52642	5.010	ug/l	99
81) trans-1,4-Dichloro-2-b...	11.079	75	86983	64.269	ug/l	# 15
82) 4-Chlorotoluene	11.451	91	5885	0.583	ug/l	# 45
83) tert-Butylbenzene	11.756	119	36933	3.633	ug/l	# 51
84) 1,2,4-Trimethylbenzene	11.756	105	307220	29.864	ug/l	98
85) sec-Butylbenzene	11.756	105	307220	23.677	ug/l	# 56
86) p-Isopropyltoluene	11.975	119	3652	0.332	ug/l	93
89) n-Butylbenzene	12.329	91	5387	0.572	ug/l	# 21
90) Hexachloroethane	12.615	117	2220	1.202	ug/l	# 10
95) Naphthalene	13.780	128	99652	8.820	ug/l	99

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041422\
Data File : VX028116.D
Acq On : 14 Apr 2022 18:45
Operator : JC/MD
Sample : N2403-06DL 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-46DL

Quant Time: Apr 15 03:17:18 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X041222W.M
Quant Title : SW846 8260
QLast Update : Tue Apr 12 22:07:23 2022
Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


(#)=qualifier out of range (m)=manual integration (+)=signals summed						

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041422\
Data File : VX028116.D
Acq On : 14 Apr 2022 18:45
Operator : JC/MD
Sample : N2403-06DL 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-46DL

Quant Time: Apr 15 03:17:18 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X041222W.M
Quant Title : SW846 8260
QLast Update : Tue Apr 12 22:07:23 2022
Response via : Initial Calibration




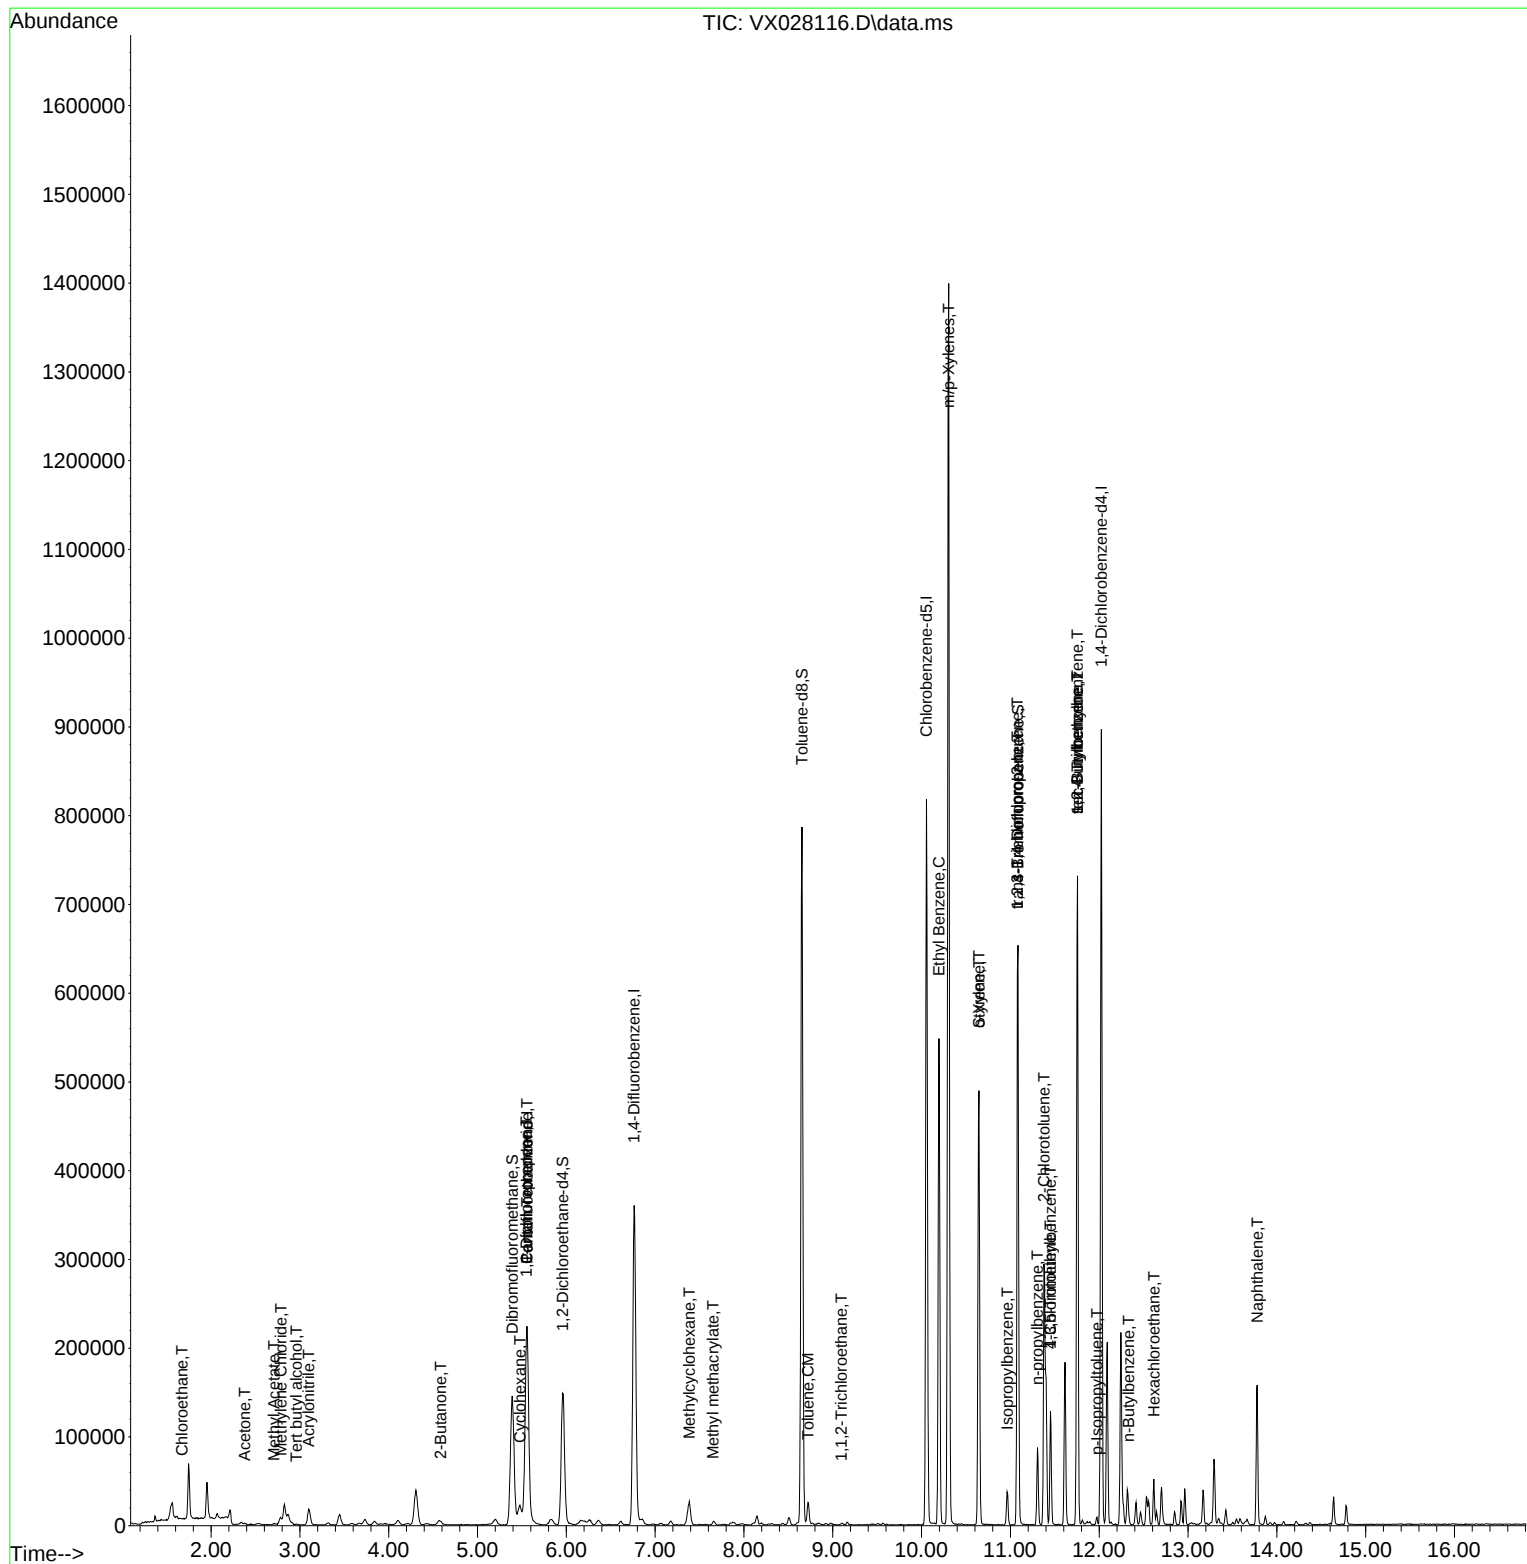




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.556 min Scan# 71
Delta R.T. -0.000 min
Lab File: VX028116.D
Acq: 14 Apr 2022 18:45




Instrument :
MSVOA_X
ClientSampleId :
MW-46DL


Tgt Ion:168 Resp: 215776
Ion Ratio Lower Upper
168 100
99 54.4 41.7 62.5

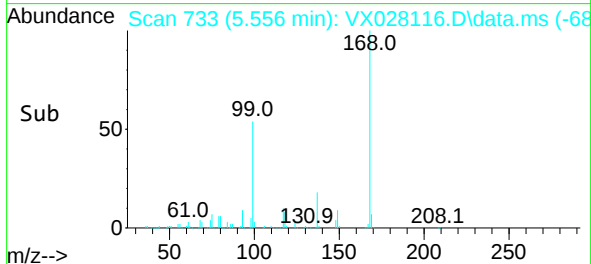

#6
Chloroethane
Concen: 2.667 ug/l
RT: 1.672 min Scan# 96
Delta R.T. -0.007 min
Lab File: VX028116.D
Acq: 14 Apr 2022 18:45

Tgt Ion: 64 Resp: 157
Ion Ratio Lower Upper
64 100
66 31.5 25.3 37.9

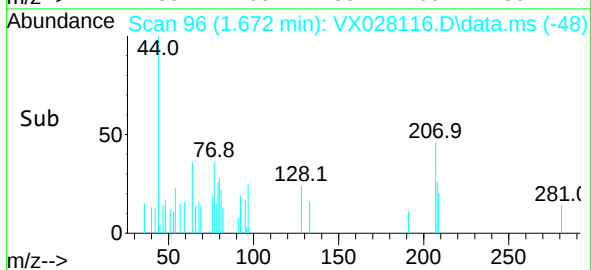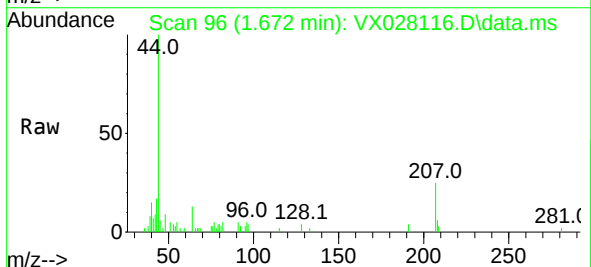



#11

Tert butyl alcohol

Concen: 0.920 ug/l

RT: 2.958 min Scan# 308

Delta R.T. -0.007 min

Lab File: VX028116.D

Acq: 14 Apr 2022 18:45

Instrument :

MSVOA_X

ClientSampleId :





MW-46DL

Tgt Ion: 59 Resp: 625

Ion Ratio Lower Upper

59 100

57 0.0 8.3 12.5#

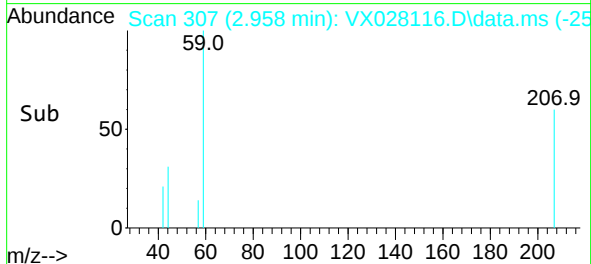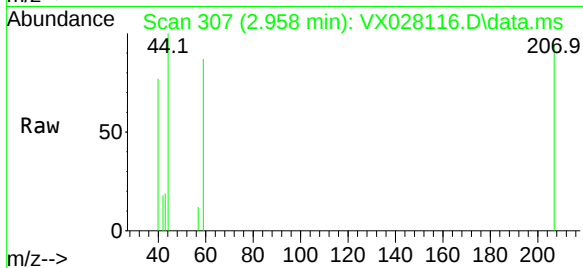

#13

Acrolein

Concen: Below Cal

RT: 2.209 min Scan# 184

Delta R.T. -0.024 min

Lab File: VX028116.D




Acq: 14 Apr 2022 18:45


Tgt Ion: 56 Resp: 450

Ion Ratio Lower Upper

56 100

55 1108.2 55.0 82.6#


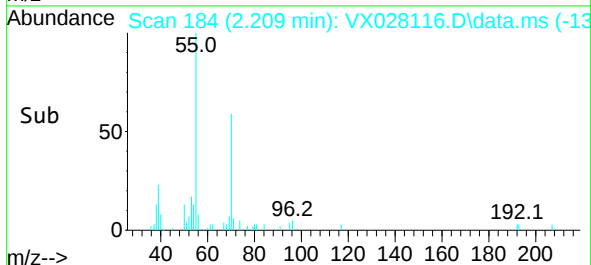

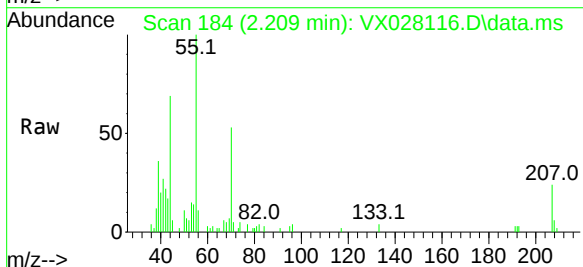




#15
Acrylonitrile
Concen: 0.341 ug/l
RT: 3.099 min Scan# 311
Delta R.T. 0.037 min
Lab File: VX028116.D
Acq: 14 Apr 2022 18:45




Instrument :
MSVOA_X
ClientSampleId :
MW-46DL


Tgt Ion: 53 Resp: 480
Ion Ratio Lower Upper
53 100
52 11.7 65.7 98.5#
51 0.0 28.4 42.6#

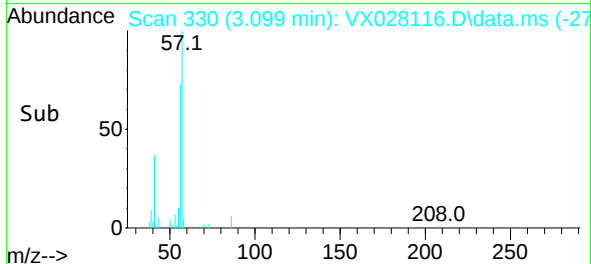

#16
Acetone
Concen: 1.623 ug/l
RT: 2.379 min Scan# 212
Delta R.T. -0.001 min
Lab File: VX028116.D
Acq: 14 Apr 2022 18:45

Tgt Ion: 43 Resp: 1979
Ion Ratio Lower Upper
43 100
58 21.1 28.8 43.2#


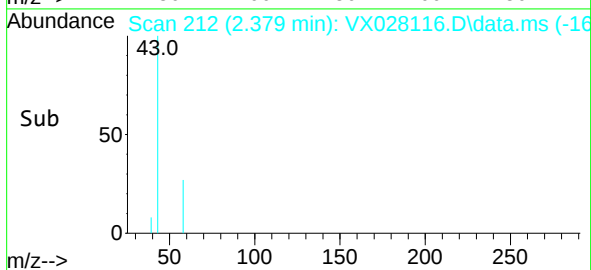

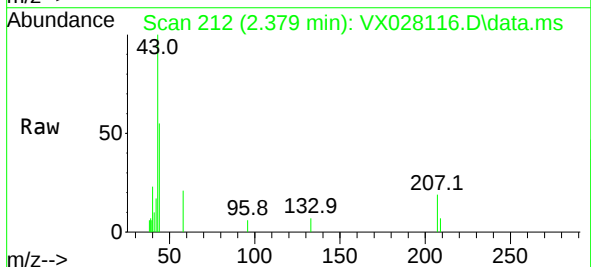




#18
Methyl Acetate
Concen: 0.205 ug/l
RT: 2.708 min Scan# 266
Delta R.T. 0.005 min
Lab File: VX028116.D
Acq: 14 Apr 2022 18:45




Instrument :
MSVOA_X
ClientSampleId :
MW-46DL


Tgt Ion: 43 Resp: 668
Ion Ratio Lower Upper
43 100
74 15.3 22.8 34.2#

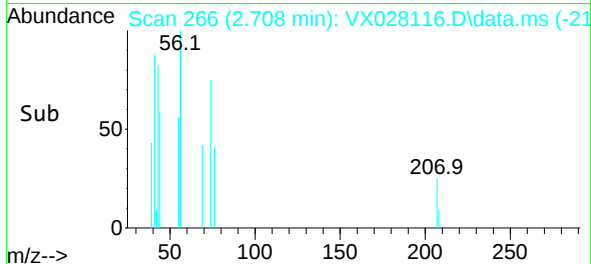

#20
Methylene Chloride
Concen: 0.203 ug/l
RT: 2.788 min Scan# 279
Delta R.T. -0.000 min
Lab File: VX028116.D
Acq: 14 Apr 2022 18:45

Tgt Ion: 84 Resp: 492
Ion Ratio Lower Upper
84 100
49 80.0 85.5 128.3#
51 45.8 26.6 39.8#
86 70.3 51.5 77.3


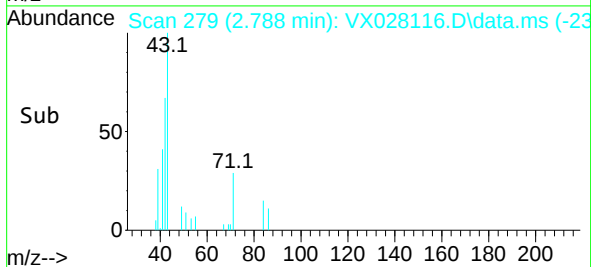

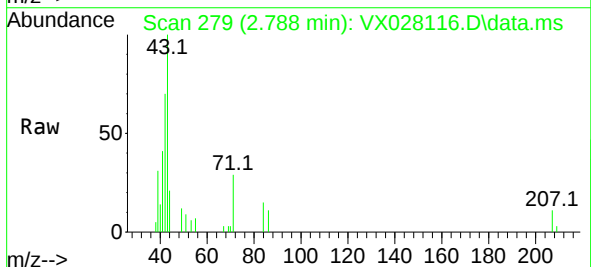




#25
2-Butanone
Concen: 0.527 ug/l
RT: 4.586 min Scan# 511
Delta R.T. 0.030 min
Lab File: VX028116.D
Acq: 14 Apr 2022 18:45




Instrument :
MSVOA_X
ClientSampleId :
MW-46DL


Tgt Ion: 43 Resp: 1112
Ion Ratio Lower Upper
43 100
72 0.0 24.4 36.6#

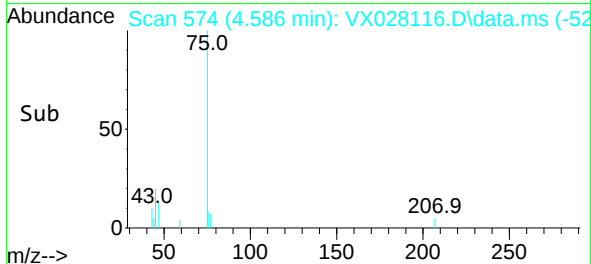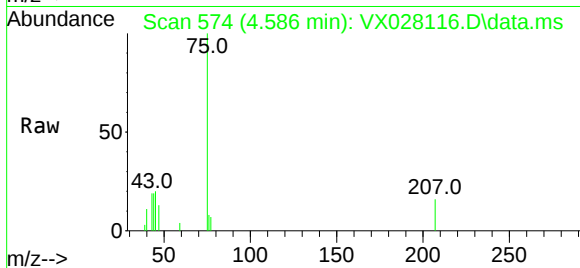

#31
Cyclohexane
Concen: 3.563 ug/l
RT: 5.476 min Scan# 720
Delta R.T. -0.001 min
Lab File: VX028116.D
Acq: 14 Apr 2022 18:45

Tgt Ion: 56 Resp: 14343
Ion Ratio Lower Upper
56 100
69 29.1 26.7 40.1
84 87.9 77.2 115.8

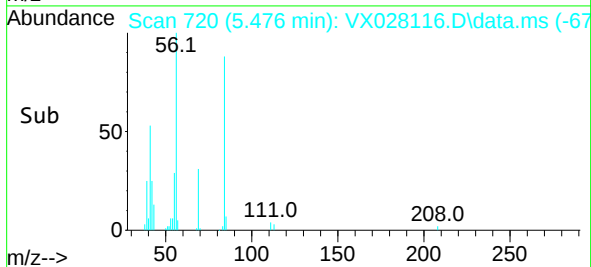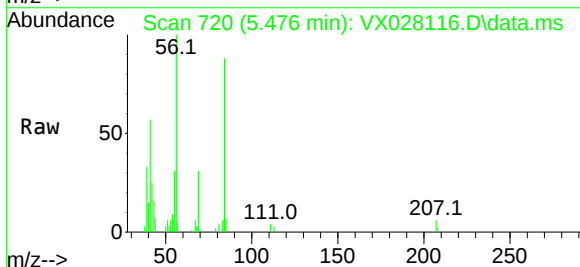

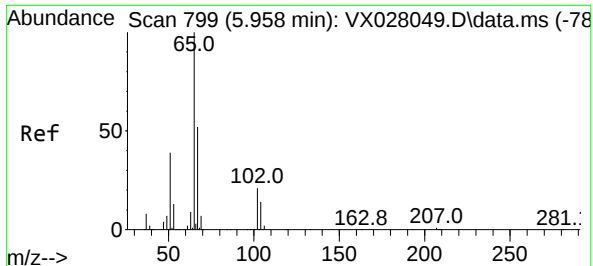

#33

1,2-Dichloroethane-d4

Concen: 46.670 ug/l

RT: 5.958 min Scan# 799

Delta R.T. -0.000 min

Lab File: VX028116.D

Acq: 14 Apr 2022 18:45

Instrument :

MSVOA_X

ClientSampleId :





MW-46DL

Tgt Ion: 65 Resp: 136621

Ion Ratio Lower Upper

65 100

67 52.3 0.0 107.4

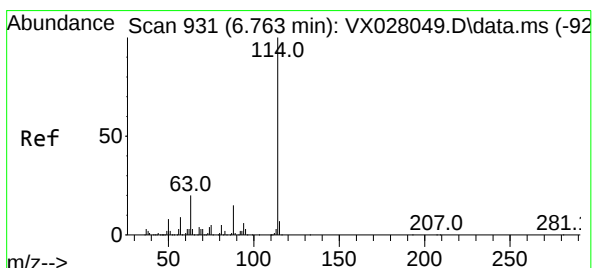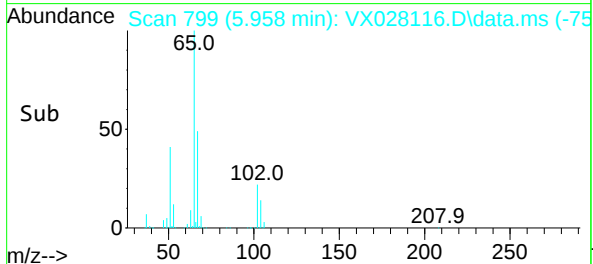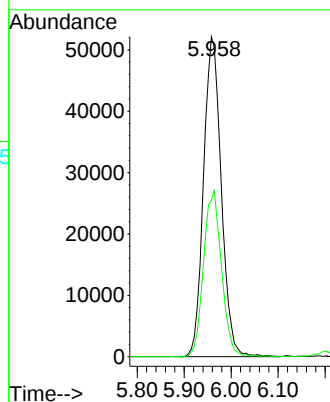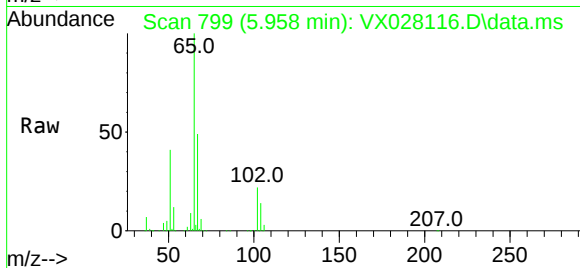

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.763 min Scan# 931

Delta R.T. -0.000 min

Lab File: VX028116.D

Acq: 14 Apr 2022 18:45




Tgt Ion: 114 Resp: 372666


Ion Ratio Lower Upper

114 100

63 18.8 0.0 36.8

88 14.6 0.0 32.4

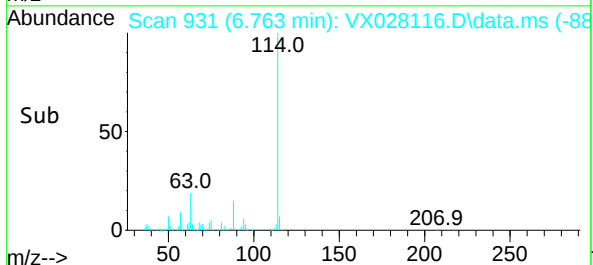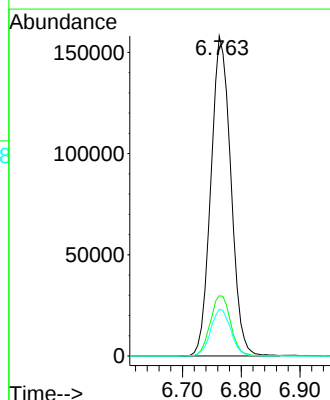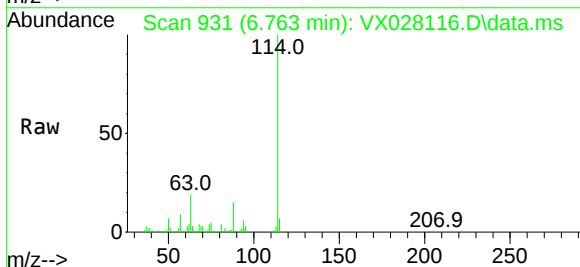

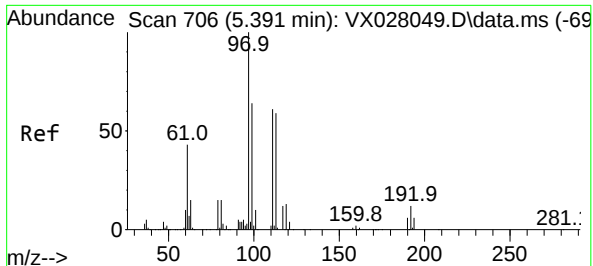

#35

Dibromofluoromethane

Concen: 49.187 ug/l

RT: 5.391 min Scan# 706

Delta R.T. -0.000 min

Lab File: VX028116.D

Acq: 14 Apr 2022 18:45

Instrument :

MSVOA_X

ClientSampleId :

MW-46DL





Tgt Ion:113 Resp: 120113

Ion Ratio Lower Upper

113 100

111 102.9 82.8 124.2

192 20.1 16.9 25.3

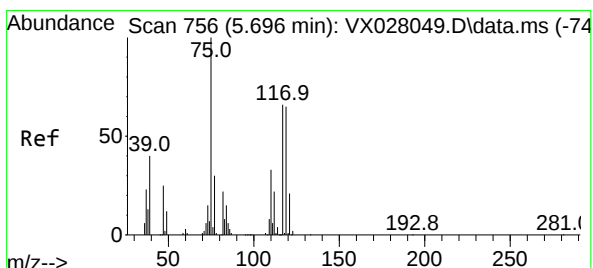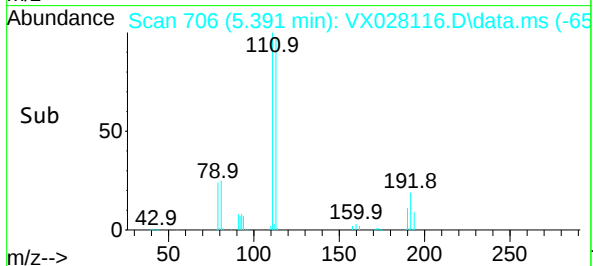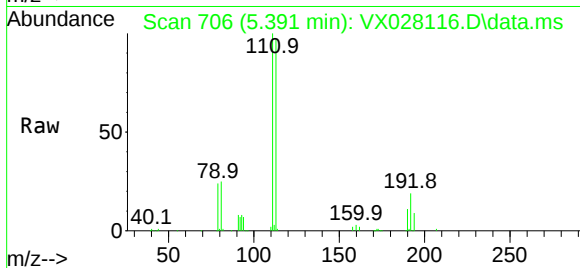

#36

1,1-Dichloropropene

Concen: 4.424 ug/l

RT: 5.549 min Scan# 732

Delta R.T. -0.147 min

Lab File: VX028116.D

Acq: 14 Apr 2022 18:45




Tgt Ion: 75 Resp: 16488


Ion Ratio Lower Upper

75 100

110 10.2 18.3 54.8#

77 0.1 24.8 37.2#


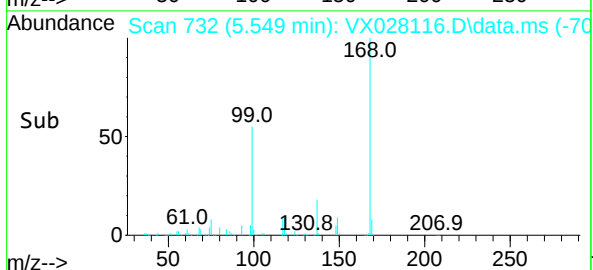

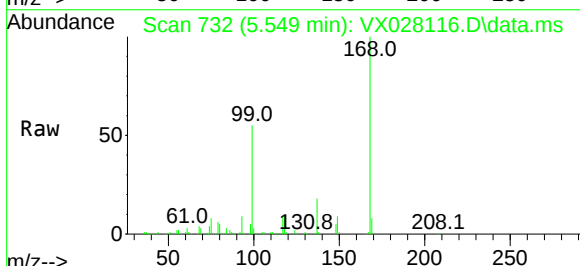




#38
Carbon Tetrachloride
Concen: 5.157 ug/l
RT: 5.556 min Scan# 71
Delta R.T. -0.128 min
Lab File: VX028116.D
Acq: 14 Apr 2022 18:45




Instrument :
MSVOA_X
ClientSampleId :
MW-46DL


Tgt Ion:117 Resp: 20518
Ion Ratio Lower Upper
117 100
119 5.7 77.3 115.9#
121 0.0 24.2 36.2#

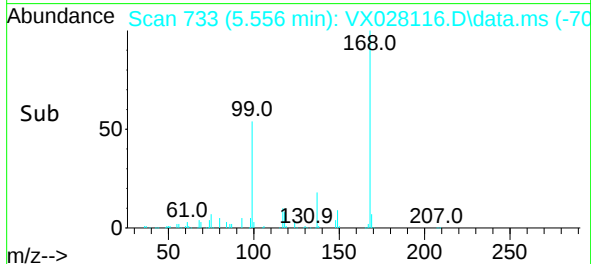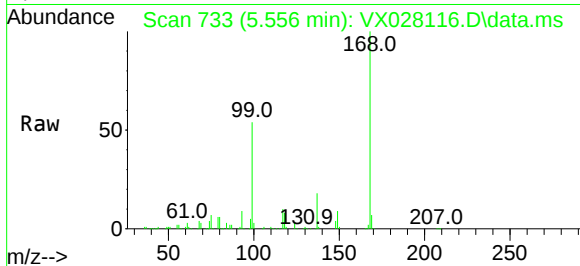

#39
Methylcyclohexane
Concen: 2.472 ug/l
RT: 7.384 min Scan# 1033
Delta R.T. -0.001 min
Lab File: VX028116.D
Acq: 14 Apr 2022 18:45

Tgt Ion: 83 Resp: 10890
Ion Ratio Lower Upper
83 100
55 65.3 54.6 81.8
98 58.1 37.4 56.2#


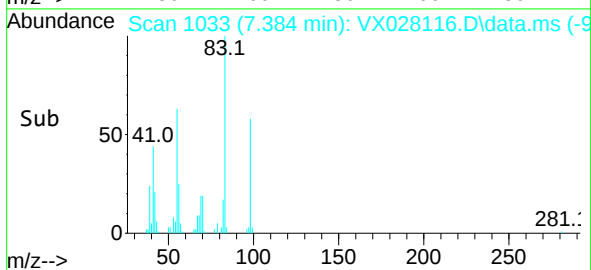

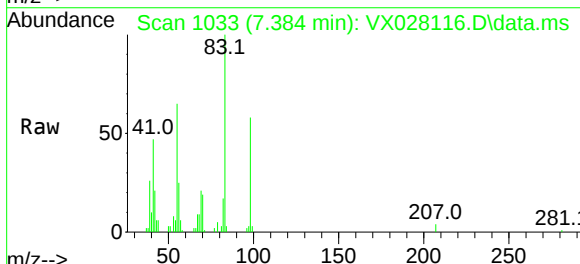




#48
Methyl methacrylate
Concen: 0.361 ug/l
RT: 7.653 min Scan# 1084
Delta R.T. -0.043 min
Lab File: VX028116.D
Acq: 14 Apr 2022 18:45




Instrument :
MSVOA_X
ClientSampleId :
MW-46DL


Tgt Ion: 41 Resp: 1191
Ion Ratio Lower Upper
41 100
69 113.4 82.5 123.7
39 66.0 43.8 65.8#

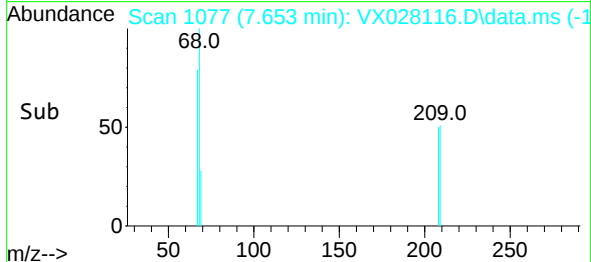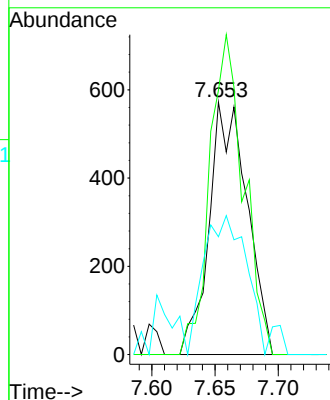

#50
Toluene-d8
Concen: 49.851 ug/l
RT: 8.653 min Scan# 1241
Delta R.T. -0.000 min
Lab File: VX028116.D
Acq: 14 Apr 2022 18:45

Tgt Ion: 98 Resp: 454021
Ion Ratio Lower Upper
98 100
100 65.2 52.6 78.8


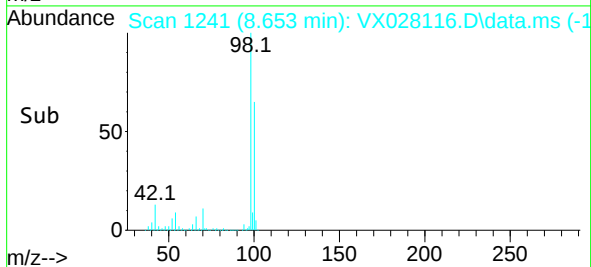
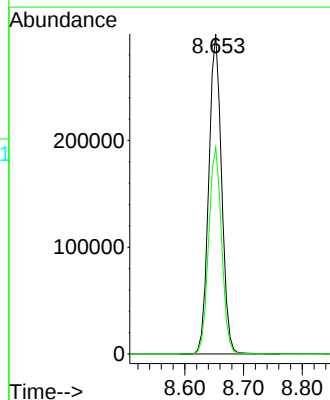
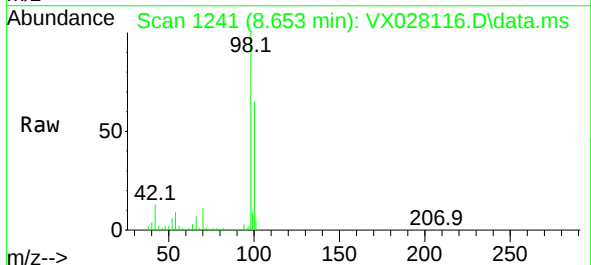




#52
Toluene
Concen: 1.328 ug/l
RT: 8.720 min Scan# 11
Delta R.T. -0.000 min
Lab File: VX028116.D
Acq: 14 Apr 2022 18:45




Instrument :
MSVOA_X
ClientSampleId :
MW-46DL


Tgt Ion: 92 Resp: 9601
Ion Ratio Lower Upper
92 100
91 172.2 137.5 206.3

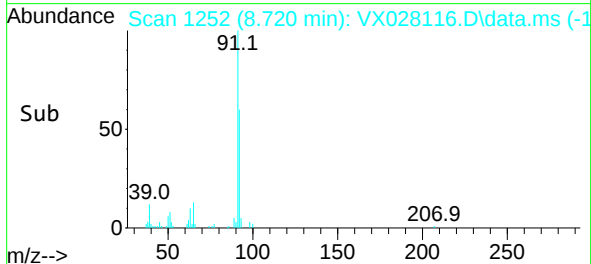

#55
1,1,2-Trichloroethane
Concen: 0.221 ug/l
RT: 9.098 min Scan# 1314
Delta R.T. -0.055 min
Lab File: VX028116.D
Acq: 14 Apr 2022 18:45

Tgt Ion: 97 Resp: 647
Ion Ratio Lower Upper
97 100
83 0.0 66.2 99.4#
85 0.0 42.9 64.3#
99 0.0 49.0 73.6#


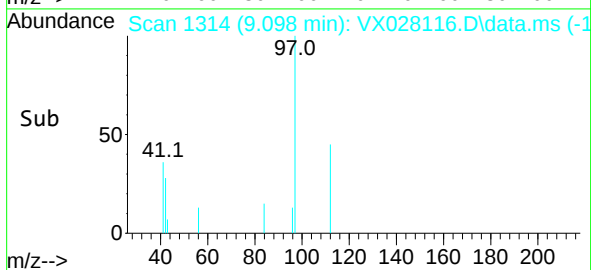

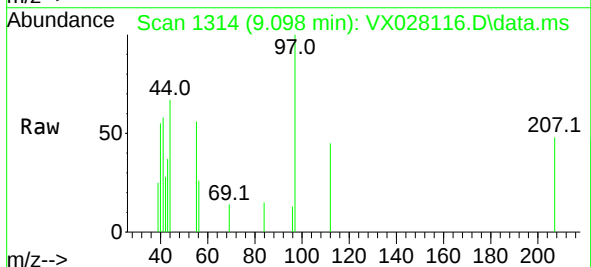




#62
4-Bromofluorobenzene
Concen: 45.930 ug/l
RT: 11.085 min Scan# 1640
Delta R.T. 0.006 min
Lab File: VX028116.D
Acq: 14 Apr 2022 18:45




Instrument :
MSVOA_X
ClientSampleId :
MW-46DL


Tgt Ion: 95 Resp: 156187
Ion Ratio Lower Upper
95 100
174 87.6 0.0 163.0
176 85.1 0.0 155.0

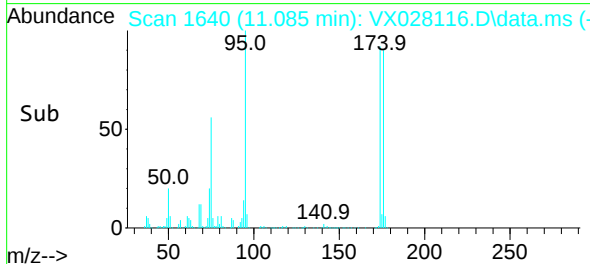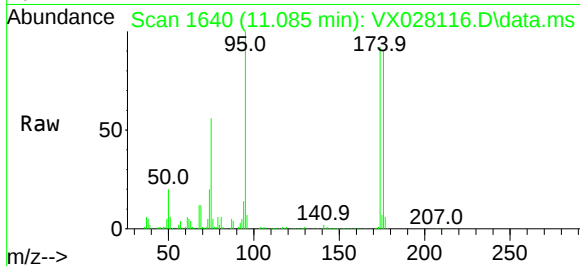

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. -0.000 min
Lab File: VX028116.D
Acq: 14 Apr 2022 18:45

Tgt Ion: 117 Resp: 354130
Ion Ratio Lower Upper
117 100
82 53.4 41.8 62.8
119 31.4 24.8 37.2


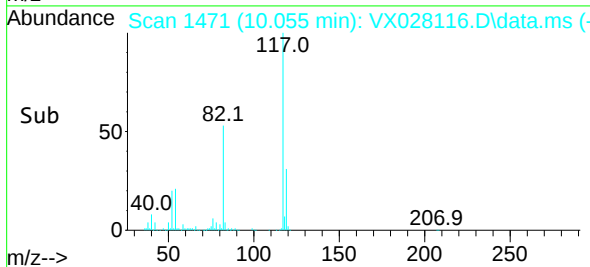

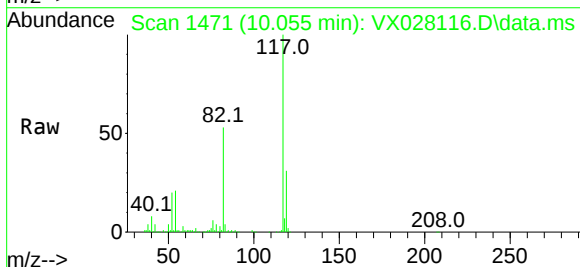




#67
Ethyl Benzene
Concen: 22.583 ug/l
RT: 10.195 min Scan# 1494
Delta R.T. -0.000 min
Lab File: VX028116.D
Acq: 14 Apr 2022 18:45




Instrument :
MSVOA_X
ClientSampleId :
MW-46DL


Tgt Ion: 91 Resp: 307287
Ion Ratio Lower Upper
91 100
106 31.7 24.6 36.8

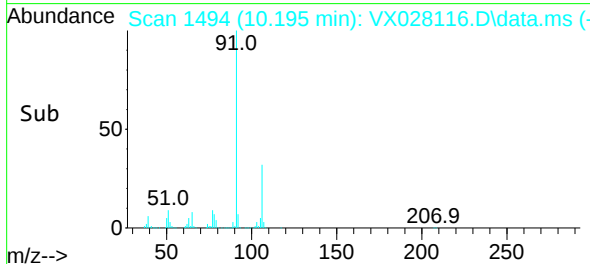

#68
m/p-Xylenes
Concen: 57.270 ug/l
RT: 10.305 min Scan# 1512
Delta R.T. -0.000 min
Lab File: VX028116.D
Acq: 14 Apr 2022 18:45

Tgt Ion:106 Resp: 325400
Ion Ratio Lower Upper
106 100
91 194.7 160.4 240.6


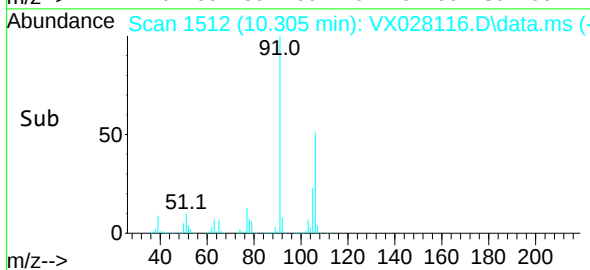

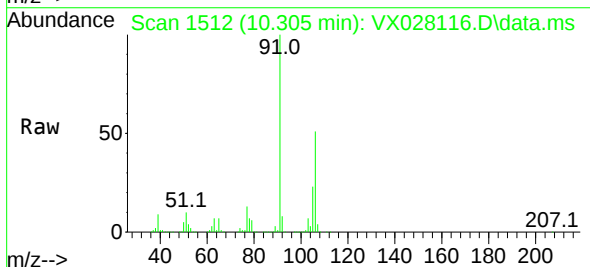




#69
o-Xylene
Concen: 19.178 ug/l
RT: 10.646 min Scan# 1567
Delta R.T. 0.006 min
Lab File: VX028116.D
Acq: 14 Apr 2022 18:45




Instrument :
MSVOA_X
ClientSampleId :
MW-46DL


Tgt Ion:106 Resp: 105925
Ion Ratio Lower Upper
106 100
91 214.3 106.1 318.1

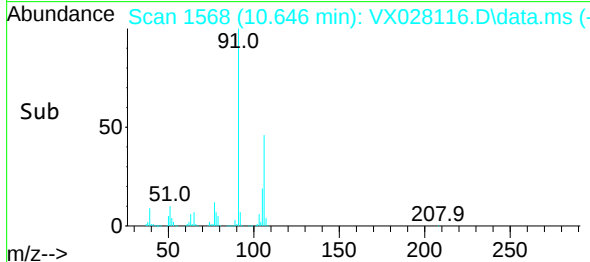

#70
Styrene
Concen: 5.152 ug/l
RT: 10.646 min Scan# 1568
Delta R.T. -0.013 min
Lab File: VX028116.D
Acq: 14 Apr 2022 18:45

Tgt Ion:104 Resp: 5380
Ion Ratio Lower Upper
104 100
78 310.6 38.6 57.8#
103 271.1 43.8 65.8#


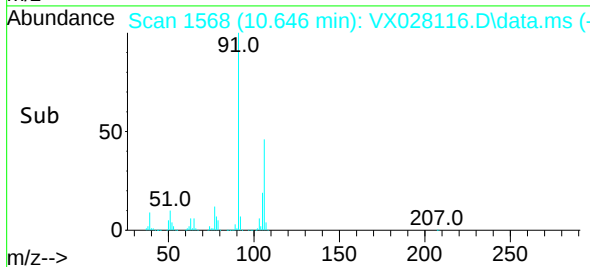

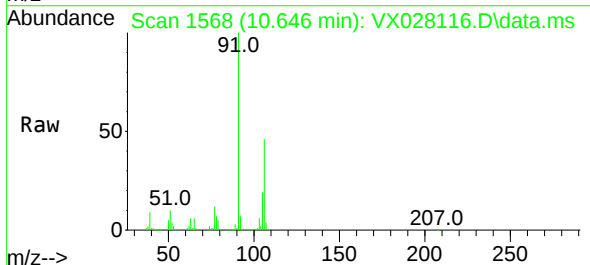




#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 11
Delta R.T. -0.000 min
Lab File: VX028116.D
Acq: 14 Apr 2022 18:45




Instrument :
MSVOA_X
ClientSampleId :
MW-46DL


Tgt Ion:152 Resp: 171225
Ion Ratio Lower Upper
152 100
115 58.3 37.5 112.7
150 157.4 0.0 338.2

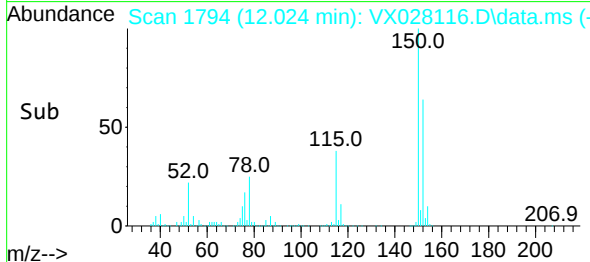

#73
Isopropylbenzene
Concen: 1.634 ug/l
RT: 10.963 min Scan# 1620
Delta R.T. 0.000 min
Lab File: VX028116.D
Acq: 14 Apr 2022 18:45

Tgt Ion:105 Resp: 19877
Ion Ratio Lower Upper
105 100
120 27.4 13.5 40.5


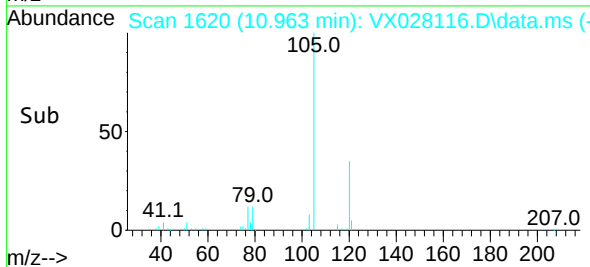

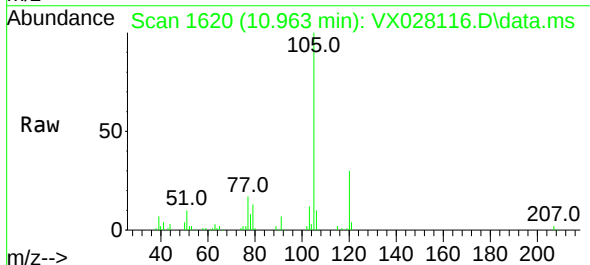




#76
1,2,3-Trichloropropane
Concen: 22.819 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.165 min
Lab File: VX028116.D
Acq: 14 Apr 2022 18:45




Instrument :
MSVOA_X
ClientSampleId :
MW-46DL


Tgt Ion: 75 Resp: 86983
Ion Ratio Lower Upper
75 100
77 1.0 19.4 58.2#

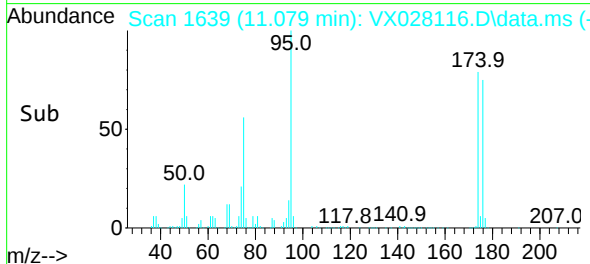

#78
n-propylbenzene
Concen: 3.656 ug/l
RT: 11.305 min Scan# 1676
Delta R.T. -0.000 min
Lab File: VX028116.D
Acq: 14 Apr 2022 18:45

Tgt Ion: 91 Resp: 51687
Ion Ratio Lower Upper
91 100
120 23.5 11.6 34.8


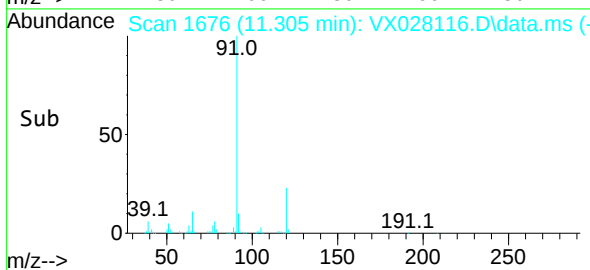

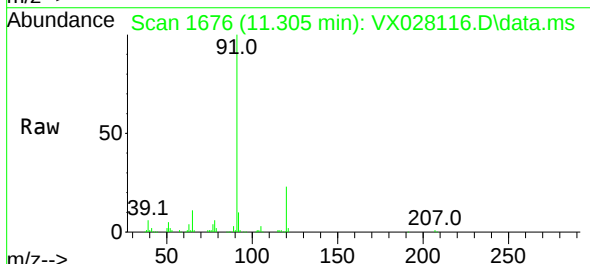




#79
2-Chlorotoluene
Concen: 3.121 ug/l
RT: 11.378 min Scan# 1
Delta R.T. 0.012 min
Lab File: VX028116.D
Acq: 14 Apr 2022 18:45




Instrument :
MSVOA_X
ClientSampleId :
MW-46DL


Tgt Ion: 91 Resp: 26754
Ion Ratio Lower Upper
91 100
126 0.0 17.3 51.9#

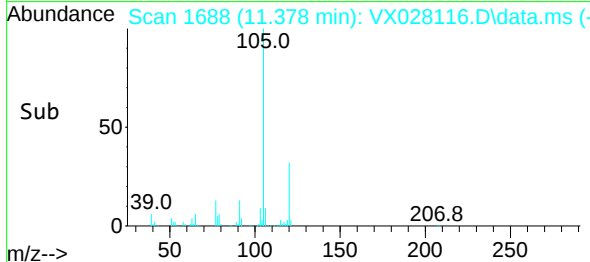

#80
1,3,5-Trimethylbenzene
Concen: 5.010 ug/l
RT: 11.451 min Scan# 1700
Delta R.T. -0.000 min
Lab File: VX028116.D
Acq: 14 Apr 2022 18:45

Tgt Ion: 105 Resp: 52642
Ion Ratio Lower Upper
105 100
120 49.5 24.3 72.9


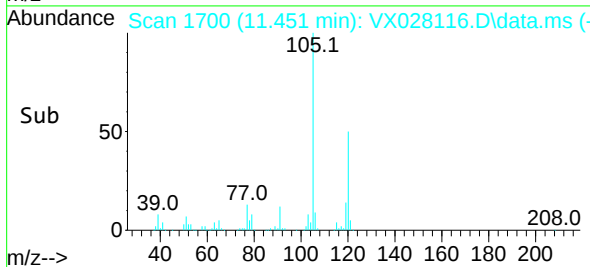

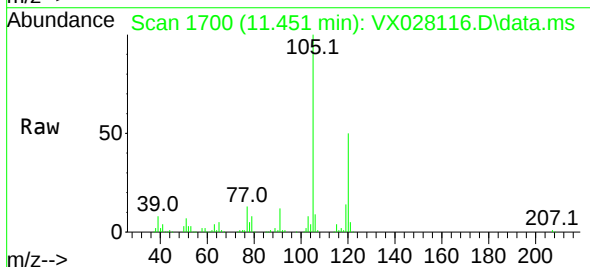




#81
trans-1,4-Dichloro-2-butene
Concen: 64.269 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.061 min
Lab File: VX028116.D
Acq: 14 Apr 2022 18:45




Instrument :
MSVOA_X
ClientSampleId :
MW-46DL


Tgt Ion: 75 Resp: 86983
Ion Ratio Lower Upper
75 100
53 0.0 69.0 103.4#
89 0.0 37.0 55.6#

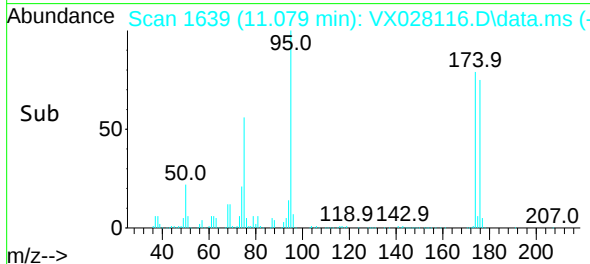

#82
4-Chlorotoluene
Concen: 0.583 ug/l
RT: 11.451 min Scan# 1700
Delta R.T. -0.006 min
Lab File: VX028116.D
Acq: 14 Apr 2022 18:45

Tgt Ion: 91 Resp: 5885
Ion Ratio Lower Upper
91 100
126 0.0 14.9 44.5#


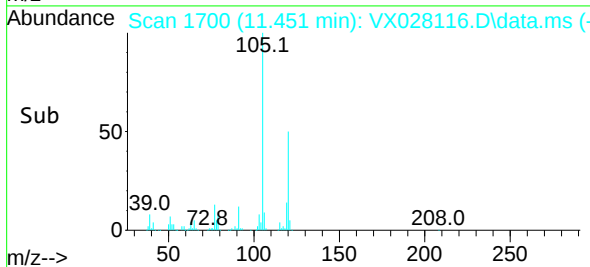

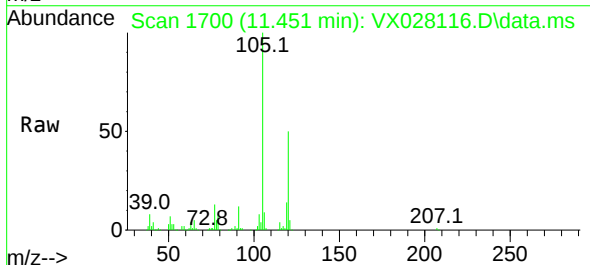




#83
tert-Butylbenzene
Concen: 3.633 ug/l
RT: 11.756 min Scan# 1743
Delta R.T. 0.043 min
Lab File: VX028116.D
Acq: 14 Apr 2022 18:45




Instrument :
MSVOA_X
ClientSampleId :
MW-46DL


Tgt Ion:119 Resp: 36933
Ion Ratio Lower Upper
119 100
91 89.6 26.9 80.6#
134 0.0 11.4 34.2#

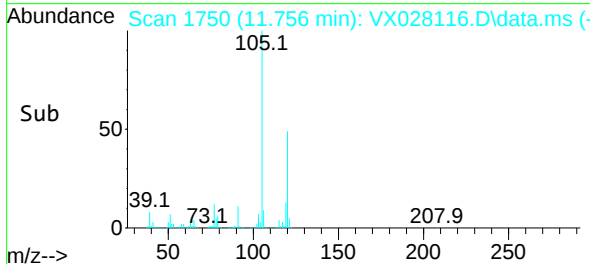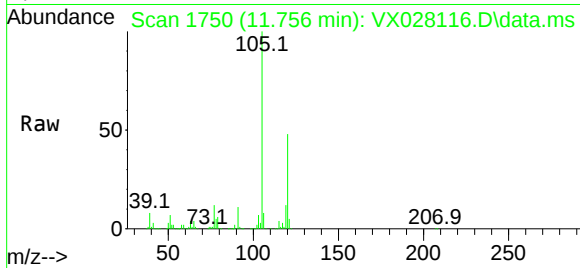

#84
1,2,4-Trimethylbenzene
Concen: 29.864 ug/l
RT: 11.756 min Scan# 1750
Delta R.T. -0.000 min
Lab File: VX028116.D
Acq: 14 Apr 2022 18:45

Tgt Ion:105 Resp: 307220
Ion Ratio Lower Upper
105 100
120 46.7 22.6 67.8


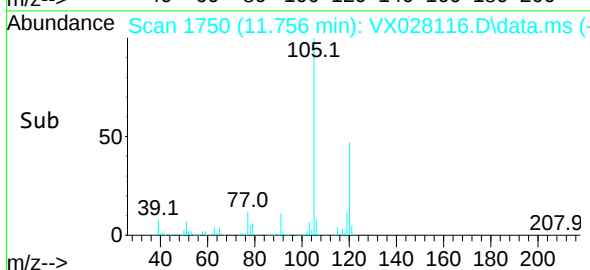

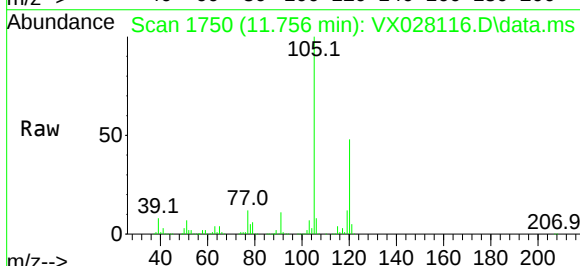




#85
 sec-Butylbenzene
 Concen: 23.677 ug/l
 RT: 11.756 min Scan# 1750
 Delta R.T. -0.134 min
 Lab File: VX028116.D
 Acq: 14 Apr 2022 18:45




Instrument :
 MSVOA_X
 ClientSampleId :
 MW-46DL


Tgt Ion:105 Resp: 307220
 Ion Ratio Lower Upper
 105 100
 134 0.0 10.2 30.4#

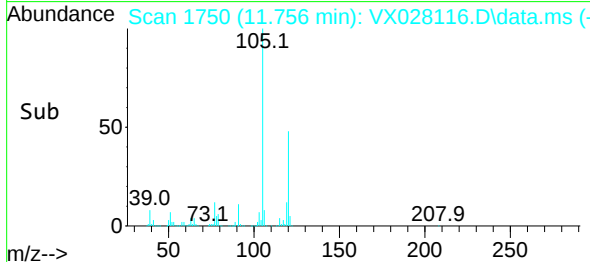

#86
 p-Isopropyltoluene
 Concen: 0.332 ug/l
 RT: 11.975 min Scan# 1786
 Delta R.T. -0.037 min
 Lab File: VX028116.D
 Acq: 14 Apr 2022 18:45

Tgt Ion:119 Resp: 3652
 Ion Ratio Lower Upper
 119 100
 134 27.9 13.0 39.0
 91 27.8 11.3 33.9

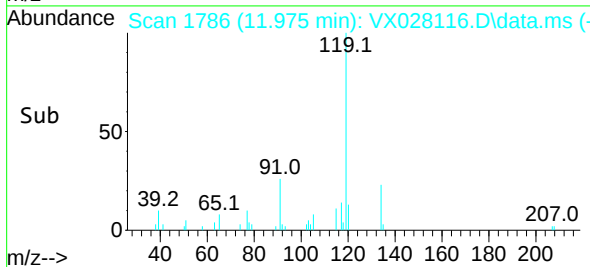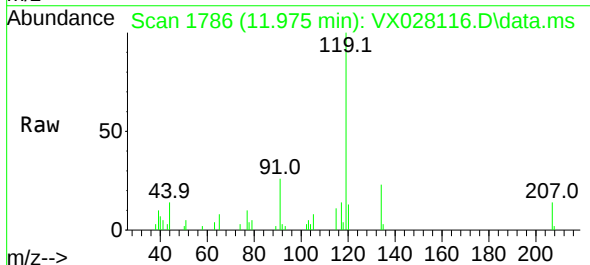



#89

n-Butylbenzene

Concen: 0.572 ug/l

RT: 12.329 min Scan# 1844

Delta R.T. -0.006 min

Lab File: VX028116.D

Acq: 14 Apr 2022 18:45

Instrument :

MSVOA_X

ClientSampleId :

MW-46DL





Tgt Ion: 91 Resp: 5387

Ion Ratio Lower Upper

91 100

92 28.9 27.8 83.3

134 112.8 13.3 39.8#

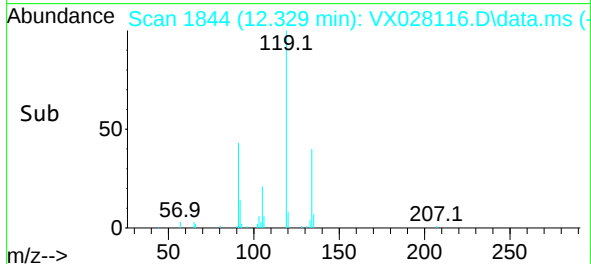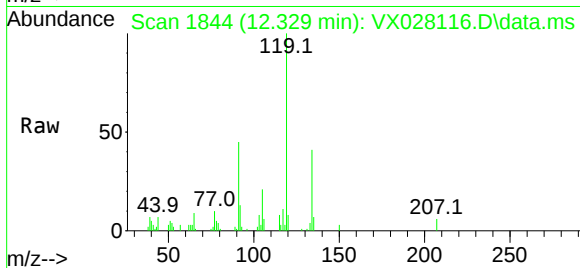

#90

Hexachloroethane

Concen: 1.202 ug/l

RT: 12.615 min Scan# 1891

Delta R.T. 0.073 min

Lab File: VX028116.D




Acq: 14 Apr 2022 18:45


Tgt Ion: 117 Resp: 2220

Ion Ratio Lower Upper

117 100

201 0.0 39.5 118.5#

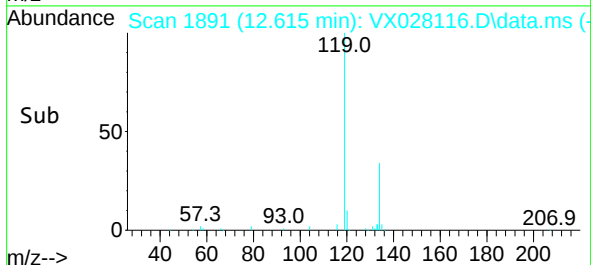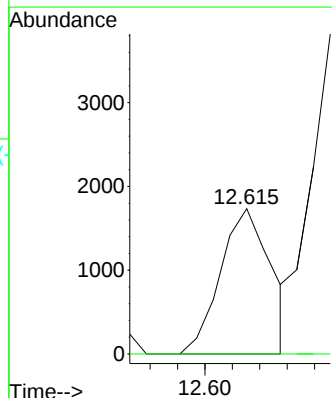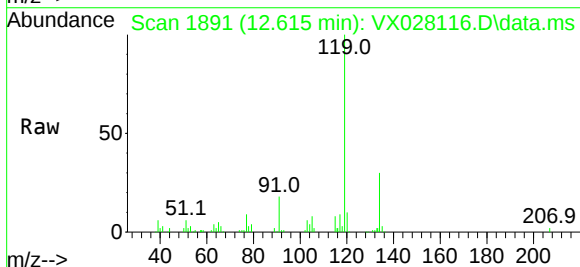

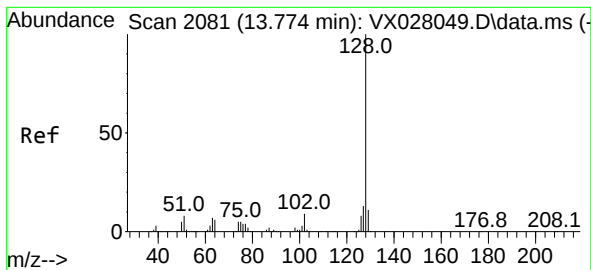

#95

Naphthalene

Concen: 8.820 ug/l

RT: 13.780 min Scan# 20

Delta R.T. 0.006 min

Lab File: VX028116.D


Acq: 14 Apr 2022 18:45

Instrument :

MSVOA_X

ClientSampleId :

MW-46DL

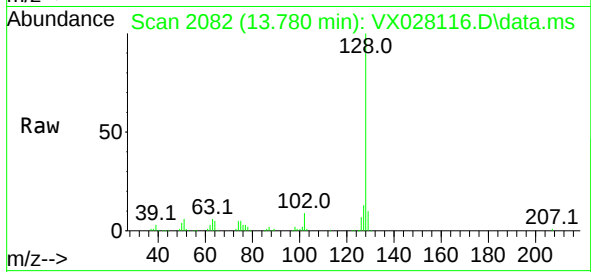

Tgt Ion:128 Resp: 99652

Ion Ratio Lower Upper

128 100

127 12.6 10.2 15.4

129 10.3 8.7 13.1

