

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041422\
 Data File : VX028112.D
 Acq On : 14 Apr 2022 17:11
 Operator : JC/MD
 Sample : N2406-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 220413004-02-VOA

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X041222W.M
 Title : SW846 8260

Signal : TIC: VX028112.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.173	12	14	24	rVB2	19494	26805	2.06%	0.272%
2	1.355	40	44	52	rVB2	25516	29412	2.26%	0.298%
3	1.557	70	77	82	rBV3	24319	45771	3.51%	0.464%
4	1.843	120	124	129	rVB2	8867	13716	1.05%	0.139%
5	2.136	167	172	179	rVB	51850	76527	5.87%	0.777%
6	2.392	206	214	215	rBV2	30000	46560	3.57%	0.472%
7	2.404	215	216	226	rVB2	27828	46338	3.56%	0.470%
8	2.959	298	307	323	rBV	104926	227638	17.47%	2.310%
9	4.568	558	571	590	rBV2	150077	492027	37.77%	4.993%
10	5.007	630	643	663	rBV2	216819	672611	51.63%	6.826%
11	5.391	695	706	718	rBV	146748	424751	32.60%	4.310%
12	5.556	722	733	751	rVB	227223	646147	49.60%	6.557%
13	5.958	789	799	809	rBV	156108	412268	31.65%	4.184%
14	6.050	809	814	822	rVB2	10063	26094	2.00%	0.265%
15	6.245	838	846	855	rBV3	5874	16536	1.27%	0.168%
16	6.763	918	931	950	rBV	370015	879764	67.53%	8.928%
17	7.665	1071	1079	1088	rBV2	11798	27612	2.12%	0.280%
18	7.903	1111	1118	1126	rBV5	7175	15268	1.17%	0.155%
19	8.653	1233	1241	1248	rBV	784286	1224936	94.03%	12.431%
20	8.720	1248	1252	1261	rVB4	12284	24506	1.88%	0.249%
21	8.805	1261	1266	1271	rBV	11528	18987	1.46%	0.193%
22	9.378	1352	1360	1367	rBV	13113	24273	1.86%	0.246%
23	9.494	1373	1379	1385	rVV	20200	29915	2.30%	0.304%
24	10.055	1461	1471	1484	rBV2	829140	1302746	100.00%	13.220%
25	10.195	1490	1494	1507	rBV4	9195	25827	1.98%	0.262%
26	10.305	1507	1512	1518	rVB	77317	110603	8.49%	1.122%
27	10.646	1563	1568	1574	rVB	55358	73244	5.62%	0.743%
28	10.963	1614	1620	1624	rBV2	16137	22607	1.74%	0.229%
29	11.085	1634	1640	1647	rBV	657041	843222	64.73%	8.557%
30	11.378	1682	1688	1691	rBV2	13342	24362	1.87%	0.247%
31	11.616	1723	1727	1735	rVB	27473	38229	2.93%	0.388%
32	11.750	1745	1749	1754	rVB	38629	48701	3.74%	0.494%
33	11.890	1765	1772	1780	rVB2	30897	44459	3.41%	0.451%
34	12.024	1787	1794	1801	rBV2	871672	1213757	93.17%	12.317%
35	12.091	1801	1805	1809	rVB	22561	28892	2.22%	0.293%
36	12.244	1822	1830	1835	rBV2	50188	70974	5.45%	0.720%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041422\
 Data File : VX028112.D
 Acq On : 14 Apr 2022 17:11
 Operator : JC/MD
 Sample : N2406-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 220413004-02-VOA

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X041222W.M
 Title : SW846 8260

37	12.335	1839	1845	1851	rVB3	11851	23448	1.80%	0.238%
38	12.414	1853	1858	1863	rBV5	7669	16274	1.25%	0.165%
39	12.542	1873	1879	1885	rVB4	8339	18522	1.42%	0.188%
40	12.616	1887	1891	1894	rVB	14846	16712	1.28%	0.170%
41	12.908	1935	1939	1945	rVV2	60262	93275	7.16%	0.947%
42	12.963	1945	1948	1952	rVB5	14210	18851	1.45%	0.191%
43	13.292	1997	2002	2007	rBV2	29338	39869	3.06%	0.405%
44	13.426	2020	2024	2028	rBV2	14906	19139	1.47%	0.194%
45	13.475	2028	2032	2035	rVV	36402	50495	3.88%	0.512%
46	13.512	2035	2038	2046	rVB2	37778	53938	4.14%	0.547%
47	13.780	2077	2082	2088	rVB	74738	97109	7.45%	0.985%
48	13.932	2101	2107	2114	rBV7	11082	26502	2.03%	0.269%
49	14.640	2219	2223	2226	rBV	15681	24838	1.91%	0.252%
50	14.664	2226	2227	2232	rVB4	14380	14630	1.12%	0.148%
51	14.780	2242	2246	2253	rVB2	18633	26001	2.00%	0.264%
52	16.334	2495	2501	2507	rVB3	9362	18352	1.41%	0.186%




Sum of corrected areas: 9854040

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041422\
Data File : VX028112.D
Acq On : 14 Apr 2022 17:11
Operator : JC/MD
Sample : N2406-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
220413004-02-VOA

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X041222W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

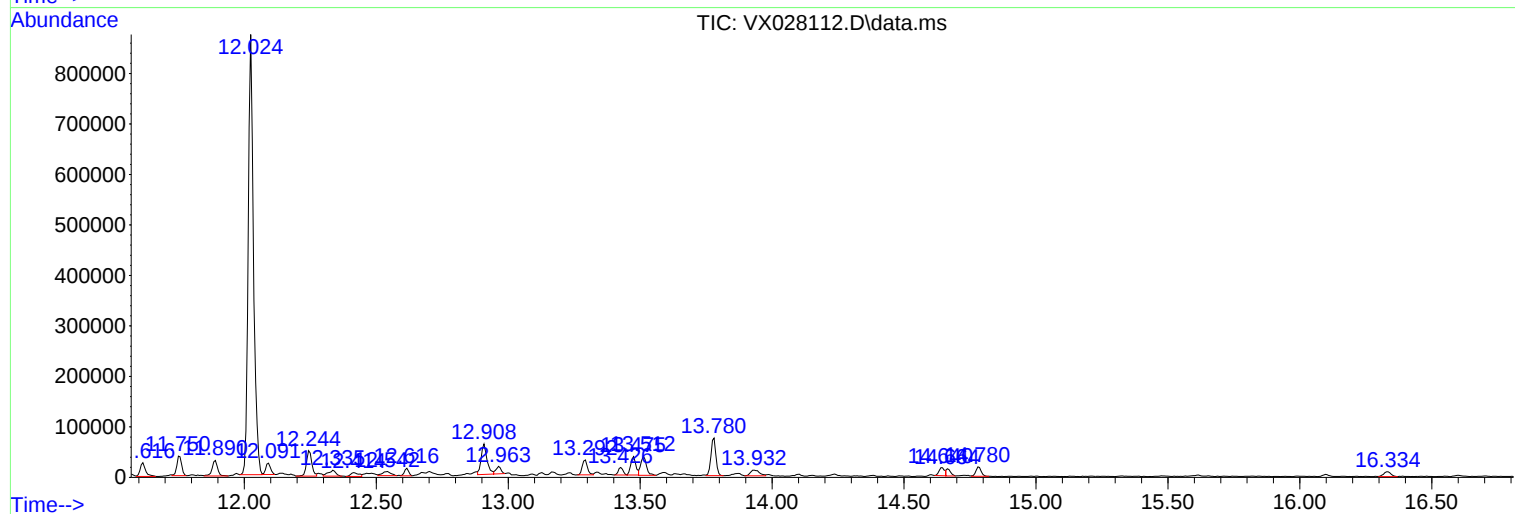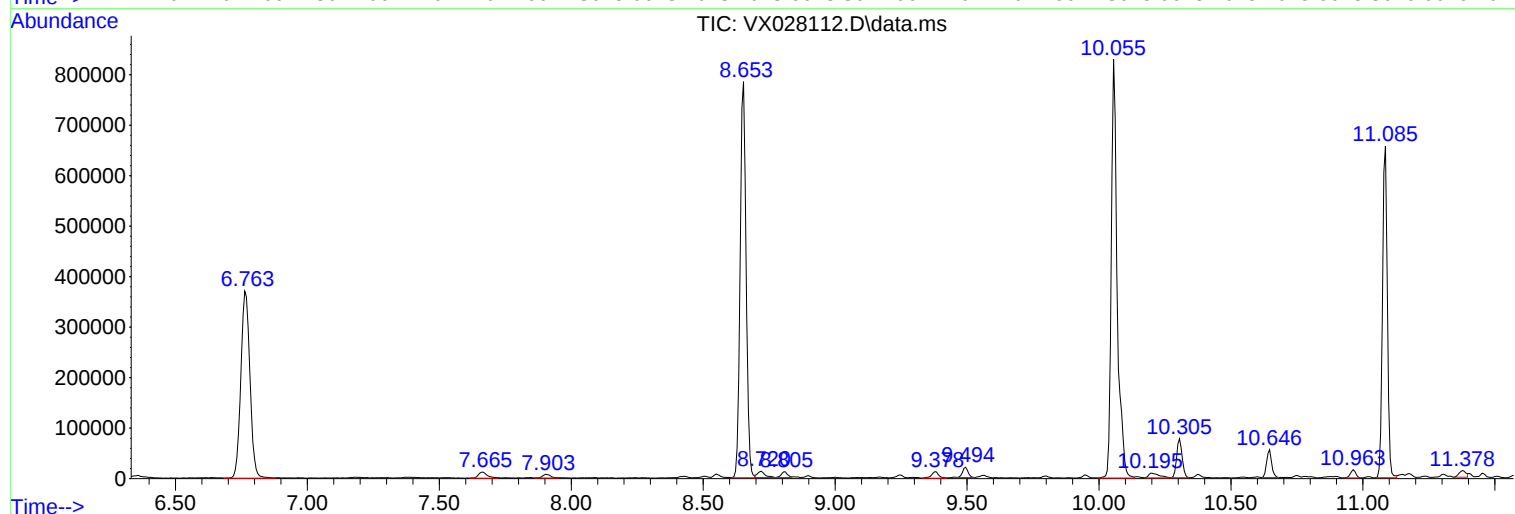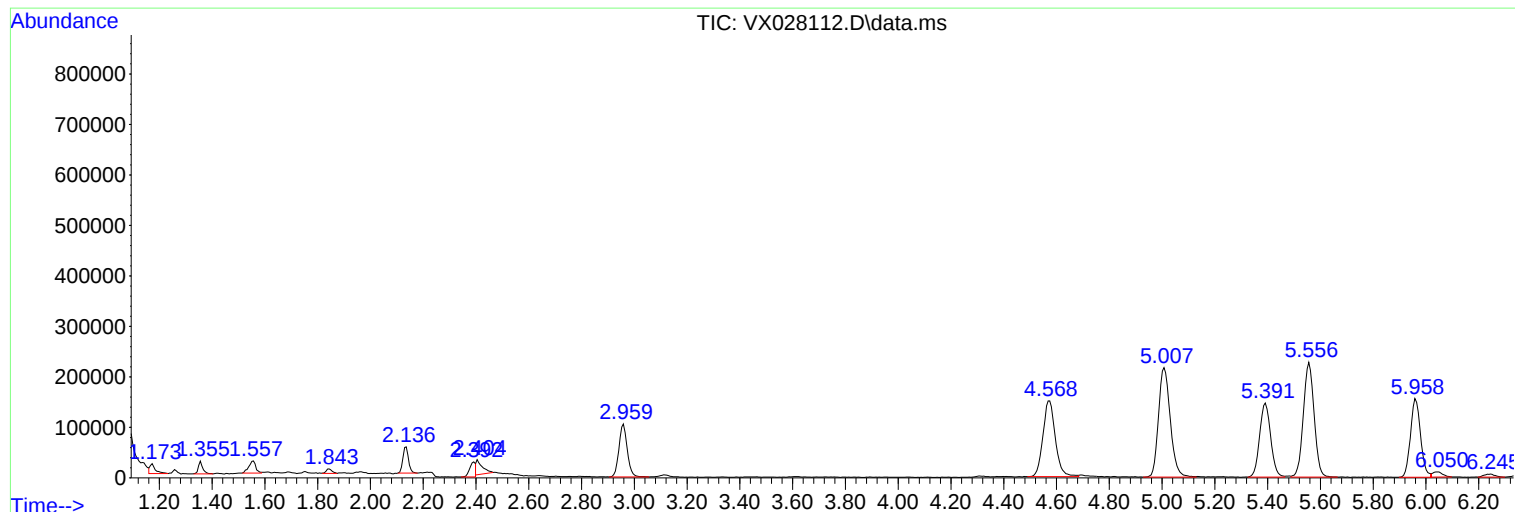

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041422\
Data File : VX028112.D
Acq On : 14 Apr 2022 17:11
Operator : JC/MD
Sample : N2406-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
220413004-02-VOA

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X041222W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041422\
Data File : VX028112.D
Acq On : 14 Apr 2022 17:11
Operator : JC/MD
Sample : N2406-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
220413004-02-VOA

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X041222W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------