

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041422\
 Data File : VX028115.D
 Acq On : 14 Apr 2022 18:21
 Operator : JC/MD
 Sample : N2403-01DL 4X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MW-24DL

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X041222W.M
 Title : SW846 8260

Signal : TIC: VX028115.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.264	26	29	33	rBV	27956	26239	2.06%	0.164%
2	1.367	43	46	51	rBV	153335	154113	12.08%	0.964%
3	1.556	69	77	83	rBV5	18552	44424	3.48%	0.278%
4	1.745	103	108	120	rVB	860281	1191569	93.41%	7.453%
5	1.953	137	142	156	rVB2	151480	245050	19.21%	1.533%
6	2.068	157	161	167	rVV2	12499	17647	1.38%	0.110%
7	2.215	179	185	196	rVB	175764	253682	19.89%	1.587%
8	2.337	198	205	211	rBV	29653	61182	4.80%	0.383%
9	2.782	262	278	281	rBV2	82682	203555	15.96%	1.273%
10	2.824	281	285	288	rVV	102167	202954	15.91%	1.269%
11	2.867	288	292	303	rVV2	136102	300532	23.56%	1.880%
12	2.959	303	307	314	rVB3	6435	13351	1.05%	0.084%
13	3.105	322	331	343	rVB2	114710	268702	21.06%	1.681%
14	3.318	358	366	375	rBV3	9723	22334	1.75%	0.140%
15	3.733	424	434	444	rBV	49432	124683	9.77%	0.780%
16	3.843	444	452	459	rBV	34600	85542	6.71%	0.535%
17	3.995	469	477	484	rBV2	7803	21859	1.71%	0.137%
18	4.105	485	495	503	rVV2	31256	89595	7.02%	0.560%
19	4.214	506	513	518	rVV2	13965	40116	3.14%	0.251%
20	4.306	518	528	540	rVV	195508	550176	43.13%	3.441%
21	4.428	540	548	563	rVB2	25035	78320	6.14%	0.490%
22	4.574	563	572	582	rBV2	6285	19673	1.54%	0.123%
23	5.196	664	674	686	rVB	47224	153176	12.01%	0.958%
24	5.391	693	706	713	rBV	147789	439503	34.45%	2.749%
25	5.476	713	720	726	rVV	103647	297630	23.33%	1.862%
26	5.556	726	733	741	rVB	192485	501177	39.29%	3.135%
27	5.836	767	779	790	rBV6	24433	81741	6.41%	0.511%
28	5.958	790	799	805	rVV	152516	393769	30.87%	2.463%
29	6.043	805	813	825	rVV	378625	1011106	79.26%	6.325%
30	6.245	825	846	857	rVV7	69712	374190	29.33%	2.341%
31	6.360	857	865	877	rVB3	30045	85686	6.72%	0.536%
32	6.763	921	931	941	rBV	365628	913710	71.63%	5.715%
33	6.854	942	946	956	rVB4	29821	78236	6.13%	0.489%
34	6.982	959	967	975	rBV6	6828	17474	1.37%	0.109%
35	7.177	990	999	1007	rBV	32475	73213	5.74%	0.458%
36	7.378	1019	1032	1043	rBV3	98352	260310	20.41%	1.628%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041422\
 Data File : VX028115.D
 Acq On : 14 Apr 2022 18:21
 Operator : JC/MD
 Sample : N2403-01DL 4X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MW-24DL

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X041222W.M
 Title : SW846 8260

37	7.500	1043	1052	1057	rBV8	5118	13077	1.03%	0.082%
38	7.659	1072	1078	1086	rVB4	11109	22592	1.77%	0.141%
39	7.775	1091	1097	1103	rVB3	7158	13899	1.09%	0.087%
40	7.860	1103	1111	1112	rBV3	14467	25249	1.98%	0.158%
41	7.884	1112	1115	1123	rVV7	20492	42907	3.36%	0.268%
42	7.982	1123	1131	1142	rVB2	24363	64036	5.02%	0.401%
43	8.110	1142	1152	1155	rBV2	40811	88335	6.92%	0.553%
44	8.147	1155	1158	1163	rVV	54158	86467	6.78%	0.541%
45	8.195	1163	1166	1176	rVB5	10828	21014	1.65%	0.131%
46	8.311	1178	1185	1192	rBV7	7307	16803	1.32%	0.105%
47	8.433	1200	1205	1210	rBV3	13219	21739	1.70%	0.136%
48	8.506	1211	1217	1225	rVB2	61054	104380	8.18%	0.653%
49	8.653	1225	1241	1248	rBV	804599	1275631	100.00%	7.979%
50	8.720	1248	1252	1258	rVB2	18364	29782	2.33%	0.186%
51	8.811	1263	1267	1269	rVV	14436	22955	1.80%	0.144%
52	8.842	1269	1272	1280	rVV	19192	31046	2.43%	0.194%
53	8.927	1280	1286	1289	rVV2	9902	16508	1.29%	0.103%
54	8.976	1289	1294	1300	rVV5	10676	22246	1.74%	0.139%
55	9.098	1311	1314	1320	rVV2	9588	16001	1.25%	0.100%
56	9.165	1320	1325	1335	rVB	30290	52080	4.08%	0.326%
57	9.378	1356	1360	1365	rBV2	16021	22967	1.80%	0.144%
58	9.457	1365	1373	1378	rVV	128634	202434	15.87%	1.266%
59	9.500	1378	1380	1386	rVB4	10175	15973	1.25%	0.100%
60	9.561	1386	1390	1394	rBV4	11340	17074	1.34%	0.107%
61	10.055	1461	1471	1477	rBV	824707	1119631	87.77%	7.003%
62	10.195	1491	1494	1499	rVV2	36187	62190	4.88%	0.389%
63	10.250	1500	1503	1508	rVV2	19447	31153	2.44%	0.195%
64	10.305	1508	1512	1518	rVB	83218	107378	8.42%	0.672%
65	10.415	1526	1530	1535	rVB2	17348	25456	2.00%	0.159%
66	10.646	1563	1568	1573	rVB2	13929	19852	1.56%	0.124%
67	10.872	1598	1605	1614	rBV4	23840	55332	4.34%	0.346%
68	10.963	1614	1620	1625	rVV	46519	64658	5.07%	0.404%
69	11.085	1634	1640	1645	rVV	670376	850376	66.66%	5.319%
70	11.170	1649	1654	1661	rVB	32279	46320	3.63%	0.290%
71	11.305	1668	1676	1681	rBV	58090	75618	5.93%	0.473%
72	11.402	1686	1692	1696	rBV	20730	29158	2.29%	0.182%
73	11.494	1703	1707	1712	rVB	16702	22843	1.79%	0.143%
74	11.616	1722	1727	1733	rBV	94128	122265	9.58%	0.765%
75	11.713	1738	1743	1746	rVV4	19830	30795	2.41%	0.193%
76	11.756	1746	1750	1755	rVB	24911	33256	2.61%	0.208%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041422\
 Data File : VX028115.D
 Acq On : 14 Apr 2022 18:21
 Operator : JC/MD
 Sample : N2403-01DL 4X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MW-24DL

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X041222W.M
 Title : SW846 8260

77	12.024	1788	1794	1800	rBV	884130	1068640	83.77%	6.684%
78	12.091	1800	1805	1809	rVV	26311	35523	2.78%	0.222%
79	12.243	1825	1830	1835	rBV	458754	561304	44.00%	3.511%
80	12.317	1839	1842	1850	rVB4	12629	21357	1.67%	0.134%
81	12.408	1853	1857	1861	rBV2	11601	15405	1.21%	0.096%
82	12.463	1862	1866	1872	rVB	19716	27144	2.13%	0.170%
83	12.530	1872	1877	1885	rBV3	12641	22187	1.74%	0.139%
84	12.615	1885	1891	1894	rBV	38598	49637	3.89%	0.310%
85	12.646	1894	1896	1900	rVB	17880	19488	1.53%	0.122%
86	12.701	1900	1905	1912	rBV	94013	118446	9.29%	0.741%
87	12.847	1925	1929	1933	rVB3	9774	13453	1.05%	0.084%
88	12.926	1933	1942	1945	rBV	27485	41624	3.26%	0.260%
89	12.963	1945	1948	1953	rVB	13101	16332	1.28%	0.102%
90	13.030	1953	1959	1965	rBV4	7089	13234	1.04%	0.083%
91	13.170	1978	1982	1992	rVB	32625	47125	3.69%	0.295%
92	13.292	1998	2002	2007	rBV2	76658	99691	7.82%	0.624%
93	13.341	2007	2010	2014	rVB4	11404	15416	1.21%	0.096%
94	13.426	2020	2024	2029	rVB2	19884	25696	2.01%	0.161%
95	13.780	2077	2082	2091	rVB	91596	119331	9.35%	0.746%
96	14.780	2242	2246	2252	rVB2	12646	18277	1.43%	0.114%




Sum of corrected areas: 15987005

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041422\
Data File : VX028115.D
Acq On : 14 Apr 2022 18:21
Operator : JC/MD
Sample : N2403-01DL 4X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-24DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X041222W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

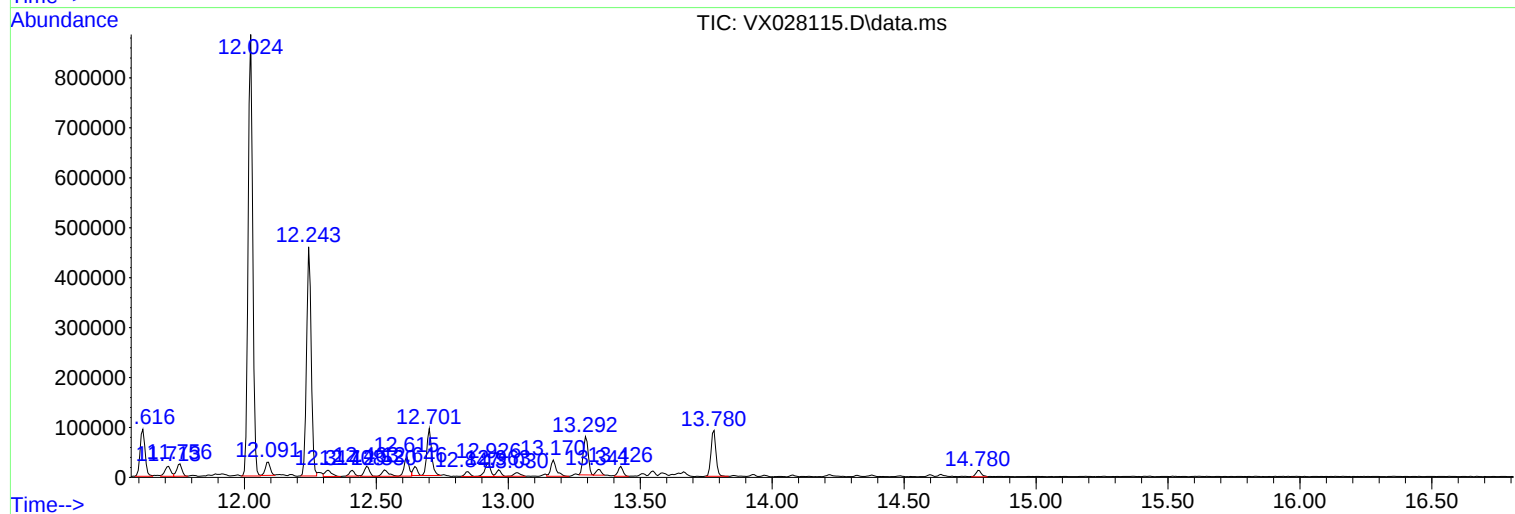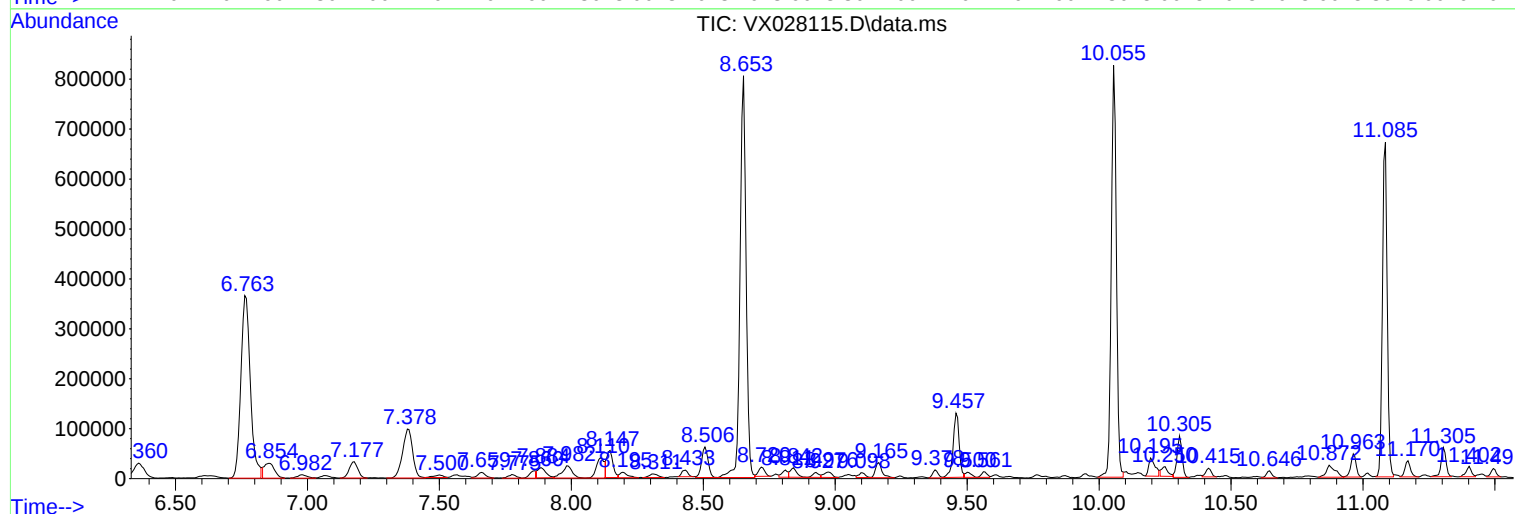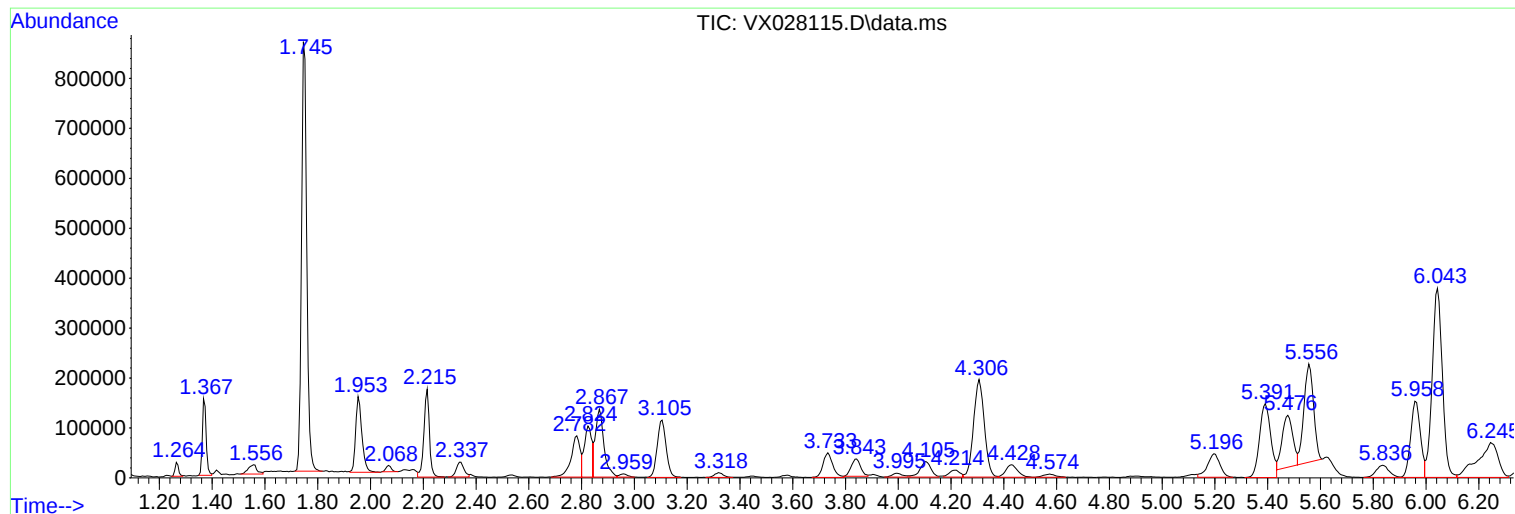

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041422\
Data File : VX028115.D
Acq On : 14 Apr 2022 18:21
Operator : JC/MD
Sample : N2403-01DL 4X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-24DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X041222W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041422\
Data File : VX028115.D
Acq On : 14 Apr 2022 18:21
Operator : JC/MD
Sample : N2403-01DL 4X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-24DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X041222W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------