

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041423\
 Data File : VX035066.D
 Acq On : 13 Apr 2023 16:01
 Operator : JC/MD
 Sample : IBLK
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 IBLK

Quant Time: Apr 14 05:42:11 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032923W.M
 Quant Title : SW846 8260
 QLast Update : Sat Apr 01 01:50:18 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.556	168	262859	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	440716	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	387318	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	167959	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	174960	43.522	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	=	87.040%
35) Dibromofluoromethane	5.385	113	130307	44.702	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	89.400%
50) Toluene-d8	8.647	98	521608	48.479	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	=	96.960%
62) 4-Bromofluorobenzene	11.079	95	189465	45.505	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	91.020%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041423\
Data File : VX035066.D
Acq On : 13 Apr 2023 16:01
Operator : JC/MD
Sample : IBLK
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
IBLK

Quant Time: Apr 14 05:42:11 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032923W.M
Quant Title : SW846 8260
QLast Update : Sat Apr 01 01:50:18 2023
Response via : Initial Calibration




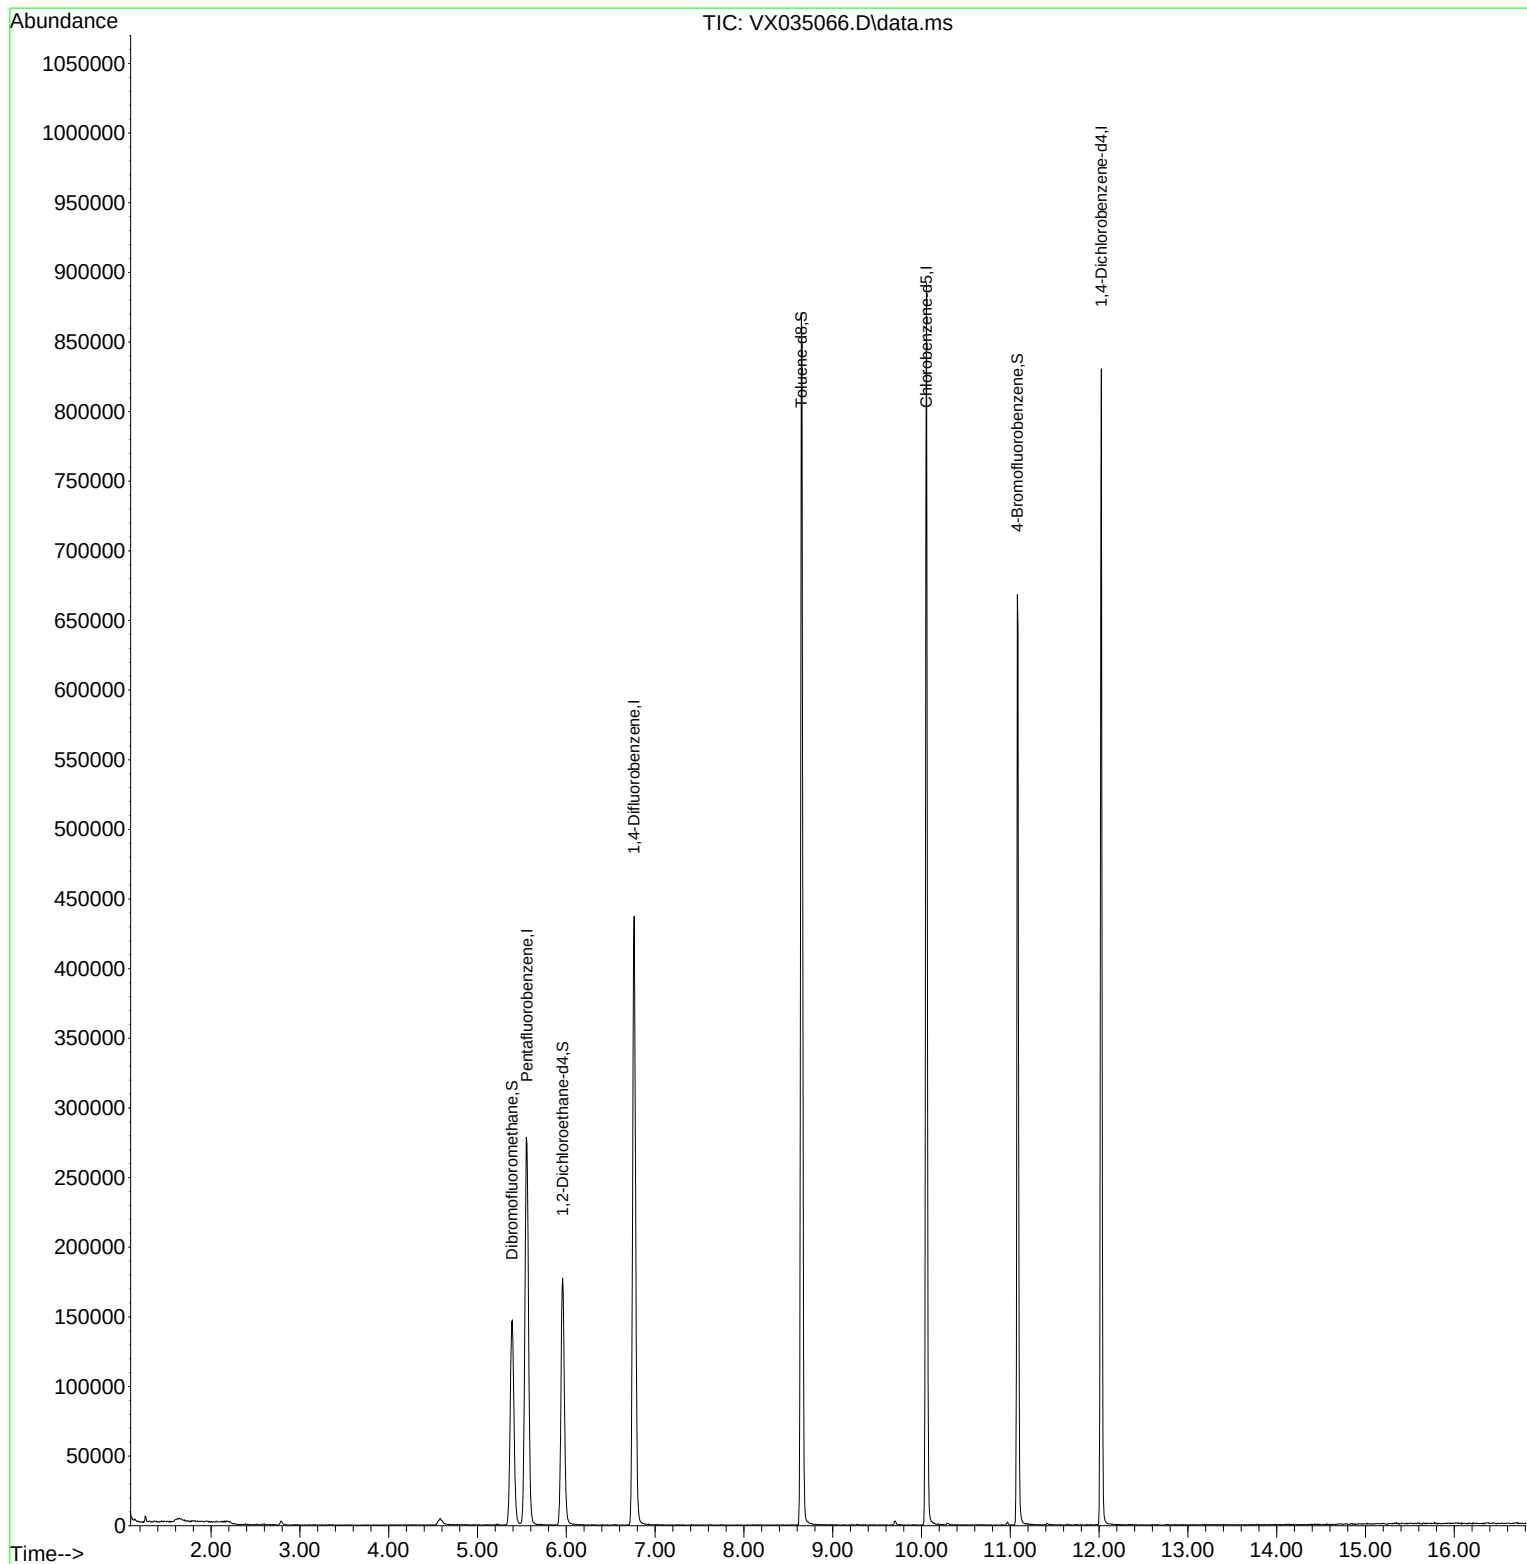


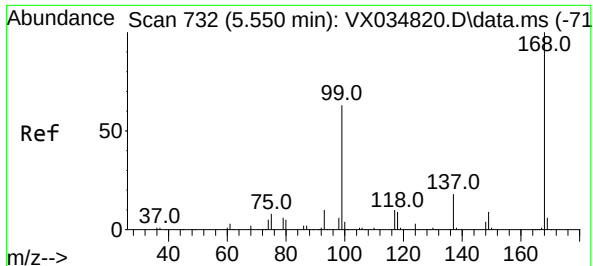

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.556 min Scan# 71
Delta R.T. 0.006 min
Lab File: VX035066.D
Acq: 13 Apr 2023 16:01




Instrument :
MSVOA_X
ClientSampleId :
IBLK


Tgt Ion:168 Resp: 262859
Ion Ratio Lower Upper
168 100
99 59.1 45.7 68.5

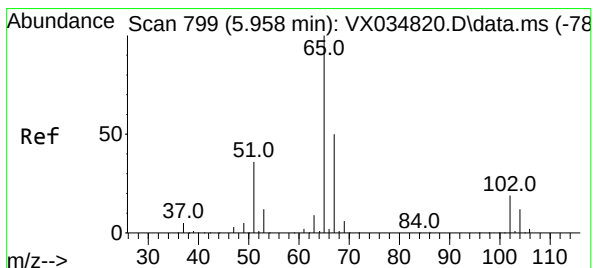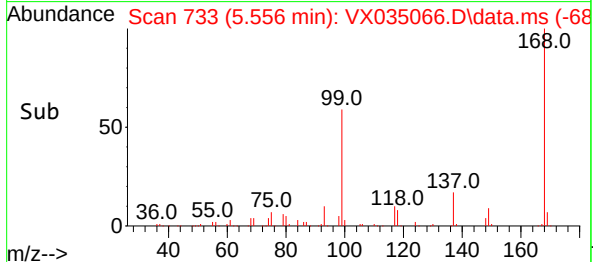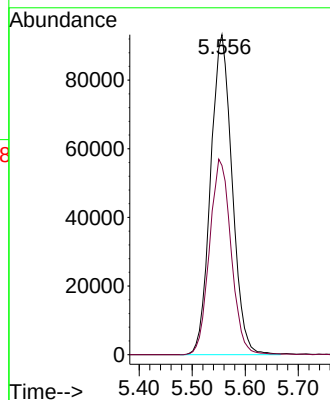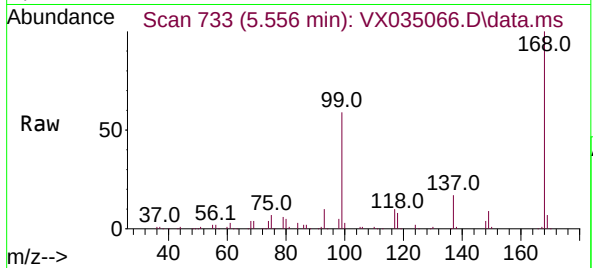

#33
1,2-Dichloroethane-d4
Concen: 43.522 ug/l
RT: 5.958 min Scan# 799
Delta R.T. 0.000 min
Lab File: VX035066.D
Acq: 13 Apr 2023 16:01

Tgt Ion: 65 Resp: 174960
Ion Ratio Lower Upper
65 100
67 51.2 0.0 104.0


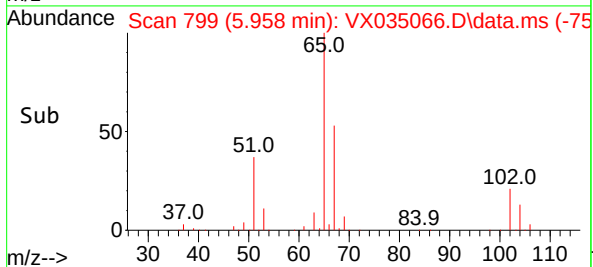
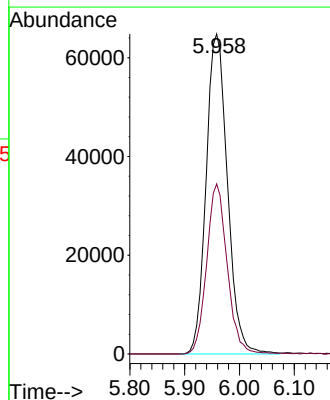
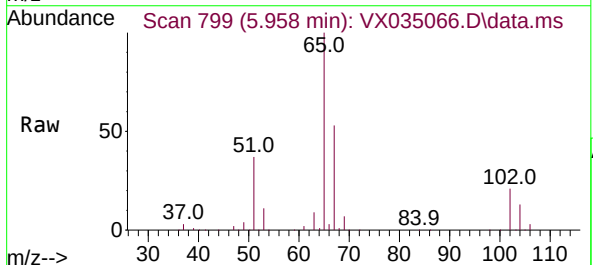


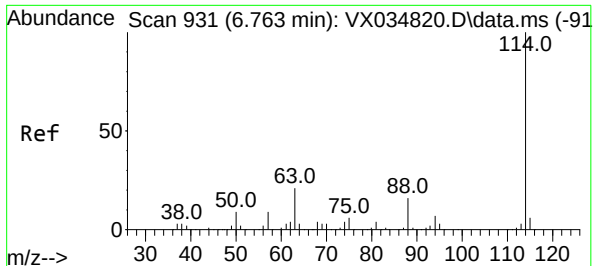

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.763 min Scan# 91
Delta R.T. 0.000 min
Lab File: VX035066.D
Acq: 13 Apr 2023 16:01




Instrument :
MSVOA_X
ClientSampleId :
IBLK


Tgt Ion:114 Resp: 440716
Ion Ratio Lower Upper
114 100
63 21.8 0.0 42.2
88 17.0 0.0 33.2

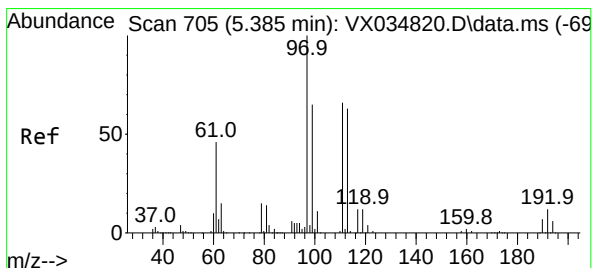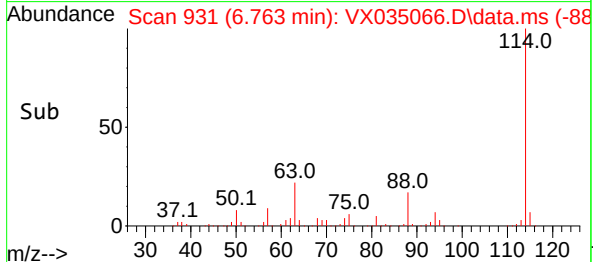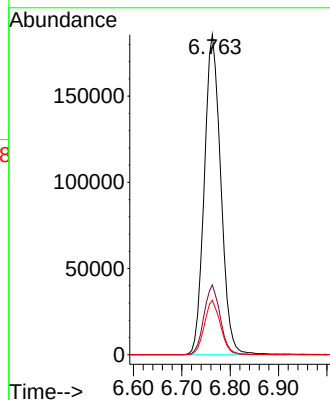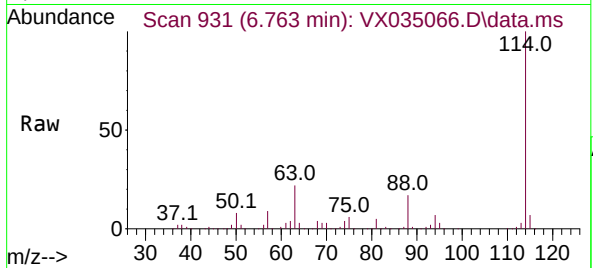

#35
Dibromofluoromethane
Concen: 44.702 ug/l
RT: 5.385 min Scan# 705
Delta R.T. 0.000 min
Lab File: VX035066.D
Acq: 13 Apr 2023 16:01

Tgt Ion:113 Resp: 130307
Ion Ratio Lower Upper
113 100
111 103.9 83.7 125.5
192 19.5 15.4 23.2


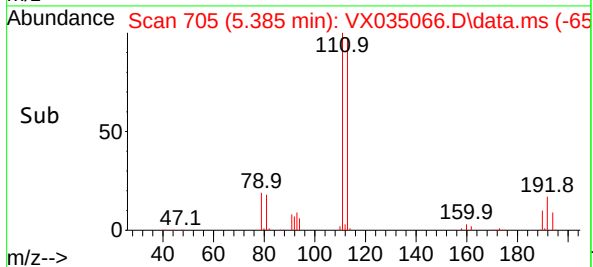
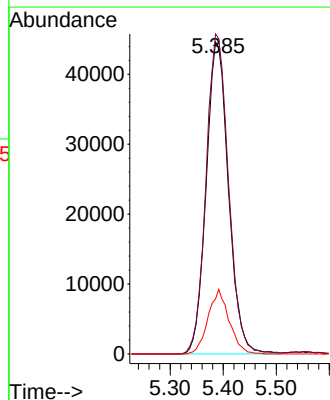
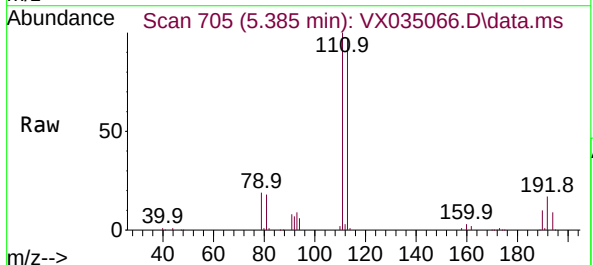


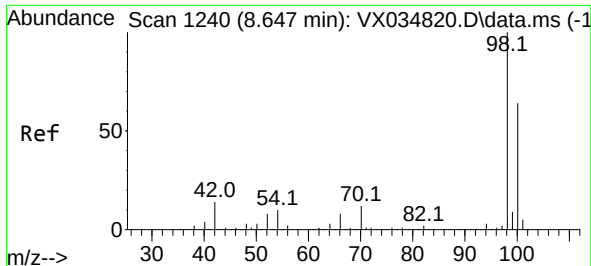

#50
Toluene-d8
Concen: 48.479 ug/l
RT: 8.647 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX035066.D
Acq: 13 Apr 2023 16:01




Instrument :
MSVOA_X
ClientSampleId :
IBLK


Tgt Ion: 98 Resp: 521608
Ion Ratio Lower Upper
98 100
100 67.2 52.5 78.7

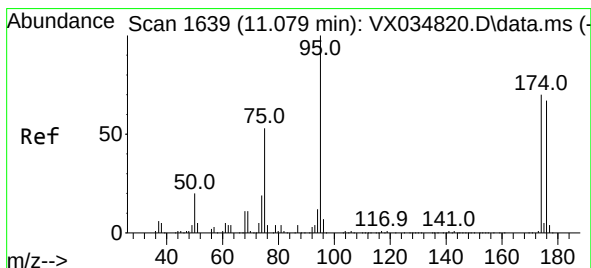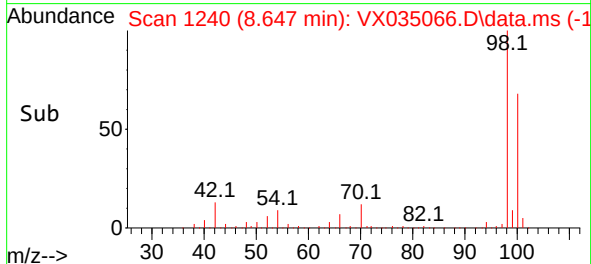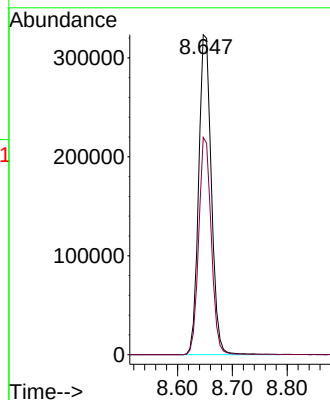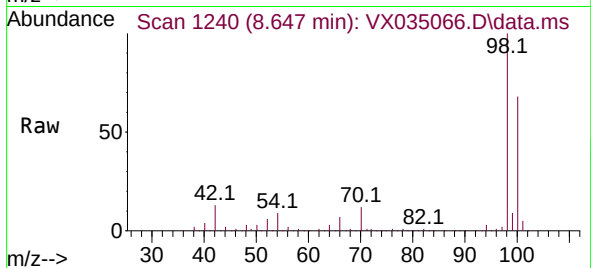

#62
4-Bromofluorobenzene
Concen: 45.505 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.000 min
Lab File: VX035066.D
Acq: 13 Apr 2023 16:01

Tgt Ion: 95 Resp: 189465
Ion Ratio Lower Upper
95 100
174 72.9 0.0 147.4
176 72.0 0.0 140.6


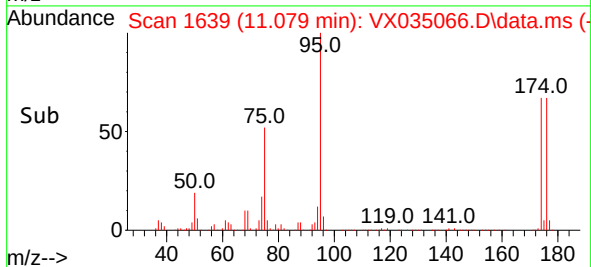
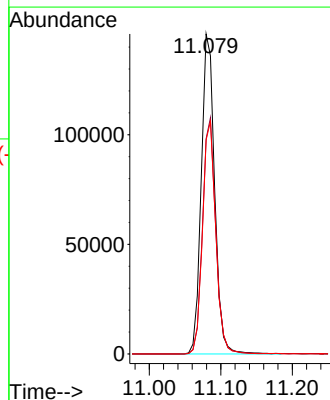
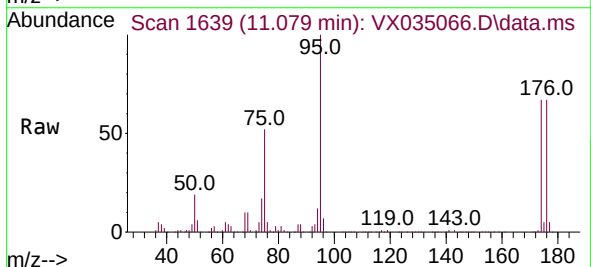


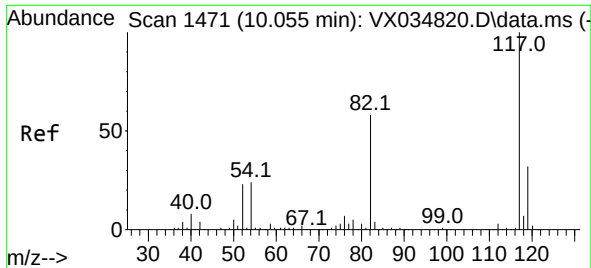

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX035066.D
Acq: 13 Apr 2023 16:01

Instrument :
MSVOA_X
ClientSampleId :
IBLK

Tgt Ion:117 Resp: 387318
Ion Ratio Lower Upper
117 100
82 56.3 45.0 67.4
119 32.2 26.0 39.0

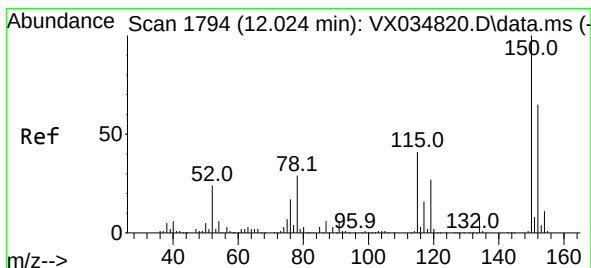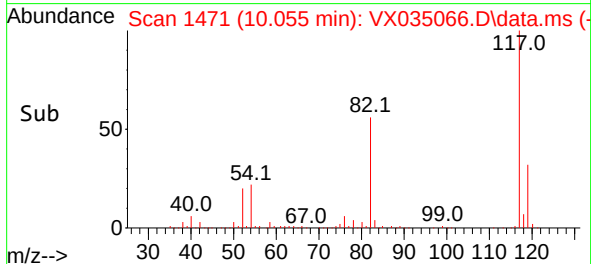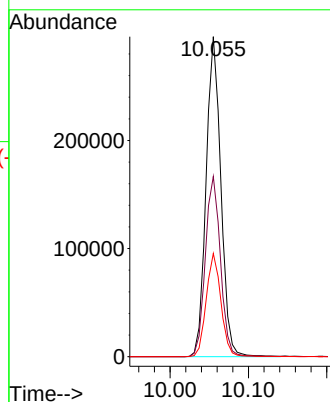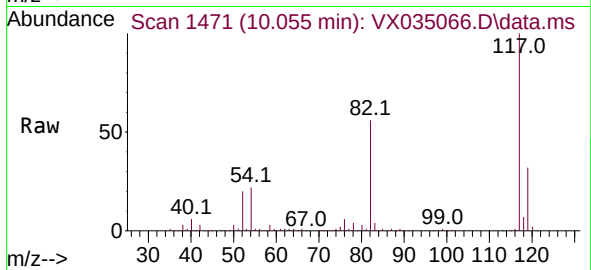

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. 0.000 min
Lab File: VX035066.D
Acq: 13 Apr 2023 16:01

Tgt Ion:152 Resp: 167959
Ion Ratio Lower Upper
152 100
115 62.3 45.0 135.0
150 158.2 0.0 352.4

