

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041425\
 Data File : VX045768.D
 Acq On : 14 Apr 2025 15:12
 Operator : JC/MD
 Sample : Q1771-04
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 TP-6C

Quant Time: Apr 15 01:29:06 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X040225W.M
 Quant Title : SW846 8260
 QLast Update : Wed Apr 02 03:11:43 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.544	168	68783	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.757	114	135123	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.049	117	132172	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.018	152	56416	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.952	65	68050	54.100	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	= 108.200%	
35) Dibromofluoromethane	5.385	113	48552	50.644	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	= 101.280%	
50) Toluene-d8	8.647	98	172726	51.618	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	= 103.240%	
62) 4-Bromofluorobenzene	11.079	95	67752	55.586	ug/l	0.00
Spiked Amount	50.000	Range	77 - 121	Recovery	= 111.180%	
Target Compounds						
					Qvalue	
11) Tert butyl alcohol	2.989	59	242	1.432	ug/l #	72
13) Acrolein	2.239	56	388	1.667	ug/l #	49
14) Allyl chloride	2.648	41	489	0.312	ug/l #	40
16) Acetone	2.386	43	27317	52.887	ug/l	100
18) Methyl Acetate	2.709	43	1825	1.535	ug/l #	85
20) Methylene Chloride	2.782	84	3124	3.231	ug/l	85
25) 2-Butanone	4.580	43	4252	5.624	ug/l #	84
29) Tetrahydrofuran	5.044	42	366	0.747	ug/l #	39
31) Cyclohexane	5.544	56	2160	1.400	ug/l #	1
36) 1,1-Dichloropropene	5.538	75	6773	5.232	ug/l #	50
37) Ethyl Acetate	4.580	43	4252	2.607	ug/l #	71
38) Carbon Tetrachloride	5.544	117	8434	6.029	ug/l #	14
41) Methacrylonitrile	5.044	41	326	0.379	ug/l #	37
43) Isopropyl Acetate	6.348	43	7783	3.148	ug/l	98
48) Methyl methacrylate	7.799	41	36646	28.707	ug/l #	50
49) 1,4-Dioxane	7.793	88	57	2.468	ug/l #	1
51) 4-Methyl-2-Pentanone	8.549	43	31735	19.363	ug/l #	49
53) t-1,3-Dichloropropene	8.958	75	131	2.375	ug/l #	43
54) cis-1,3-Dichloropropene	8.549	75	12693	8.932	ug/l #	64
57) 1,3-Dichloropropane	9.482	76	1138	0.686	ug/l #	42
59) 2-Hexanone	9.372	43	8928	7.356	ug/l #	28
67) Ethyl Benzene	10.195	91	1172	0.232	ug/l	99
69) o-Xylene	10.646	106	444	0.245	ug/l	99
73) Isopropylbenzene	10.963	105	925	0.205	ug/l	81
76) 1,2,3-Trichloropropane	11.079	75	38509	27.984	ug/l #	37
78) n-propylbenzene	11.311	91	1104	0.212	ug/l	86
80) 1,3,5-Trimethylbenzene	11.451	105	1294	0.346	ug/l	82
81) trans-1,4-Dichloro-2-b...	11.079	75	38509	94.973	ug/l #	1
84) 1,2,4-Trimethylbenzene	11.750	105	2732	0.728	ug/l	95
85) sec-Butylbenzene	11.884	105	1629	0.358	ug/l	97
86) p-Isopropyltoluene	11.969	119	971	0.259	ug/l	93
89) n-Butylbenzene	12.329	91	1016	0.313	ug/l #	46
90) Hexachloroethane	12.616	117	472	0.733	ug/l #	19
95) Naphthalene	13.774	128	14440	3.689	ug/l #	96

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041425\
Data File : VX045768.D
Acq On : 14 Apr 2025 15:12
Operator : JC/MD
Sample : Q1771-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TP-6C

Quant Time: Apr 15 01:29:06 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X040225W.M
Quant Title : SW846 8260
QLast Update : Wed Apr 02 03:11:43 2025
Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


(#)=qualifier out of range (m)=manual integration (+)=signals summed						

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041425\
Data File : VX045768.D
Acq On : 14 Apr 2025 15:12
Operator : JC/MD
Sample : Q1771-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TP-6C

Quant Time: Apr 15 01:29:06 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X040225W.M
Quant Title : SW846 8260
QLast Update : Wed Apr 02 03:11:43 2025
Response via : Initial Calibration




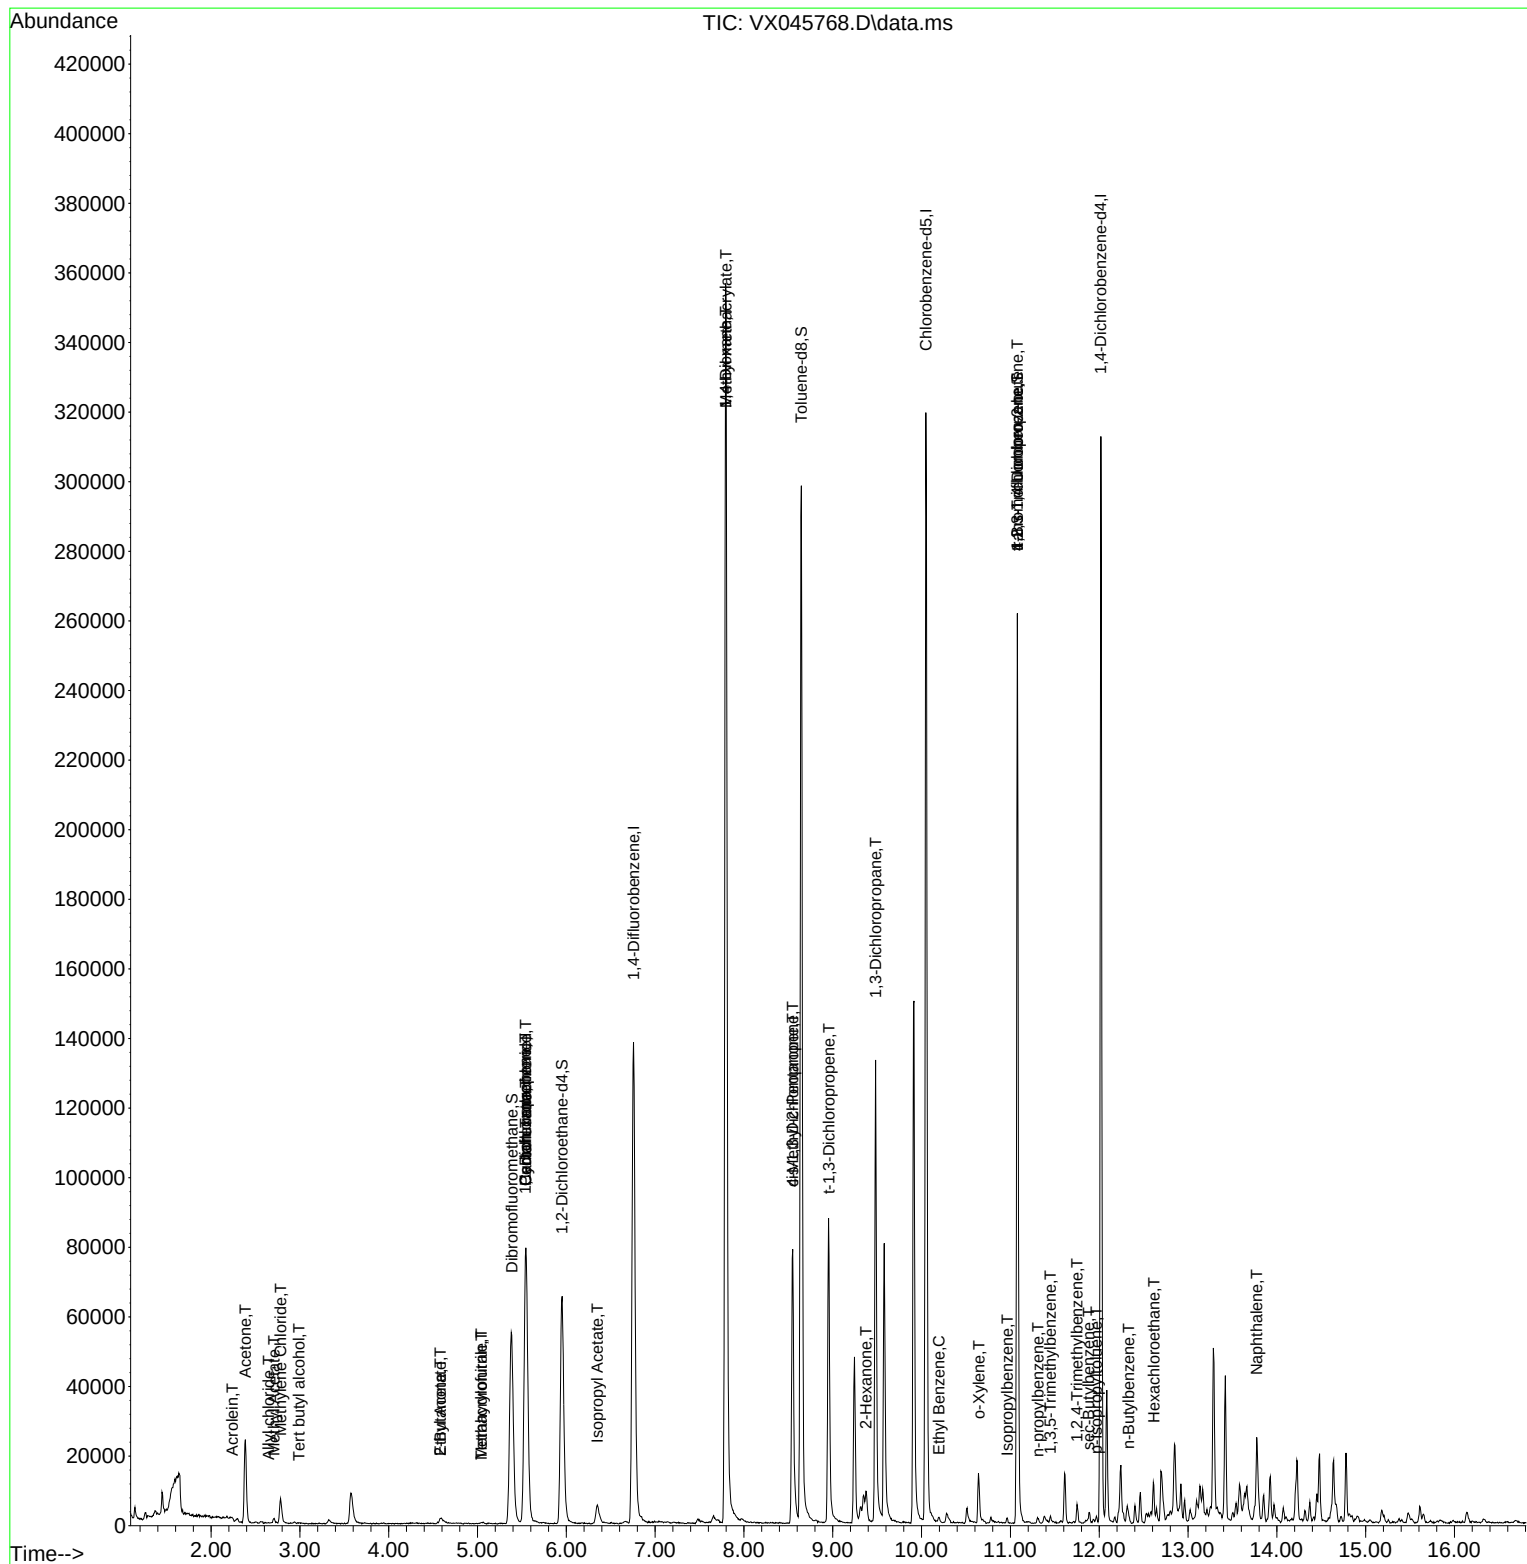




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.544 min Scan# 71
Delta R.T. -0.006 min
Lab File: VX045768.D
Acq: 14 Apr 2025 15:12




Instrument :
MSVOA_X
ClientSampleId :
TP-6C


Tgt Ion:168 Resp: 68783
Ion Ratio Lower Upper
168 100
99 70.6 52.3 78.5

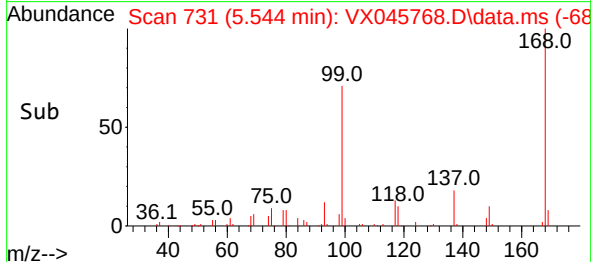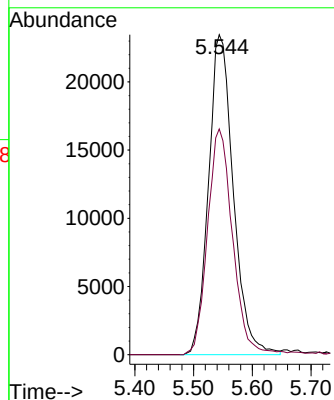

#11
Tert butyl alcohol
Concen: 1.432 ug/l
RT: 2.989 min Scan# 312
Delta R.T. 0.012 min
Lab File: VX045768.D
Acq: 14 Apr 2025 15:12

Tgt Ion: 59 Resp: 242
Ion Ratio Lower Upper
59 100
57 0.0 8.6 12.8#


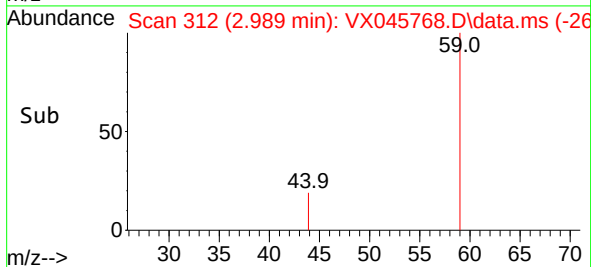
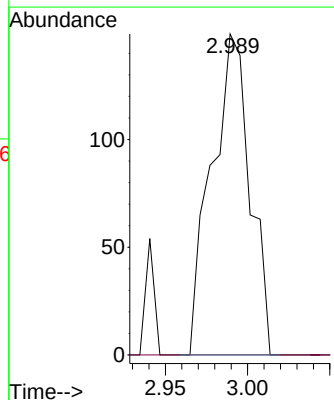
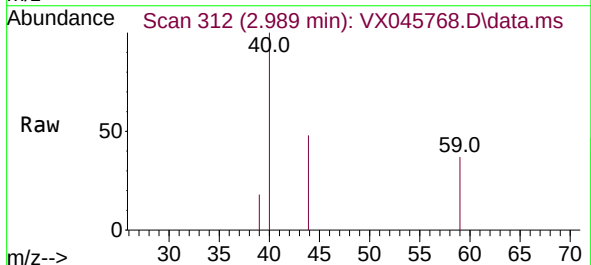




#13
Acrolein
Concen: 1.667 ug/l
RT: 2.239 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX045768.D
Acq: 14 Apr 2025 15:12




Instrument :
MSVOA_X
ClientSampleId :
TP-6C


Tgt Ion: 56 Resp: 388
Ion Ratio Lower Upper
56 100
55 111.9 56.2 84.2#



#14
Allyl chloride
Concen: 0.312 ug/l
RT: 2.648 min Scan# 256
Delta R.T. -0.012 min
Lab File: VX045768.D
Acq: 14 Apr 2025 15:12

Tgt Ion: 41 Resp: 489
Ion Ratio Lower Upper
41 100
39 22.3 60.2 90.2#
76 0.0 24.6 36.8#


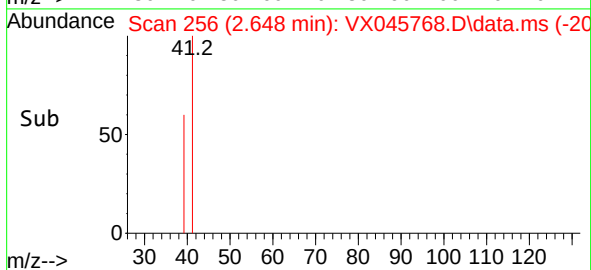

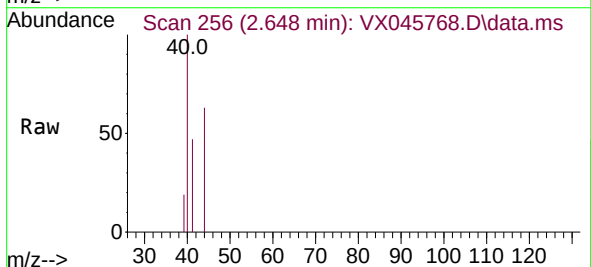




#16
Acetone
Concen: 52.887 ug/l
RT: 2.386 min Scan# 213
Delta R.T. 0.000 min
Lab File: VX045768.D
Acq: 14 Apr 2025 15:12




Instrument :
MSVOA_X
ClientSampleId :
TP-6C


Tgt Ion: 43 Resp: 27317
Ion Ratio Lower Upper
43 100
58 27.9 22.3 33.5

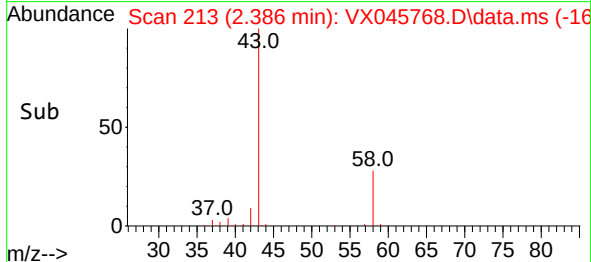

#18
Methyl Acetate
Concen: 1.535 ug/l
RT: 2.709 min Scan# 266
Delta R.T. 0.006 min
Lab File: VX045768.D
Acq: 14 Apr 2025 15:12

Tgt Ion: 43 Resp: 1825
Ion Ratio Lower Upper
43 100
74 14.6 17.5 26.3#


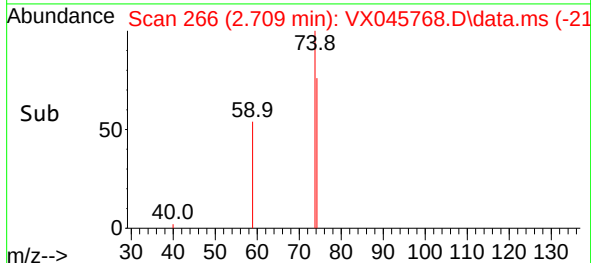
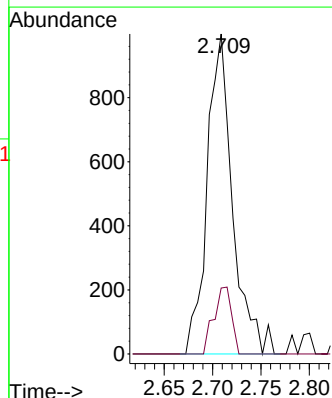
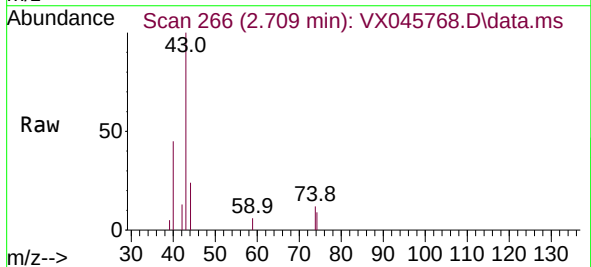




#20
Methylene Chloride
Concen: 3.231 ug/l
RT: 2.782 min Scan# 21
Delta R.T. 0.000 min
Lab File: VX045768.D
Acq: 14 Apr 2025 15:12




Instrument :
MSVOA_X
ClientSampleId :
TP-6C


Tgt Ion:	84	Resp:	3124
Ion	Ratio	Lower	Upper
84	100		
49	160.7	107.5	161.3
51	45.8	33.0	49.6
86	57.6	50.1	75.1

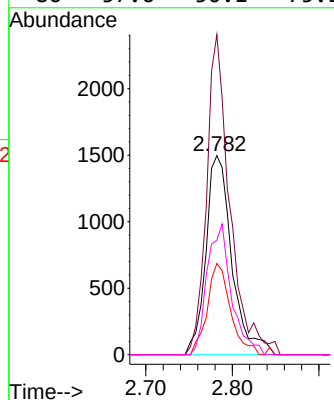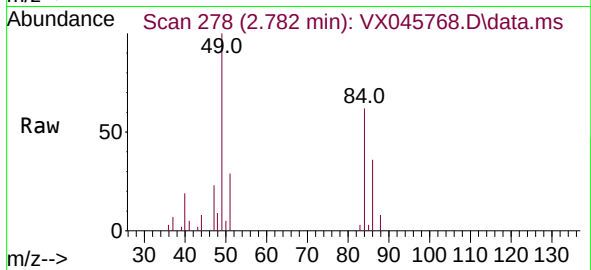

#25
2-Butanone
Concen: 5.624 ug/l
RT: 4.580 min Scan# 573
Delta R.T. 0.024 min
Lab File: VX045768.D
Acq: 14 Apr 2025 15:12

Tgt Ion:	43	Resp:	4252
Ion	Ratio	Lower	Upper
43	100		
72	15.7	18.6	28.0#

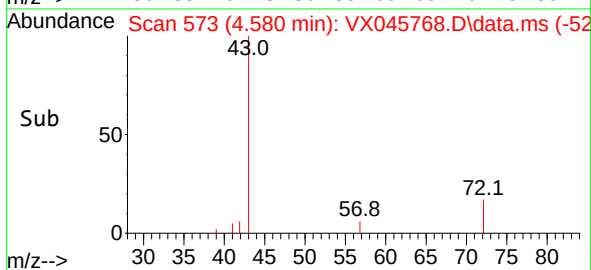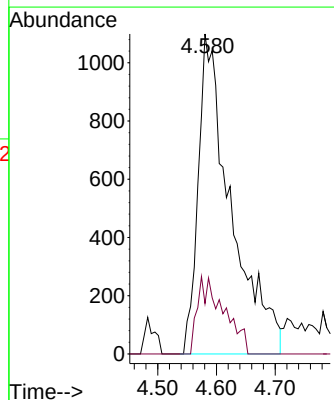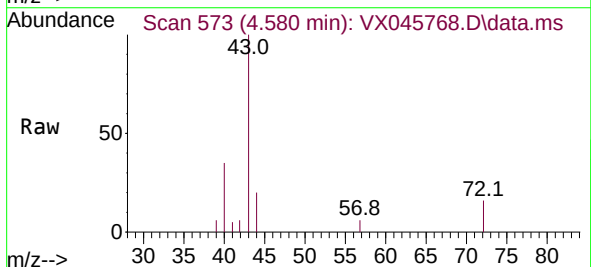

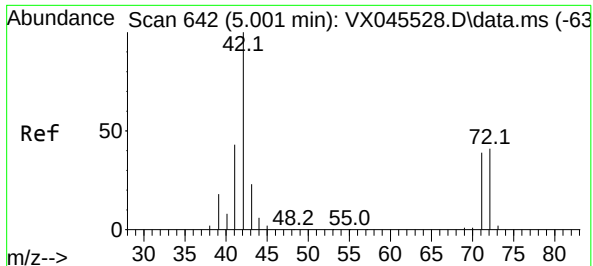

#29

Tetrahydrofuran

Concen: 0.747 ug/l

RT: 5.044 min Scan# 642

Delta R.T. 0.043 min

Lab File: VX045768.D

Acq: 14 Apr 2025 15:12





Instrument :

MSVOA_X

ClientSampleId :

TP-6C

Tgt Ion:	42	Resp:	366
Ion	Ratio	Lower	Upper
42	100		
72	5.2	33.4	50.0#
71	0.0	31.4	47.0#

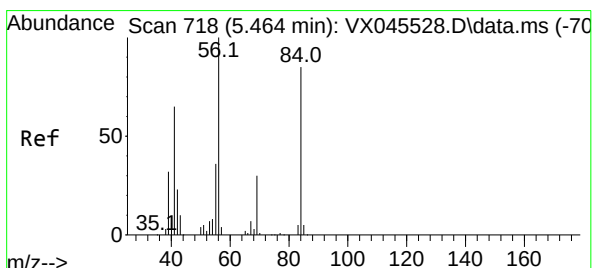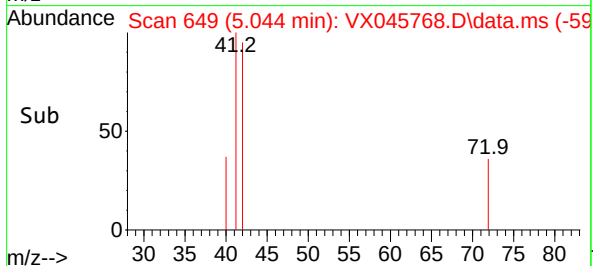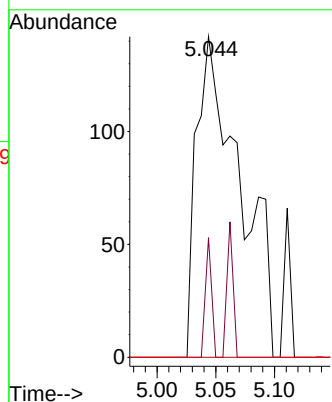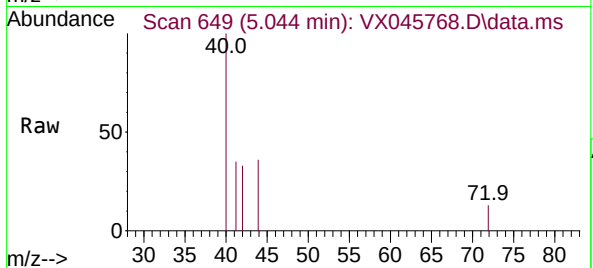

#31

Cyclohexane

Concen: 1.400 ug/l




RT: 5.544 min Scan# 731


Delta R.T. 0.079 min

Lab File: VX045768.D

Acq: 14 Apr 2025 15:12

Tgt Ion:	56	Resp:	2160
Ion	Ratio	Lower	Upper
56	100		
69	187.0	23.6	35.4#
84	114.4	67.7	101.5#

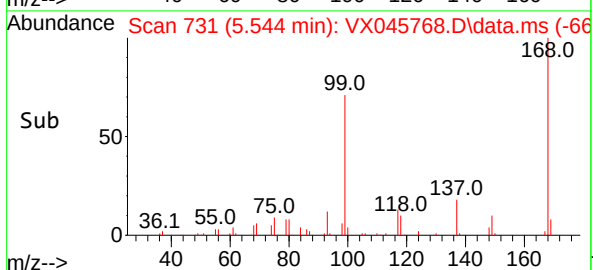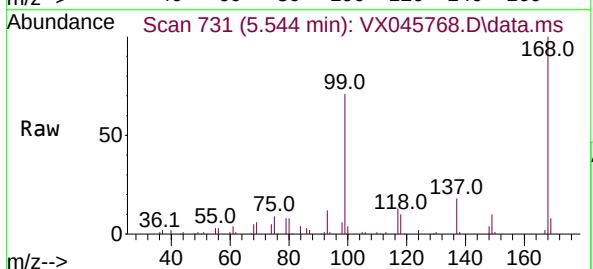



#33

1,2-Dichloroethane-d4

Concen: 54.100 ug/l

RT: 5.952 min Scan# 798

Delta R.T. 0.000 min

Lab File: VX045768.D

Acq: 14 Apr 2025 15:12

Instrument :

MSVOA_X

ClientSampleId :





TP-6C

Tgt Ion: 65 Resp: 68050

Ion Ratio Lower Upper

65 100

67 48.9 0.0 99.0

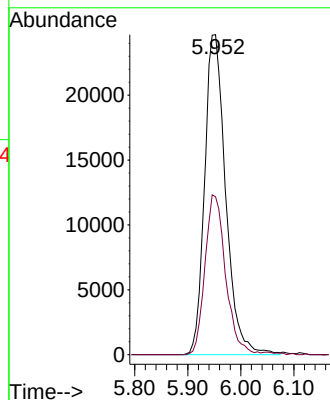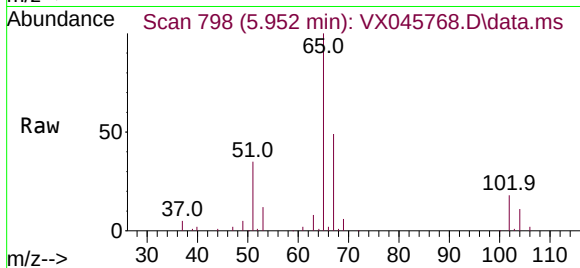

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.757 min Scan# 930

Delta R.T. 0.000 min

Lab File: VX045768.D

Acq: 14 Apr 2025 15:12




Tgt Ion: 114 Resp: 135123


Ion Ratio Lower Upper

114 100

63 23.8 0.0 46.8

88 17.3 0.0 35.4


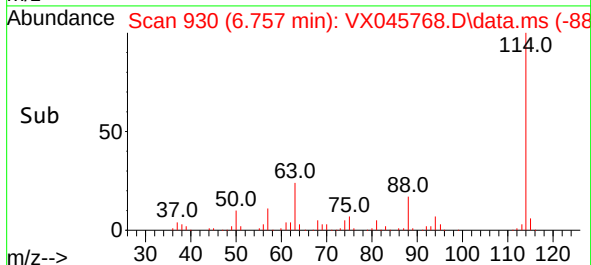
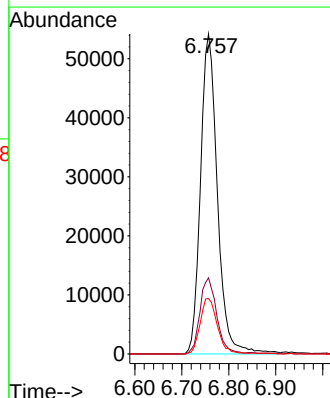
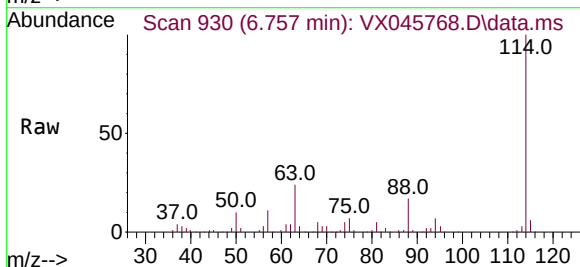




#35
Dibromofluoromethane
Concen: 50.644 ug/l
RT: 5.385 min Scan# 704
Delta R.T. 0.006 min
Lab File: VX045768.D
Acq: 14 Apr 2025 15:12




Instrument :
MSVOA_X
ClientSampleId :
TP-6C


Tgt Ion:113 Resp: 48552
Ion Ratio Lower Upper
113 100
111 101.5 81.8 122.6
192 16.5 13.8 20.6

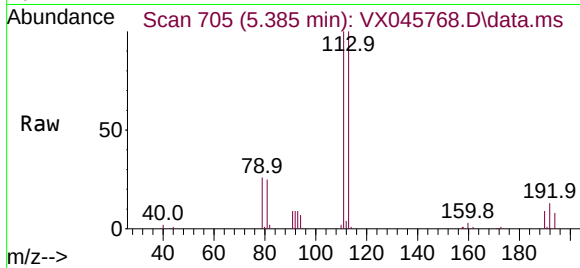

#36
1,1-Dichloropropene
Concen: 5.232 ug/l
RT: 5.538 min Scan# 730
Delta R.T. -0.146 min
Lab File: VX045768.D
Acq: 14 Apr 2025 15:12

Tgt Ion: 75 Resp: 6773
Ion Ratio Lower Upper
75 100
110 9.1 16.9 50.6#
77 0.0 25.0 37.4#

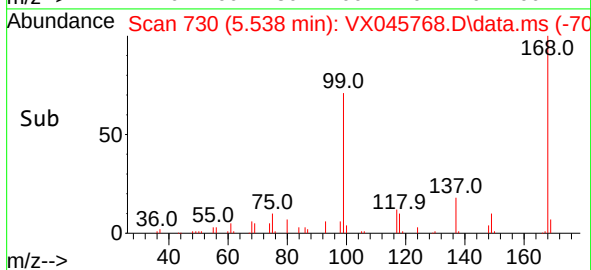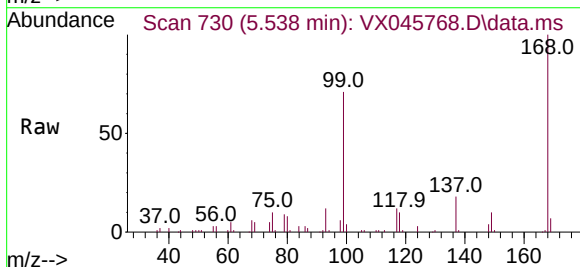



#37

Ethyl Acetate

Concen: 2.607 ug/l

RT: 4.580 min Scan# 51

Delta R.T. -0.134 min

Lab File: VX045768.D

Acq: 14 Apr 2025 15:12

Instrument :

MSVOA_X

ClientSampleId :

TP-6C





Tgt Ion: 43 Resp: 4252

Ion Ratio Lower Upper

43 100

61 0.0 9.9 14.9#

70 0.0 7.5 11.3#

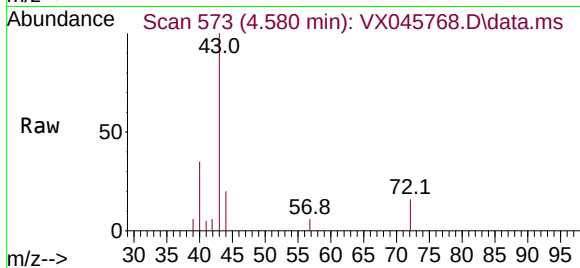

#38

Carbon Tetrachloride

Concen: 6.029 ug/l

RT: 5.544 min Scan# 731

Delta R.T. -0.128 min

Lab File: VX045768.D

Acq: 14 Apr 2025 15:12




Tgt Ion: 117 Resp: 8434


Ion Ratio Lower Upper

117 100

119 3.3 76.9 115.3#

121 0.0 24.2 36.2#


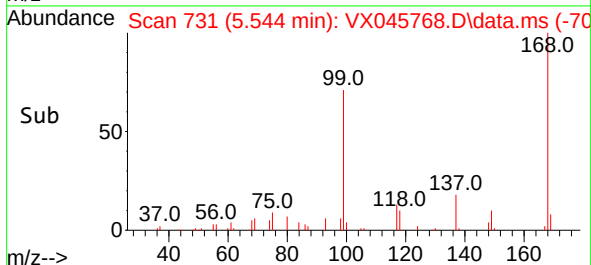
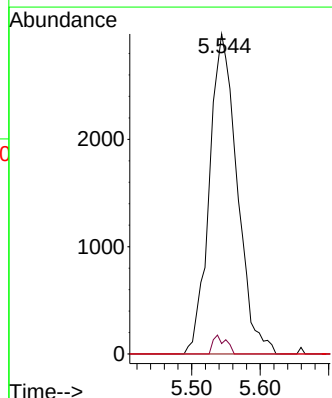
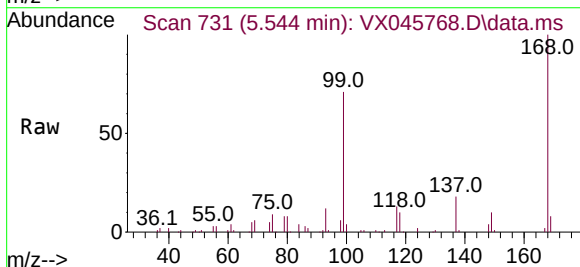




#41
Methacrylonitrile
Concen: 0.379 ug/l
RT: 5.044 min Scan# 649
Delta R.T. 0.122 min
Lab File: VX045768.D
Acq: 14 Apr 2025 15:12




Instrument :
MSVOA_X
ClientSampleId :
TP-6C


Tgt Ion:	41	Resp:	326
Ion	Ratio	Lower	Upper
41	100		
39	27.3	47.0	70.6#
67	0.0	53.2	79.8#
52	0.0	25.0	37.6#

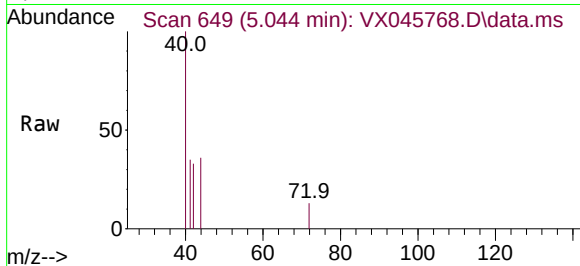

#43
Isopropyl Acetate
Concen: 3.148 ug/l
RT: 6.348 min Scan# 863
Delta R.T. 0.012 min
Lab File: VX045768.D
Acq: 14 Apr 2025 15:12

Tgt Ion:	43	Resp:	7783
Ion	Ratio	Lower	Upper
43	100		
61	16.3	14.1	21.1
87	11.4	9.2	13.8


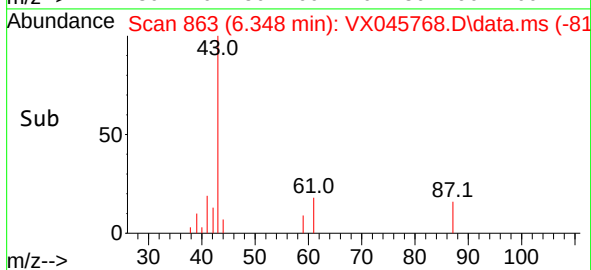

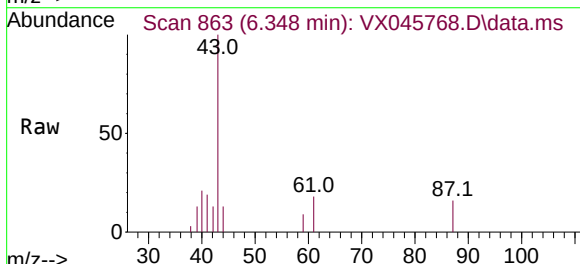


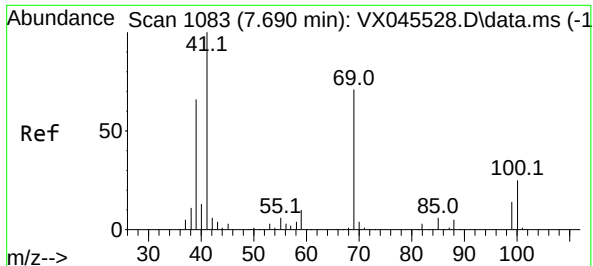

#48
Methyl methacrylate
Concen: 28.707 ug/l
RT: 7.799 min Scan# 1101
Delta R.T. 0.110 min
Lab File: VX045768.D
Acq: 14 Apr 2025 15:12




Instrument :
MSVOA_X
ClientSampleId :
TP-6C


Tgt Ion: 41 Resp: 36646
Ion Ratio Lower Upper
41 100
69 0.0 58.2 87.2#
39 58.7 53.6 80.4

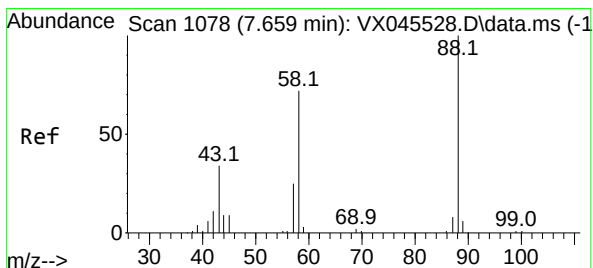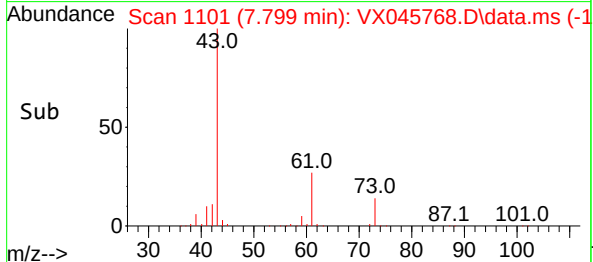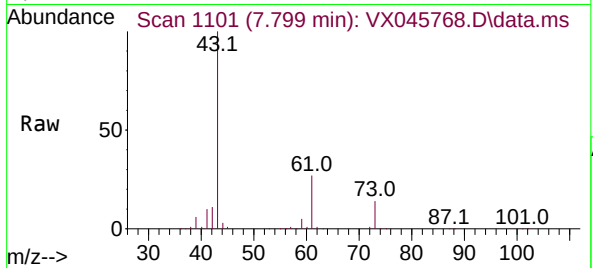

#49
1,4-Dioxane
Concen: 2.468 ug/l
RT: 7.793 min Scan# 1100
Delta R.T. 0.134 min
Lab File: VX045768.D
Acq: 14 Apr 2025 15:12

Tgt Ion: 88 Resp: 57
Ion Ratio Lower Upper
88 100
43 625824.6 32.2 48.4#
58 2852.6 58.6 88.0#


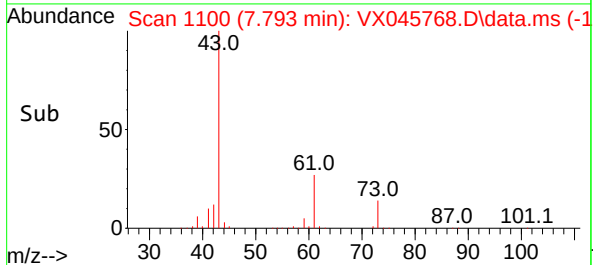

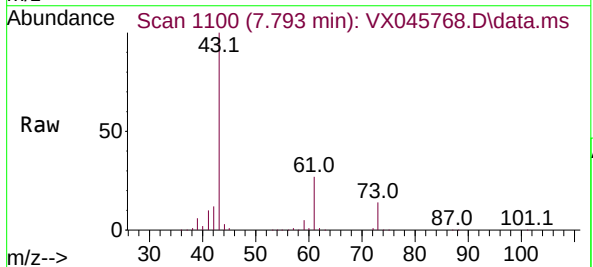


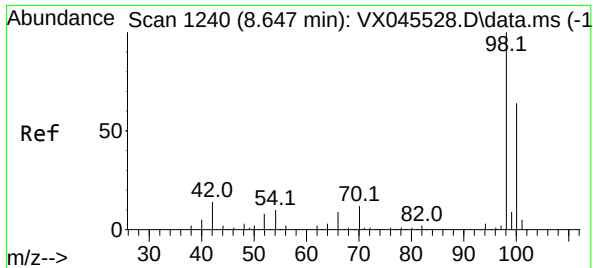

#50
Toluene-d8
Concen: 51.618 ug/l
RT: 8.647 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX045768.D
Acq: 14 Apr 2025 15:12




Instrument :
MSVOA_X
ClientSampleId :
TP-6C


Tgt Ion: 98 Resp: 172726
Ion Ratio Lower Upper
98 100
100 65.6 52.2 78.4

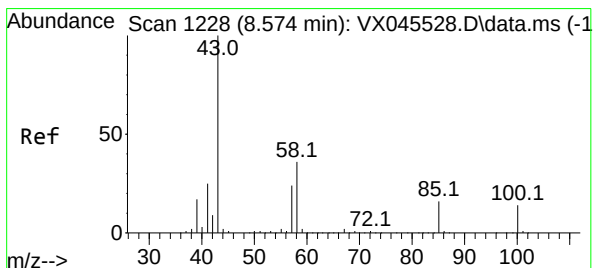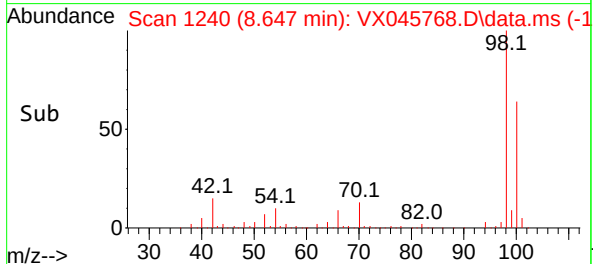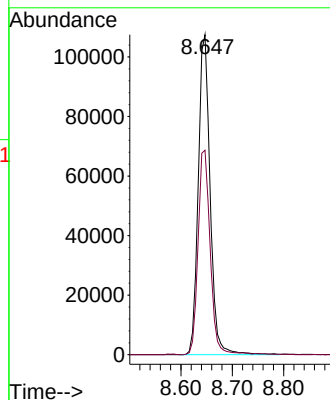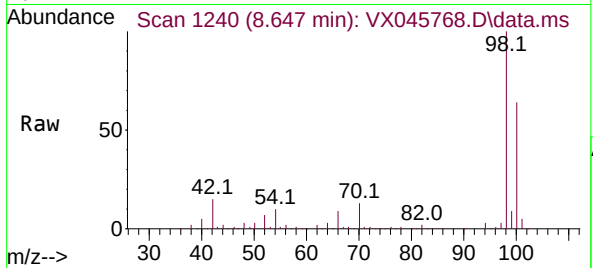

#51
4-Methyl-2-Pentanone
Concen: 19.363 ug/l
RT: 8.549 min Scan# 1224
Delta R.T. -0.024 min
Lab File: VX045768.D
Acq: 14 Apr 2025 15:12

Tgt Ion: 43 Resp: 31735
Ion Ratio Lower Upper
43 100
58 5.7 28.5 42.7#

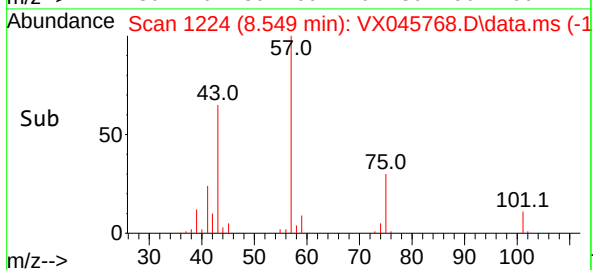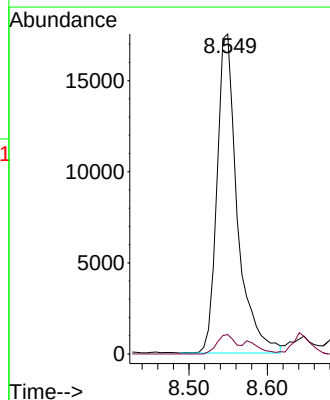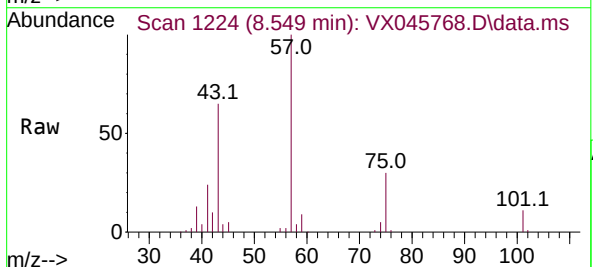

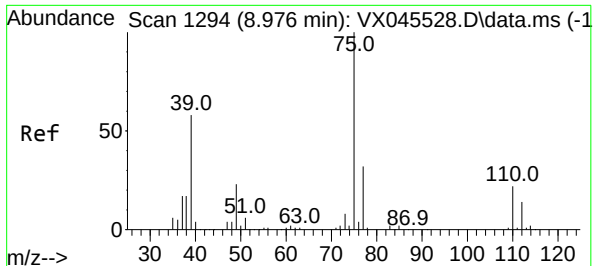

#53

t-1,3-Dichloropropene

Concen: 2.375 ug/l

RT: 8.958 min Scan# 11

Delta R.T. -0.018 min

Lab File: VX045768.D

Acq: 14 Apr 2025 15:12

Instrument :

MSVOA_X

ClientSampleId :





TP-6C

Tgt Ion: 75 Resp: 131

Ion Ratio Lower Upper

75 100

77 0.0 25.4 38.0#

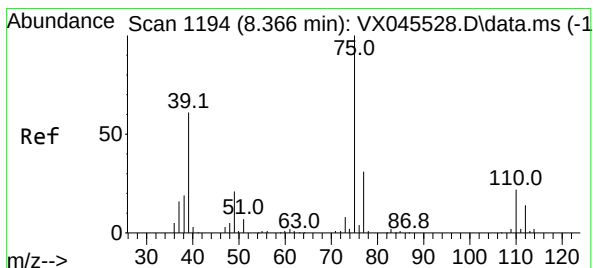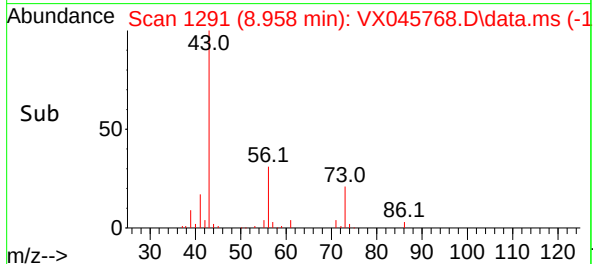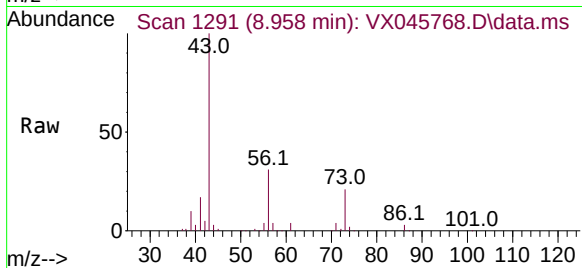

#54

cis-1,3-Dichloropropene

Concen: 8.932 ug/l

RT: 8.549 min Scan# 1224

Delta R.T. 0.183 min

Lab File: VX045768.D

Acq: 14 Apr 2025 15:12




Tgt Ion: 75 Resp: 12693


Ion Ratio Lower Upper

75 100

77 0.0 24.6 36.8#

39 41.0 48.4 72.6#

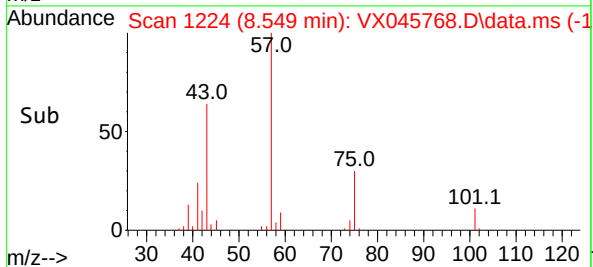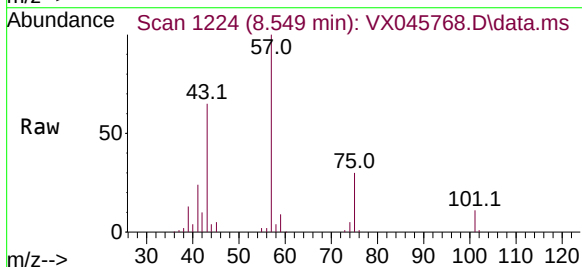



#57

1,3-Dichloropropane

Concen: 0.686 ug/l

RT: 9.482 min Scan# 11

Delta R.T. 0.177 min

Lab File: VX045768.D

Acq: 14 Apr 2025 15:12

Instrument :

MSVOA_X

ClientSampleId :





TP-6C

Tgt Ion: 76 Resp: 1138

Ion Ratio Lower Upper

76 100

78 0.0 26.0 39.0#

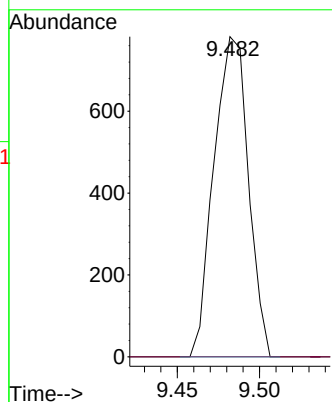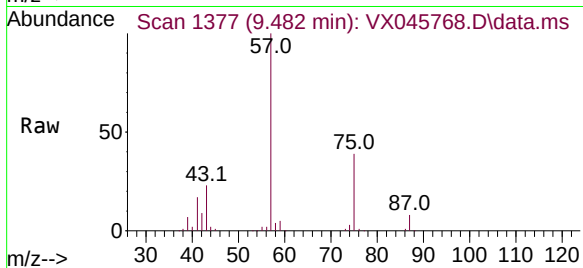

#59

2-Hexanone

Concen: 7.356 ug/l

RT: 9.372 min Scan# 1359

Delta R.T. -0.055 min

Lab File: VX045768.D




Acq: 14 Apr 2025 15:12


Tgt Ion: 43 Resp: 8928

Ion Ratio Lower Upper

43 100

58 0.0 24.9 74.6#


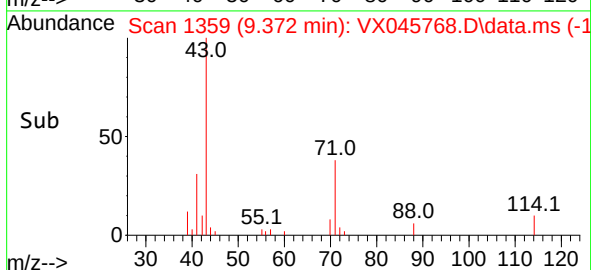

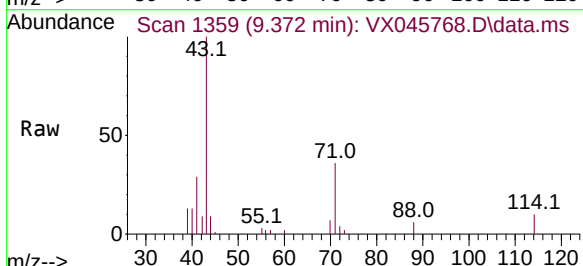




#62
4-Bromofluorobenzene
Concen: 55.586 ug/l
RT: 11.079 min Scan# 1
Delta R.T. 0.000 min
Lab File: VX045768.D
Acq: 14 Apr 2025 15:12




Instrument :
MSVOA_X
ClientSampleId :
TP-6C


Tgt Ion: 95 Resp: 67752
Ion Ratio Lower Upper
95 100
174 67.5 0.0 135.8
176 64.9 0.0 131.4

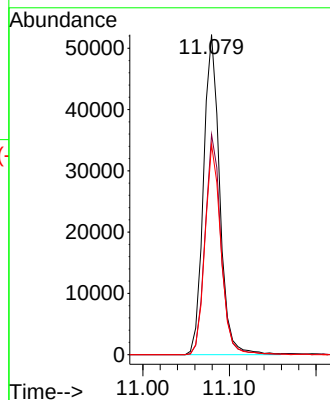

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.049 min Scan# 1470
Delta R.T. 0.000 min
Lab File: VX045768.D
Acq: 14 Apr 2025 15:12

Tgt Ion: 117 Resp: 132172
Ion Ratio Lower Upper
117 100
82 63.6 49.2 73.8
119 32.1 25.1 37.7

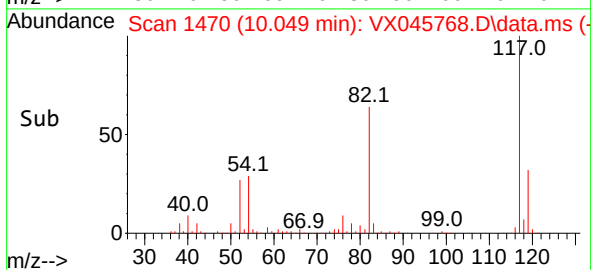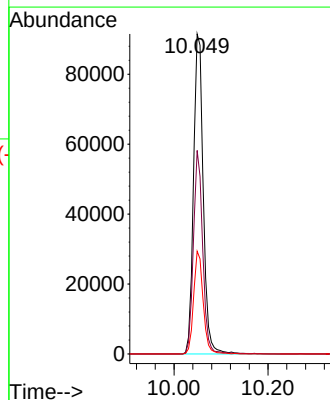



#67

Ethyl Benzene

Concen: 0.232 ug/l

RT: 10.195 min Scan# 1493

Delta R.T. 0.006 min

Lab File: VX045768.D

Acq: 14 Apr 2025 15:12

Instrument :

MSVOA_X

ClientSampleId :





TP-6C

Tgt Ion: 91 Resp: 1172

Ion Ratio Lower Upper

91 100

106 29.3 23.7 35.5



#69

o-Xylene

Concen: 0.245 ug/l

RT: 10.646 min Scan# 1568

Delta R.T. 0.006 min

Lab File: VX045768.D




Acq: 14 Apr 2025 15:12


Tgt Ion:106 Resp: 444

Ion Ratio Lower Upper

106 100

91 229.1 113.6 340.6


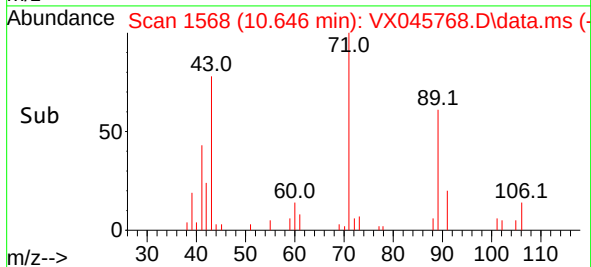

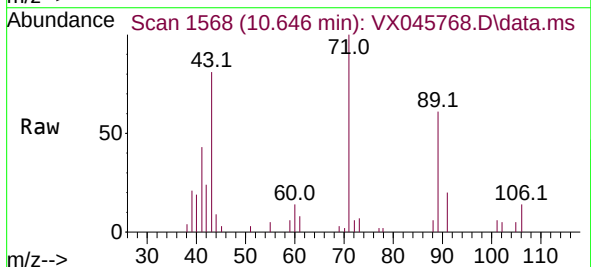




#72
 1,4-Dichlorobenzene-d4
 Concen: 50.000 ug/l
 RT: 12.018 min Scan# 1
 Delta R.T. 0.000 min
 Lab File: VX045768.D
 Acq: 14 Apr 2025 15:12




Instrument :
 MSVOA_X
 ClientSampleId :
 TP-6C


Tgt Ion:152 Resp: 56416
 Ion Ratio Lower Upper
 152 100
 115 67.0 46.9 140.7
 150 159.7 0.0 349.4

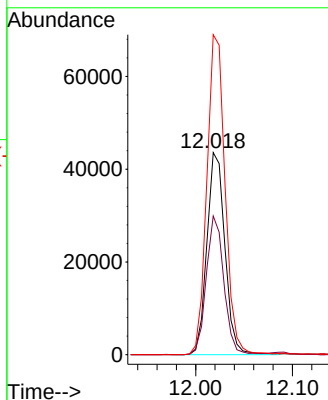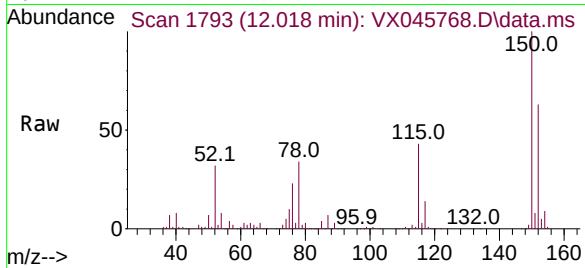

#73
 Isopropylbenzene
 Concen: 0.205 ug/l
 RT: 10.963 min Scan# 1620
 Delta R.T. 0.006 min
 Lab File: VX045768.D
 Acq: 14 Apr 2025 15:12

Tgt Ion:105 Resp: 925
 Ion Ratio Lower Upper
 105 100
 120 15.9 12.7 38.0


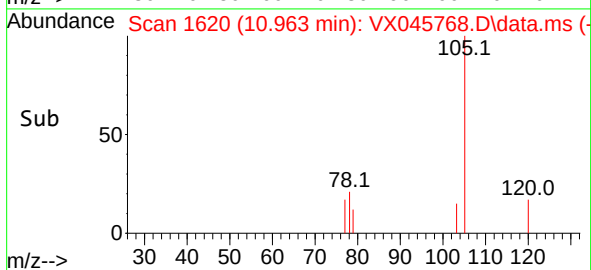
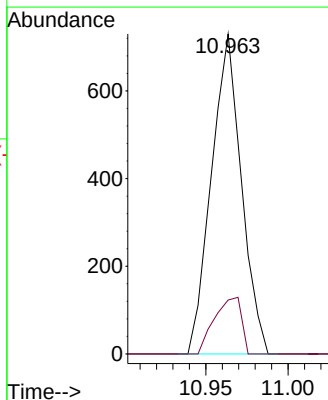
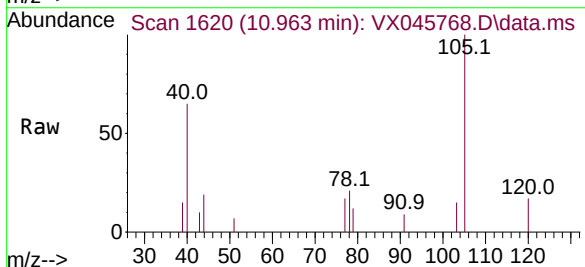




#76
1,2,3-Trichloropropane
Concen: 27.984 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.158 min
Lab File: VX045768.D
Acq: 14 Apr 2025 15:12




Instrument :
MSVOA_X
ClientSampleId :
TP-6C


Tgt Ion: 75 Resp: 38509
Ion Ratio Lower Upper
75 100
77 1.0 20.0 59.9#

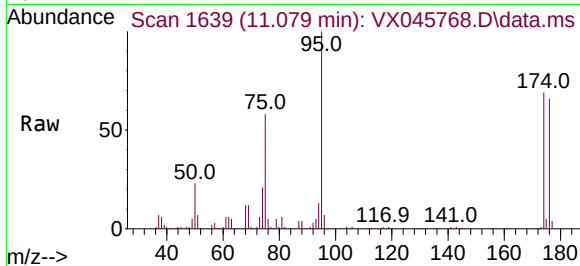

#78
n-propylbenzene
Concen: 0.212 ug/l
RT: 11.311 min Scan# 1677
Delta R.T. 0.012 min
Lab File: VX045768.D
Acq: 14 Apr 2025 15:12

Tgt Ion: 91 Resp: 1104
Ion Ratio Lower Upper
91 100
120 27.9 10.8 32.3




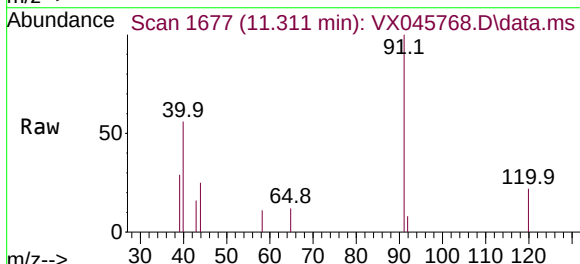




#80
1,3,5-Trimethylbenzene
Concen: 0.346 ug/l
RT: 11.451 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX045768.D
Acq: 14 Apr 2025 15:12




Instrument :
MSVOA_X
ClientSampleId :
TP-6C


Tgt Ion:105 Resp: 1294
Ion Ratio Lower Upper
105 100
120 34.1 23.0 69.0

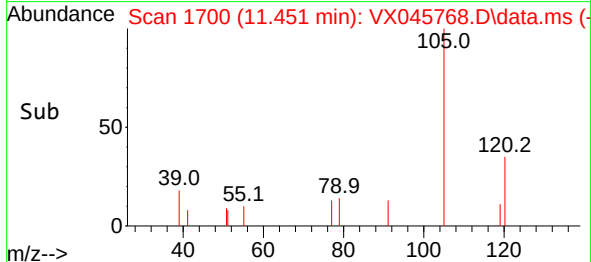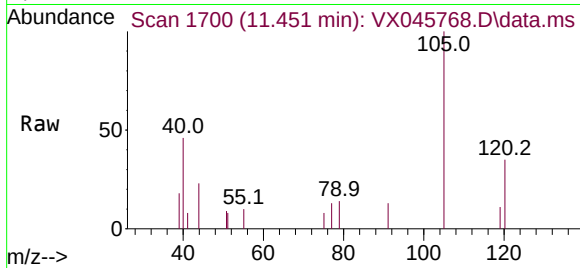

#81
trans-1,4-Dichloro-2-butene
Concen: 94.973 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.061 min
Lab File: VX045768.D
Acq: 14 Apr 2025 15:12

Tgt Ion: 75 Resp: 38509
Ion Ratio Lower Upper
75 100
53 0.0 101.8 152.6#
89 0.0 37.2 55.8#

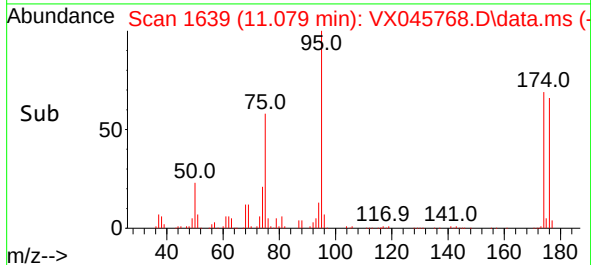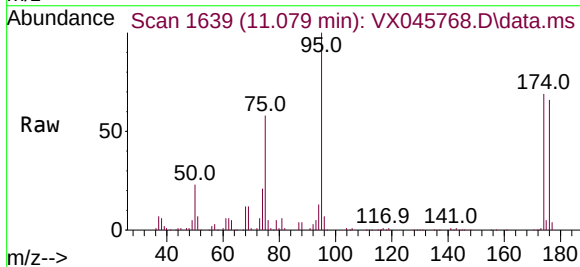



#84

1,2,4-Trimethylbenzene

Concen: 0.728 ug/l

RT: 11.750 min Scan# 11

Delta R.T. 0.000 min

Lab File: VX045768.D

Acq: 14 Apr 2025 15:12

Instrument :

MSVOA_X

ClientSampleId :





TP-6C

Tgt Ion:105 Resp: 2732

Ion Ratio Lower Upper

105 100

120 39.9 21.4 64.3

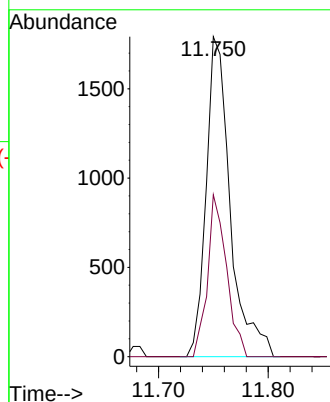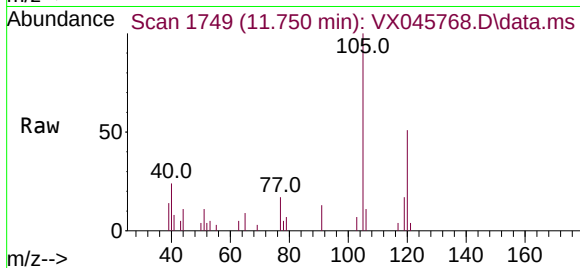

#85

sec-Butylbenzene

Concen: 0.358 ug/l

RT: 11.884 min Scan# 1771

Delta R.T. -0.006 min

Lab File: VX045768.D




Acq: 14 Apr 2025 15:12


Tgt Ion:105 Resp: 1629

Ion Ratio Lower Upper

105 100

134 20.5 9.6 28.6


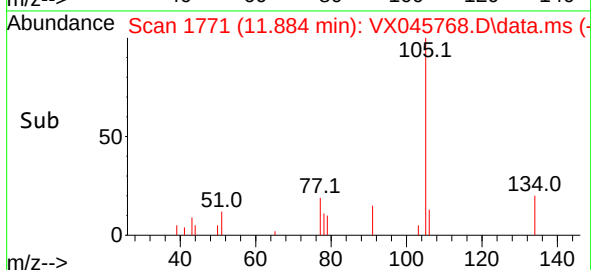
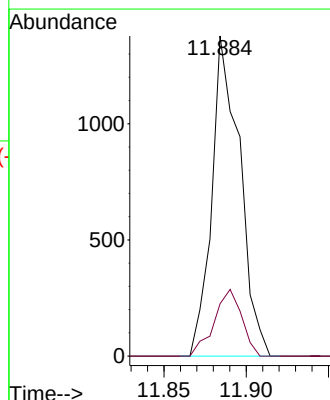
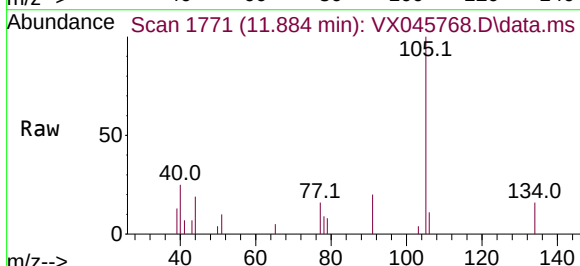




#86
p-Isopropyltoluene
Concen: 0.259 ug/l
RT: 11.969 min Scan# 119
Delta R.T. -0.037 min
Lab File: VX045768.D
Acq: 14 Apr 2025 15:12




Instrument :
MSVOA_X
ClientSampleId :
TP-6C


Tgt Ion:	119	Resp:	971
Ion	Ratio	Lower	Upper
119	100		
134	21.5	12.6	37.8
91	23.5	13.7	41.1

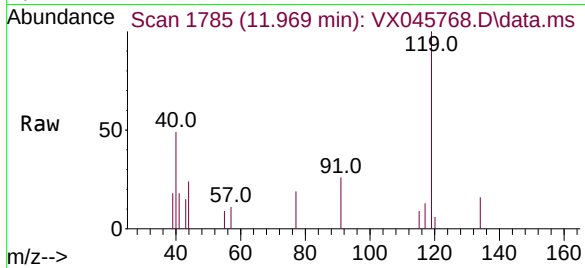

#89
n-Butylbenzene
Concen: 0.313 ug/l
RT: 12.329 min Scan# 1844
Delta R.T. 0.000 min
Lab File: VX045768.D
Acq: 14 Apr 2025 15:12

Tgt Ion:	91	Resp:	1016
Ion	Ratio	Lower	Upper
91	100		
92	34.2	26.9	80.6
134	79.1	11.9	35.7


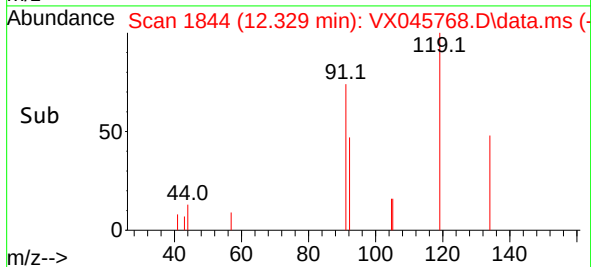

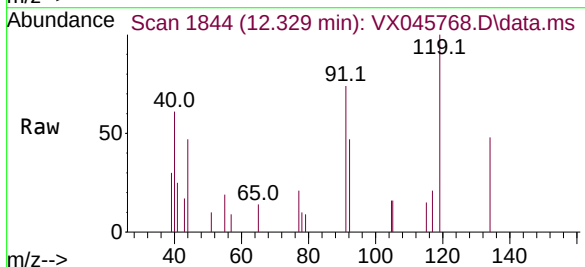




#90
Hexachloroethane
Concen: 0.733 ug/l
RT: 12.616 min Scan# 1878
Delta R.T. 0.079 min
Lab File: VX045768.D
Acq: 14 Apr 2025 15:12

Instrument :
MSVOA_X
ClientSampleId :
TP-6C

Tgt Ion:117 Resp: 472
Ion Ratio Lower Upper
117 100
201 0.0 31.2 93.6#

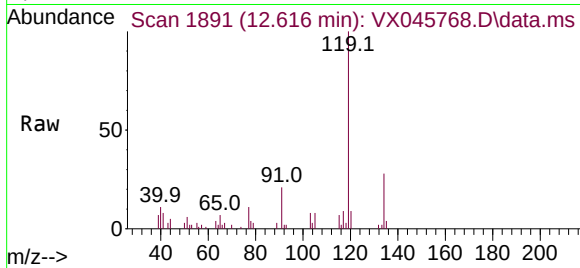

#95
Naphthalene
Concen: 3.689 ug/l
RT: 13.774 min Scan# 2081
Delta R.T. 0.000 min
Lab File: VX045768.D
Acq: 14 Apr 2025 15:12

Tgt Ion:128 Resp: 14440
Ion Ratio Lower Upper
128 100
127 13.3 10.3 15.5
129 13.3 8.6 12.8#

