




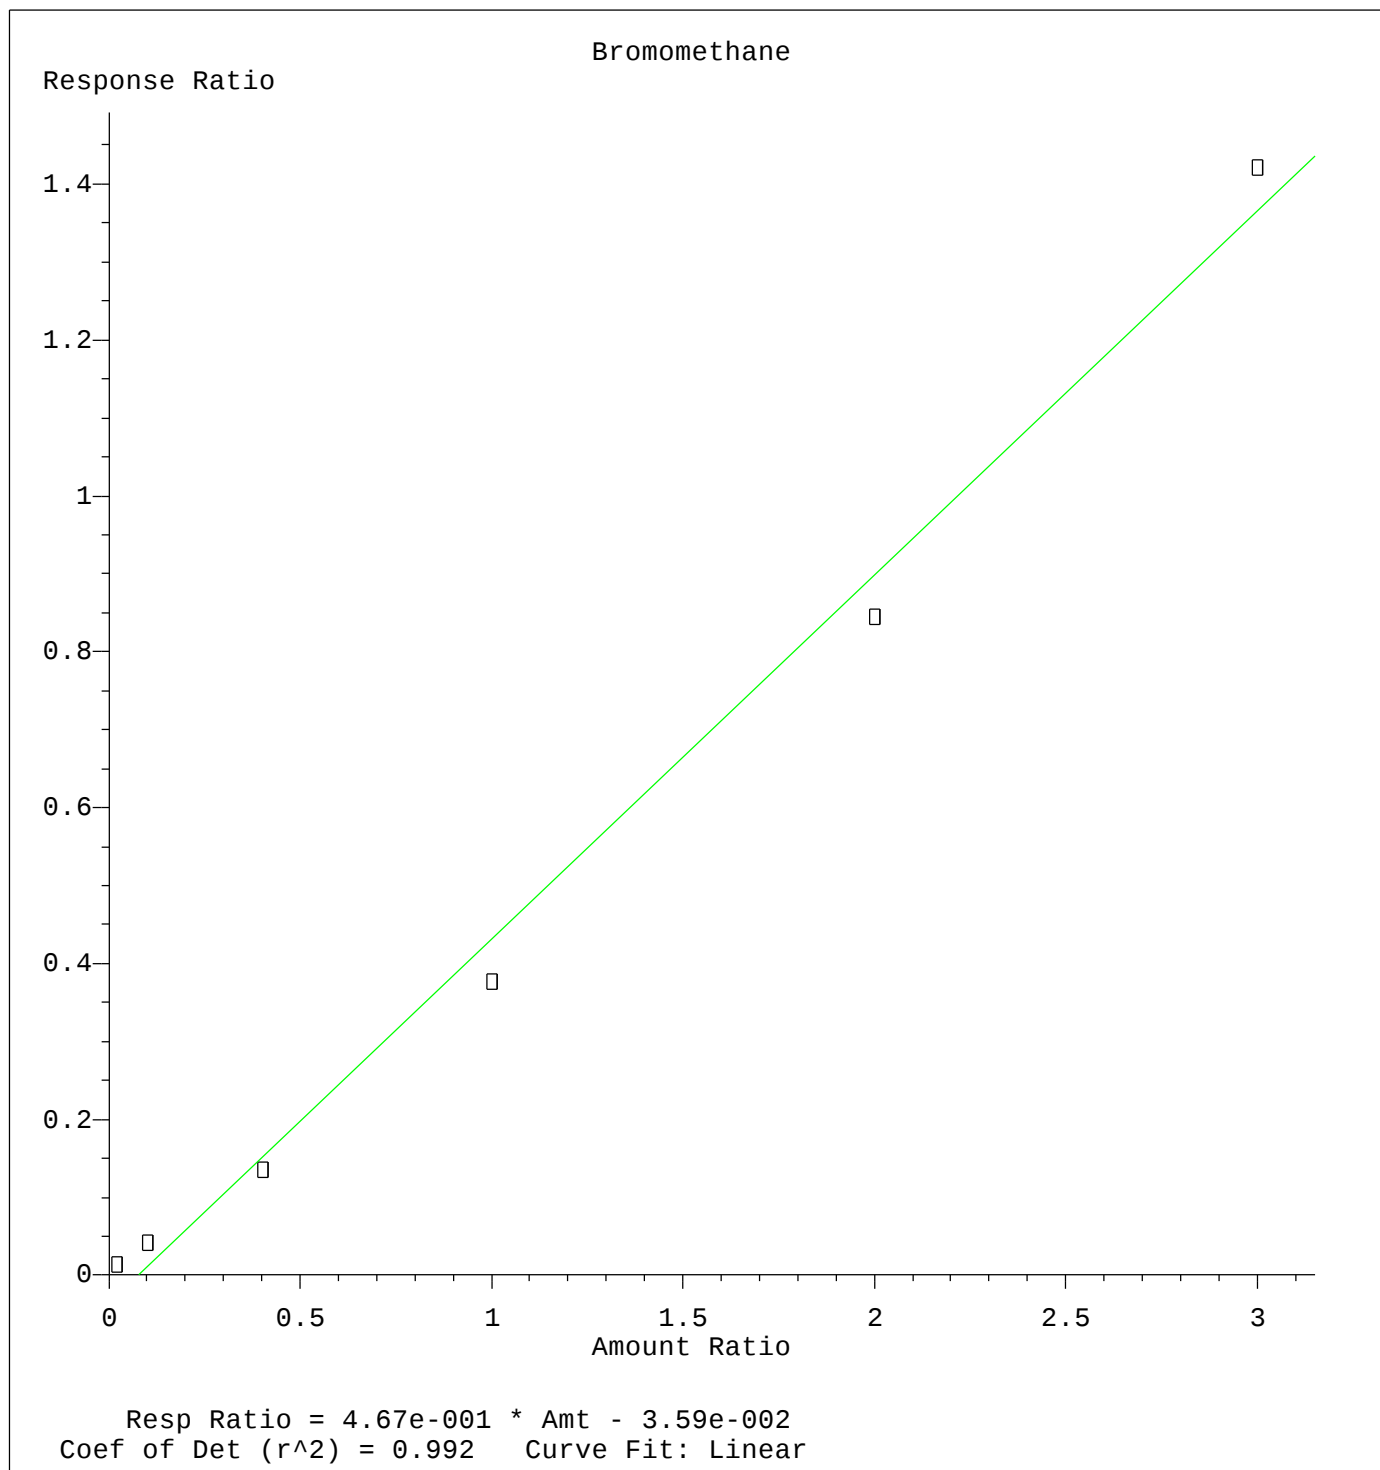

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X041519W.M
Calibration Table Last Updated: Tue Apr 16 09:35:21 2019

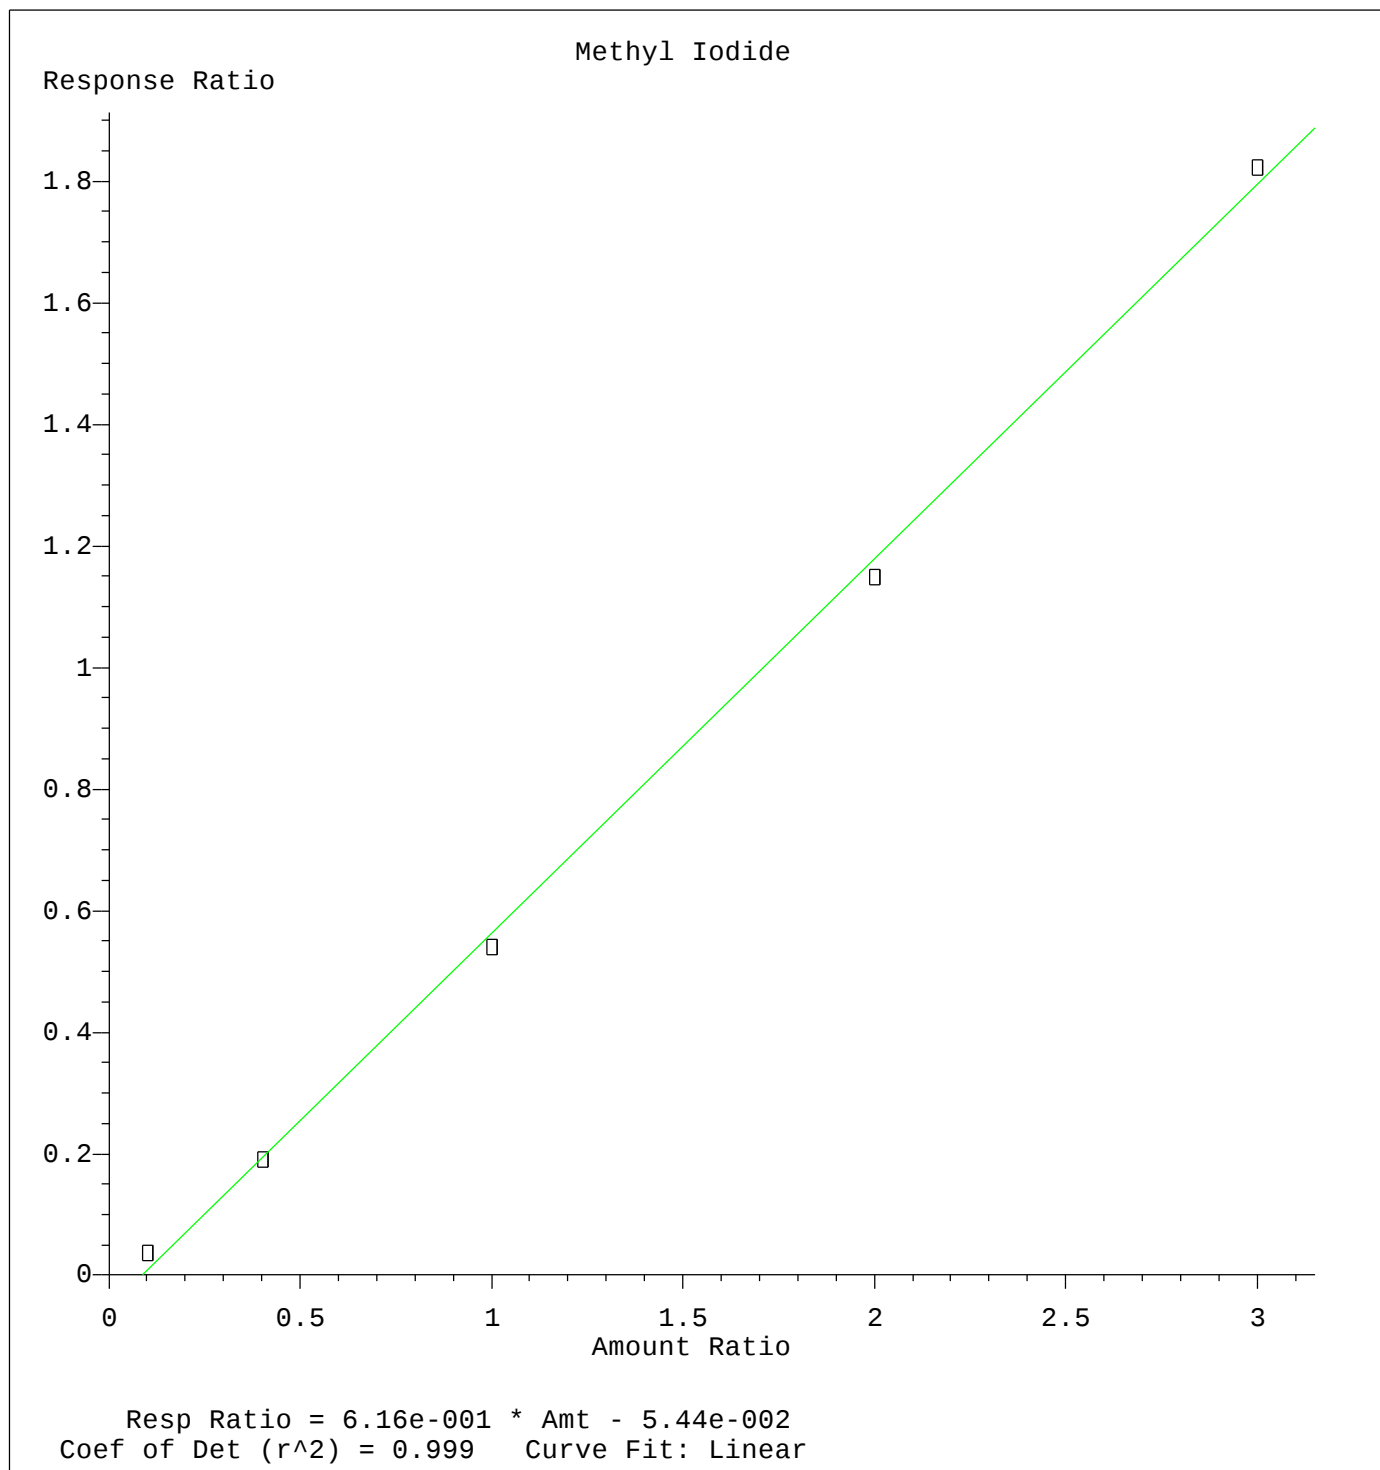


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X041519W.M
Calibration Table Last Updated: Tue Apr 16 09:35:21 2019

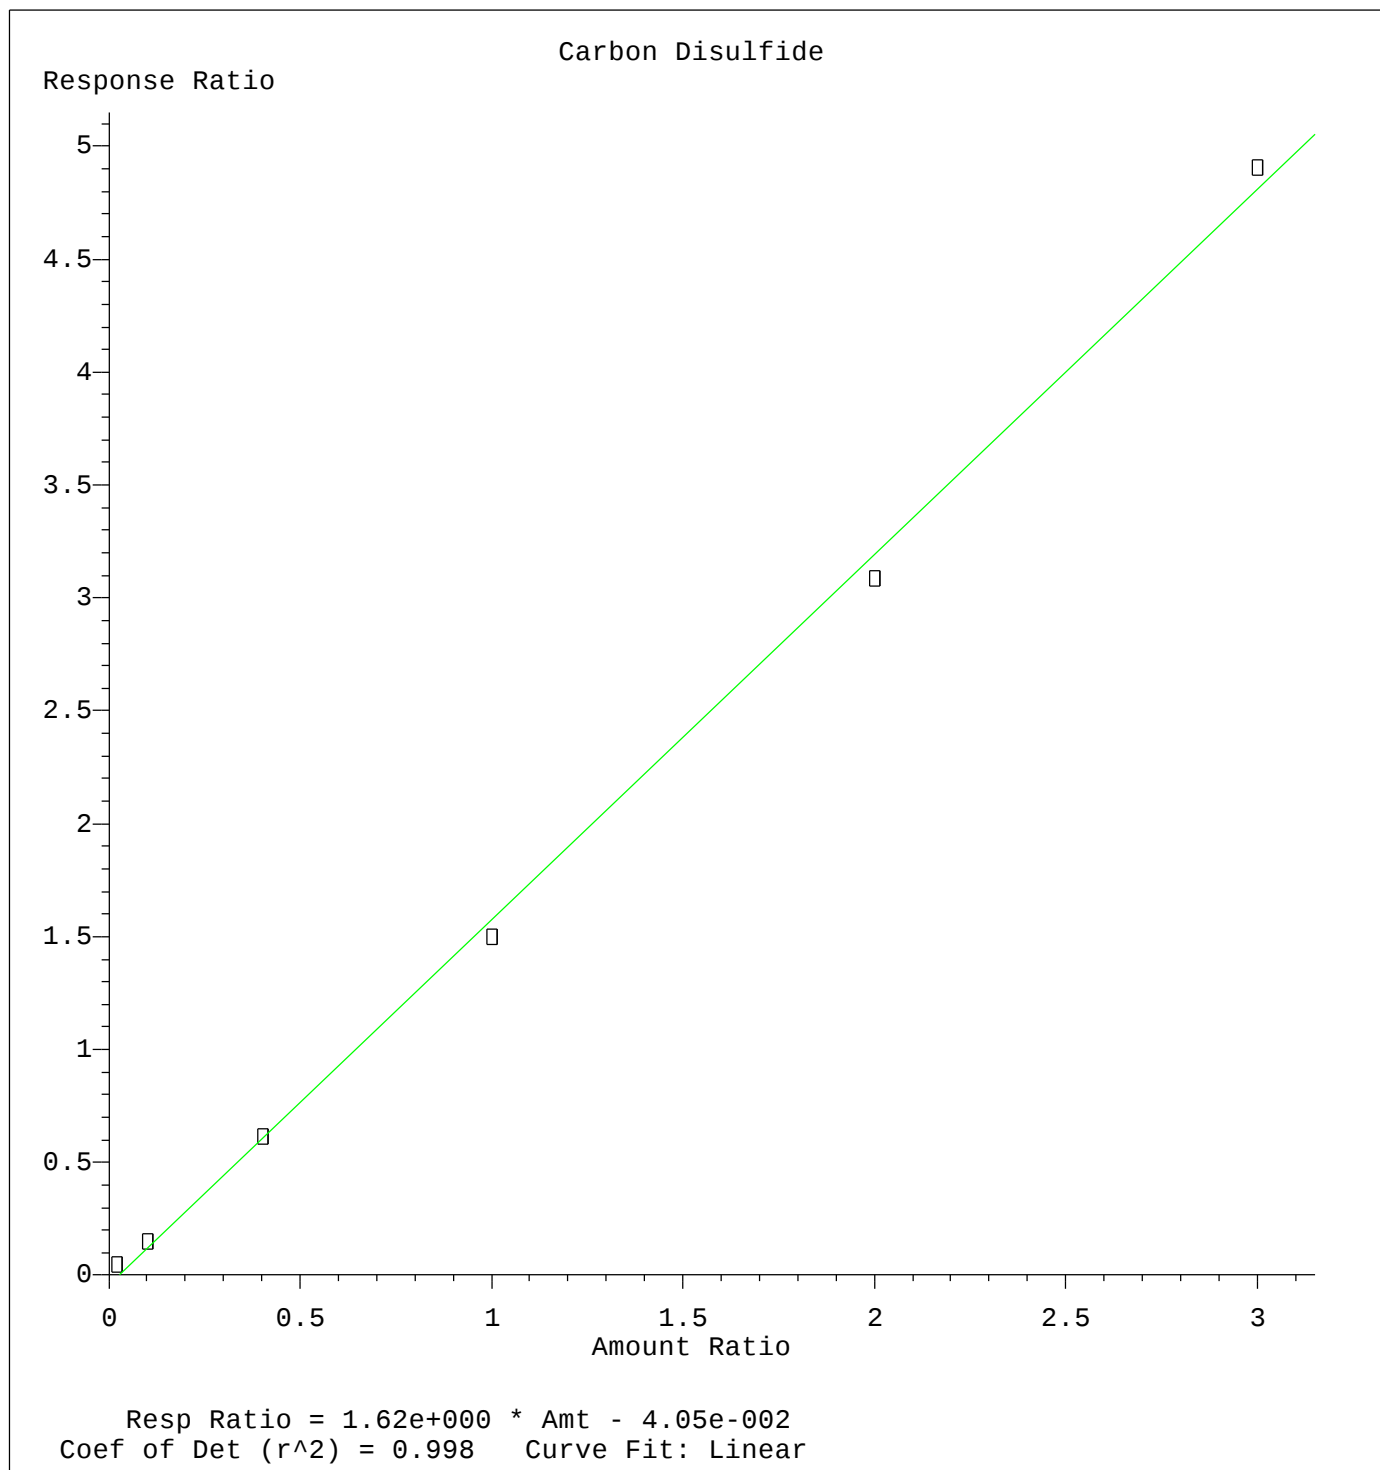

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X041519W.M
Calibration Table Last Updated: Tue Apr 16 09:35:21 2019

Bromochloromethane

Response Ratio

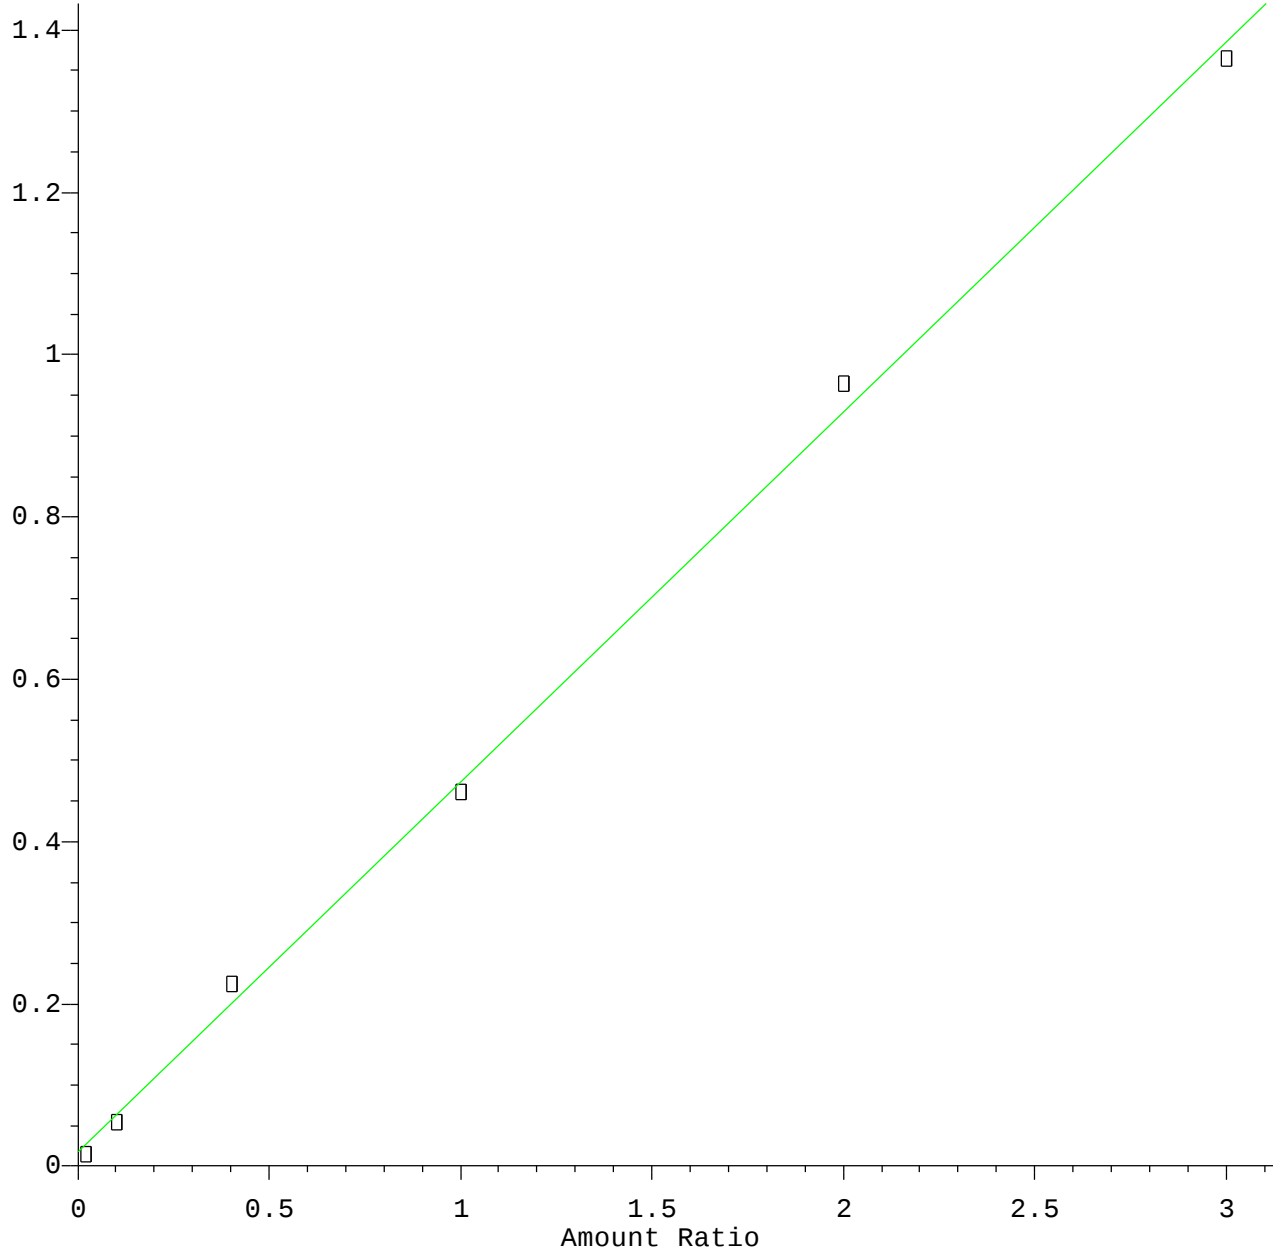

Resp Ratio = $4.56 \times 10^{-1} \times \text{Amt} + 1.83 \times 10^{-2}$
Coef of Det (r^2) = 0.998 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X041519W.M
Calibration Table Last Updated: Tue Apr 16 09:35:21 2019