

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041522\
 Data File : VX028137.D
 Acq On : 15 Apr 2022 16:46
 Operator : JC/MD
 Sample : N2392-02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VNJ-212

Quant Time: Apr 16 02:26:43 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X041222W.M
 Quant Title : SW846 8260
 QLast Update : Tue Apr 12 22:07:23 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.556	168	217899	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	379601	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	359411	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	165617	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	141448	47.848	ug/l	0.00
Spiked Amount	50.000	Range	61 - 141	Recovery	=	95.700%
35) Dibromofluoromethane	5.391	113	123374	49.599	ug/l	0.00
Spiked Amount	50.000	Range	69 - 133	Recovery	=	99.200%
50) Toluene-d8	8.653	98	465027	50.127	ug/l	0.00
Spiked Amount	50.000	Range	65 - 126	Recovery	=	100.260%
62) 4-Bromofluorobenzene	11.079	95	152152	43.926	ug/l	0.00
Spiked Amount	50.000	Range	58 - 135	Recovery	=	87.860%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041522\
Data File : VX028137.D
Acq On : 15 Apr 2022 16:46
Operator : JC/MD
Sample : N2392-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VNJ-212

Quant Time: Apr 16 02:26:43 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X041222W.M
Quant Title : SW846 8260
QLast Update : Tue Apr 12 22:07:23 2022
Response via : Initial Calibration




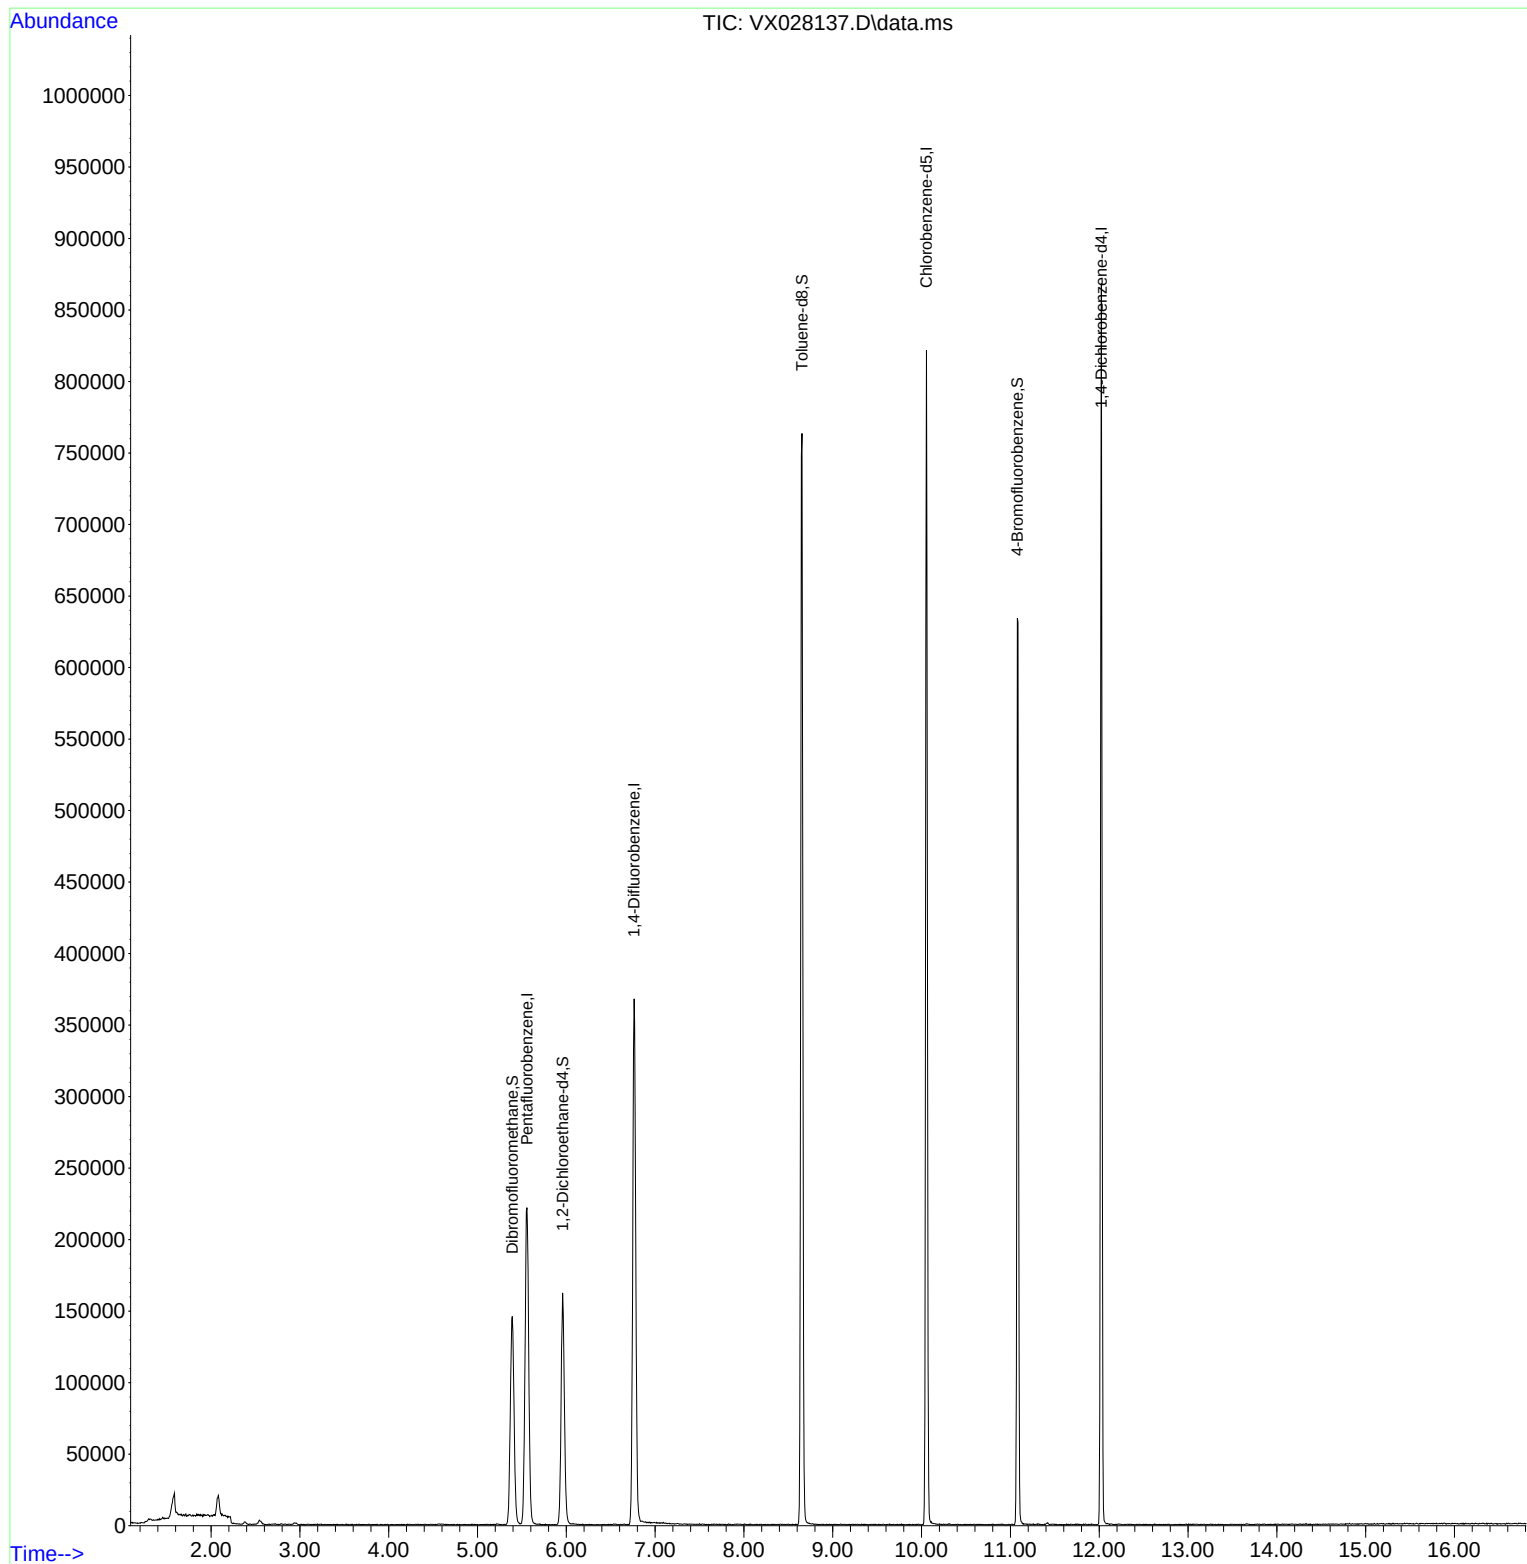


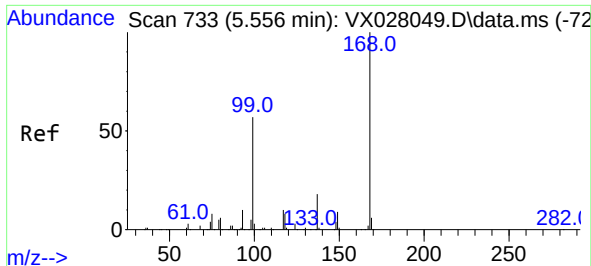

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.556 min Scan# 733
Delta R.T. -0.000 min
Lab File: VX028137.D
Acq: 15 Apr 2022 16:46




Instrument :
MSVOA_X
ClientSampleId :
VNJ-212


Tgt Ion:168 Resp: 217899
Ion Ratio Lower Upper
168 100
99 51.6 41.7 62.5

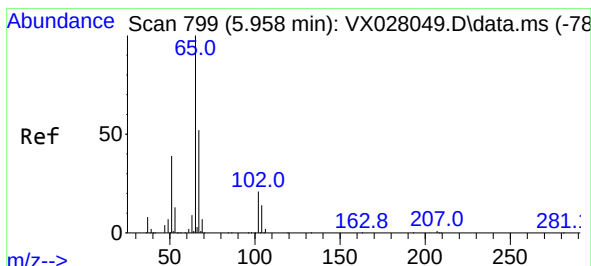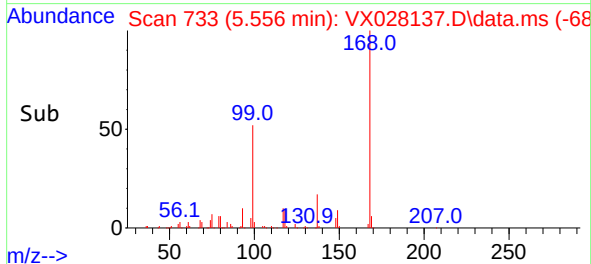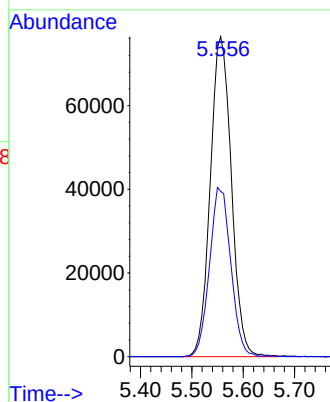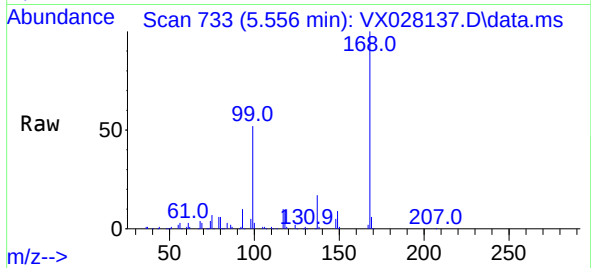

#33
1,2-Dichloroethane-d4
Concen: 47.848 ug/l
RT: 5.958 min Scan# 799
Delta R.T. 0.000 min
Lab File: VX028137.D
Acq: 15 Apr 2022 16:46

Tgt Ion: 65 Resp: 141448
Ion Ratio Lower Upper
65 100
67 51.3 0.0 107.4


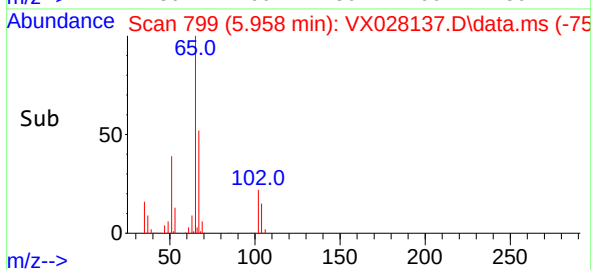
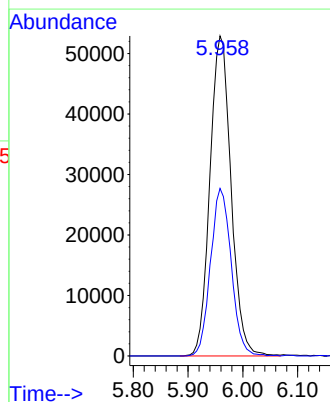
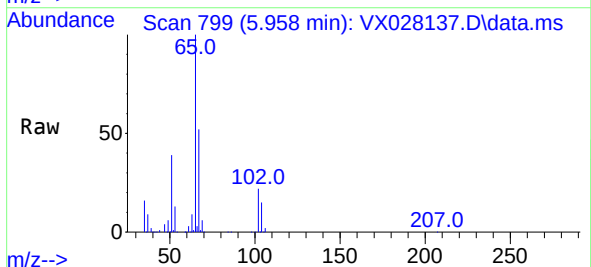


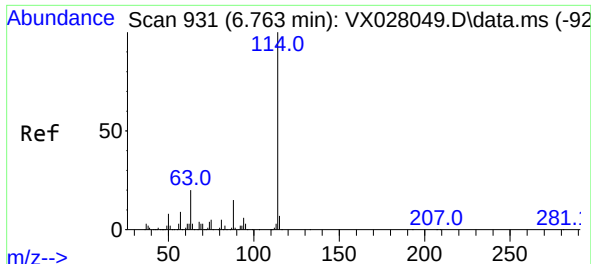

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.763 min Scan# 91
Delta R.T. 0.000 min
Lab File: VX028137.D
Acq: 15 Apr 2022 16:46




Instrument :
MSVOA_X
ClientSampleId :
VNJ-212


Tgt Ion:114 Resp: 379601
Ion Ratio Lower Upper
114 100
63 18.0 0.0 36.8
88 14.0 0.0 32.4

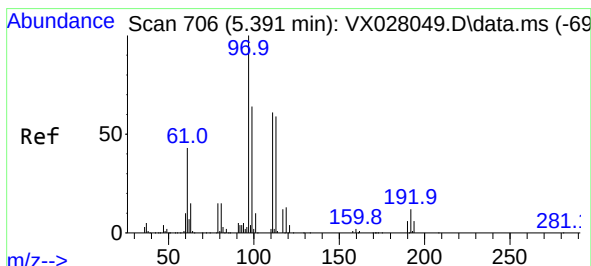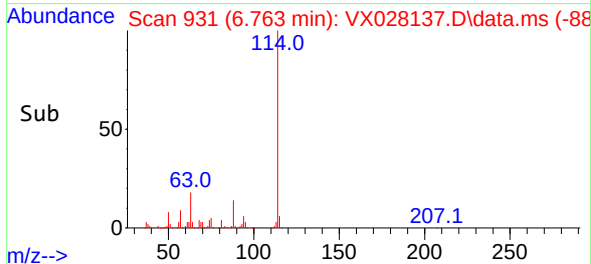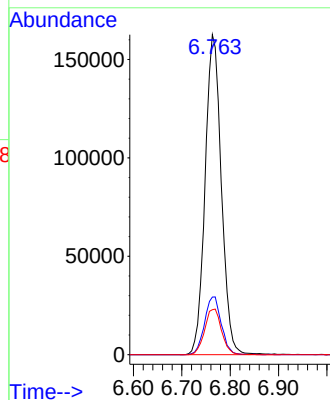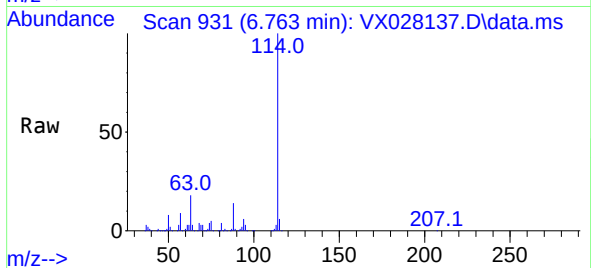

#35
Dibromofluoromethane
Concen: 49.599 ug/l
RT: 5.391 min Scan# 706
Delta R.T. 0.000 min
Lab File: VX028137.D
Acq: 15 Apr 2022 16:46

Tgt Ion:113 Resp: 123374
Ion Ratio Lower Upper
113 100
111 102.4 82.8 124.2
192 19.3 16.9 25.3


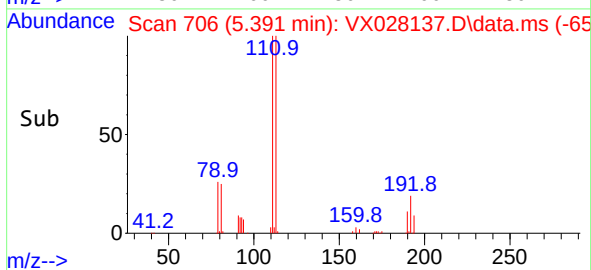
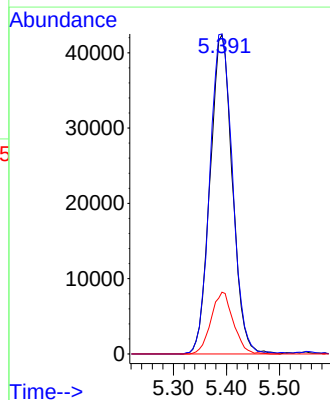
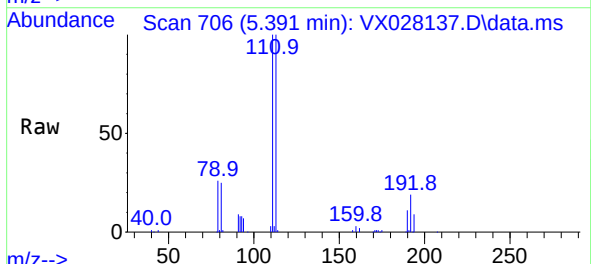


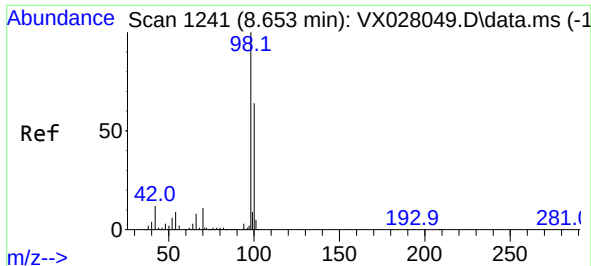

#50
Toluene-d8
Concen: 50.127 ug/l
RT: 8.653 min Scan# 11
Delta R.T. -0.000 min
Lab File: VX028137.D
Acq: 15 Apr 2022 16:46




Instrument :
MSVOA_X
ClientSampleId :
VNJ-212


Tgt Ion: 98 Resp: 465027
Ion Ratio Lower Upper
98 100
100 64.3 52.6 78.8

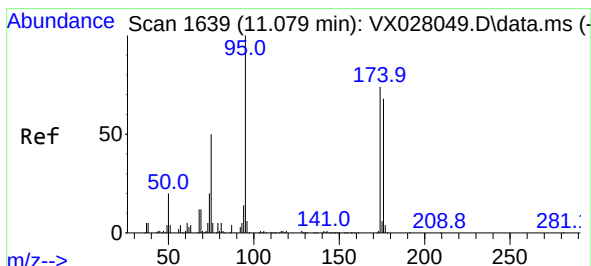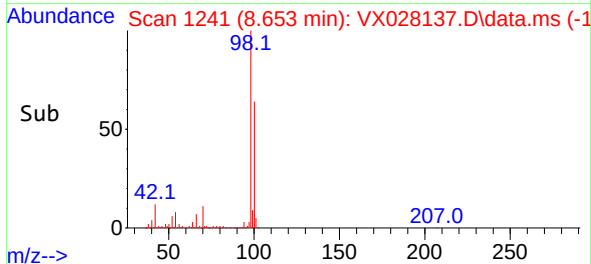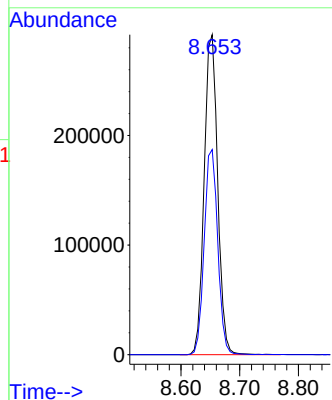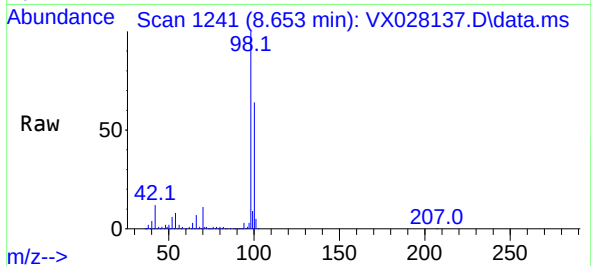

#62
4-Bromofluorobenzene
Concen: 43.926 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.000 min
Lab File: VX028137.D
Acq: 15 Apr 2022 16:46

Tgt Ion: 95 Resp: 152152
Ion Ratio Lower Upper
95 100
174 88.0 0.0 163.0
176 86.8 0.0 155.0


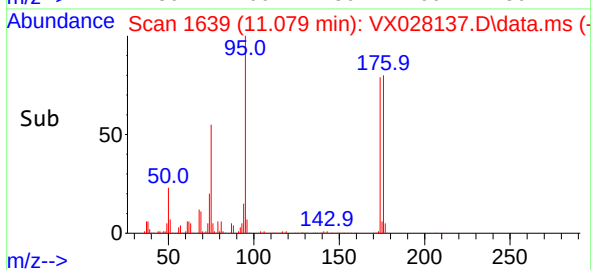
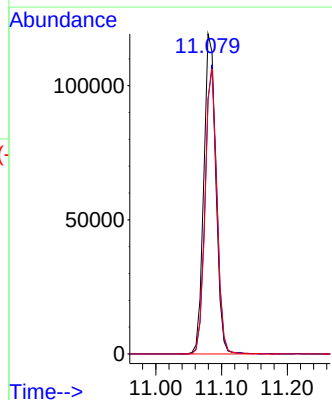
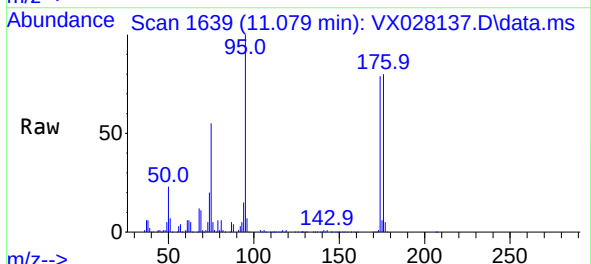


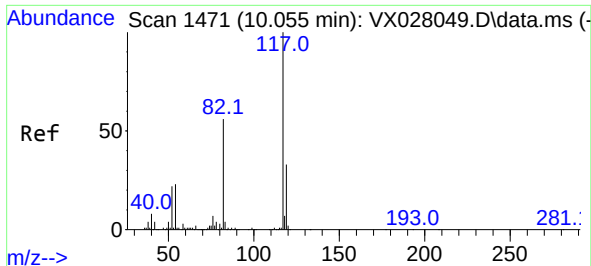

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX028137.D
Acq: 15 Apr 2022 16:46

Instrument :
MSVOA_X
ClientSampleId :
VNJ-212

Tgt Ion:117 Resp: 359411
Ion Ratio Lower Upper
117 100
82 53.5 41.8 62.8
119 31.4 24.8 37.2

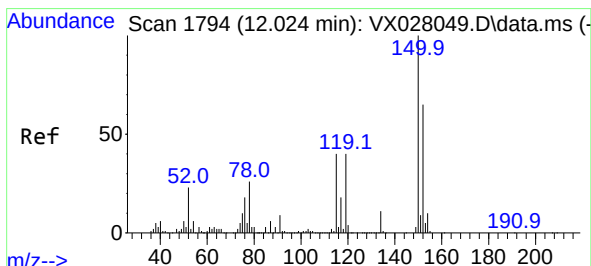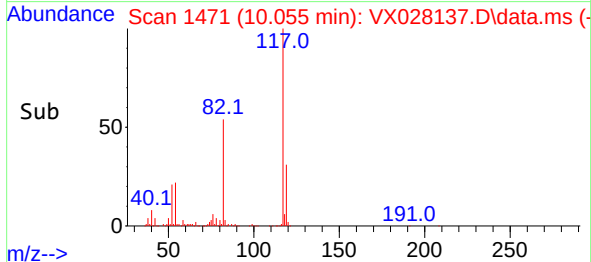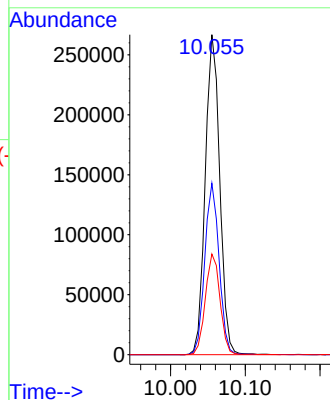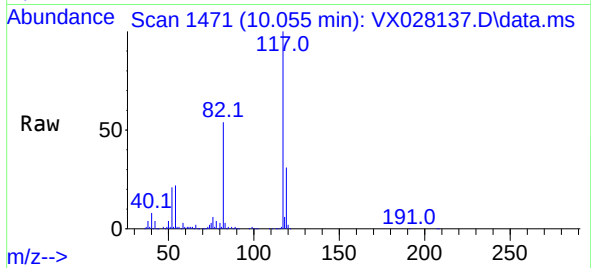

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. 0.000 min
Lab File: VX028137.D
Acq: 15 Apr 2022 16:46

Tgt Ion:152 Resp: 165617
Ion Ratio Lower Upper
152 100
115 58.5 37.5 112.7
150 158.2 0.0 338.2

