

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041522\
 Data File : VX028132.D
 Acq On : 15 Apr 2022 14:50
 Operator : JC/MD
 Sample : N2440-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BP-TB-20220411

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X041222W.M
 Title : SW846 8260

Signal : TIC: VX028132.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	6.763	917	931	952	rBV	411681	1241748	1.18%	0.385%
2	7.799	1094	1101	1111	rBV	1464846	2387241	2.27%	0.739%
3	8.653	1234	1241	1247	rBV	837755	1295857	1.23%	0.401%
4	9.482	1373	1377	1383	rVB	2283507	2778172	2.64%	0.861%
5	10.055	1467	1471	1475	rVB	866439	1106842	1.05%	0.343%
6	11.177	1646	1655	1662	rBV	1072307	1530023	1.45%	0.474%
7	11.890	1766	1772	1780	rVB	7680313	9729976	9.25%	3.014%
8	12.018	1788	1793	1800	rVB3	5218304	7422502	7.05%	2.299%
9	12.109	1800	1808	1813	rBV	29758802	37287042	35.43%	11.550%
10	13.005	1950	1955	1960	rBV	2004724	2445707	2.32%	0.758%
11	13.127	1967	1975	1979	rBV	10745769	14785555	14.05%	4.580%
12	13.182	1979	1984	1988	rVV	73756653	105243473	100.00%	32.600%
13	13.219	1988	1990	1995	rVB	5493222	5846866	5.56%	1.811%
14	13.341	2005	2010	2020	rVB	1001447	1683033	1.60%	0.521%
15	13.475	2027	2032	2035	rBV	1922124	2637198	2.51%	0.817%
16	13.518	2035	2039	2043	rVV	6313512	8428480	8.01%	2.611%
17	13.572	2043	2048	2058	rVV	24547002	34055077	32.36%	10.549%
18	13.670	2058	2064	2071	rVV	58783291	80009860	76.02%	24.784%
19	13.871	2092	2097	2102	rBV	1302271	1760630	1.67%	0.545%
20	14.469	2191	2195	2209	rVB	782729	1155112	1.10%	0.358%


Sum of corrected areas: 322830394

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041522\
Data File : VX028132.D
Acq On : 15 Apr 2022 14:50
Operator : JC/MD
Sample : N2440-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BP-TB-20220411

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X041222W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

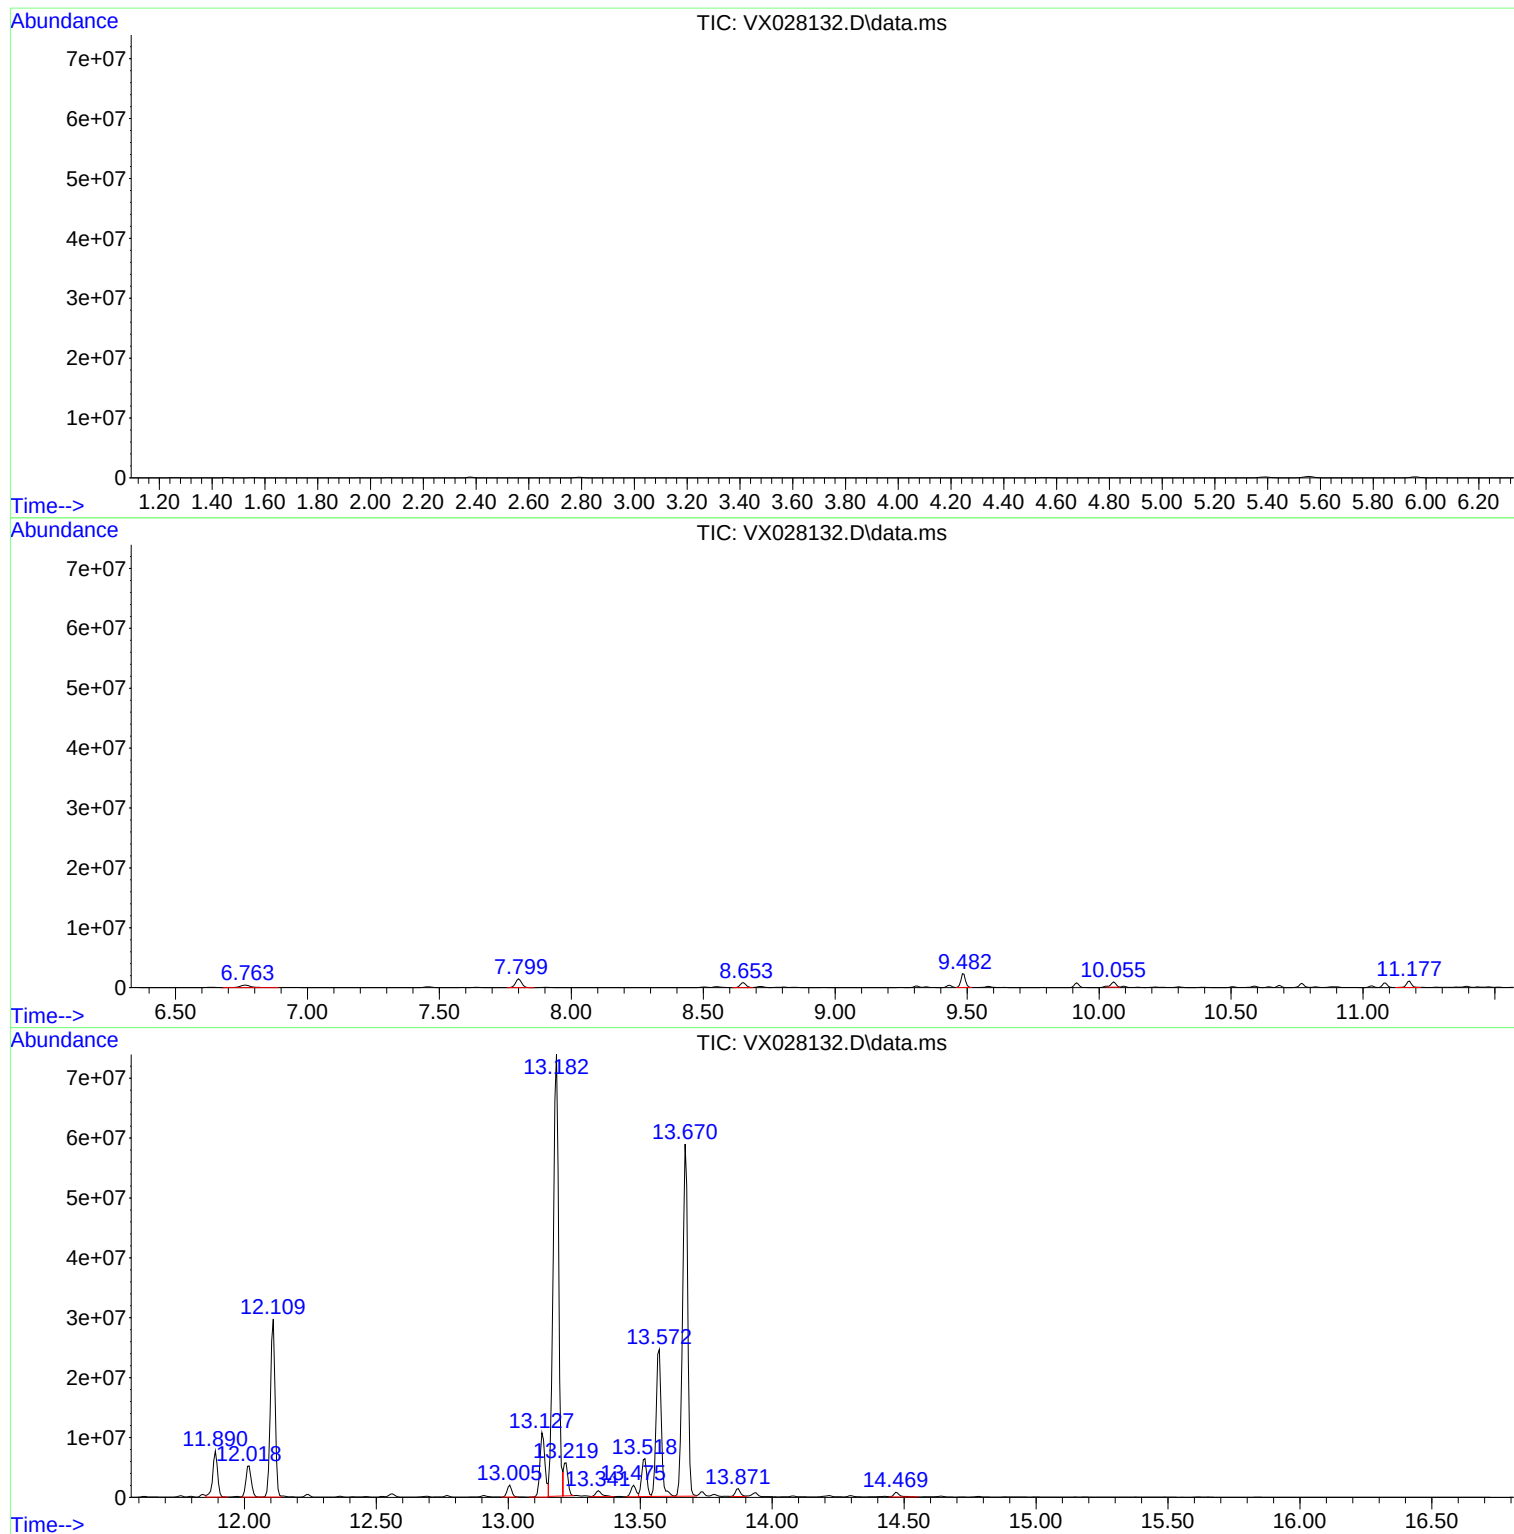

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041522\
Data File : VX028132.D
Acq On : 15 Apr 2022 14:50
Operator : JC/MD
Sample : N2440-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BP-TB-20220411

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X041222W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041522\
Data File : VX028132.D
Acq On : 15 Apr 2022 14:50
Operator : JC/MD
Sample : N2440-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BP-TB-20220411

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X041222W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------