

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041523\
 Data File : VX035091.D
 Acq On : 14 Apr 2023 18:17
 Operator : JC/MD
 Sample : 02353-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BUR-1253

Quant Time: Apr 17 08:58:09 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032923W.M
 Quant Title : SW846 8260
 QLast Update : Sat Apr 01 01:50:18 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.556	168	264013	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	439948	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	390272	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	180693	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	167206	41.411	ug/l	0.00
Spiked Amount 50.000	Range 78 - 117		Recovery =	82.820%		
35) Dibromofluoromethane	5.391	113	130551	44.864	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery =	89.720%		
50) Toluene-d8	8.647	98	524330	48.817	ug/l	0.00
Spiked Amount 50.000	Range 92 - 112		Recovery =	97.640%		
62) 4-Bromofluorobenzene	11.079	95	196952	47.386	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery =	94.780%		
Target Compounds						
					Qvalue	
2) Dichlorodifluoromethane	1.313	85	1240	0.471	ug/l #	42
11) Tert butyl alcohol	2.983	59	3797	5.360	ug/l #	93
13) Acrolein	2.240	56	397	0.544	ug/l #	14
16) Acetone	2.386	43	8716	5.314	ug/l	91
20) Methylene Chloride	2.788	84	832	0.257	ug/l #	77
25) 2-Butanone	4.587	43	954	0.400	ug/l	95
31) Cyclohexane	5.550	56	6372	1.296	ug/l #	4
36) 1,1-Dichloropropene	5.550	75	20315	4.712	ug/l #	51
38) Carbon Tetrachloride	5.550	117	26979	6.638	ug/l #	17
51) 4-Methyl-2-Pentanone	8.580	43	2065	0.463	ug/l	96
52) Toluene	8.720	92	26867	3.330	ug/l	100
67) Ethyl Benzene	10.195	91	55686	3.786	ug/l	96
68) m/p-Xylenes	10.299	106	82065	14.605	ug/l	98
69) o-Xylene	10.647	106	84062	15.271	ug/l	99
70) Styrene	10.640	104	4034	0.459	ug/l #	1
73) Isopropylbenzene	10.964	105	19899	1.503	ug/l	98
76) 1,2,3-Trichloropropane	11.378	75	4130	1.134	ug/l #	1
78) n-propylbenzene	11.305	91	70112	4.585	ug/l	100
79) 2-Chlorotoluene	11.378	91	54355	5.630	ug/l #	42
80) 1,3,5-Trimethylbenzene	11.451	105	168654	15.240	ug/l	99
81) trans-1,4-Dichloro-2-b...	11.079	75	98304	80.918	ug/l #	9
82) 4-Chlorotoluene	11.451	91	18459	1.647	ug/l #	47
83) tert-Butylbenzene	11.750	119	73624	7.085	ug/l #	62
84) 1,2,4-Trimethylbenzene	11.750	105	597778	53.117	ug/l	99
85) sec-Butylbenzene	11.890	105	28012	2.216	ug/l	90
86) p-Isopropyltoluene	12.012	119	23804	2.258	ug/l	100
89) n-Butylbenzene	12.329	91	94615	10.273	ug/l #	29
90) Hexachloroethane	12.530	117	16816	10.296	ug/l #	15
92) 1,2-Dibromo-3-Chloropr...	12.963	75	2808	3.101	ug/l #	7
95) Naphthalene	13.774	128	203552	16.933	ug/l	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041523\
Data File : VX035091.D
Acq On : 14 Apr 2023 18:17
Operator : JC/MD
Sample : 02353-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BUR-1253

Quant Time: Apr 17 08:58:09 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032923W.M
Quant Title : SW846 8260
QLast Update : Sat Apr 01 01:50:18 2023
Response via : Initial Calibration




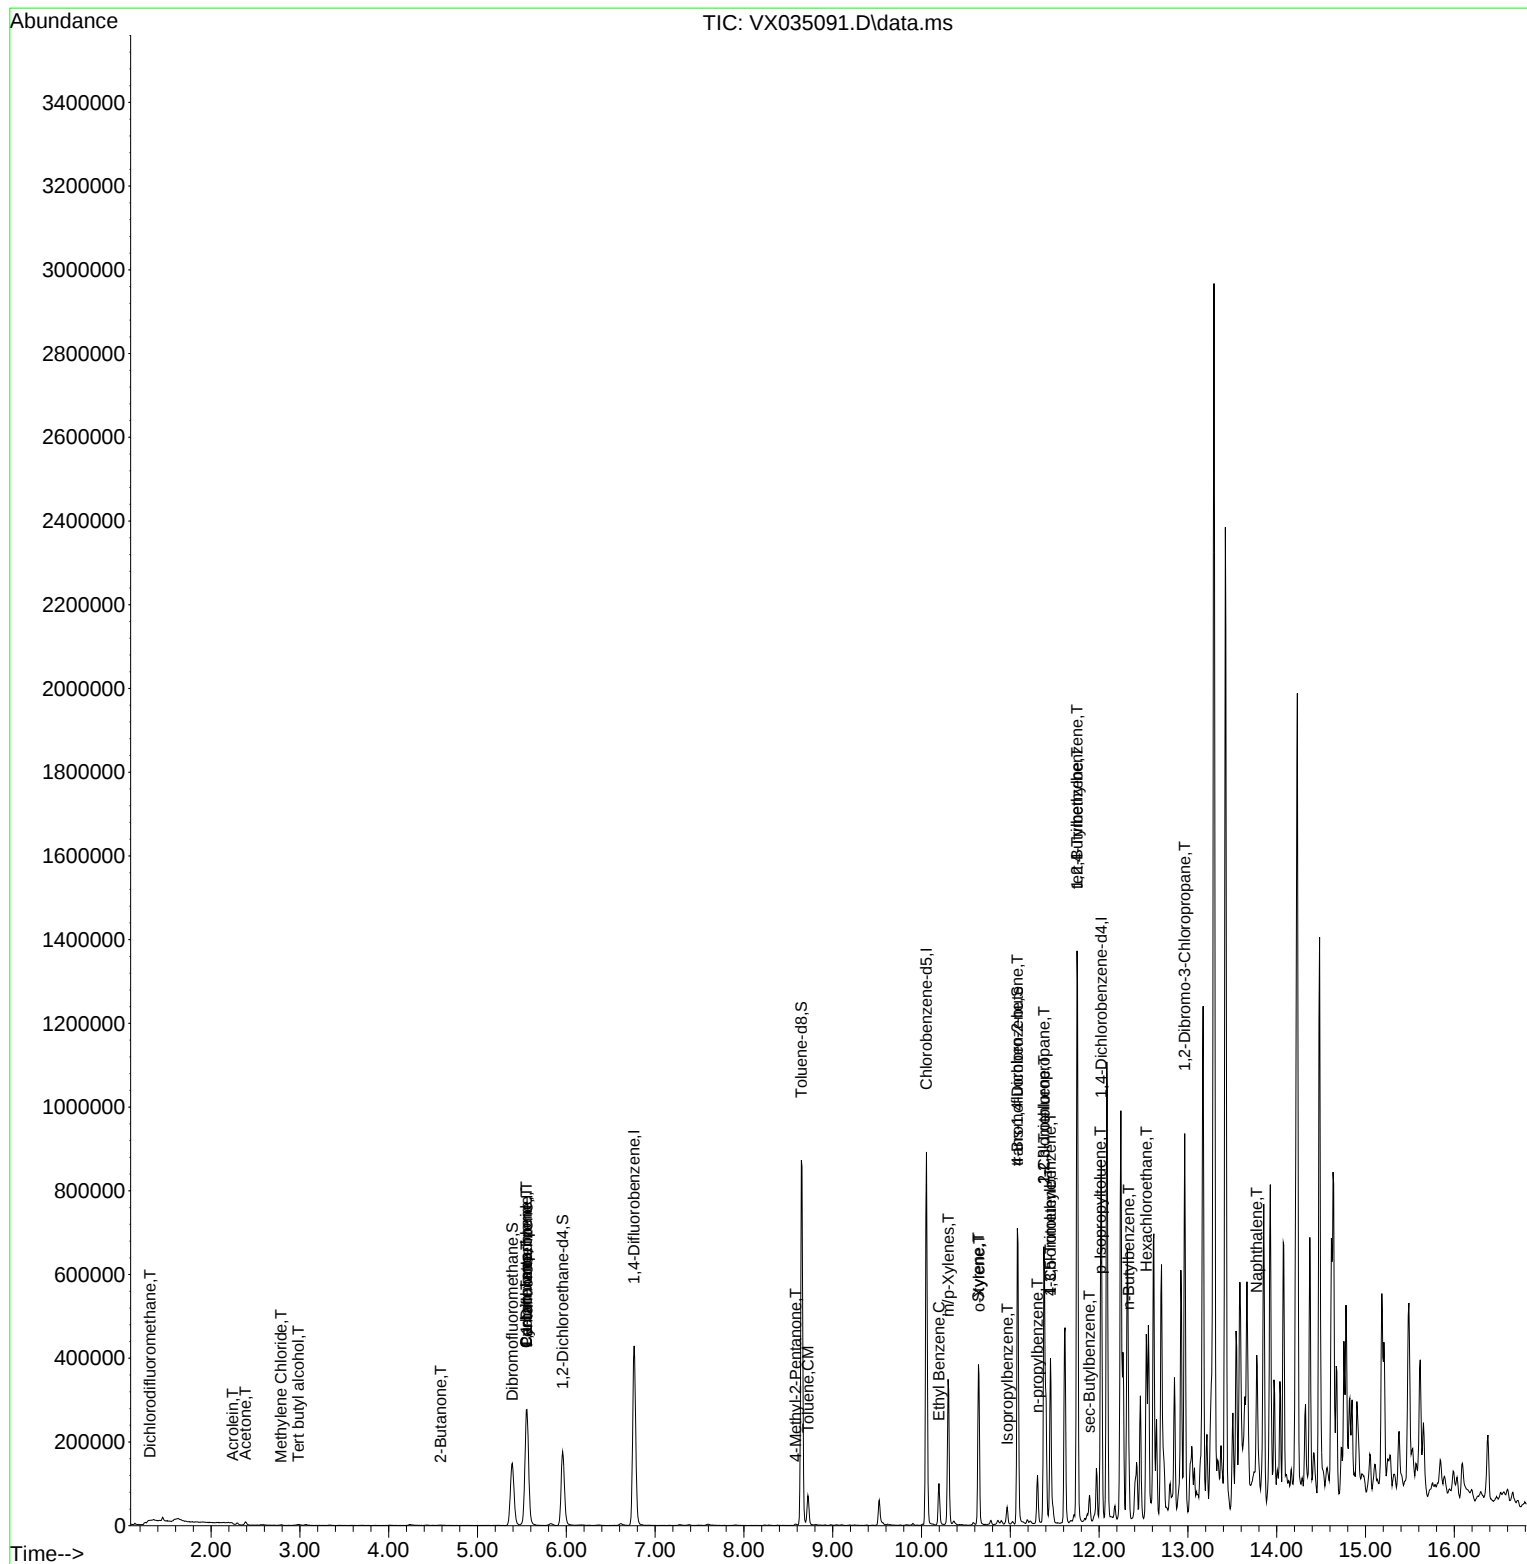




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.556 min Scan# 71
Delta R.T. 0.006 min
Lab File: VX035091.D
Acq: 14 Apr 2023 18:17




Instrument :
MSVOA_X
ClientSampleId :
BUR-1253


Tgt Ion:168 Resp: 264013
Ion Ratio Lower Upper
168 100
99 59.1 45.7 68.5



#2
Dichlorodifluoromethane
Concen: 0.471 ug/l
RT: 1.313 min Scan# 37
Delta R.T. 0.146 min
Lab File: VX035091.D
Acq: 14 Apr 2023 18:17

Tgt Ion: 85 Resp: 1240
Ion Ratio Lower Upper
85 100
87 0.0 16.4 49.1#

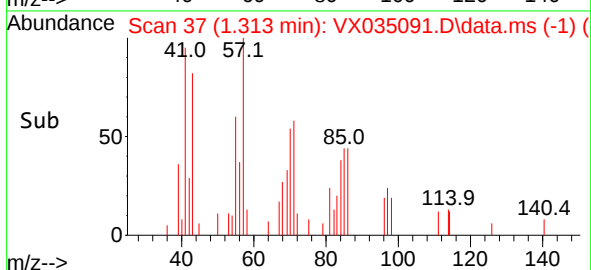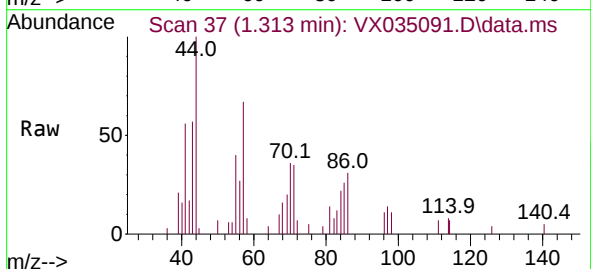

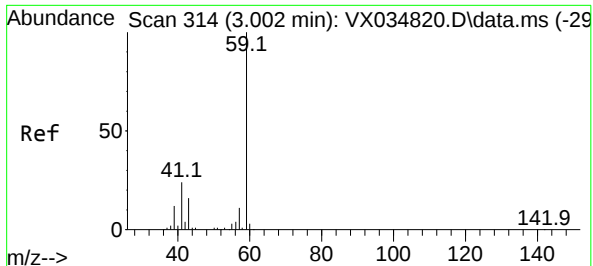

#11

Tert butyl alcohol

Concen: 5.360 ug/l

RT: 2.983 min Scan# 314

Delta R.T. -0.018 min

Lab File: VX035091.D

Acq: 14 Apr 2023 18:17

Instrument :

MSVOA_X

ClientSampleId :





BUR-1253

Tgt Ion: 59 Resp: 3797

Ion Ratio Lower Upper

59 100

57 7.6 8.1 12.1#

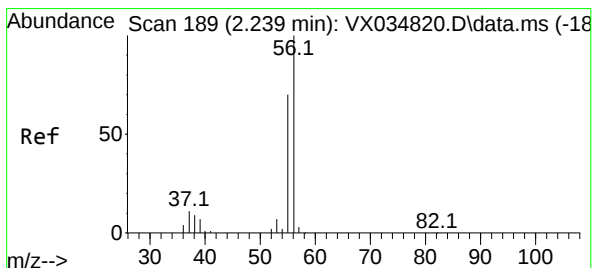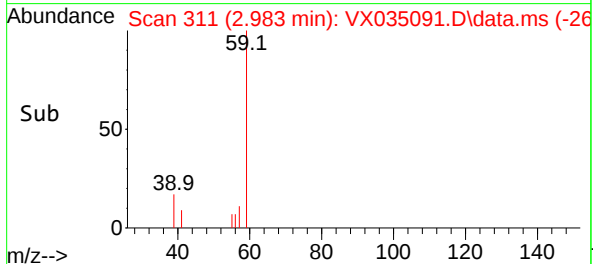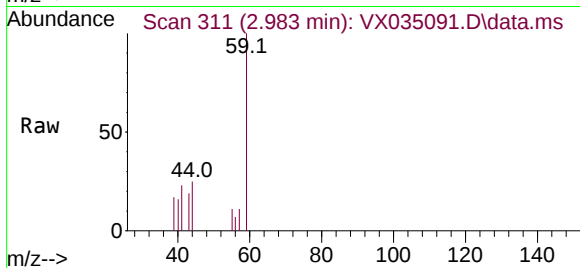

#13

Acrolein

Concen: 0.544 ug/l

RT: 2.240 min Scan# 189

Delta R.T. 0.000 min

Lab File: VX035091.D




Acq: 14 Apr 2023 18:17


Tgt Ion: 56 Resp: 397

Ion Ratio Lower Upper

56 100

55 0.0 56.6 85.0#

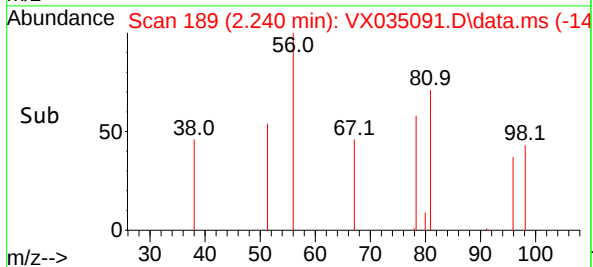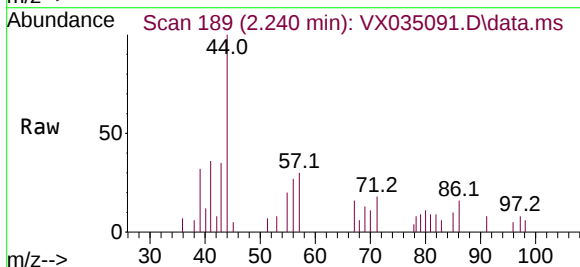



#16

Acetone

Concen: 5.314 ug/l

RT: 2.386 min Scan# 213

Delta R.T. 0.000 min

Lab File: VX035091.D

Acq: 14 Apr 2023 18:17

Instrument :

MSVOA_X

ClientSampleId :





BUR-1253

Tgt Ion: 43 Resp: 8716

Ion Ratio Lower Upper

43 100

58 25.7 24.7 37.1

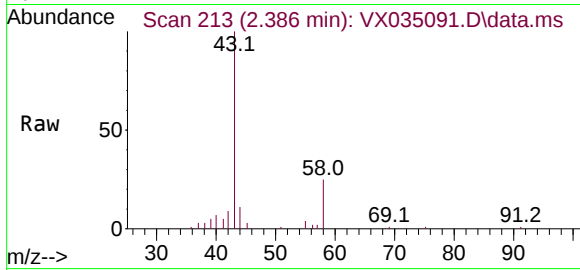

#20

Methylene Chloride

Concen: 0.257 ug/l

RT: 2.788 min Scan# 279

Delta R.T. 0.000 min

Lab File: VX035091.D

Acq: 14 Apr 2023 18:17

Tgt Ion: 84 Resp: 832




Ion Ratio Lower Upper


84 100

49 88.1 103.8 155.8#

51 38.4 31.8 47.8

86 55.9 51.4 77.2


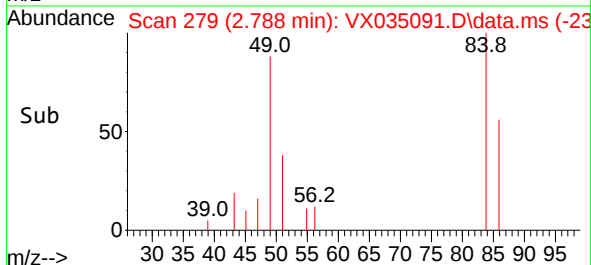
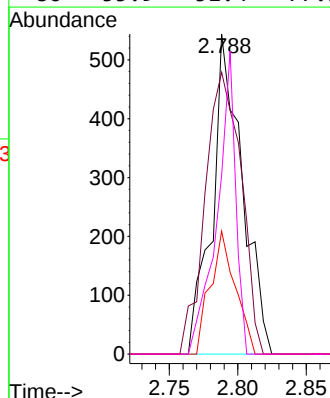
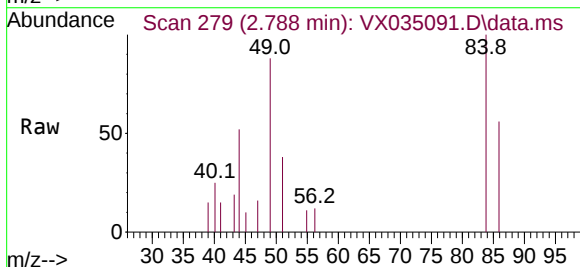




#25
2-Butanone
Concen: 0.400 ug/l
RT: 4.587 min Scan# 51
Delta R.T. 0.031 min
Lab File: VX035091.D
Acq: 14 Apr 2023 18:17




Instrument :
MSVOA_X
ClientSampleId :
BUR-1253


Tgt Ion: 43 Resp: 954
Ion Ratio Lower Upper
43 100
72 21.8 19.3 28.9

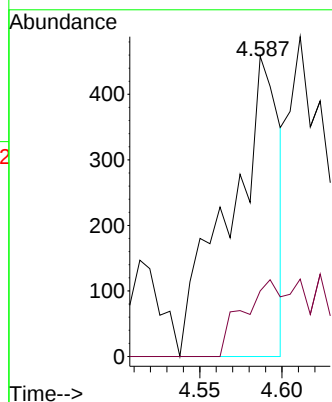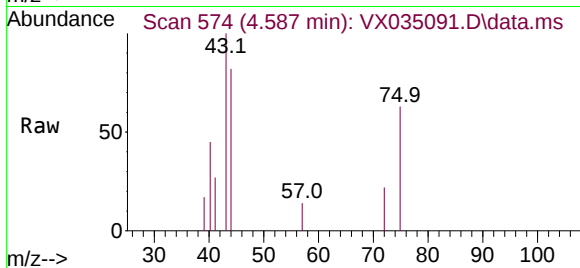

#31
Cyclohexane
Concen: 1.296 ug/l
RT: 5.550 min Scan# 732
Delta R.T. 0.079 min
Lab File: VX035091.D
Acq: 14 Apr 2023 18:17

Tgt Ion: 56 Resp: 6372
Ion Ratio Lower Upper
56 100
69 161.4 23.7 35.5#
84 126.7 68.5 102.7#

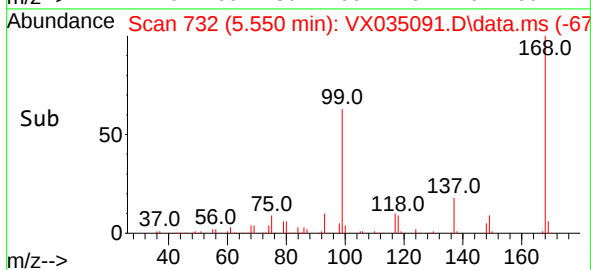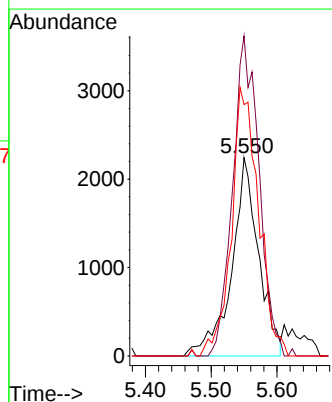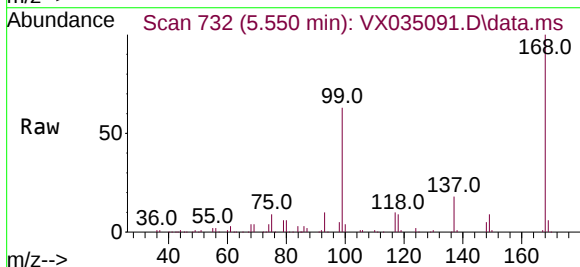



#33

1,2-Dichloroethane-d4

Concen: 41.411 ug/l

RT: 5.958 min Scan# 799

Delta R.T. 0.000 min

Lab File: VX035091.D

Acq: 14 Apr 2023 18:17

Instrument :

MSVOA_X

ClientSampleId :





BUR-1253

Tgt Ion: 65 Resp: 167206

Ion Ratio Lower Upper

65 100

67 52.2 0.0 104.0

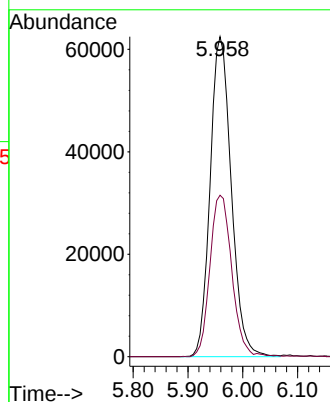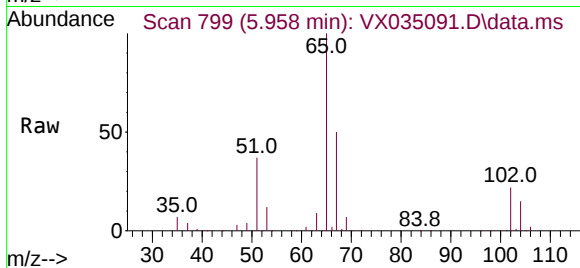

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.763 min Scan# 931

Delta R.T. 0.000 min

Lab File: VX035091.D

Acq: 14 Apr 2023 18:17




Tgt Ion: 114 Resp: 439948


Ion Ratio Lower Upper

114 100

63 21.1 0.0 42.2

88 16.9 0.0 33.2

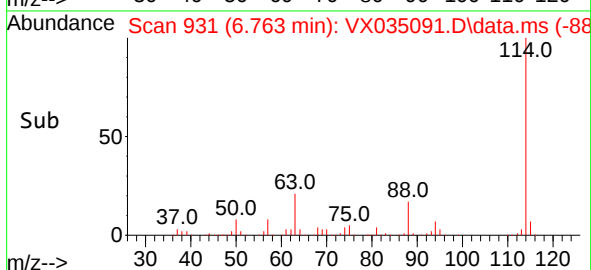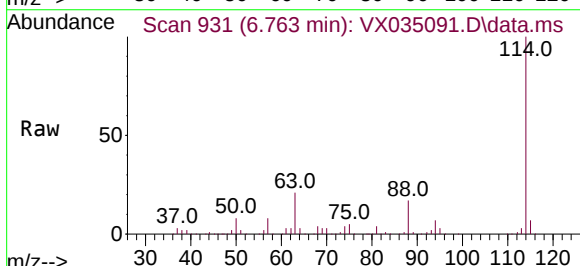

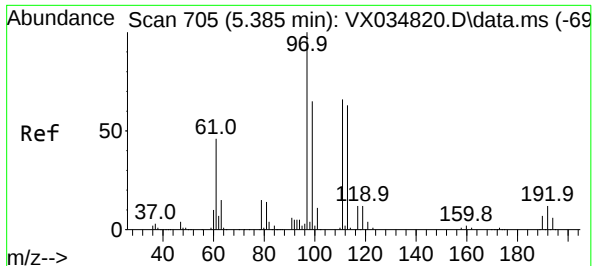

#35

Dibromofluoromethane

Concen: 44.864 ug/l

RT: 5.391 min Scan# 705

Delta R.T. 0.006 min

Lab File: VX035091.D

Acq: 14 Apr 2023 18:17

Instrument :

MSVOA_X

ClientSampleId :

BUR-1253





Tgt Ion:113 Resp: 130551

Ion Ratio Lower Upper

113 100

111 103.8 83.7 125.5

192 19.4 15.4 23.2

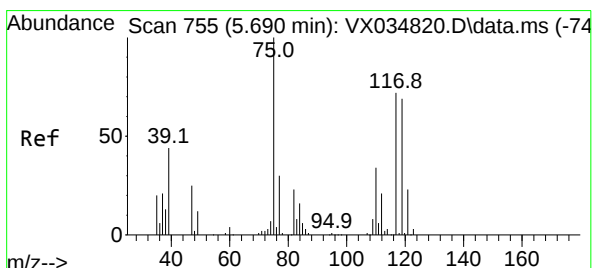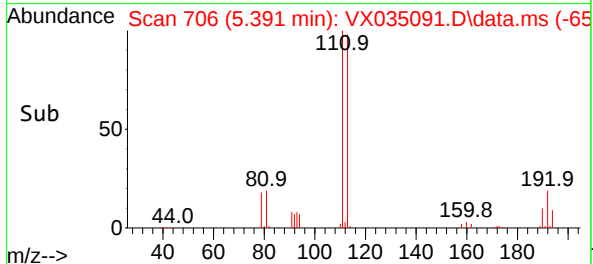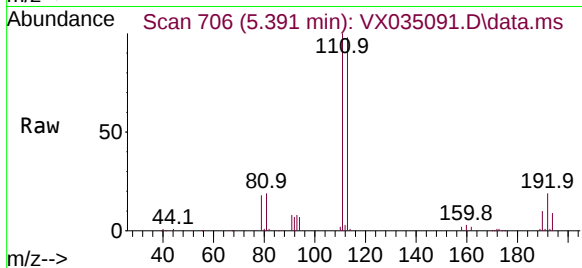

#36

1,1-Dichloropropene

Concen: 4.712 ug/l

RT: 5.550 min Scan# 732

Delta R.T. -0.140 min

Lab File: VX035091.D

Acq: 14 Apr 2023 18:17




Tgt Ion: 75 Resp: 20315


Ion Ratio Lower Upper

75 100

110 10.0 17.5 52.5#


77 0.0 24.3 36.5#

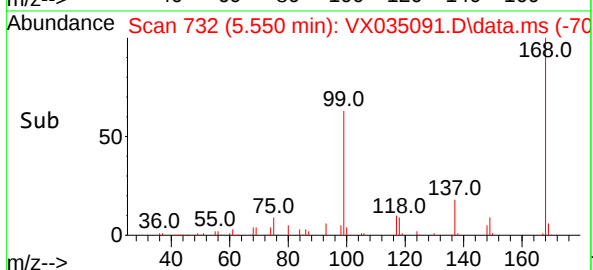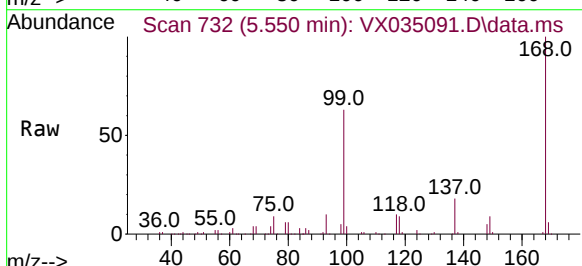






#38
Carbon Tetrachloride
Concen: 6.638 ug/l
RT: 5.550 min Scan# 71
Delta R.T. -0.128 min
Lab File: VX035091.D
Acq: 14 Apr 2023 18:17

Instrument :
MSVOA_X
ClientSampleId :
BUR-1253



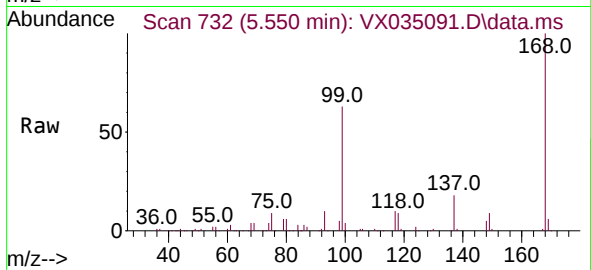



Tgt Ion:117 Resp: 26979
Ion Ratio Lower Upper
117 100
119 6.2 76.6 114.8#
121 0.0 23.8 35.6#



#50
Toluene-d8
Concen: 48.817 ug/l
RT: 8.647 min Scan# 1240
Delta R.T. 0.000 min
Lab File: VX035091.D
Acq: 14 Apr 2023 18:17

Tgt Ion: 98 Resp: 524330
Ion Ratio Lower Upper
98 100
100 66.8 52.5 78.7

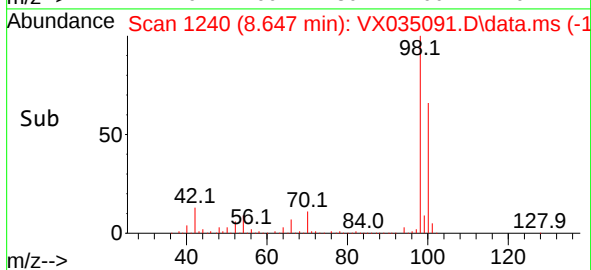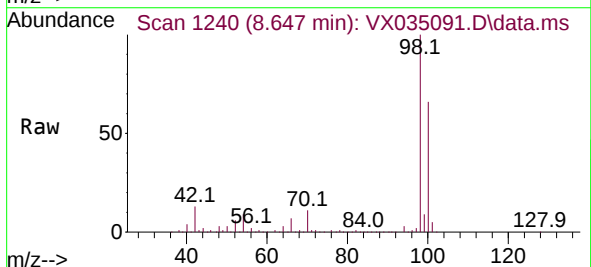



#51

4-Methyl-2-Pentanone

Concen: 0.463 ug/l

RT: 8.580 min Scan# 11

Delta R.T. 0.006 min

Lab File: VX035091.D

Acq: 14 Apr 2023 18:17

Instrument :

MSVOA_X

ClientSampleId :





BUR-1253

Tgt Ion: 43 Resp: 2065

Ion Ratio Lower Upper

43 100

58 40.9 30.6 46.0



#52

Toluene

Concen: 3.330 ug/l

RT: 8.720 min Scan# 1252

Delta R.T. 0.000 min

Lab File: VX035091.D




Acq: 14 Apr 2023 18:17


Tgt Ion: 92 Resp: 26867

Ion Ratio Lower Upper

92 100

91 171.6 136.8 205.2


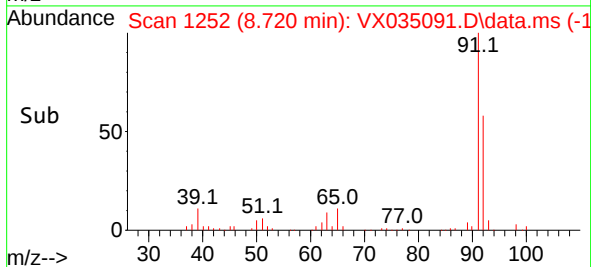

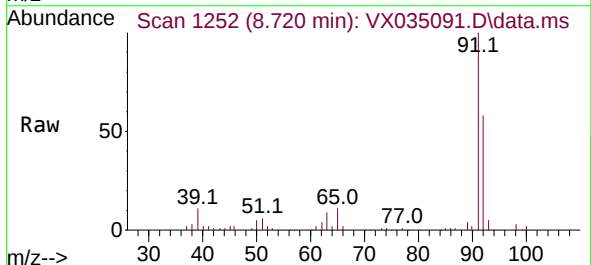




#62
4-Bromofluorobenzene
Concen: 47.386 ug/l
RT: 11.079 min Scan# 1
Delta R.T. 0.000 min
Lab File: VX035091.D
Acq: 14 Apr 2023 18:17




Instrument :
MSVOA_X
ClientSampleId :
BUR-1253


Tgt Ion: 95 Resp: 196952
Ion Ratio Lower Upper
95 100
174 75.3 0.0 147.4
176 72.8 0.0 140.6

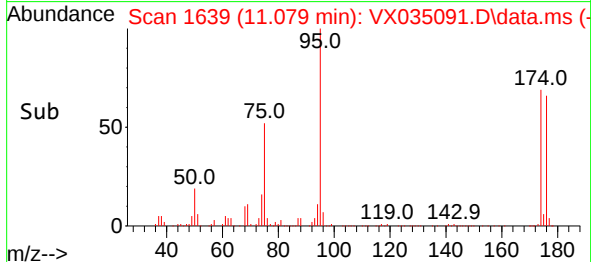

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX035091.D
Acq: 14 Apr 2023 18:17

Tgt Ion: 117 Resp: 390272
Ion Ratio Lower Upper
117 100
82 57.6 45.0 67.4
119 31.5 26.0 39.0

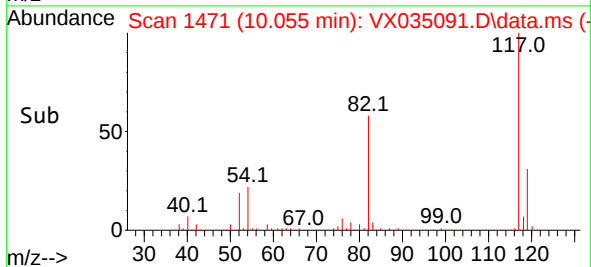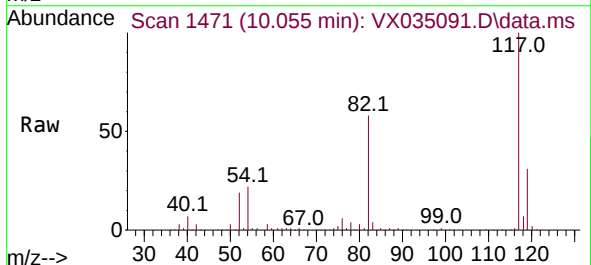



#67

Ethyl Benzene

Concen: 3.786 ug/l

RT: 10.195 min Scan# 1494

Delta R.T. 0.000 min

Lab File: VX035091.D

Acq: 14 Apr 2023 18:17

Instrument :

MSVOA_X

ClientSampleId :





BUR-1253

Tgt Ion: 91 Resp: 55686

Ion Ratio Lower Upper

91 100

106 29.7 25.6 38.4

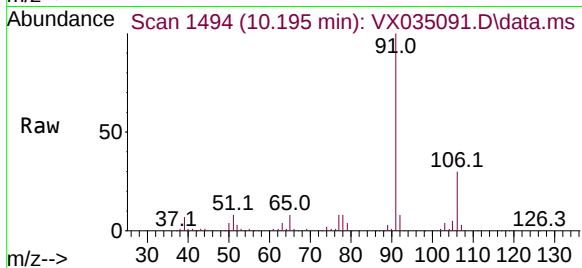

#68

m/p-Xylenes

Concen: 14.605 ug/l

RT: 10.299 min Scan# 1511

Delta R.T. 0.000 min

Lab File: VX035091.D




Acq: 14 Apr 2023 18:17


Tgt Ion: 106 Resp: 82065

Ion Ratio Lower Upper

106 100

91 202.2 164.0 246.0


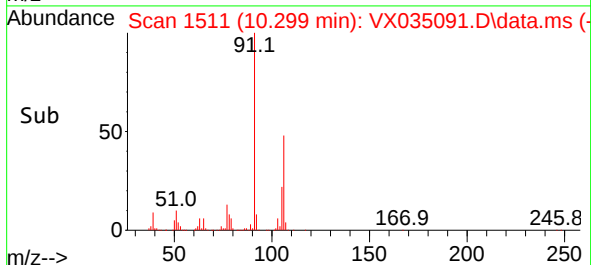
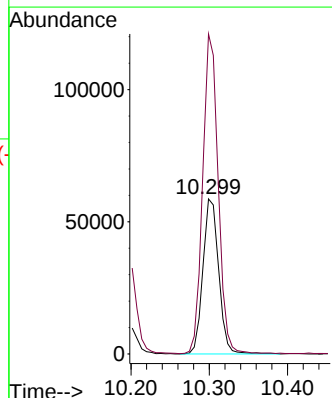
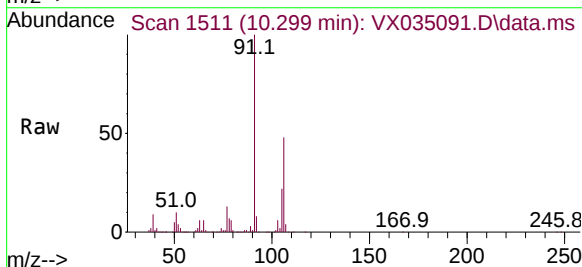




#69
o-Xylene
Concen: 15.271 ug/l
RT: 10.647 min Scan# 1
Delta R.T. 0.006 min
Lab File: VX035091.D
Acq: 14 Apr 2023 18:17




Instrument :
MSVOA_X
ClientSampleId :
BUR-1253


Tgt Ion:106 Resp: 84062
Ion Ratio Lower Upper
106 100
91 217.9 108.5 325.3

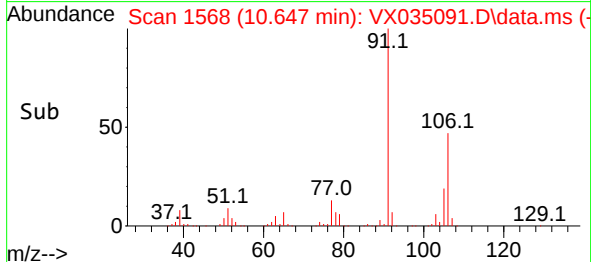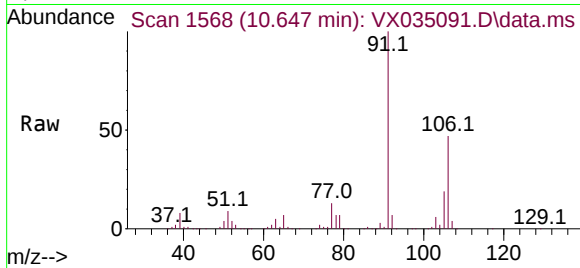

#70
Styrene
Concen: 0.459 ug/l
RT: 10.640 min Scan# 1567
Delta R.T. -0.013 min
Lab File: VX035091.D
Acq: 14 Apr 2023 18:17

Tgt Ion:104 Resp: 4034
Ion Ratio Lower Upper
104 100
78 315.5 43.4 65.2#
103 287.0 44.2 66.2#


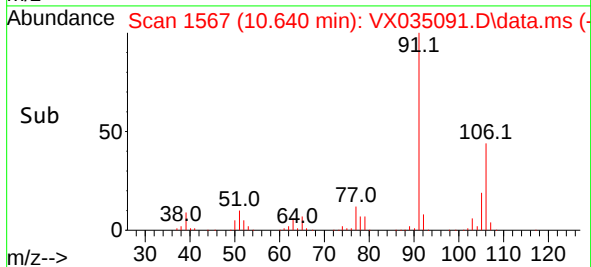

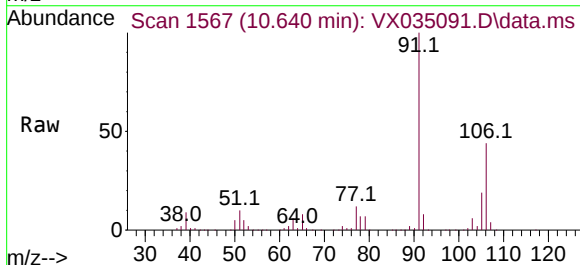




#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX035091.D
Acq: 14 Apr 2023 18:17




Instrument :
MSVOA_X
ClientSampleId :
BUR-1253


Tgt Ion:152 Resp: 180693
Ion Ratio Lower Upper
152 100
115 62.2 45.0 135.0
150 155.6 0.0 352.4

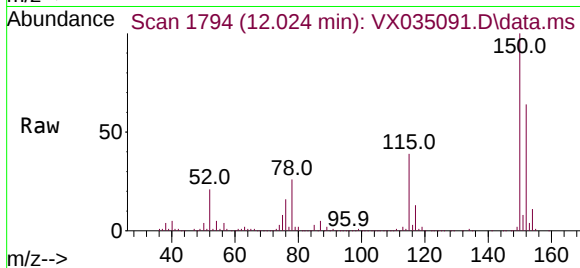

#73
Isopropylbenzene
Concen: 1.503 ug/l
RT: 10.964 min Scan# 1620
Delta R.T. 0.001 min
Lab File: VX035091.D
Acq: 14 Apr 2023 18:17

Tgt Ion:105 Resp: 19899
Ion Ratio Lower Upper
105 100
120 25.8 13.3 39.9

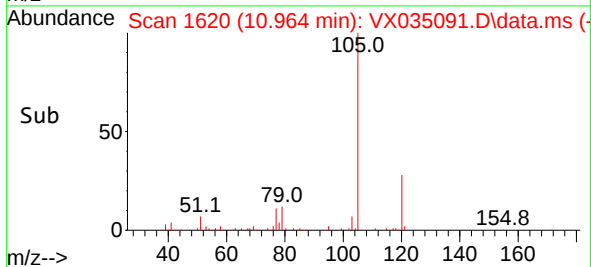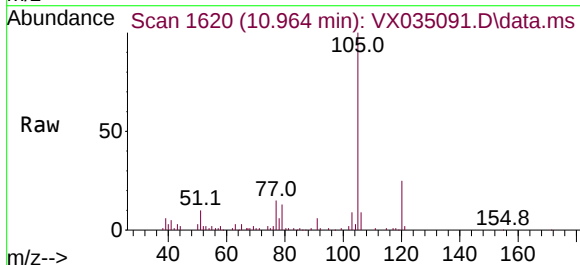

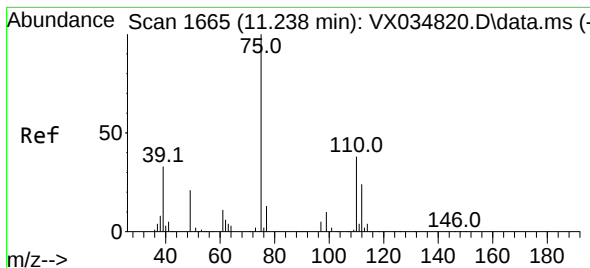

#76

1,2,3-Trichloropropane

Concen: 1.134 ug/l

RT: 11.378 min Scan# 1688

Delta R.T. 0.140 min

Lab File: VX035091.D

Acq: 14 Apr 2023 18:17

Instrument :

MSVOA_X

ClientSampleId :





BUR-1253

Tgt Ion: 75 Resp: 4130

Ion Ratio Lower Upper

75 100

77 1256.5 21.6 64.8#

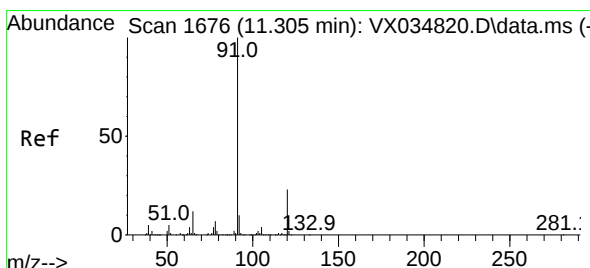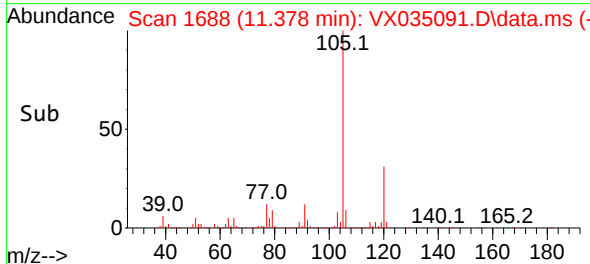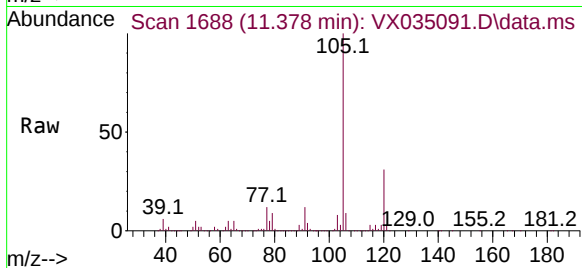

#78

n-propylbenzene

Concen: 4.585 ug/l

RT: 11.305 min Scan# 1676

Delta R.T. -0.000 min

Lab File: VX035091.D




Acq: 14 Apr 2023 18:17


Tgt Ion: 91 Resp: 70112

Ion Ratio Lower Upper

91 100

120 22.9 11.5 34.5

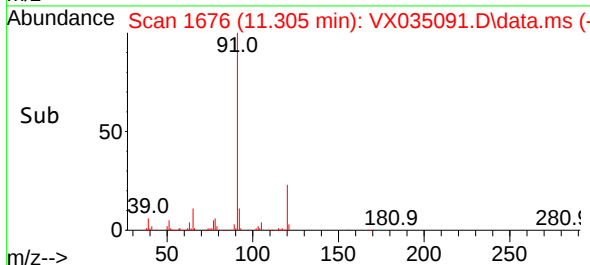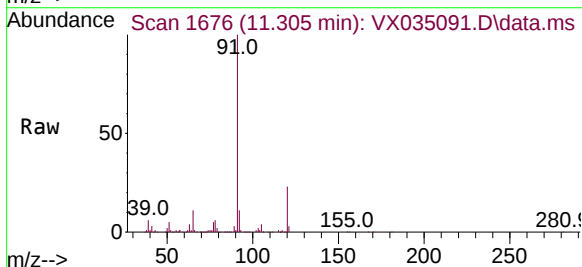



#79

2-Chlorotoluene

Concen: 5.630 ug/l

RT: 11.378 min Scan# 1

Delta R.T. 0.012 min

Lab File: VX035091.D

Acq: 14 Apr 2023 18:17

Instrument :

MSVOA_X

ClientSampleId :





BUR-1253

Tgt Ion: 91 Resp: 54355

Ion Ratio Lower Upper

91 100

126 0.0 16.3 48.9#

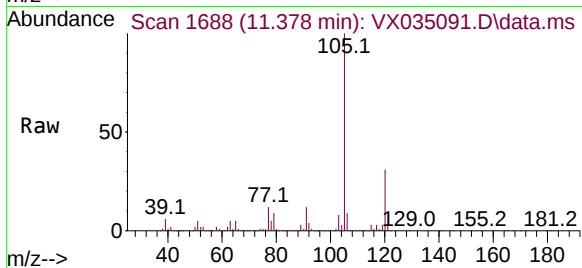

#80

1,3,5-Trimethylbenzene

Concen: 15.240 ug/l

RT: 11.451 min Scan# 1700

Delta R.T. 0.000 min

Lab File: VX035091.D




Acq: 14 Apr 2023 18:17


Tgt Ion: 105 Resp: 168654

Ion Ratio Lower Upper

105 100

120 48.3 23.7 71.1


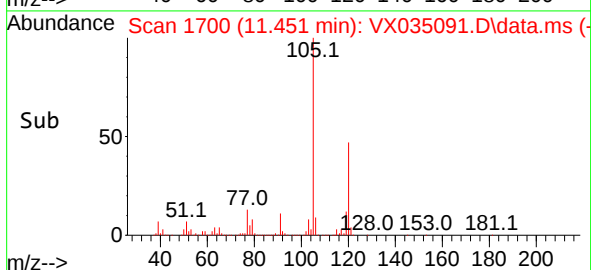

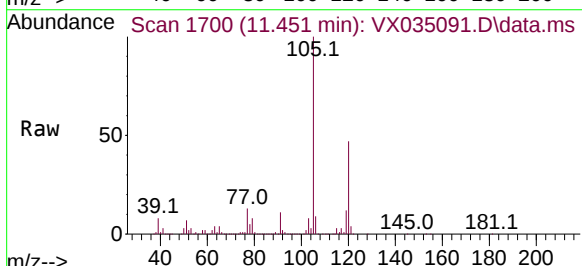




#81
trans-1,4-Dichloro-2-butene
Concen: 80.918 ug/l
RT: 11.079 min Scan# 1
Delta R.T. 0.061 min
Lab File: VX035091.D
Acq: 14 Apr 2023 18:17




Instrument :
MSVOA_X
ClientSampleId :
BUR-1253


Tgt Ion: 75 Resp: 98304
Ion Ratio Lower Upper
75 100
53 0.2 82.6 124.0#
89 0.0 36.9 55.3#

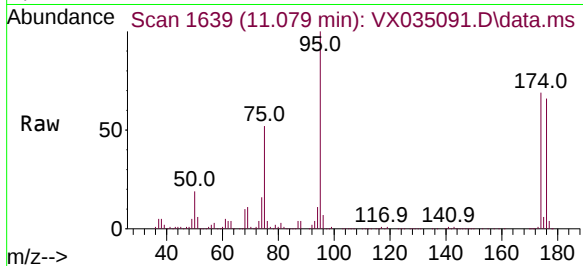

#82
4-Chlorotoluene
Concen: 1.647 ug/l
RT: 11.451 min Scan# 1700
Delta R.T. 0.000 min
Lab File: VX035091.D
Acq: 14 Apr 2023 18:17

Tgt Ion: 91 Resp: 18459
Ion Ratio Lower Upper
91 100
126 0.2 14.2 42.6#

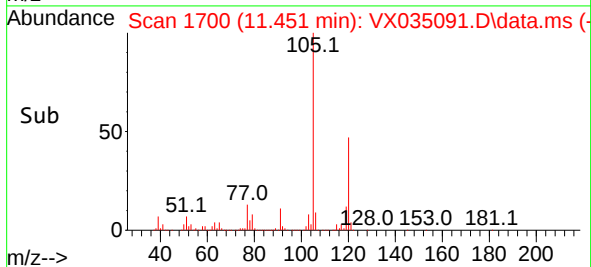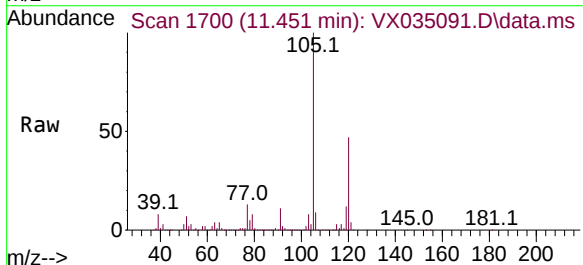



#83

tert-Butylbenzene

Concen: 7.085 ug/l

RT: 11.750 min Scan# 11

Delta R.T. 0.037 min

Lab File: VX035091.D

Acq: 14 Apr 2023 18:17

Instrument :

MSVOA_X

ClientSampleId :

BUR-1253





Tgt Ion:119 Resp: 73624

Ion Ratio Lower Upper

119 100

91 87.5 30.6 92.0

134 0.0 11.8 35.4#

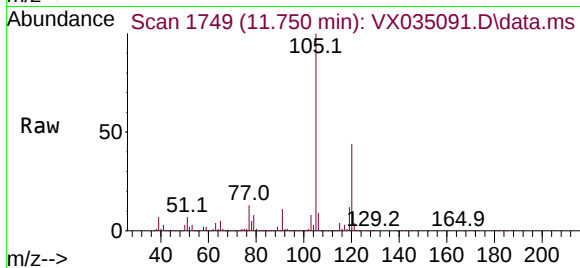

#84

1,2,4-Trimethylbenzene

Concen: 53.117 ug/l

RT: 11.750 min Scan# 1749

Delta R.T. 0.000 min

Lab File: VX035091.D




Acq: 14 Apr 2023 18:17


Tgt Ion:105 Resp: 597778

Ion Ratio Lower Upper

105 100

120 45.5 22.4 67.0

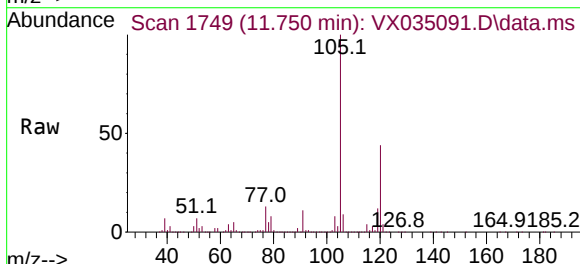

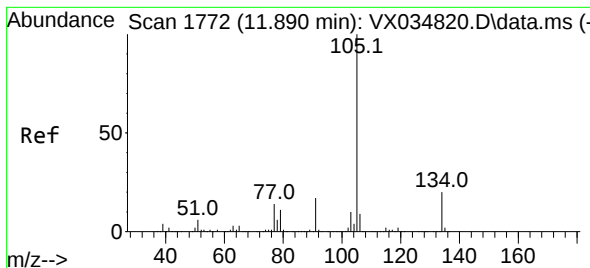

#85

sec-Butylbenzene

Concen: 2.216 ug/l

RT: 11.890 min Scan# 1772

Delta R.T. 0.000 min

Lab File: VX035091.D

Acq: 14 Apr 2023 18:17

Instrument :

MSVOA_X

ClientSampleId :





BUR-1253

Tgt Ion:105 Resp: 28012

Ion Ratio Lower Upper

105 100

134 25.0 10.2 30.4

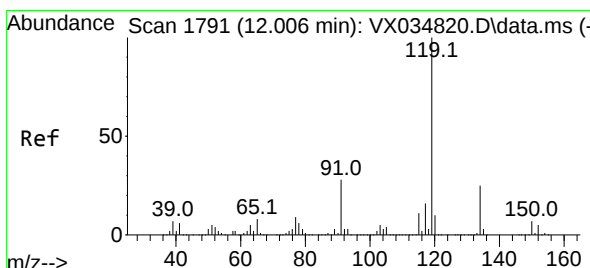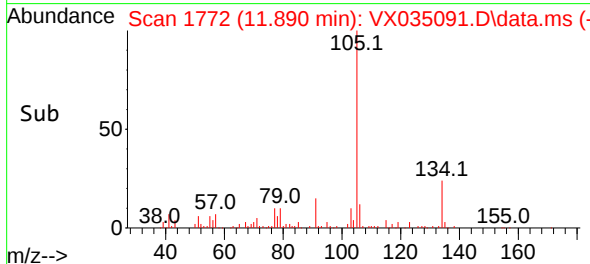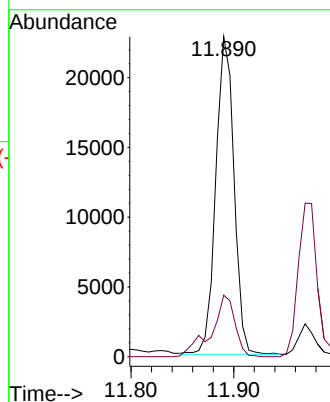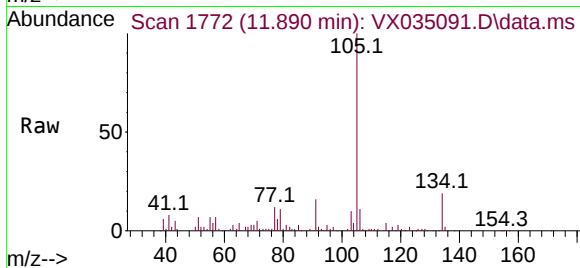

#86

p-Isopropyltoluene

Concen: 2.258 ug/l

RT: 12.012 min Scan# 1792

Delta R.T. 0.006 min

Lab File: VX035091.D

Acq: 14 Apr 2023 18:17




Tgt Ion:119 Resp: 23804


Ion Ratio Lower Upper

119 100

134 26.7 13.2 39.5

91 25.7 12.9 38.7

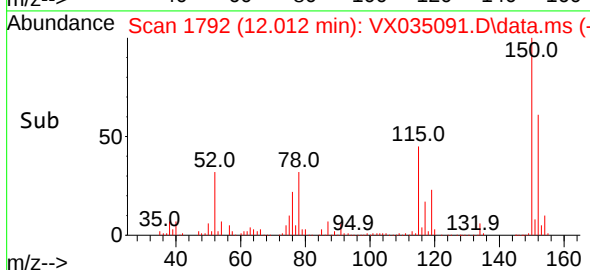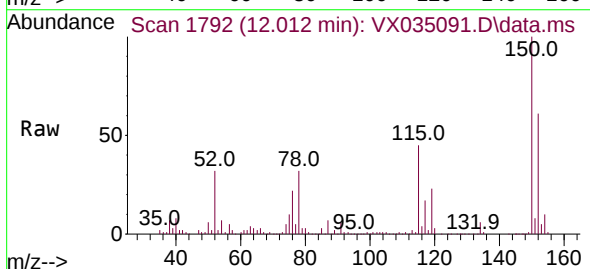



#89

n-Butylbenzene

Concen: 10.273 ug/l

RT: 12.329 min Scan# 1844

Delta R.T. 0.000 min

Lab File: VX035091.D

Acq: 14 Apr 2023 18:17

Instrument :

MSVOA_X

ClientSampleId :

BUR-1253





Tgt Ion: 91 Resp: 94615

Ion Ratio Lower Upper

91 100

92 33.3 27.7 83.0

134 105.7 13.0 38.9#

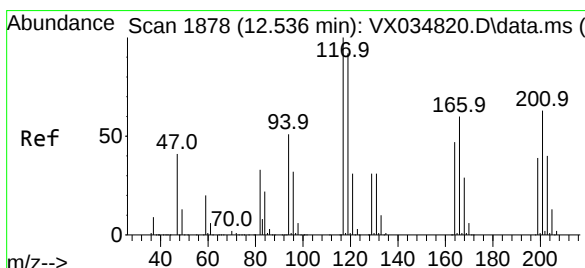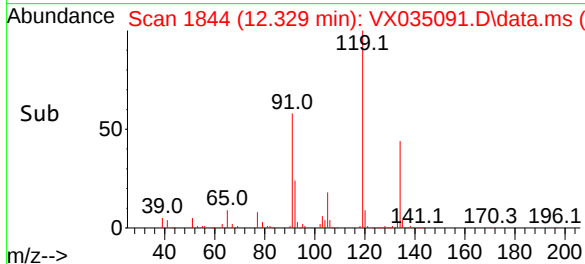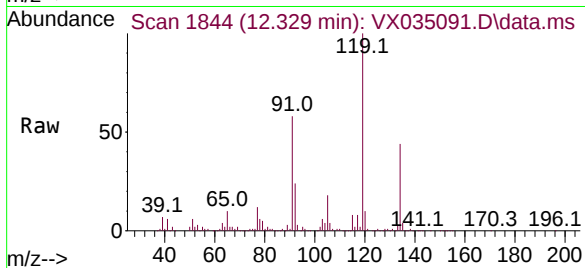

#90

Hexachloroethane

Concen: 10.296 ug/l

RT: 12.530 min Scan# 1877

Delta R.T. -0.006 min

Lab File: VX035091.D




Acq: 14 Apr 2023 18:17


Tgt Ion: 117 Resp: 16816

Ion Ratio Lower Upper

117 100

201 0.0 34.4 103.1#


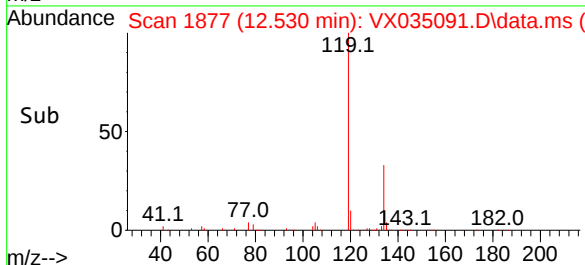

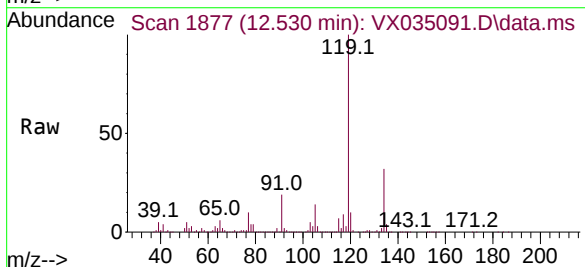




#92
1,2-Dibromo-3-Chloropropane
Concen: 3.101 ug/l
RT: 12.963 min Scan# 1948
Delta R.T. 0.018 min
Lab File: VX035091.D
Acq: 14 Apr 2023 18:17

Instrument :
MSVOA_X
ClientSampleId :
BUR-1253

Tgt Ion: 75 Resp: 2808
Ion Ratio Lower Upper
75 100
155 0.0 38.4 115.1#
157 4.3 49.9 149.7#

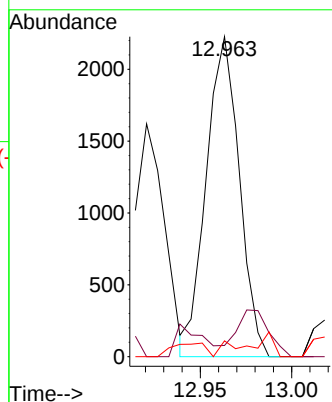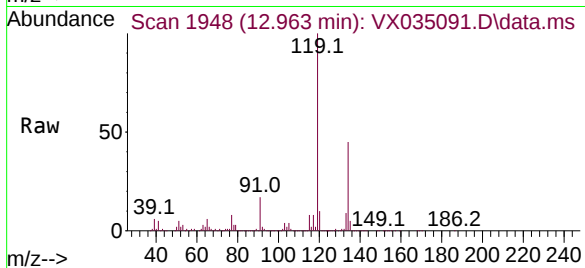

#95
Naphthalene
Concen: 16.933 ug/l
RT: 13.774 min Scan# 2081
Delta R.T. 0.000 min
Lab File: VX035091.D
Acq: 14 Apr 2023 18:17

Tgt Ion: 128 Resp: 203552
Ion Ratio Lower Upper
128 100
127 13.2 10.2 15.4
129 12.1 8.6 13.0

