

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041524\
 Data File : VX041072.D
 Acq On : 15 Apr 2024 12:50
 Operator : JC/MD
 Sample : P2049-07
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :

Quant Time: Apr 16 02:50:01 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Apr 16 02:47:54 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.763	114	278098	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	266719	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	140474	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.367	65	79167	40.023	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	80.040%		
7) Chloroethane-d5	1.672	69	70851	43.919	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	87.840%		
11) 1,1-Dichloroethene-d2	2.306	65	34039	40.307	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	80.620%		
21) 2-Butanone-d5	4.452	46	127374	118.216	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	118.220%		
24) Chloroform-d	5.056	84	159687	43.267	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	86.540%		
26) 1,2-Dichloroethane-d4	5.958	65	106063	44.179	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	88.360%		
32) Benzene-d6	5.976	84	314464	43.428	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	86.860%		
36) 1,2-Dichloropropane-d6	7.305	67	94546	44.770	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	89.540%		
41) Toluene-d8	8.646	98	289176	40.878	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	81.760%		
43) trans-1,3-Dichloroprop...	8.951	79	43824	41.237	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	82.480%		
47) 2-Hexanone-d5	9.384	63	86787	97.472	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	97.470%		
56) 1,1,2,2-Tetrachloroeth...	11.189	84	145446	46.494	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	92.980%		
66) 1,2-Dichlorobenzene-d4	12.317	152	137298	48.724	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	97.440%		
Target Compounds					Qvalue	
37) 1,2-Dichloropropane	7.311	63	10913	6.093	ug/L #	84


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041524\
Data File : VX041072.D
Acq On : 15 Apr 2024 12:50
Operator : JC/MD
Sample : P2049-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :

Quant Time: Apr 16 02:50:01 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Apr 16 02:47:54 2024
Response via : Initial Calibration

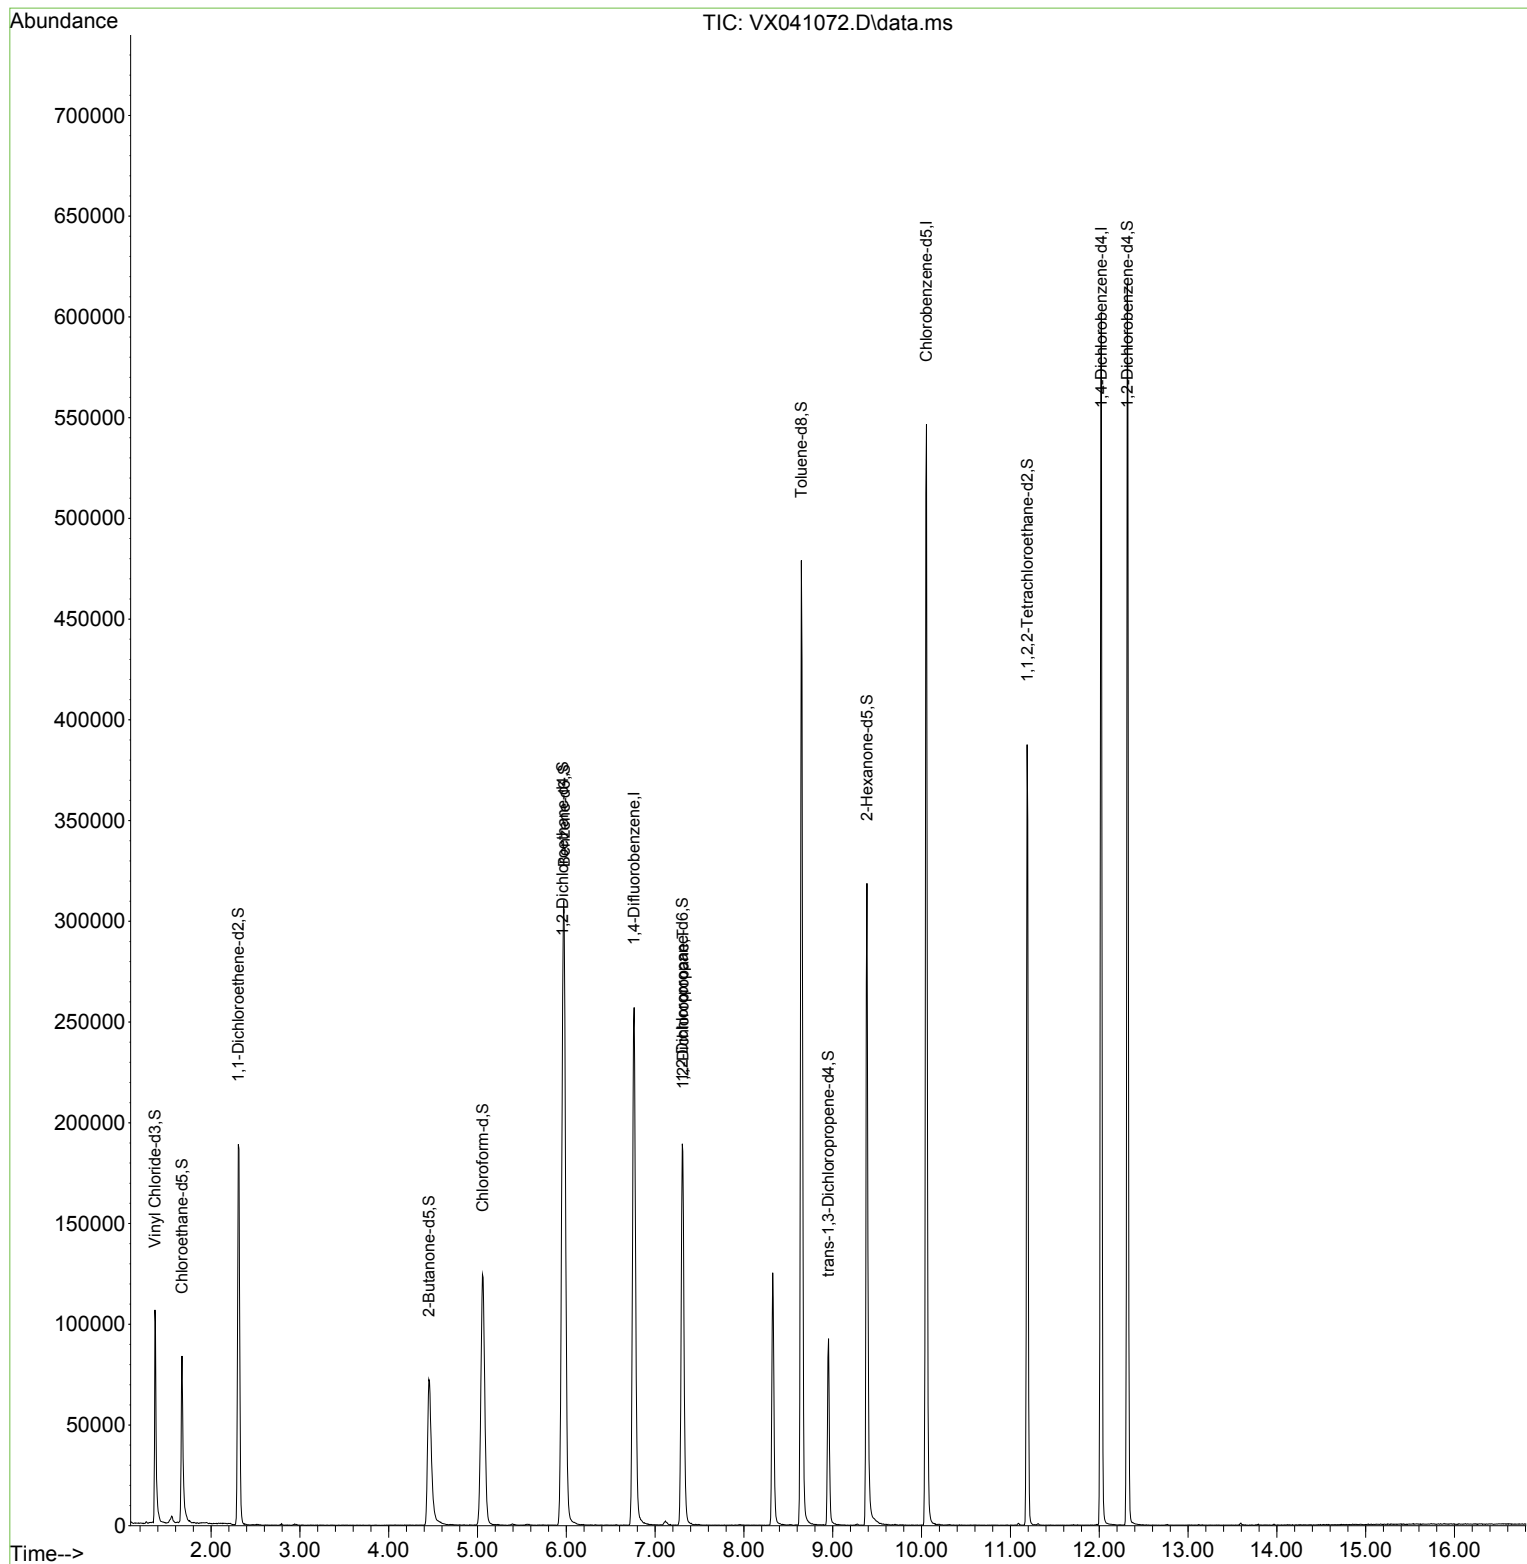

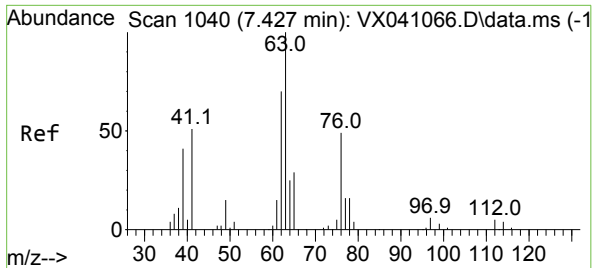

#37
 1,2-Dichloropropane
 Concen: 6.093 ug/L
 RT: 7.311 min Scan# 10
 Delta R.T. -0.116 min
 Lab File: VX041072.D
 Acq: 15 Apr 2024 12:50

Instrument :
 MSVOA_X
 ClientSampleId :

Tgt Ion: 63 Resp: 10913
 Ion Ratio Lower Upper
 63 100
 112 0.0 4.2 6.2#

