

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041524\
 Data File : VX041083.D
 Acq On : 15 Apr 2024 17:02
 Operator : JC/MD
 Sample : P2098-14
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :

Quant Time: Apr 16 02:52:12 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Apr 16 02:47:54 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.763	114	263057	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	253960	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	133084	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.367	65	77262	41.294	ug/L	0.00
Spiked Amount	50.000	Range 60 - 135	Recovery	=	82.580%	
7) Chloroethane-d5	1.672	69	70491	46.194	ug/L	0.00
Spiked Amount	50.000	Range 70 - 130	Recovery	=	92.380%	
11) 1,1-Dichloroethene-d2	2.306	65	33719	42.211	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	84.420%	
21) 2-Butanone-d5	4.452	46	122127	119.827	ug/L	0.00
Spiked Amount	100.000	Range 40 - 130	Recovery	=	119.830%	
24) Chloroform-d	5.062	84	159798	45.773	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	91.540%	
26) 1,2-Dichloroethane-d4	5.952	65	106725	46.997	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	94.000%	
32) Benzene-d6	5.976	84	311211	45.138	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	90.280%	
36) 1,2-Dichloropropane-d6	7.312	67	95413	47.450	ug/L	0.00
Spiked Amount	50.000	Range 70 - 120	Recovery	=	94.900%	
41) Toluene-d8	8.647	98	289979	43.051	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	86.100%	
43) trans-1,3-Dichloroprop...	8.951	79	43353	42.843	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	85.680%	
47) 2-Hexanone-d5	9.384	63	81464	96.091	ug/L	0.00
Spiked Amount	100.000	Range 45 - 130	Recovery	=	96.090%	
56) 1,1,2,2-Tetrachloroeth...	11.189	84	146956	49.337	ug/L	0.00
Spiked Amount	50.000	Range 65 - 120	Recovery	=	98.680%	
66) 1,2-Dichlorobenzene-d4	12.317	152	133978	50.186	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	100.380%	
Target Compounds						
37) 1,2-Dichloropropane	7.305	63	11226	6.582	ug/L	Qvalue # 84


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041524\
Data File : VX041083.D
Acq On : 15 Apr 2024 17:02
Operator : JC/MD
Sample : P2098-14
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :

Quant Time: Apr 16 02:52:12 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Apr 16 02:47:54 2024
Response via : Initial Calibration

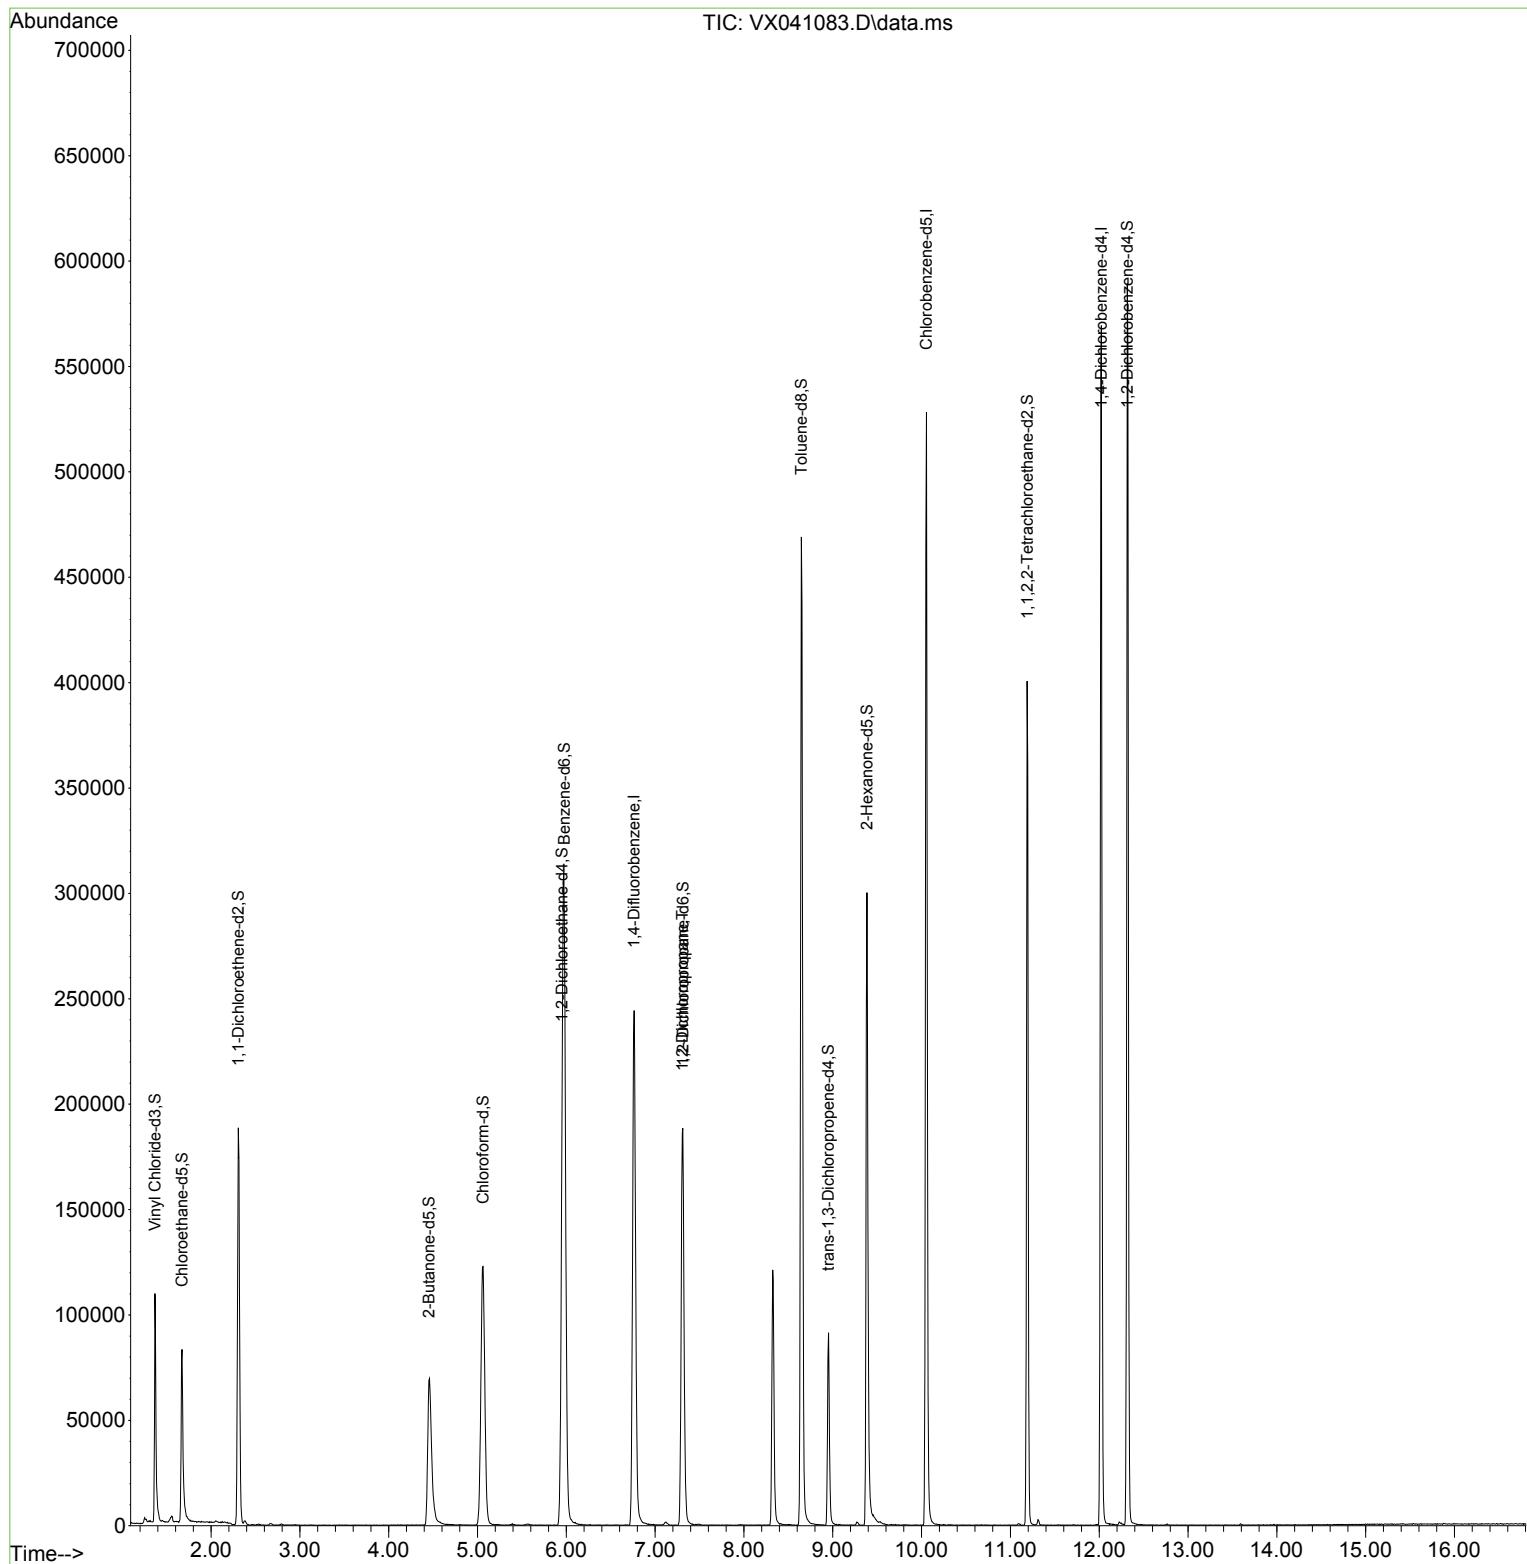

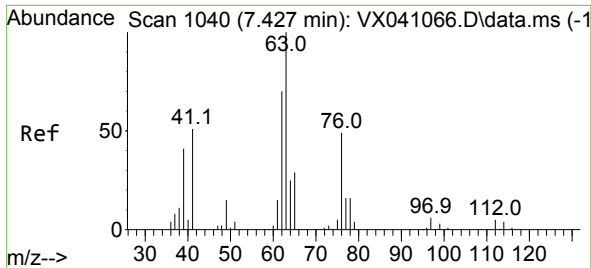

#37
 1,2-Dichloropropane
 Concen: 6.582 ug/L
 RT: 7.305 min Scan# 10
 Delta R.T. -0.122 min
 Lab File: VX041083.D
 Acq: 15 Apr 2024 17:02

Instrument :
 MSVOA_X
 ClientSampleId :

Tgt Ion: 63 Resp: 11226
 Ion Ratio Lower Upper
 63 100
 112 0.0 4.2 6.2#

