

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041524\
 Data File : VX041068.D
 Acq On : 15 Apr 2024 11:14
 Operator : JC/MD
 Sample : VX0415WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK672

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
 Title : VOC Analysis

Signal : TIC: VX041068.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	43	46	64	rVB	119122	143557	14.36%	1.786%
2	1.672	91	96	113	rVB	96622	139962	14.00%	1.741%
3	2.306	194	200	216	rVB	208099	331071	33.12%	4.119%
4	2.440	220	222	223	rBV	161	112	0.01%	0.001%
5	2.459	223	225	230	rBV3	346	488	0.05%	0.006%
6	2.794	275	280	285	rVB2	1216	2044	0.20%	0.025%
7	2.855	289	290	294	rVB2	141	112	0.01%	0.001%
8	2.892	294	296	299	rBV	140	138	0.01%	0.002%
9	2.940	299	304	305	rBV3	1106	1468	0.15%	0.018%
10	3.105	327	331	332	rBB2	152	192	0.02%	0.002%
11	3.221	348	350	353	rVB2	116	106	0.01%	0.001%
12	3.270	353	358	359	rBV2	78	109	0.01%	0.001%
13	3.520	396	399	402	rBV	144	182	0.02%	0.002%
14	3.587	409	410	413	rBV2	123	135	0.01%	0.002%
15	3.641	417	419	422	rBV2	112	131	0.01%	0.002%
16	4.062	484	488	491	rVB2	155	272	0.03%	0.003%
17	4.105	494	495	497	rBV2	117	115	0.01%	0.001%
18	4.452	543	552	581	rBV	72840	231972	23.21%	2.886%
19	4.818	610	612	614	rVB	246	183	0.02%	0.002%
20	4.903	625	626	628	rBV	120	107	0.01%	0.001%
21	4.940	631	632	636	rBV2	165	156	0.02%	0.002%
22	5.056	639	651	670	rBV	132178	410543	41.07%	5.108%
23	5.367	700	702	703	rBV2	182	163	0.02%	0.002%
24	5.495	721	723	724	rVB	228	125	0.01%	0.002%
25	5.562	727	734	735	rBV3	337	665	0.07%	0.008%
26	5.641	745	747	749	rBV	127	126	0.01%	0.002%
27	5.970	789	801	823	rBV2	335108	999502	100.00%	12.435%
28	6.184	834	836	838	rVB2	368	200	0.02%	0.002%
29	6.275	849	851	854	rVB2	202	218	0.02%	0.003%
30	6.397	869	871	874	rBV2	211	184	0.02%	0.002%
31	6.458	877	881	885	rBV2	244	380	0.04%	0.005%
32	6.501	885	888	890	rBB2	195	197	0.02%	0.002%
33	6.525	890	892	893	rBV2	126	129	0.01%	0.002%
34	6.684	916	918	921	rVB	112	127	0.01%	0.002%
35	6.763	921	931	956	rBV	262717	640875	64.12%	7.973%
36	7.007	969	971	973	rVB2	227	129	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041524\
 Data File : VX041068.D
 Acq On : 15 Apr 2024 11:14
 Operator : JC/MD
 Sample : VX0415WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK672

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
 Title : VOC Analysis

37	7.056	977	979	981	rVB	201	108	0.01%	0.001%
38	7.123	983	990	997	rVV6	2123	5235	0.52%	0.065%
39	7.190	1000	1001	1004	rBV2	200	230	0.02%	0.003%
40	7.305	1010	1020	1044	rBV	202366	450231	45.05%	5.602%
41	7.879	1111	1114	1117	rBV	108	113	0.01%	0.001%
42	7.946	1123	1125	1126	rBV2	145	109	0.01%	0.001%
43	8.013	1135	1136	1138	rBV	154	110	0.01%	0.001%
44	8.147	1155	1158	1160	rVV	167	114	0.01%	0.001%
45	8.324	1181	1187	1202	rBV	137698	227474	22.76%	2.830%
46	8.488	1213	1214	1216	rBV	248	224	0.02%	0.003%
47	8.647	1234	1240	1261	rBV	514956	825004	82.54%	10.264%
48	8.952	1284	1290	1306	rBV	96910	150584	15.07%	1.873%
49	9.153	1321	1323	1325	rBV	242	115	0.01%	0.001%
50	9.177	1325	1327	1329	rVB	164	123	0.01%	0.002%
51	9.275	1339	1343	1348	rVB3	403	708	0.07%	0.009%
52	9.384	1355	1361	1388	rBV	322443	491945	49.22%	6.121%
53	9.634	1400	1402	1403	rVB2	299	152	0.02%	0.002%
54	9.701	1409	1413	1418	rVB4	599	1143	0.11%	0.014%
55	9.829	1430	1434	1436	rBV3	215	297	0.03%	0.004%
56	9.903	1443	1446	1448	rBV2	156	224	0.02%	0.003%
57	9.927	1448	1450	1452	rVV2	139	112	0.01%	0.001%
58	9.951	1452	1454	1456	rVV	145	125	0.01%	0.002%
59	9.976	1456	1458	1459	rVB	204	110	0.01%	0.001%
60	9.988	1459	1460	1462	rBV2	151	117	0.01%	0.001%
61	10.055	1465	1471	1493	rVV	556076	793353	79.37%	9.870%
62	10.317	1509	1514	1517	rBV	251	354	0.04%	0.004%
63	10.506	1540	1545	1547	rBV2	114	220	0.02%	0.003%
64	10.726	1579	1581	1583	rBV2	110	130	0.01%	0.002%
65	10.854	1601	1602	1605	rBV	169	116	0.01%	0.001%
66	10.927	1611	1614	1617	rBV	178	161	0.02%	0.002%
67	10.963	1617	1620	1621	rBV2	211	165	0.02%	0.002%
68	11.091	1636	1641	1646	rVB4	1054	1488	0.15%	0.019%
69	11.189	1652	1657	1672	rVB	411334	528813	52.91%	6.579%
70	11.707	1738	1742	1747	rBV	125	185	0.02%	0.002%
71	11.762	1748	1751	1753	rVV	174	205	0.02%	0.003%
72	11.817	1758	1760	1763	rBV	217	115	0.01%	0.001%
73	11.969	1781	1785	1788	rBV3	695	863	0.09%	0.011%
74	12.018	1788	1793	1805	rBV	631715	814363	81.48%	10.132%
75	12.317	1837	1842	1857	rBV	654581	827430	82.78%	10.294%
76	12.518	1871	1875	1878	rBV	158	229	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041524\
 Data File : VX041068.D
 Acq On : 15 Apr 2024 11:14
 Operator : JC/MD
 Sample : VX0415WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK672

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
 Title : VOC Analysis

77	12.768	1913	1916	1920	rBV	298	395	0.04%	0.005%
78	12.859	1929	1931	1935	rVB	183	174	0.02%	0.002%
79	12.926	1939	1942	1944	rBV2	148	199	0.02%	0.002%
80	12.969	1947	1949	1951	rBV2	196	177	0.02%	0.002%
81	13.061	1960	1964	1969	rVB2	132	196	0.02%	0.002%
82	13.115	1969	1973	1979	rBV3	490	774	0.08%	0.010%
83	13.237	1991	1993	1996	rBV2	121	136	0.01%	0.002%
84	13.335	2007	2009	2014	rVB2	132	161	0.02%	0.002%
85	13.384	2015	2017	2022	rVB	166	172	0.02%	0.002%
86	13.597	2048	2052	2056	rVV	1435	1756	0.18%	0.022%
87	13.634	2056	2058	2061	rVB2	201	139	0.01%	0.002%
88	13.676	2064	2065	2068	rBV2	144	135	0.01%	0.002%
89	13.701	2068	2069	2071	rVB	173	123	0.01%	0.002%
90	13.786	2078	2083	2090	rVB	537	980	0.10%	0.012%
91	13.841	2090	2092	2094	rVB2	147	116	0.01%	0.001%
92	13.865	2094	2096	2097	rBV2	179	151	0.02%	0.002%
93	13.932	2103	2107	2108	rVB	159	154	0.02%	0.002%
94	13.963	2108	2112	2118	rBV4	775	1322	0.13%	0.016%
95	14.188	2146	2149	2152	rBB3	154	195	0.02%	0.002%
96	14.280	2161	2164	2165	rBV2	199	273	0.03%	0.003%
97	14.694	2228	2232	2233	rBV2	265	263	0.03%	0.003%
98	14.713	2233	2235	2236	rBV	216	133	0.01%	0.002%
99	14.768	2242	2244	2245	rBV2	288	249	0.02%	0.003%
100	16.286	2491	2493	2494	rBV2	394	209	0.02%	0.003%




Sum of corrected areas: 8037654

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041524\
Data File : VX041068.D
Acq On : 15 Apr 2024 11:14
Operator : JC/MD
Sample : VX0415WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK672

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

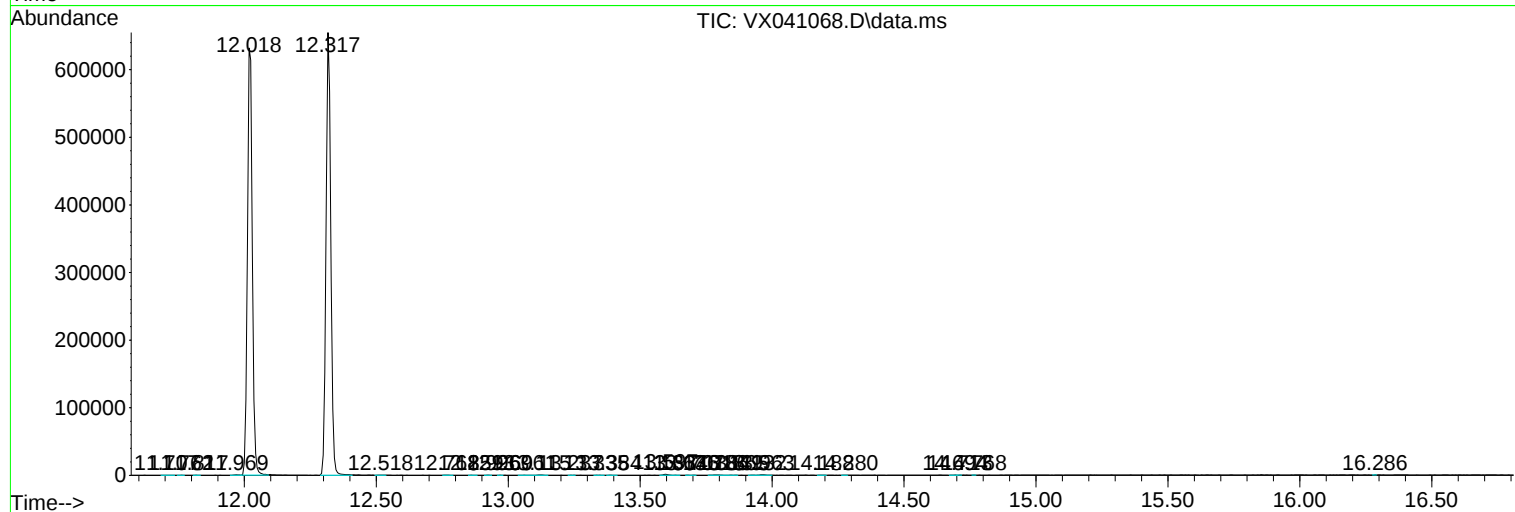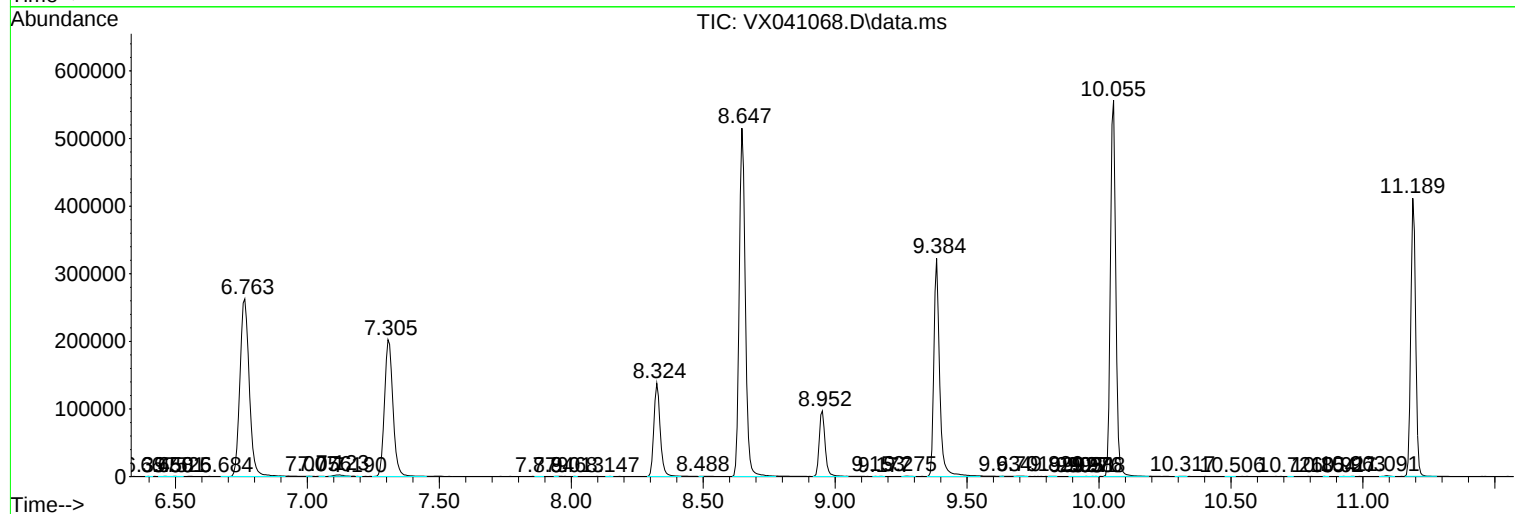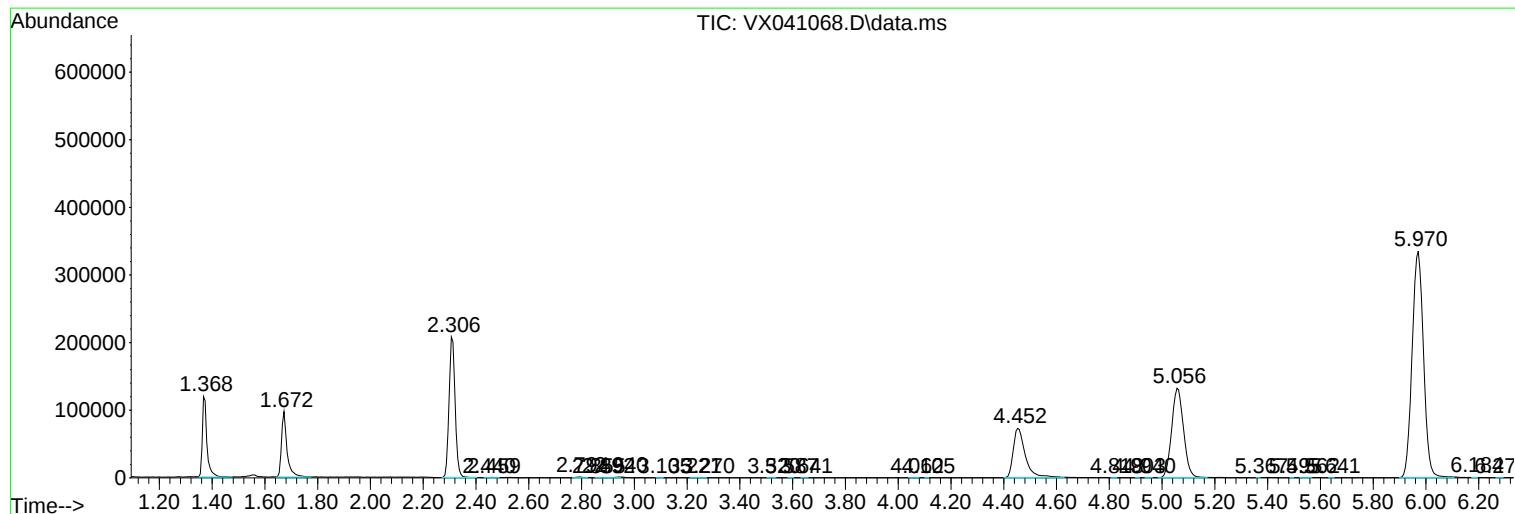

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041524\
Data File : VX041068.D
Acq On : 15 Apr 2024 11:14
Operator : JC/MD
Sample : VX0415WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK672

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM041024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041524\
Data File : VX041068.D
Acq On : 15 Apr 2024 11:14
Operator : JC/MD
Sample : VX0415WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK672

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc