

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041524\
 Data File : VX041074.D
 Acq On : 15 Apr 2024 13:35
 Operator : JC/MD
 Sample : P2098-03 10X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0RJ5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
 Title : VOC Analysis

Signal : TIC: VX041074.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	43	46	61	rBV	114618	131387	13.74%	1.693%
2	1.666	91	95	116	rVB	84590	131969	13.81%	1.701%
3	2.306	194	200	209	rBV	197281	304863	31.89%	3.929%
4	2.502	230	232	233	rBV	218	216	0.02%	0.003%
5	2.538	233	238	245	rVB	1847	3523	0.37%	0.045%
6	2.745	270	272	274	rVB	170	114	0.01%	0.001%
7	2.794	275	280	285	rVV2	990	1844	0.19%	0.024%
8	2.849	288	289	292	rBV2	112	116	0.01%	0.001%
9	2.947	298	305	316	rVV	5694	12620	1.32%	0.163%
10	3.087	325	328	331	rVB2	113	144	0.02%	0.002%
11	3.117	331	333	335	rBV	172	95	0.01%	0.001%
12	3.623	413	416	418	rBV2	171	187	0.02%	0.002%
13	3.648	418	420	423	rBV	106	119	0.01%	0.002%
14	3.715	428	431	432	rVB	125	95	0.01%	0.001%
15	3.733	432	434	438	rBV	122	166	0.02%	0.002%
16	3.940	465	468	469	rVB	120	104	0.01%	0.001%
17	3.959	469	471	472	rBV	137	113	0.01%	0.001%
18	3.983	472	475	478	rBV2	150	201	0.02%	0.003%
19	4.343	531	534	536	rBV	218	223	0.02%	0.003%
20	4.452	543	552	566	rBV	74020	227809	23.83%	2.936%
21	4.965	634	636	637	rBV	186	97	0.01%	0.001%
22	5.056	639	651	667	rVV	125631	392105	41.02%	5.053%
23	5.391	699	706	709	rBV4	645	1492	0.16%	0.019%
24	5.550	729	732	741	rVB4	688	1690	0.18%	0.022%
25	5.647	746	748	749	rBV	90	93	0.01%	0.001%
26	5.751	763	765	767	rBV	114	104	0.01%	0.001%
27	5.775	767	769	770	rVB2	154	96	0.01%	0.001%
28	5.830	776	778	781	rBV2	104	101	0.01%	0.001%
29	5.970	788	801	819	rBV2	322496	955948	100.00%	12.320%
30	6.227	841	843	845	rBV2	199	193	0.02%	0.002%
31	6.306	852	856	859	rBV2	196	346	0.04%	0.004%
32	6.361	863	865	867	rVB2	169	139	0.01%	0.002%
33	6.696	918	920	921	rBV	168	100	0.01%	0.001%
34	6.763	921	931	949	rBV	254847	622916	65.16%	8.028%
35	7.117	984	989	999	rVB3	1469	3167	0.33%	0.041%
36	7.184	999	1000	1002	rVB2	242	135	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041524\
 Data File : VX041074.D
 Acq On : 15 Apr 2024 13:35
 Operator : JC/MD
 Sample : P2098-03 10X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0RJ5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
 Title : VOC Analysis

37	7.214	1002	1005	1006	rBV2	141	141	0.01%	0.002%
38	7.306	1011	1020	1037	rBV	191554	431123	45.10%	5.556%
39	7.763	1093	1095	1098	rVB	118	138	0.01%	0.002%
40	7.818	1102	1104	1107	rBV2	140	185	0.02%	0.002%
41	7.934	1121	1123	1124	rBV2	133	97	0.01%	0.001%
42	8.055	1141	1143	1144	rBV	232	213	0.02%	0.003%
43	8.232	1170	1172	1174	rVB	119	92	0.01%	0.001%
44	8.269	1174	1178	1181	rBV2	134	235	0.02%	0.003%
45	8.324	1181	1187	1201	rBV	131355	215427	22.54%	2.776%
46	8.574	1226	1228	1230	rBB	190	134	0.01%	0.002%
47	8.647	1234	1240	1261	rBV	493233	780262	81.62%	10.056%
48	8.952	1284	1290	1302	rBV	94932	142539	14.91%	1.837%
49	9.195	1327	1330	1331	rBV2	246	227	0.02%	0.003%
50	9.275	1337	1343	1348	rVB	5036	8411	0.88%	0.108%
51	9.384	1355	1361	1383	rBV	323469	495124	51.79%	6.381%
52	9.945	1451	1453	1457	rBV2	170	170	0.02%	0.002%
53	10.012	1463	1464	1465	rBV	210	117	0.01%	0.002%
54	10.055	1465	1471	1489	rBV	553003	770665	80.62%	9.932%
55	10.195	1492	1494	1496	rVB2	279	172	0.02%	0.002%
56	10.281	1507	1508	1510	rVB	251	120	0.01%	0.002%
57	10.305	1510	1512	1516	rBV3	381	514	0.05%	0.007%
58	10.543	1549	1551	1552	rVB	191	104	0.01%	0.001%
59	10.622	1562	1564	1566	rBV2	154	142	0.01%	0.002%
60	10.689	1574	1575	1578	rVB2	154	130	0.01%	0.002%
61	10.738	1581	1583	1586	rVB2	137	149	0.02%	0.002%
62	10.762	1586	1587	1590	rBV2	206	181	0.02%	0.002%
63	10.793	1590	1592	1593	rBV2	100	101	0.01%	0.001%
64	10.957	1617	1619	1623	rVB	133	141	0.01%	0.002%
65	11.085	1637	1640	1647	rVB4	891	1611	0.17%	0.021%
66	11.146	1647	1650	1652	rBV2	105	172	0.02%	0.002%
67	11.189	1652	1657	1668	rBV	406949	524083	54.82%	6.754%
68	11.311	1673	1677	1682	rVV	6536	8968	0.94%	0.116%
69	11.409	1691	1693	1697	rBV	204	177	0.02%	0.002%
70	11.476	1702	1704	1707	rBV2	111	134	0.01%	0.002%
71	11.524	1710	1712	1716	rVB2	119	160	0.02%	0.002%
72	11.567	1716	1719	1721	rBV	145	177	0.02%	0.002%
73	11.689	1737	1739	1740	rBV	161	138	0.01%	0.002%
74	11.707	1740	1742	1744	rVV	205	176	0.02%	0.002%
75	11.957	1780	1783	1784	rBV	161	152	0.02%	0.002%
76	11.975	1784	1786	1788	rVV	446	403	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041524\
 Data File : VX041074.D
 Acq On : 15 Apr 2024 13:35
 Operator : JC/MD
 Sample : P2098-03 10X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0RJ5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M

Title : VOC Analysis

77	12.018	1788	1793	1807	rVV	605176	783067	81.92%	10.092%
78	12.317	1837	1842	1857	rBV	616283	790970	82.74%	10.194%
79	12.542	1877	1879	1882	rBV2	166	119	0.01%	0.002%
80	12.762	1911	1915	1920	rBV2	969	1380	0.14%	0.018%
81	13.061	1963	1964	1967	rVV2	193	165	0.02%	0.002%
82	13.122	1970	1974	1977	rVV4	235	327	0.03%	0.004%
83	13.219	1989	1990	1992	rVB	213	101	0.01%	0.001%
84	13.256	1995	1996	2000	rBV2	171	169	0.02%	0.002%
85	13.335	2008	2009	2010	rBV	192	97	0.01%	0.001%
86	13.414	2021	2022	2025	rBV	150	102	0.01%	0.001%
87	13.439	2025	2026	2029	rVB	177	153	0.02%	0.002%
88	13.469	2029	2031	2034	rBV2	131	139	0.01%	0.002%
89	13.567	2045	2047	2048	rVV	201	105	0.01%	0.001%
90	13.591	2048	2051	2056	rVV4	1070	1492	0.16%	0.019%
91	13.719	2070	2072	2074	rVB2	186	127	0.01%	0.002%
92	13.786	2080	2083	2086	rVV2	297	424	0.04%	0.005%
93	13.914	2102	2104	2106	rVB	148	101	0.01%	0.001%
94	13.963	2106	2112	2117	rBV3	529	872	0.09%	0.011%
95	14.018	2119	2121	2122	rBV2	167	104	0.01%	0.001%
96	14.115	2135	2137	2138	rBV2	269	216	0.02%	0.003%
97	14.268	2160	2162	2165	rVB	262	257	0.03%	0.003%
98	14.292	2165	2166	2167	rBV	207	144	0.02%	0.002%
99	14.902	2264	2266	2268	rBV	295	224	0.02%	0.003%
100	16.347	2501	2503	2504	rBV2	430	215	0.02%	0.003%




Sum of corrected areas: 7759105

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041524\
Data File : VX041074.D
Acq On : 15 Apr 2024 13:35
Operator : JC/MD
Sample : P2098-03 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0RJ5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

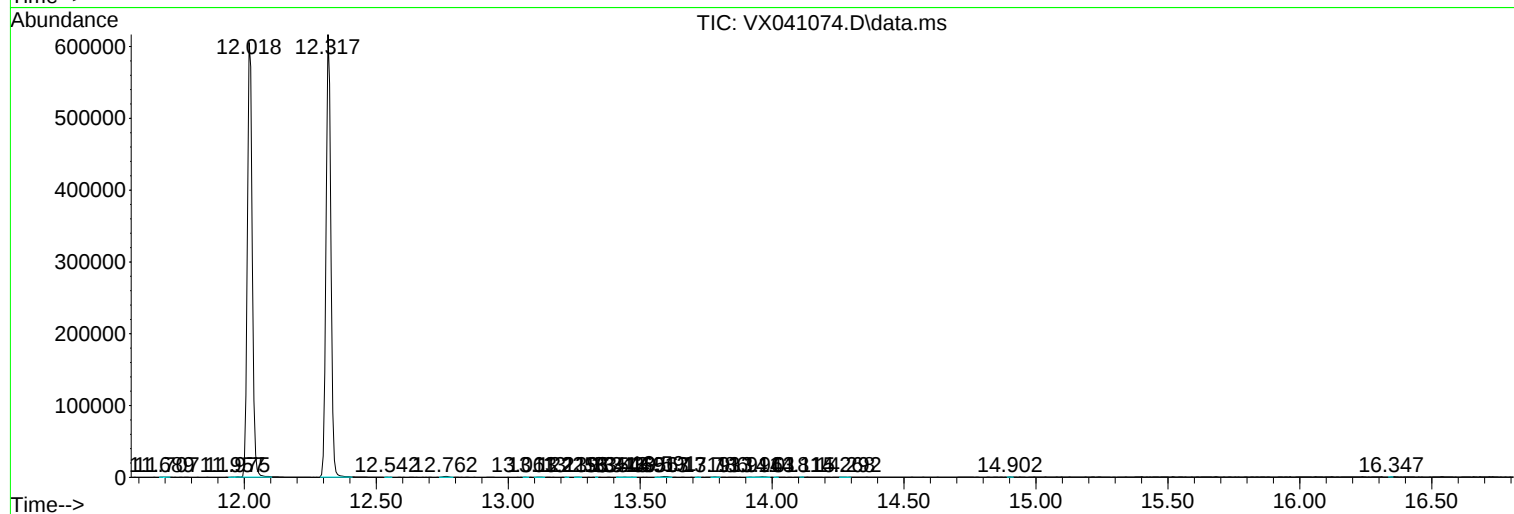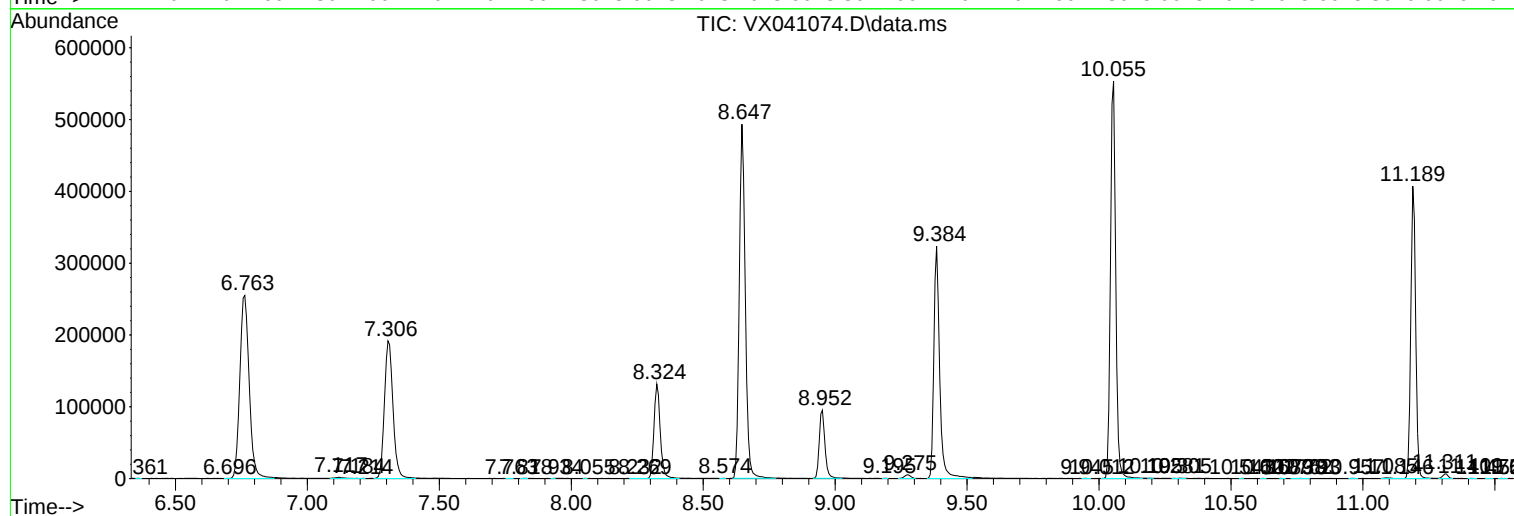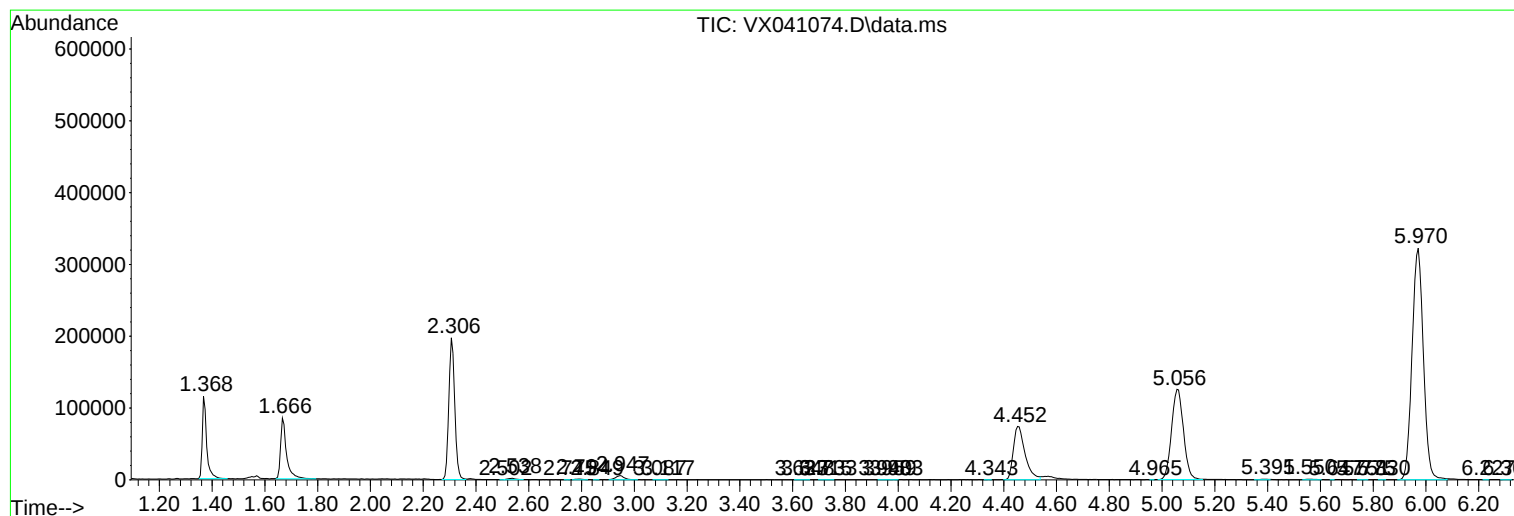

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041524\
Data File : VX041074.D
Acq On : 15 Apr 2024 13:35
Operator : JC/MD
Sample : P2098-03 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0RJ5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM041024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041524\
Data File : VX041074.D
Acq On : 15 Apr 2024 13:35
Operator : JC/MD
Sample : P2098-03 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0RJ5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------