

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041524\
 Data File : VX041075.D
 Acq On : 15 Apr 2024 13:58
 Operator : JC/MD
 Sample : P2098-04DL 1000X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MC0R55DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M

Title : VOC Analysis

Signal : TIC: VX041075.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.367	43	46	61	rVB	108104	127286	12.71%	1.583%
2	1.672	91	96	114	rVB	85605	129519	12.93%	1.611%
3	2.306	194	200	215	rBV	191003	298741	29.82%	3.715%
4	2.532	232	237	242	rVB2	786	1378	0.14%	0.017%
5	2.703	263	265	267	rBV2	131	137	0.01%	0.002%
6	2.788	274	279	285	rVB2	1011	1801	0.18%	0.022%
7	2.867	290	292	294	rVB	171	112	0.01%	0.001%
8	2.886	294	295	297	rBV2	157	104	0.01%	0.001%
9	2.946	298	305	313	rVB	2273	5250	0.52%	0.065%
10	3.032	315	319	322	rVB2	136	175	0.02%	0.002%
11	3.154	336	339	340	rVB2	145	117	0.01%	0.001%
12	3.172	340	342	346	rBV2	177	226	0.02%	0.003%
13	3.233	350	352	355	rBV2	135	235	0.02%	0.003%
14	3.318	364	366	368	rBV2	114	116	0.01%	0.001%
15	3.355	370	372	375	rVB2	178	188	0.02%	0.002%
16	3.385	375	377	378	rVB	228	133	0.01%	0.002%
17	3.422	381	383	385	rBV2	153	166	0.02%	0.002%
18	3.770	439	440	443	rVB	186	120	0.01%	0.001%
19	3.849	452	453	456	rBV	156	124	0.01%	0.002%
20	3.934	465	467	470	rVB	103	111	0.01%	0.001%
21	4.105	494	495	501	rVB2	145	146	0.01%	0.002%
22	4.257	519	520	523	rBV2	151	154	0.02%	0.002%
23	4.318	528	530	533	rVB	150	144	0.01%	0.002%
24	4.452	544	552	568	rBV	71241	222479	22.21%	2.767%
25	4.757	600	602	606	rBV3	261	301	0.03%	0.004%
26	4.818	611	612	615	rBV	173	205	0.02%	0.003%
27	4.849	615	617	621	rVB2	324	289	0.03%	0.004%
28	5.056	638	651	669	rBV	125148	385106	38.44%	4.789%
29	5.300	689	691	692	rVB2	346	203	0.02%	0.003%
30	5.330	694	696	698	rBV2	160	142	0.01%	0.002%
31	5.385	698	705	708	rBV2	649	1407	0.14%	0.017%
32	5.562	726	734	742	rVB3	856	2278	0.23%	0.028%
33	5.690	753	755	757	rVB2	224	143	0.01%	0.002%
34	5.970	789	801	807	rBV2	318386	946361	94.47%	11.768%
35	6.403	871	872	874	rBV	146	105	0.01%	0.001%
36	6.421	874	875	878	rVB2	167	123	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041524\
 Data File : VX041075.D
 Acq On : 15 Apr 2024 13:58
 Operator : JC/MD
 Sample : P2098-04DL 1000X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MC0R55DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
 Title : VOC Analysis

37	6.598	902	904	908	rVB2	159	164	0.02%	0.002%
38	6.763	921	931	947	rBV	240309	577019	57.60%	7.175%
39	7.055	978	979	983	rVV3	177	177	0.02%	0.002%
40	7.116	983	989	998	rVB4	1917	4731	0.47%	0.059%
41	7.305	1011	1020	1040	rBV	191750	422380	42.16%	5.252%
42	7.586	1065	1066	1071	rVB2	207	214	0.02%	0.003%
43	7.622	1071	1072	1073	rBV	219	117	0.01%	0.001%
44	7.757	1092	1094	1098	rBV2	125	228	0.02%	0.003%
45	7.909	1117	1119	1121	rBV2	117	105	0.01%	0.001%
46	7.952	1124	1126	1134	rVB2	314	567	0.06%	0.007%
47	8.110	1150	1152	1155	rVV2	114	117	0.01%	0.001%
48	8.238	1171	1173	1177	rBV2	111	133	0.01%	0.002%
49	8.324	1181	1187	1202	rBV	127881	211639	21.13%	2.632%
50	8.592	1229	1231	1234	rBV2	126	169	0.02%	0.002%
51	8.647	1234	1240	1258	rBV	483350	761650	76.03%	9.471%
52	8.951	1284	1290	1301	rBV	93550	139659	13.94%	1.737%
53	9.140	1318	1321	1323	rBV2	96	106	0.01%	0.001%
54	9.159	1323	1324	1327	rVB	214	113	0.01%	0.001%
55	9.226	1332	1335	1337	rBV	154	188	0.02%	0.002%
56	9.275	1340	1343	1347	rVB2	771	908	0.09%	0.011%
57	9.311	1347	1349	1350	rBV	177	112	0.01%	0.001%
58	9.384	1356	1361	1374	rBV	312447	474987	47.41%	5.907%
59	9.701	1410	1413	1418	rVB4	482	733	0.07%	0.009%
60	9.890	1443	1444	1446	rBV	166	117	0.01%	0.001%
61	9.909	1446	1447	1449	rVB2	172	123	0.01%	0.002%
62	10.055	1465	1471	1473	rBV	543344	839975	83.85%	10.445%
63	10.299	1508	1511	1513	rBV2	223	327	0.03%	0.004%
64	10.457	1533	1537	1538	rBV2	140	175	0.02%	0.002%
65	10.774	1587	1589	1592	rBV2	130	143	0.01%	0.002%
66	10.835	1597	1599	1601	rBV2	147	172	0.02%	0.002%
67	11.006	1626	1627	1630	rBV2	109	121	0.01%	0.002%
68	11.085	1638	1640	1646	rVB3	916	1498	0.15%	0.019%
69	11.189	1652	1657	1669	rBV	403820	514263	51.33%	6.395%
70	11.311	1674	1677	1681	rVB2	812	1078	0.11%	0.013%
71	11.372	1684	1687	1692	rVB	133	215	0.02%	0.003%
72	11.671	1731	1736	1738	rBV2	177	277	0.03%	0.003%
73	11.707	1740	1742	1745	rVV2	299	286	0.03%	0.004%
74	11.969	1781	1785	1788	rBV2	7163	9325	0.93%	0.116%
75	12.018	1788	1793	1811	rVB2	589297	1001780	100.00%	12.457%
76	12.219	1823	1826	1827	rBV2	175	209	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041524\
 Data File : VX041075.D
 Acq On : 15 Apr 2024 13:58
 Operator : JC/MD
 Sample : P2098-04DL 1000X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MC0R55DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM041024WMA.M
 Title : VOC Analysis

77	12.317	1837	1842	1863	rBV2	633715	935118	93.35%	11.628%
78	12.494	1869	1871	1873	rVB	270	167	0.02%	0.002%
79	12.530	1873	1877	1878	rVB	219	181	0.02%	0.002%
80	12.628	1889	1893	1894	rBV2	137	181	0.02%	0.002%
81	12.683	1901	1902	1904	rBV	121	109	0.01%	0.001%
82	12.762	1912	1915	1918	rVB3	333	468	0.05%	0.006%
83	12.939	1943	1944	1946	rVB	218	110	0.01%	0.001%
84	12.957	1946	1947	1950	rBV2	221	274	0.03%	0.003%
85	13.036	1958	1960	1963	rVB2	167	129	0.01%	0.002%
86	13.121	1970	1974	1977	rVB2	419	545	0.05%	0.007%
87	13.250	1993	1995	1996	rBV	172	115	0.01%	0.001%
88	13.378	2014	2016	2019	rVB2	119	112	0.01%	0.001%
89	13.591	2046	2051	2060	rVB	6290	8716	0.87%	0.108%
90	13.695	2065	2068	2078	rBV2	242	565	0.06%	0.007%
91	13.780	2078	2082	2086	rBV3	346	602	0.06%	0.007%
92	13.859	2093	2095	2097	rBV2	150	151	0.02%	0.002%
93	13.969	2110	2113	2116	rBV4	618	652	0.07%	0.008%
94	14.121	2136	2138	2141	rVB	268	282	0.03%	0.004%
95	14.322	2168	2171	2173	rBV3	139	206	0.02%	0.003%
96	14.426	2186	2188	2191	rBV2	332	283	0.03%	0.004%
97	14.585	2212	2214	2218	rVB2	255	228	0.02%	0.003%
98	14.621	2218	2220	2223	rBV2	232	262	0.03%	0.003%
99	14.792	2246	2248	2250	rVB	245	121	0.01%	0.002%
100	14.816	2250	2252	2253	rBV	284	155	0.02%	0.002%




Sum of corrected areas: 8041657

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041524\
Data File : VX041075.D
Acq On : 15 Apr 2024 13:58
Operator : JC/MD
Sample : P2098-04DL 1000X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MC0R55DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

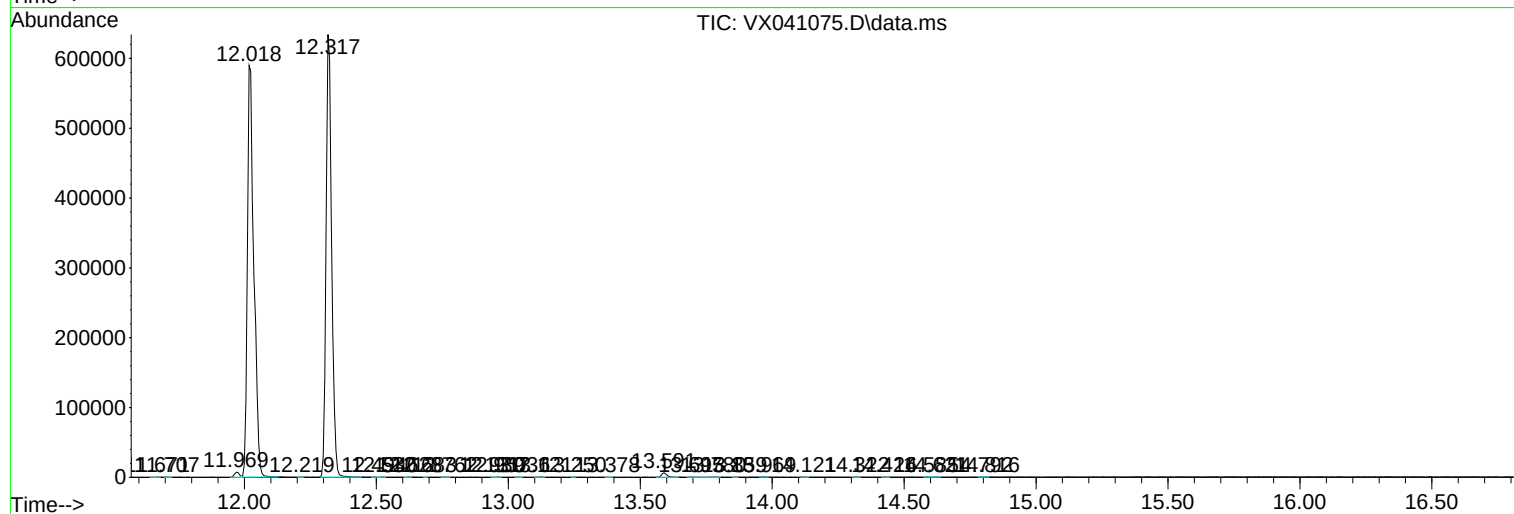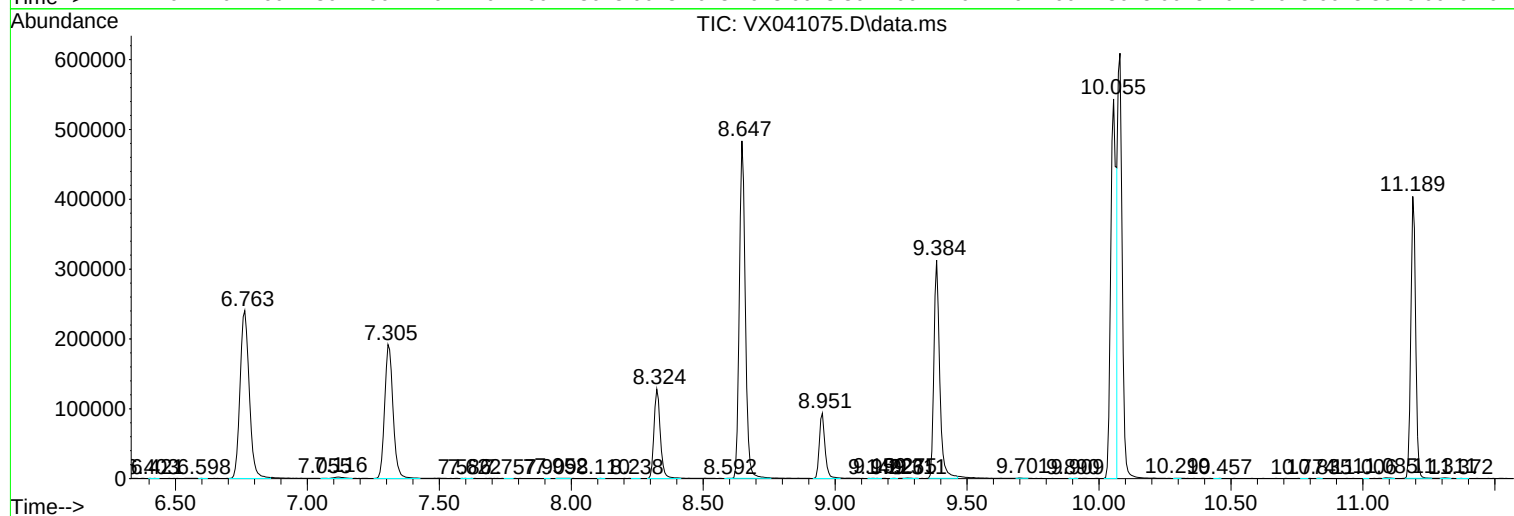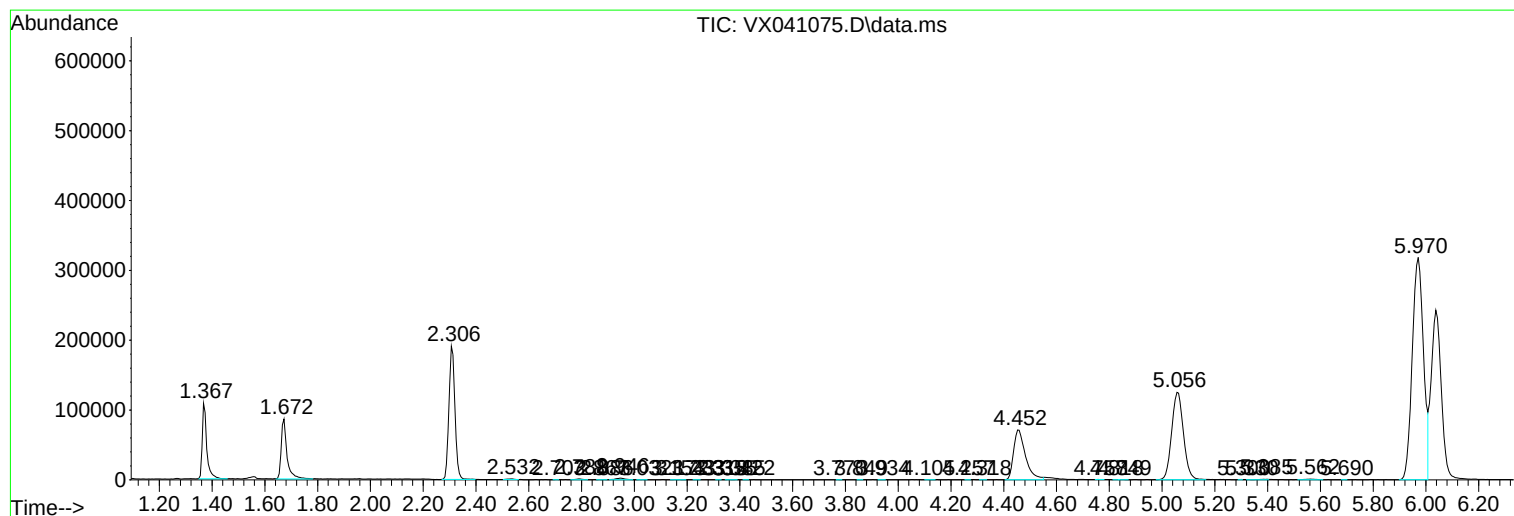

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041524\
Data File : VX041075.D
Acq On : 15 Apr 2024 13:58
Operator : JC/MD
Sample : P2098-04DL 1000X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MC0R55DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM041024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041524\
Data File : VX041075.D
Acq On : 15 Apr 2024 13:58
Operator : JC/MD
Sample : P2098-04DL 1000X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MC0R55DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
