

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041524\
 Data File : VX041086.D
 Acq On : 15 Apr 2024 18:11
 Operator : JC/MD
 Sample : P2098-16
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
 Title : VOC Analysis

Signal : TIC: VX041086.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.264	25	29	33	rBV3	1584	2649	0.29%	0.036%
2	1.368	43	46	58	rBV	106888	121106	13.34%	1.668%
3	1.672	91	96	114	rBV	80619	123391	13.59%	1.699%
4	2.306	194	200	210	rBV	184814	284697	31.36%	3.920%
5	2.538	234	238	244	rVB3	1499	2489	0.27%	0.034%
6	2.654	254	257	259	rBV2	139	195	0.02%	0.003%
7	2.794	275	280	287	rVB2	1847	3417	0.38%	0.047%
8	2.953	301	306	308	rBV3	254	361	0.04%	0.005%
9	3.014	313	316	318	rBV2	146	181	0.02%	0.002%
10	3.148	334	338	339	rBV2	153	121	0.01%	0.002%
11	3.166	339	341	343	rVB2	133	129	0.01%	0.002%
12	3.331	365	368	371	rBV2	114	192	0.02%	0.003%
13	3.690	426	427	431	rVB	161	134	0.01%	0.002%
14	3.751	434	437	438	rBV2	187	180	0.02%	0.002%
15	3.922	462	465	468	rBV2	92	137	0.02%	0.002%
16	4.160	501	504	506	rBV	214	196	0.02%	0.003%
17	4.312	527	529	530	rVB	218	141	0.02%	0.002%
18	4.330	530	532	533	rBV	139	139	0.02%	0.002%
19	4.458	544	553	575	rBV	70226	221145	24.36%	3.045%
20	4.843	613	616	619	rBV3	153	179	0.02%	0.002%
21	4.873	619	621	623	rBV2	176	132	0.01%	0.002%
22	4.916	626	628	630	rVB2	225	133	0.01%	0.002%
23	5.056	639	651	669	rBV	121894	372022	40.97%	5.123%
24	5.288	686	689	690	rBV2	203	204	0.02%	0.003%
25	5.349	697	699	702	rVB2	110	118	0.01%	0.002%
26	5.385	702	705	706	rBV2	420	477	0.05%	0.007%
27	5.513	724	726	729	rBV	185	136	0.01%	0.002%
28	5.550	729	732	733	rBV	406	503	0.06%	0.007%
29	5.684	750	754	758	rVB2	130	208	0.02%	0.003%
30	5.970	789	801	823	rBV2	303118	907926	100.00%	12.502%
31	6.300	853	855	858	rBV	149	139	0.02%	0.002%
32	6.428	872	876	878	rBV2	241	225	0.02%	0.003%
33	6.501	885	888	890	rBV2	191	165	0.02%	0.002%
34	6.550	893	896	898	rBV2	206	260	0.03%	0.004%
35	6.763	921	931	947	rBV	235211	558015	61.46%	7.684%
36	7.123	983	990	996	rBV4	1351	2891	0.32%	0.040%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041524\
 Data File : VX041086.D
 Acq On : 15 Apr 2024 18:11
 Operator : JC/MD
 Sample : P2098-16
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
 Title : VOC Analysis

37	7.171	996	998	1001	rVB3	271	249	0.03%	0.003%
38	7.202	1001	1003	1006	rBV	125	171	0.02%	0.002%
39	7.306	1011	1020	1037	rBV	185650	409337	45.08%	5.637%
40	7.671	1075	1080	1081	rBV	133	195	0.02%	0.003%
41	7.757	1093	1094	1097	rVB2	151	127	0.01%	0.002%
42	7.842	1106	1108	1111	rBV2	176	189	0.02%	0.003%
43	7.921	1120	1121	1124	rBV2	154	143	0.02%	0.002%
44	7.946	1124	1125	1128	rBV2	189	208	0.02%	0.003%
45	8.019	1136	1137	1140	rBV2	125	143	0.02%	0.002%
46	8.116	1151	1153	1155	rVV	184	133	0.01%	0.002%
47	8.238	1171	1173	1176	rVB2	167	159	0.02%	0.002%
48	8.281	1176	1180	1181	rBV	119	174	0.02%	0.002%
49	8.324	1181	1187	1201	rBV	118924	198928	21.91%	2.739%
50	8.507	1215	1217	1222	rVB5	302	447	0.05%	0.006%
51	8.574	1226	1228	1231	rBV2	161	172	0.02%	0.002%
52	8.647	1234	1240	1260	rBV	455394	737194	81.20%	10.151%
53	8.897	1280	1281	1285	rBV2	155	158	0.02%	0.002%
54	8.952	1285	1290	1301	rBV	88456	132521	14.60%	1.825%
55	9.092	1312	1313	1317	rVB2	264	263	0.03%	0.004%
56	9.275	1339	1343	1347	rVV	1216	1524	0.17%	0.021%
57	9.384	1356	1361	1385	rBV2	311770	476545	52.49%	6.562%
58	9.732	1415	1418	1419	rBV2	203	212	0.02%	0.003%
59	9.817	1429	1432	1435	rVV2	223	274	0.03%	0.004%
60	10.055	1465	1471	1487	rBV	501162	695059	76.55%	9.571%
61	10.268	1504	1506	1510	rBV2	185	263	0.03%	0.004%
62	10.305	1510	1512	1513	rBV3	177	142	0.02%	0.002%
63	10.470	1536	1539	1544	rBV2	148	262	0.03%	0.004%
64	10.720	1576	1580	1585	rBV2	174	268	0.03%	0.004%
65	11.024	1626	1630	1635	rBV2	154	310	0.03%	0.004%
66	11.098	1638	1642	1645	rBV3	762	1118	0.12%	0.015%
67	11.189	1652	1657	1671	rBV	391939	507836	55.93%	6.993%
68	11.311	1673	1677	1683	rVV	1966	2546	0.28%	0.035%
69	11.445	1696	1699	1701	rBV	150	179	0.02%	0.002%
70	11.488	1705	1706	1709	rVB	200	159	0.02%	0.002%
71	11.585	1720	1722	1725	rVB2	214	189	0.02%	0.003%
72	11.616	1725	1727	1731	rBV2	127	165	0.02%	0.002%
73	11.713	1740	1743	1747	rVB3	274	320	0.04%	0.004%
74	11.908	1774	1775	1777	rBV	170	118	0.01%	0.002%
75	11.975	1781	1786	1788	rBV3	345	524	0.06%	0.007%
76	12.024	1788	1794	1806	rBV	565934	719544	79.25%	9.908%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041524\
 Data File : VX041086.D
 Acq On : 15 Apr 2024 18:11
 Operator : JC/MD
 Sample : P2098-16
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM041024WMA.M
 Title : VOC Analysis

77	12.317	1837	1842	1851	rBV	577761	761788	83.90%	10.490%
78	12.597	1886	1888	1889	rBV	172	144	0.02%	0.002%
79	12.658	1894	1898	1899	rBV2	172	152	0.02%	0.002%
80	12.695	1902	1904	1905	rBV2	193	128	0.01%	0.002%
81	13.079	1966	1967	1970	rBV2	146	123	0.01%	0.002%
82	13.109	1970	1972	1975	rVV2	119	170	0.02%	0.002%
83	13.134	1975	1976	1980	rVV2	171	158	0.02%	0.002%
84	13.341	2008	2010	2011	rVV	305	145	0.02%	0.002%
85	13.384	2015	2017	2022	rVB2	160	185	0.02%	0.003%
86	13.432	2022	2025	2028	rBV2	146	193	0.02%	0.003%
87	13.475	2030	2032	2034	rVB	175	128	0.01%	0.002%
88	13.554	2043	2045	2048	rVB2	281	203	0.02%	0.003%
89	13.591	2048	2051	2060	rVB5	1701	2630	0.29%	0.036%
90	13.853	2092	2094	2096	rBV2	158	130	0.01%	0.002%
91	13.908	2101	2103	2105	rBV2	147	138	0.02%	0.002%
92	13.969	2108	2113	2117	rBV3	455	580	0.06%	0.008%
93	14.024	2120	2122	2124	rBV2	192	157	0.02%	0.002%
94	14.158	2140	2144	2146	rBV2	150	214	0.02%	0.003%
95	14.182	2146	2148	2149	rBV	206	118	0.01%	0.002%
96	14.213	2149	2153	2155	rVB2	195	266	0.03%	0.004%
97	14.316	2167	2170	2174	rBV3	164	250	0.03%	0.003%
98	14.463	2190	2194	2195	rBV3	217	270	0.03%	0.004%
99	14.597	2214	2216	2220	rVB3	268	269	0.03%	0.004%
100	15.828	2416	2418	2420	rBV2	357	341	0.04%	0.005%




Sum of corrected areas: 7262081

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041524\
Data File : VX041086.D
Acq On : 15 Apr 2024 18:11
Operator : JC/MD
Sample : P2098-16
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

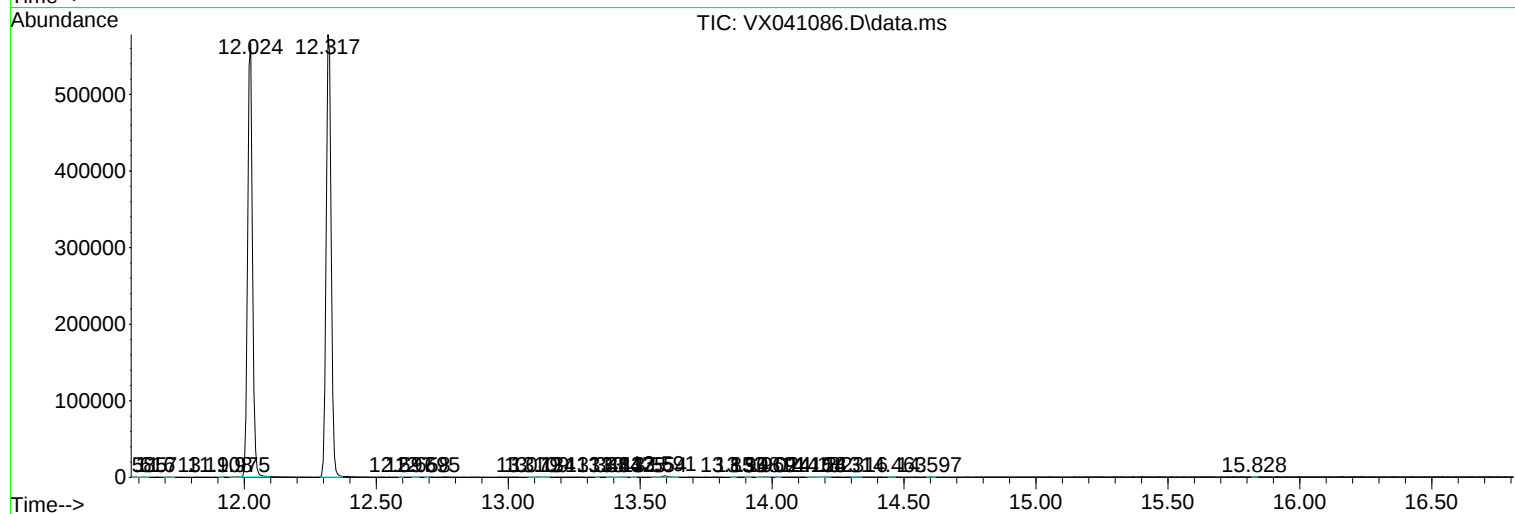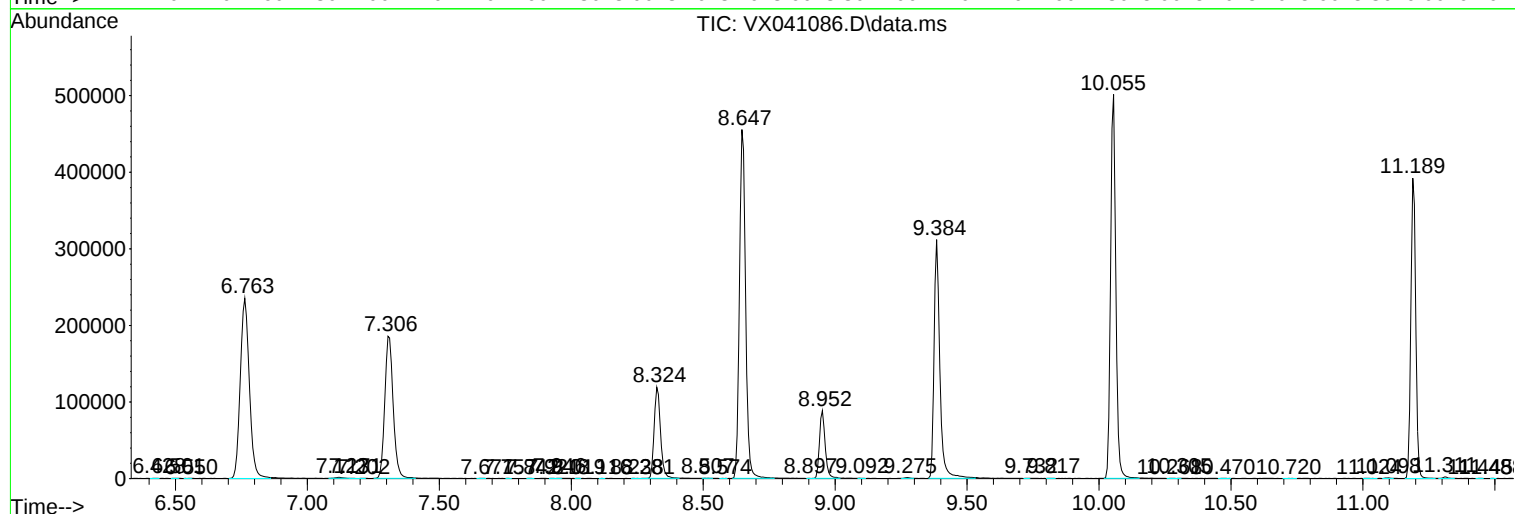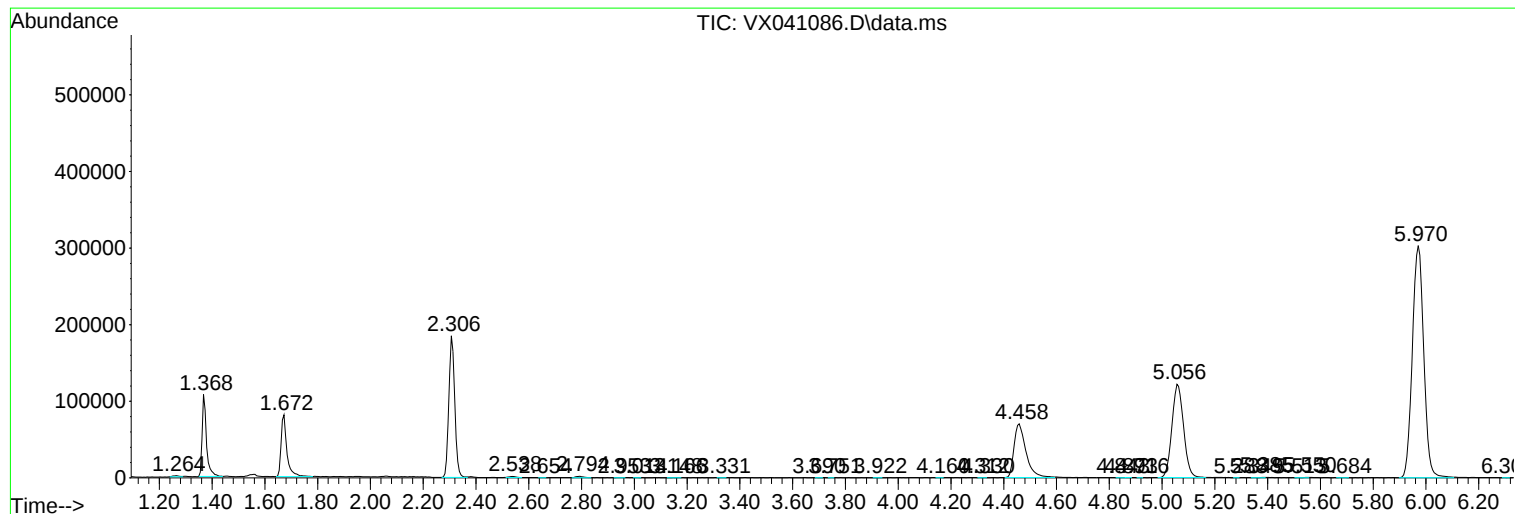

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041524\
Data File : VX041086.D
Acq On : 15 Apr 2024 18:11
Operator : JC/MD
Sample : P2098-16
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM041024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041524\
Data File : VX041086.D
Acq On : 15 Apr 2024 18:11
Operator : JC/MD
Sample : P2098-16
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
