
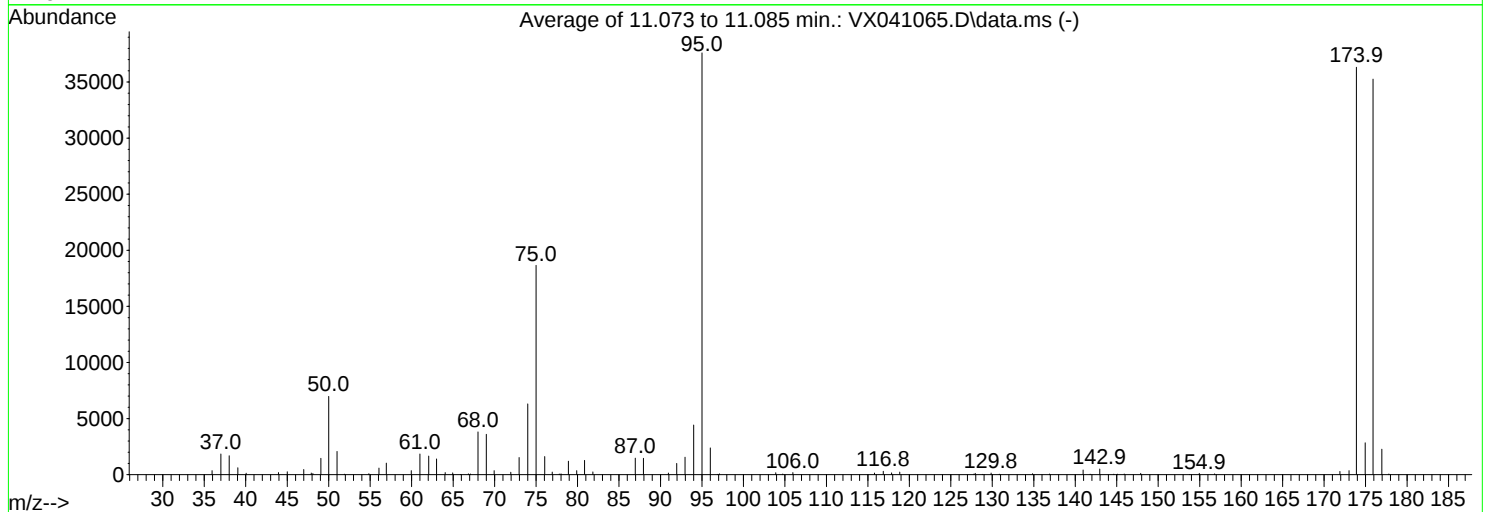


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041524\
Data File : VX041065.D
Acq On : 15 Apr 2024 09:00
Operator : JC/MD
Sample : BFB672
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB672

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM041024WMA.M
Title : VOC Analysis
Last Update : Tue Apr 16 02:47:54 2024

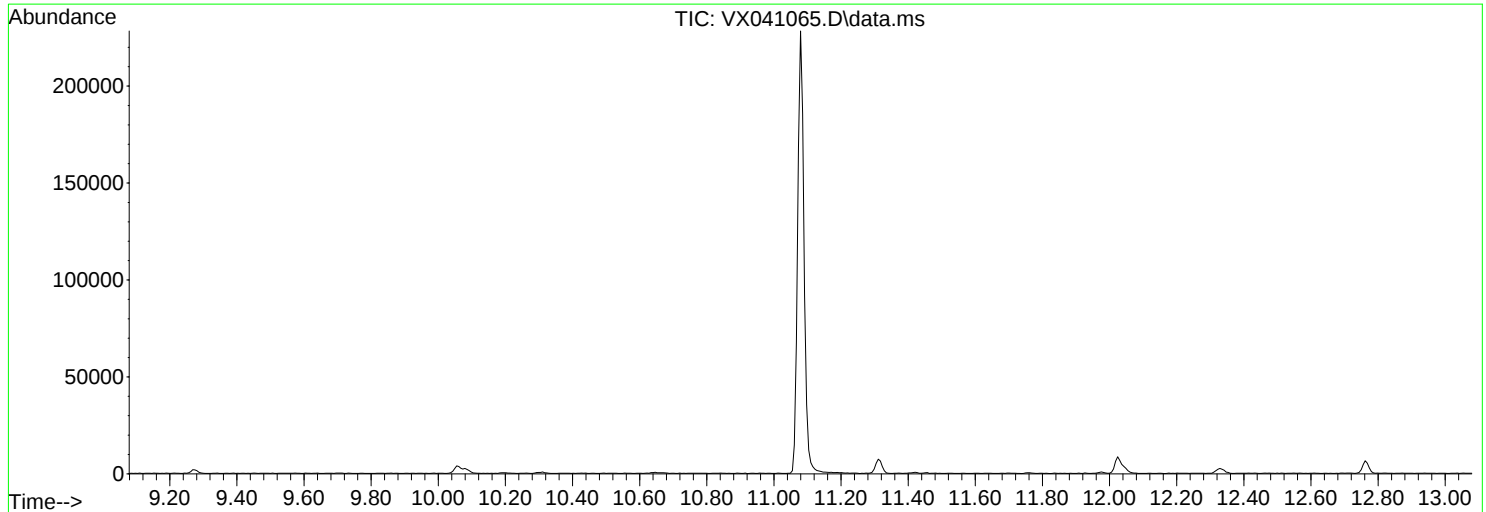

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1633

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.6	6979	PASS
75	95	30	80	49.6	18653	PASS
95	95	100	100	100.0	37605	PASS
96	95	5	9	6.3	2379	PASS
173	174	0.00	2	1.0	357	PASS
174	95	50	120	96.6	36323	PASS
175	174	5	9	7.8	2836	PASS
176	174	95	101	97.1	35261	PASS
177	176	5	9	6.4	2268	PASS

m/z	Abundance
39.90	208.0
44.00	135.0

Instrument :
MSVOA_X
ClientSampleId :
BFB672

m/z	Abundance
36.00	319.0
37.00	1756.0
38.00	1752.0
39.10	576.0
39.90	196.0
44.00	239.0
45.00	311.0
46.90	445.0
47.90	246.0
49.00	1405.0
50.00	6578.0
51.00	2012.0
51.90	93.0
54.90	113.0
56.10	567.0
56.90	959.0
60.00	394.0
61.00	1821.0
62.00	1682.0
63.00	1125.0
64.10	284.0
65.00	135.0
66.90	135.0
68.00	3481.0
69.00	3345.0
70.00	364.0
72.00	196.0
73.00	1419.0
74.00	6042.0
75.00	17080.0
76.10	1628.0
76.90	235.0
77.80	165.0
78.90	1144.0
79.90	331.0
80.80	1187.0
81.90	237.0
87.10	1492.0
87.90	1393.0
91.00	150.0
91.90	1018.0
93.00	1507.0
94.00	3956.0
95.00	34136.0
96.00	2328.0
96.90	109.0
103.80	158.0
104.70	55.0
106.00	178.0
115.80	108.0
116.80	248.0
117.80	122.0
118.80	124.0
127.80	163.0
129.80	140.0
134.90	93.0
137.00	52.0
141.00	330.0
141.80	71.0
142.90	448.0
145.10	55.0
147.80	111.0
155.00	97.0
171.90	241.0
173.90	27976.0
174.90	2139.0
175.90	27632.0
176.90	1930.0

Instrument :
MSVOA_X
ClientSampleId :
BFB672

m/z	Abundance
35.90	423.0
37.00	2330.0
38.00	1926.0
39.10	711.0
40.10	196.0
43.90	275.0
45.00	309.0
47.00	544.0
48.10	308.0
49.10	1730.0
50.00	8561.0
51.00	2433.0
51.90	53.0
54.80	99.0
56.00	651.0
57.00	1209.0
60.00	315.0
61.00	2239.0
62.00	1970.0
63.00	1751.0
63.90	134.0
64.90	179.0
65.90	52.0
67.10	109.0
68.00	4407.0
69.00	4013.0
70.00	412.0
71.90	244.0
73.00	1786.0
74.00	7157.0
75.00	22096.0
76.00	1886.0
77.00	277.0
78.00	201.0
78.90	1409.0
79.90	431.0
80.90	1548.0
81.80	267.0
86.90	1640.0
88.00	1705.0
90.90	153.0
92.00	1050.0
92.90	1782.0
94.00	5064.0
95.00	44416.0
96.00	2791.0
97.10	134.0
103.90	227.0
104.80	102.0
105.90	231.0
115.80	176.0
116.90	376.0
117.90	185.0
118.90	351.0
128.00	139.0
128.80	65.0
129.90	179.0
130.80	67.0
134.80	75.0
136.90	66.0
140.90	504.0
141.80	75.0
142.90	629.0
144.70	90.0
145.10	89.0
145.90	107.0
147.90	165.0
153.80	59.0
154.90	122.0
156.80	71.0
171.90	320.0
173.00	529.0
173.90	42616.0
175.00	3383.0
175.90	41400.0
177.00	2538.0
177.80	103.0

Instrument :
MSVOA_X
ClientSampleId :
BFB672

m/z	Abundance
36.00	340.0
37.00	1438.0
38.00	1384.0
39.00	576.0
40.00	206.0
44.00	435.0
45.00	170.0
47.10	392.0
47.90	200.0
49.10	1224.0
50.00	5797.0
51.00	1754.0
54.90	61.0
56.00	532.0
57.00	914.0
59.90	360.0
61.00	1478.0
62.10	1331.0
63.00	1305.0
64.00	129.0
65.00	152.0
66.80	63.0
67.10	63.0
68.00	3517.0
69.00	3423.0
69.90	316.0
71.90	215.0
72.90	1369.0
74.00	5734.0
75.00	16784.0
76.00	1337.0
76.90	175.0
78.90	1053.0
79.90	292.0
80.90	1056.0
81.90	243.0
86.90	1264.0
88.00	1279.0
90.90	112.0
92.00	911.0
93.00	1391.0
94.00	4244.0
95.00	34264.0
96.00	2018.0
97.10	90.0
104.00	147.0
105.90	140.0
115.80	123.0
116.90	265.0
117.80	167.0
118.90	205.0
127.90	212.0
129.00	57.0
129.90	116.0
130.90	62.0
134.90	85.0
136.80	66.0
140.90	393.0
143.00	421.0
144.60	63.0
145.90	88.0
148.00	86.0
154.90	109.0
156.80	129.0
171.90	292.0
173.00	543.0
173.90	38376.0
175.00	2987.0
175.90	36752.0
176.90	2336.0
177.80	87.0

Instrument :
MSVOA_X
ClientSampleId :
BFB672