


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX041619\
 Data File : VX008974.D
 Acq On : 16 Apr 2019 09:21
 Operator : JC/SP
 Sample : BFB
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X041519W.M
 Title : SW846 8260
 Last Update : Wed Apr 17 06:47:58 2019

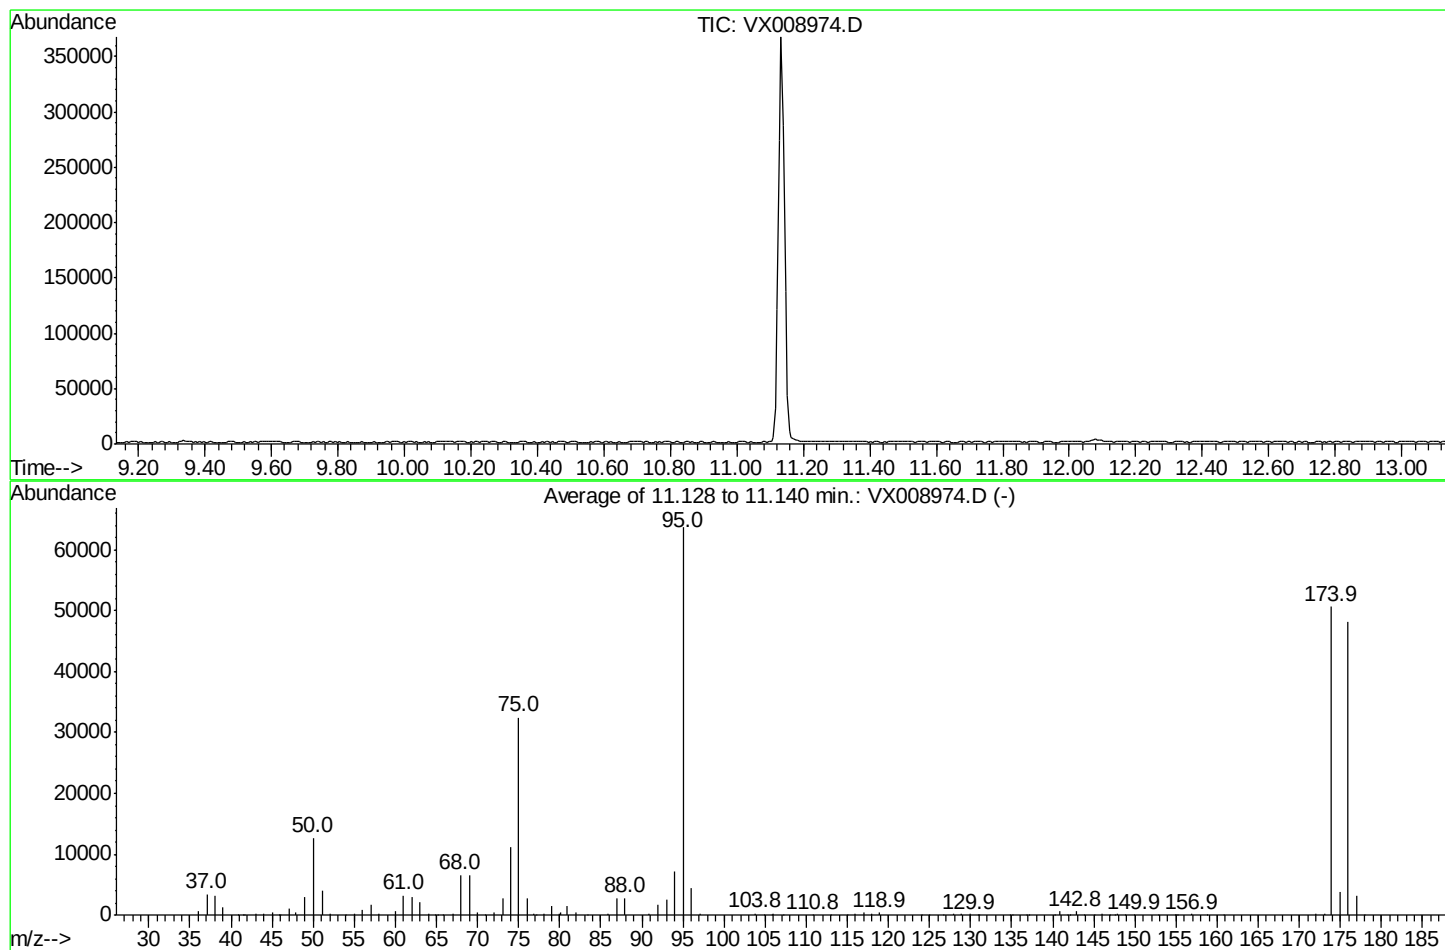

AutoFind: Scans 1636, 1637, 1638; Background Corrected with Scan 1630

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.0	12738	PASS
75	95	30	60	51.0	32501	PASS
95	95	100	100	100.0	63738	PASS
96	95	5	9	6.8	4340	PASS
173	174	0.00	2	0.6	282	PASS
174	95	50	100	79.6	50704	PASS
175	174	5	9	7.5	3792	PASS
176	174	95	101	95.1	48234	PASS
177	176	5	9	6.7	3230	PASS