


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX041620\
 Data File : VX015700.D
 Acq On : 16 Apr 2020 09:49
 Operator : JC/SP
 Sample : BFB
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X032720W.M
 Title : SW846 8260
 Last Update : Fri Mar 27 09:35:51 2020

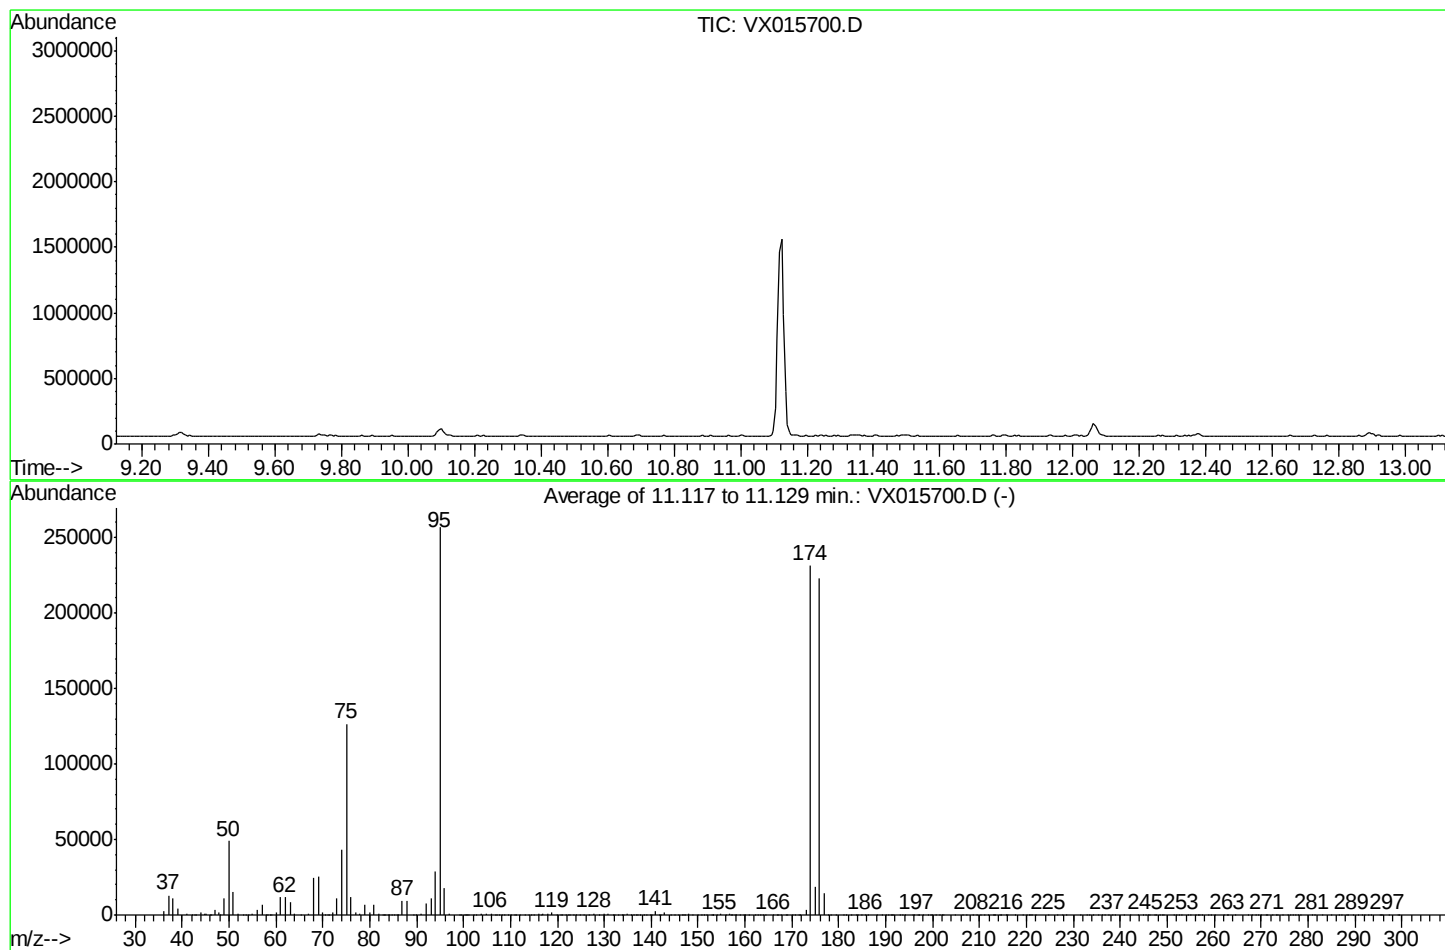

AutoFind: Scans 1678, 1679, 1680; Background Corrected with Scan 1669

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.0	48802	PASS
75	95	30	60	49.4	126791	PASS
95	95	100	100	100.0	256832	PASS
96	95	5	9	6.8	17540	PASS
173	174	0.00	2	1.3	3053	PASS
174	95	50	100	90.1	231422	PASS
175	174	5	9	8.1	18767	PASS
176	174	95	101	96.4	223189	PASS
177	176	5	9	6.5	14405	PASS