

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041624\
 Data File : VX041097.D
 Acq On : 16 Apr 2024 11:43
 Operator : JC/MD
 Sample : IBLK
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 IBLK

Quant Time: Apr 17 01:42:02 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X041624W.M
 Quant Title : SW846 8260
 QLast Update : Wed Apr 17 01:32:05 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.556	168	180193	50.000	ug/l	# 0.00
34) 1,4-Difluorobenzene	6.763	114	266648	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	261623	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	149137	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	95244	48.957	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	=	97.920%
35) Dibromofluoromethane	5.385	113	85868	48.206	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	96.420%
50) Toluene-d8	8.647	98	314287	50.373	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	=	100.740%
62) 4-Bromofluorobenzene	11.079	95	119046	50.263	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	100.520%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041624\
Data File : VX041097.D
Acq On : 16 Apr 2024 11:43
Operator : JC/MD
Sample : IBLK
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
IBLK

Quant Time: Apr 17 01:42:02 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X041624W.M
Quant Title : SW846 8260
QLast Update : Wed Apr 17 01:32:05 2024
Response via : Initial Calibration




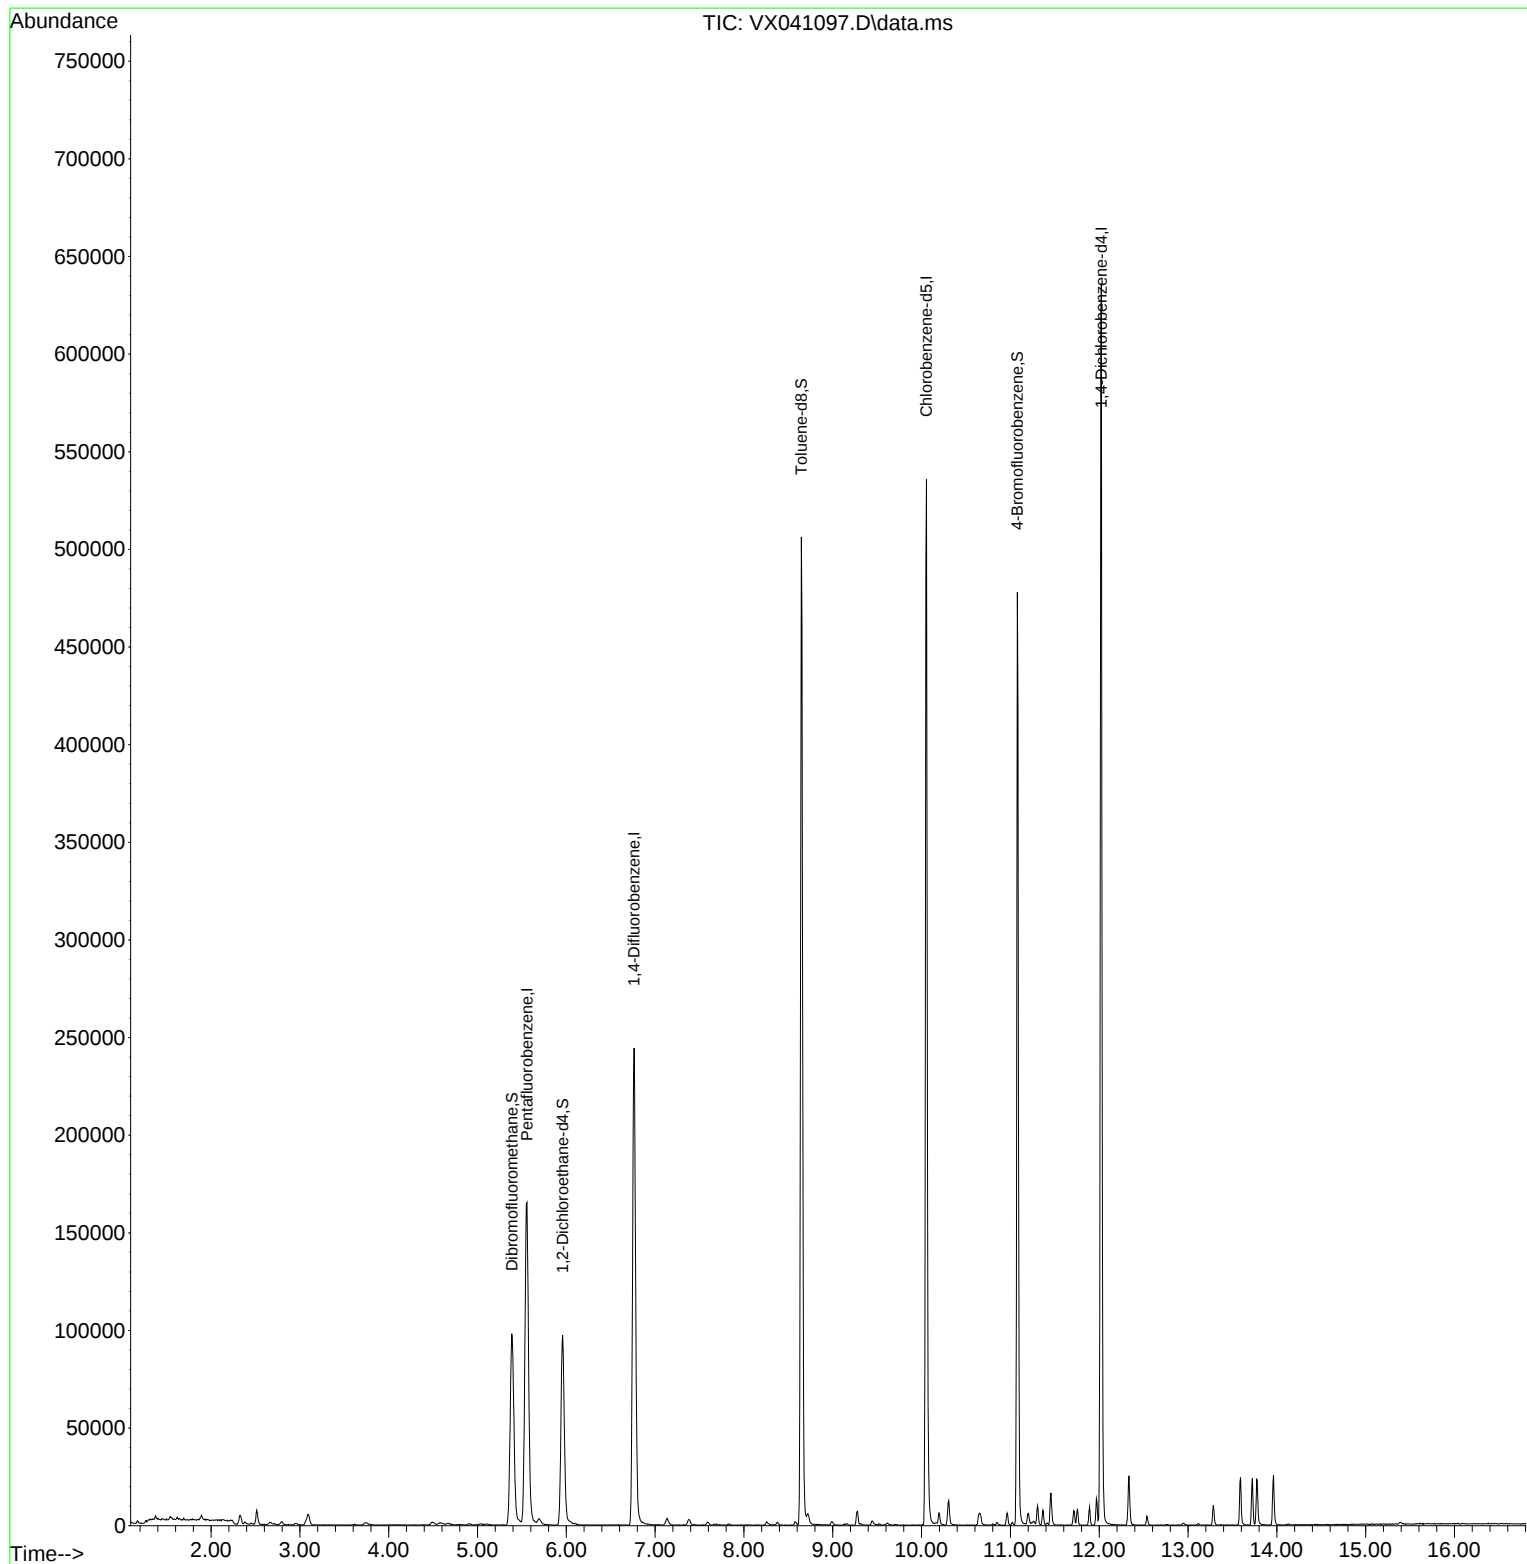


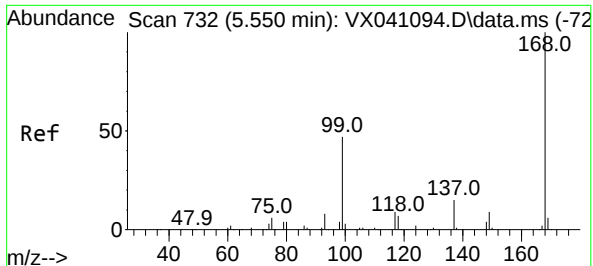

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.556 min Scan# 711
Delta R.T. 0.006 min
Lab File: VX041097.D
Acq: 16 Apr 2024 11:43




Instrument :
MSVOA_X
ClientSampleId :
IBLK


Tgt Ion:168 Resp: 180193
Ion Ratio Lower Upper
168 100
99 47.4 56.6 85.0#

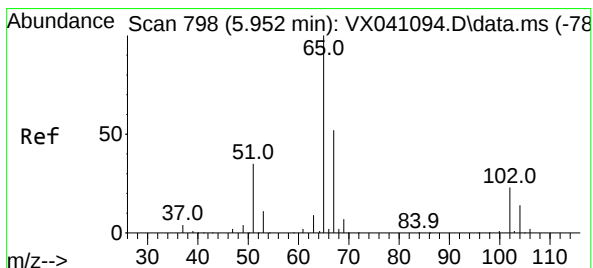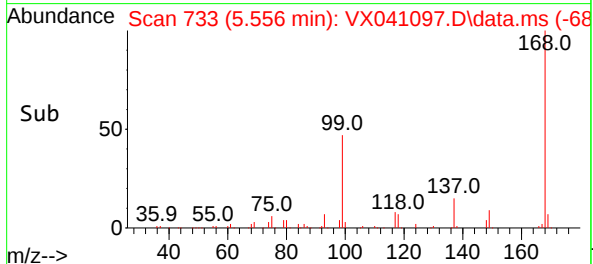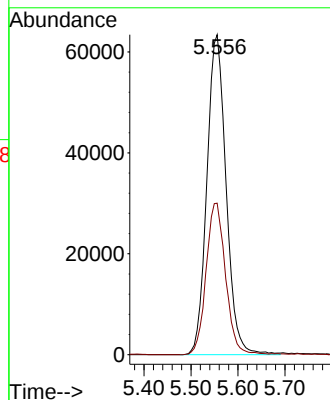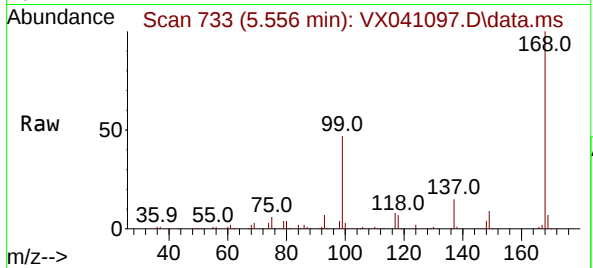

#33
1,2-Dichloroethane-d4
Concen: 48.957 ug/l
RT: 5.958 min Scan# 799
Delta R.T. 0.006 min
Lab File: VX041097.D
Acq: 16 Apr 2024 11:43

Tgt Ion: 65 Resp: 95244
Ion Ratio Lower Upper
65 100
67 51.5 0.0 100.2


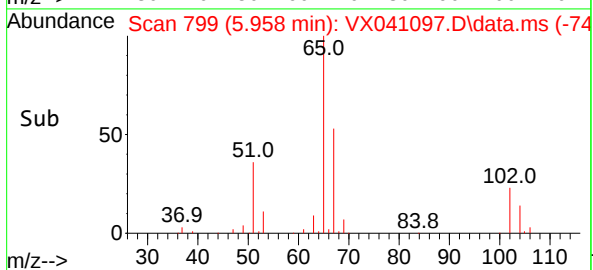
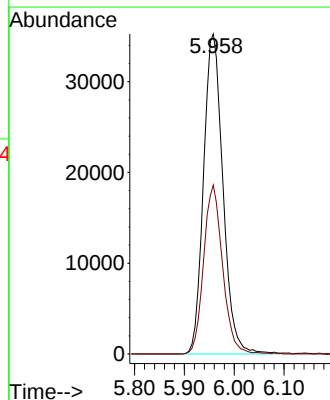
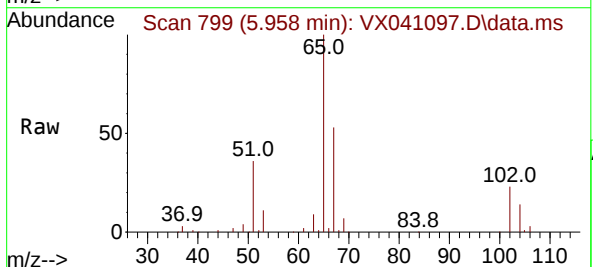


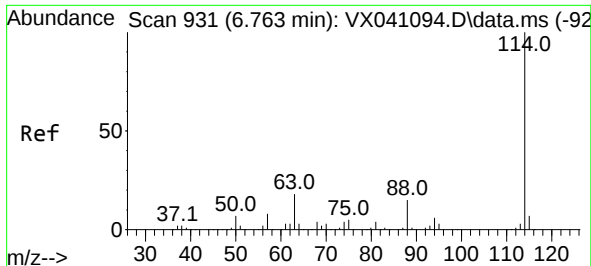

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.763 min Scan# 91
Delta R.T. -0.000 min
Lab File: VX041097.D
Acq: 16 Apr 2024 11:43




Instrument :
MSVOA_X
ClientSampleId :
IBLK


Tgt Ion:114 Resp: 266648
Ion Ratio Lower Upper
114 100
63 19.0 0.0 45.0
88 15.8 0.0 36.6

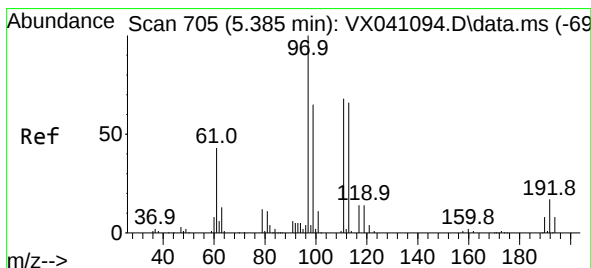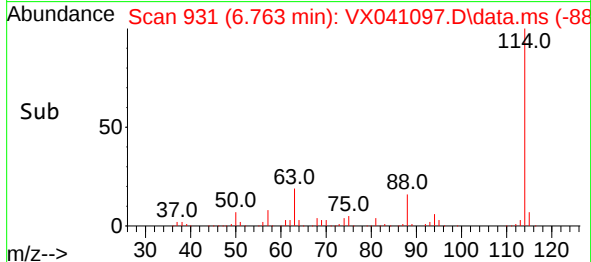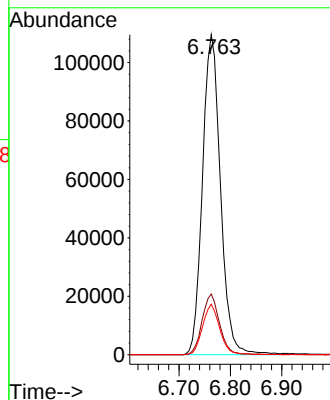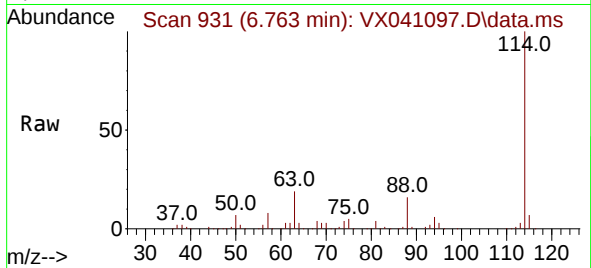

#35
Dibromofluoromethane
Concen: 48.206 ug/l
RT: 5.385 min Scan# 705
Delta R.T. -0.000 min
Lab File: VX041097.D
Acq: 16 Apr 2024 11:43

Tgt Ion:113 Resp: 85868
Ion Ratio Lower Upper
113 100
111 100.7 82.9 124.3
192 25.2 13.3 19.9#

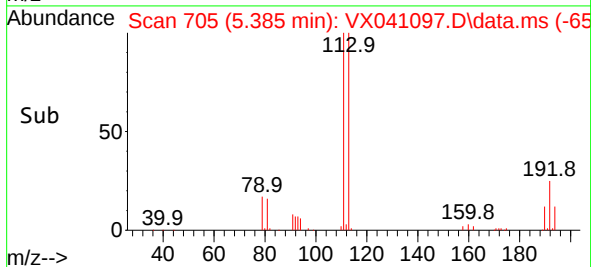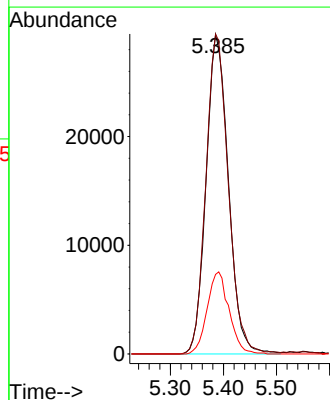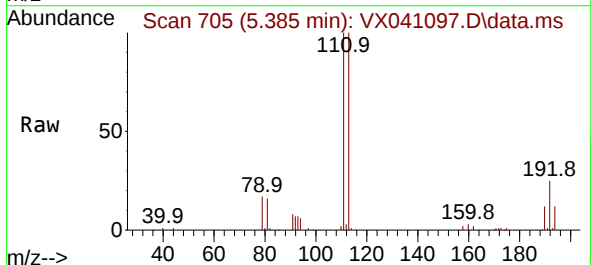

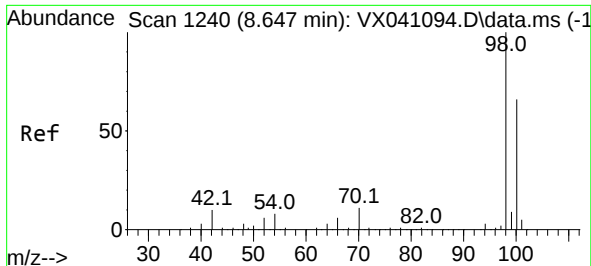

#50

Toluene-d8

Concen: 50.373 ug/l

RT: 8.647 min Scan# 11

Delta R.T. -0.000 min

Lab File: VX041097.D

Acq: 16 Apr 2024 11:43

Instrument :

MSVOA_X

ClientSampleId :





IBLK

Tgt Ion: 98 Resp: 314287

Ion Ratio Lower Upper

98 100

100 66.1 53.1 79.7

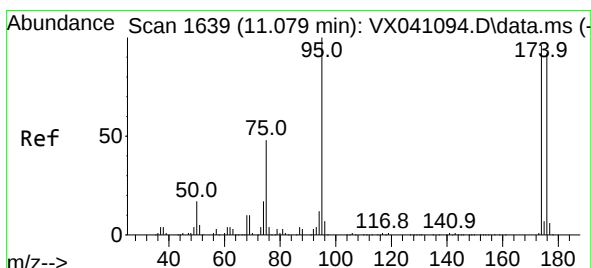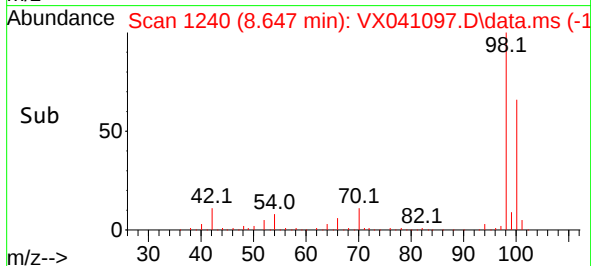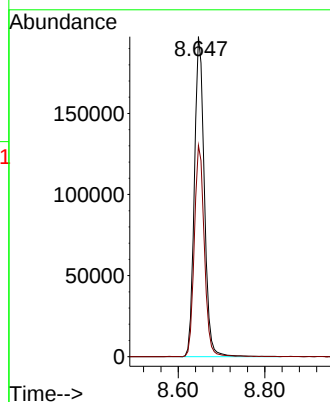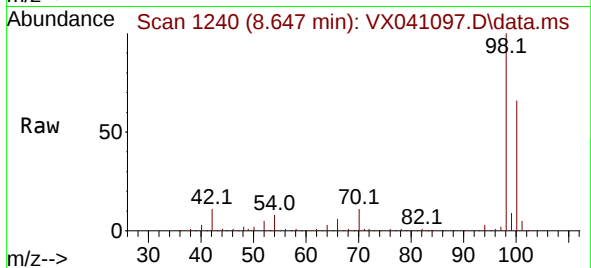

#62

4-Bromofluorobenzene

Concen: 50.263 ug/l

RT: 11.079 min Scan# 1639

Delta R.T. -0.000 min

Lab File: VX041097.D

Acq: 16 Apr 2024 11:43




Tgt Ion: 95 Resp: 119046


Ion Ratio Lower Upper

95 100

174 99.6 0.0 135.6

176 97.9 0.0 131.0

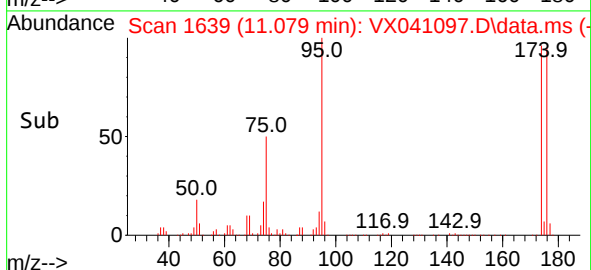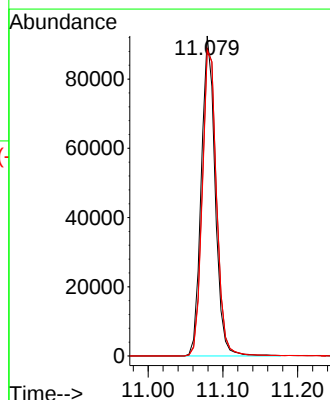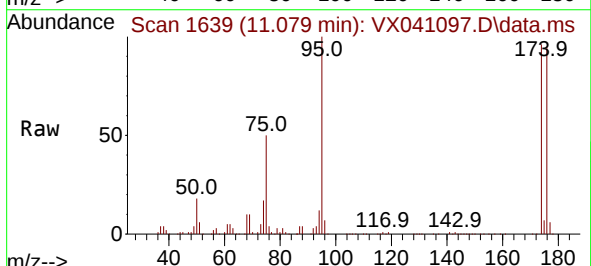

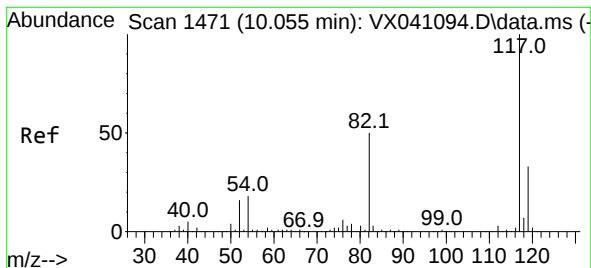

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 10.055 min Scan# 1471

Delta R.T. -0.000 min

Lab File: VX041097.D

Acq: 16 Apr 2024 11:43

Instrument :

MSVOA_X

ClientSampleId :

IBLK





Tgt Ion:117 Resp: 261623

Ion Ratio Lower Upper

117 100

82 50.8 46.2 69.4

119 32.2 25.5 38.3

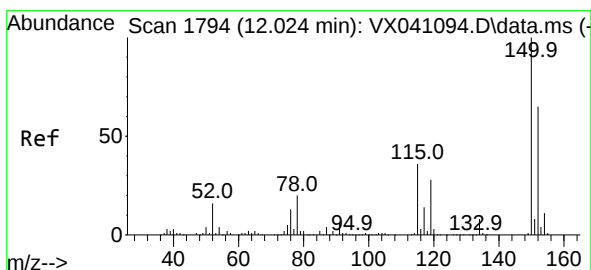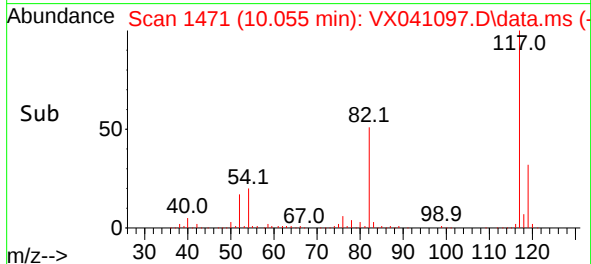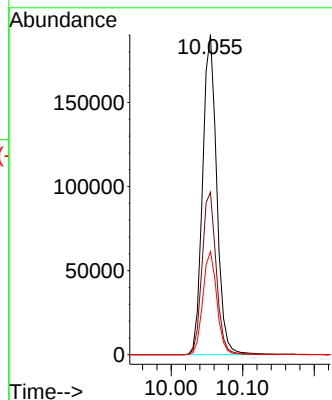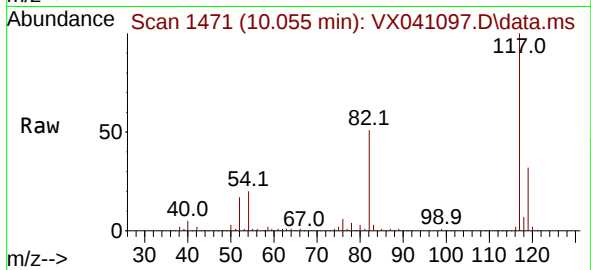

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 12.024 min Scan# 1794

Delta R.T. -0.000 min

Lab File: VX041097.D

Acq: 16 Apr 2024 11:43

Tgt Ion:152 Resp: 149137

Ion Ratio Lower Upper

152 100

115 52.8 43.3 129.9

150 153.6 0.0 345.0

