

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041624\
 Data File : VX041100.D
 Acq On : 16 Apr 2024 13:19
 Operator : JC/MD
 Sample : VX0416WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VX0416WBL01

Quant Time: Apr 17 02:08:41 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X041624W.M
 Quant Title : SW846 8260
 QLast Update : Wed Apr 17 02:04:44 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.550	168	176137	50.000	ug/l	# 0.00
34) 1,4-Difluorobenzene	6.763	114	265995	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	258252	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	144124	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.952	65	96893	50.952	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	= 101.900%	
35) Dibromofluoromethane	5.385	113	85476	48.104	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	= 96.200%	
50) Toluene-d8	8.647	98	310643	49.911	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	= 99.820%	
62) 4-Bromofluorobenzene	11.079	95	117629	49.786	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	= 99.580%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041624\
Data File : VX041100.D
Acq On : 16 Apr 2024 13:19
Operator : JC/MD
Sample : VX0416WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0416WBL01

Quant Time: Apr 17 02:08:41 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X041624W.M
Quant Title : SW846 8260
QLast Update : Wed Apr 17 02:04:44 2024
Response via : Initial Calibration




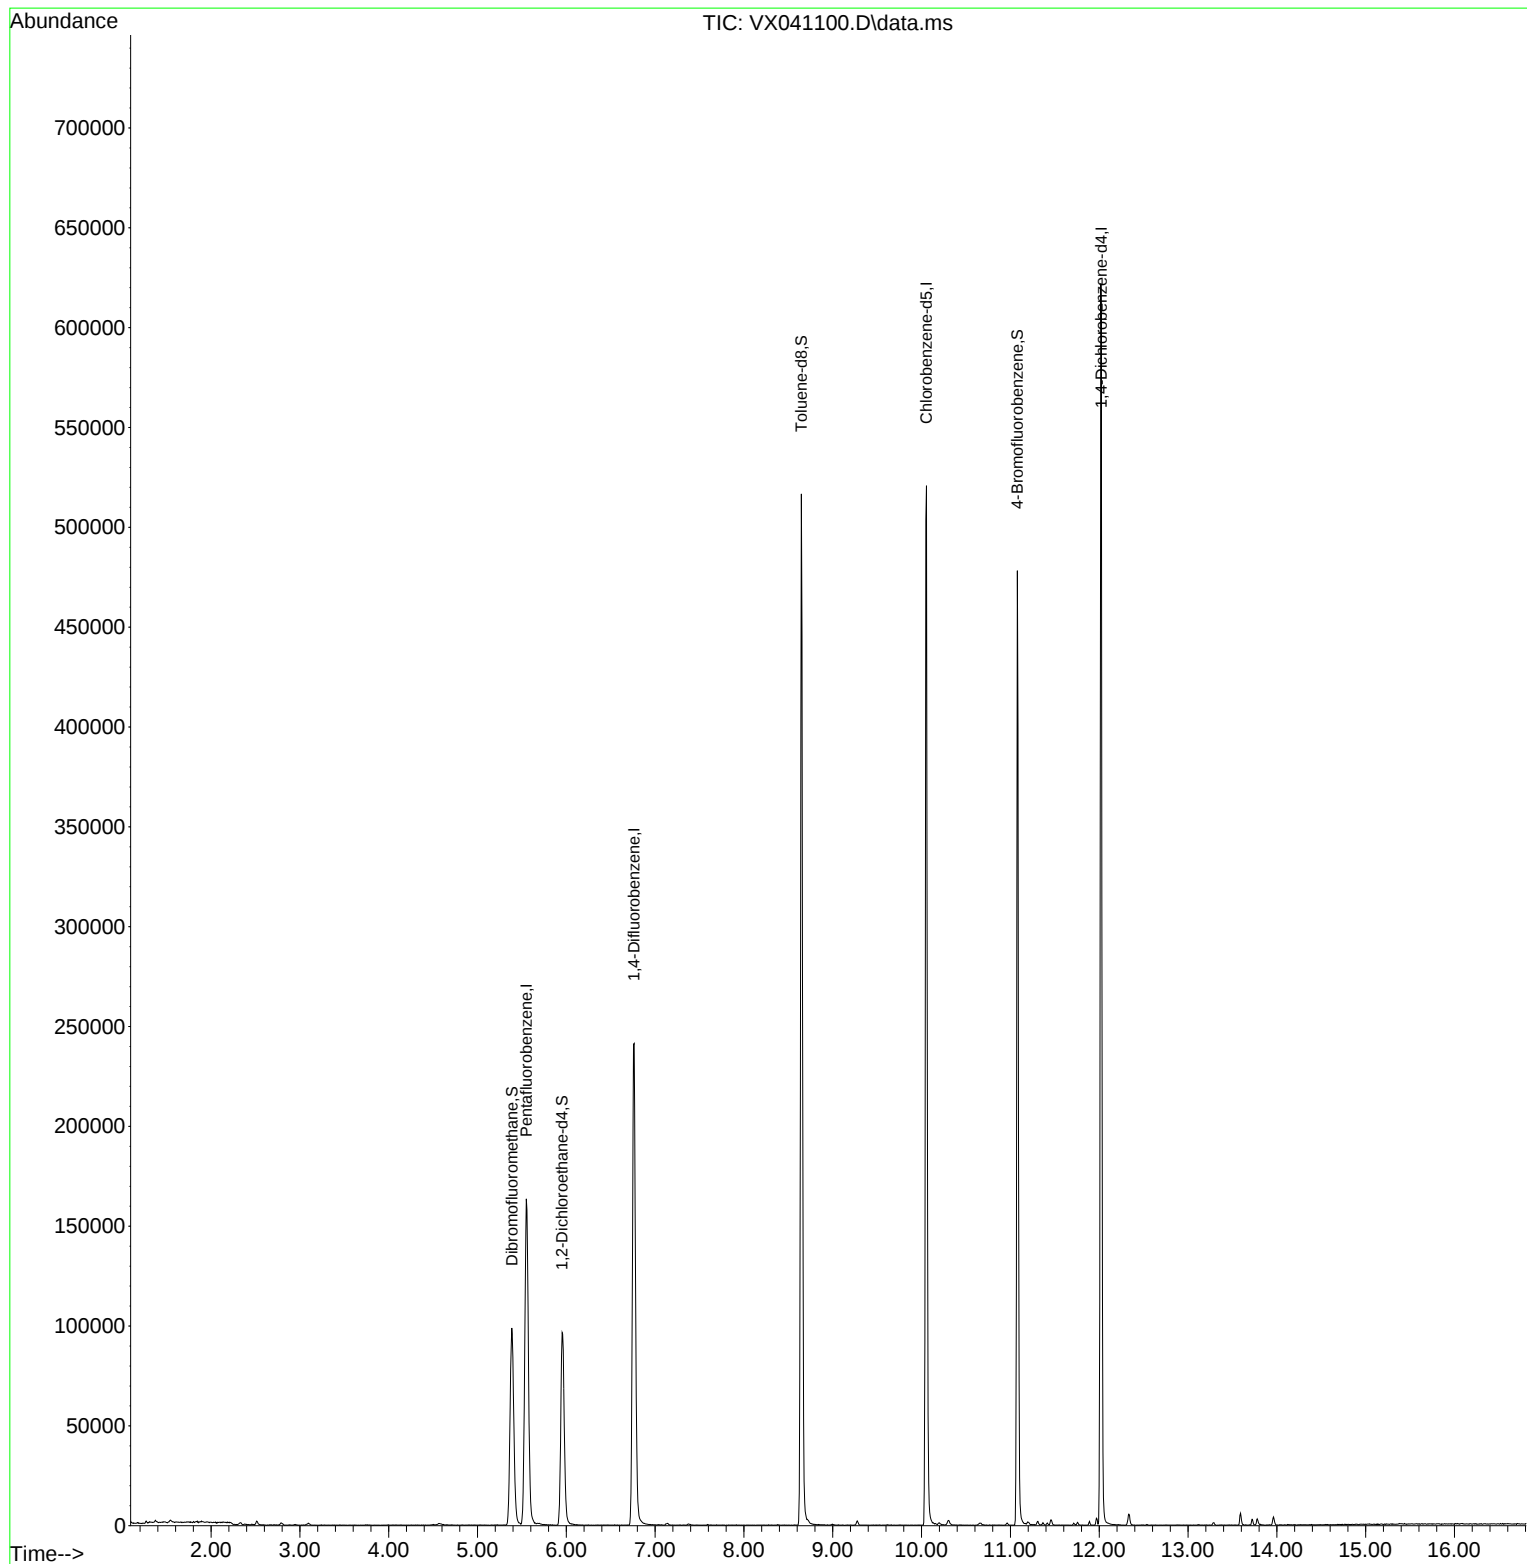


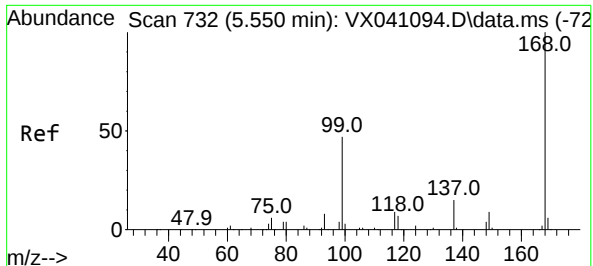

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.550 min Scan# 732
Delta R.T. -0.000 min
Lab File: VX041100.D
Acq: 16 Apr 2024 13:19




Instrument :
MSVOA_X
ClientSampleId :
VX0416WBL01

Tgt Ion:168 Resp: 176137
Ion Ratio Lower Upper
168 100
99 47.3 56.6 85.0#

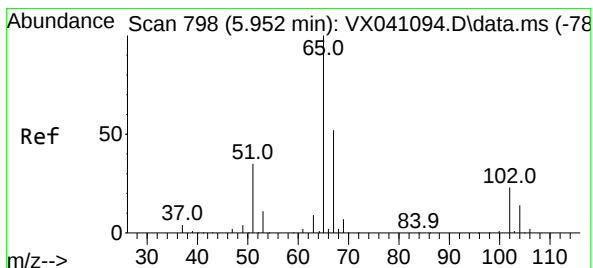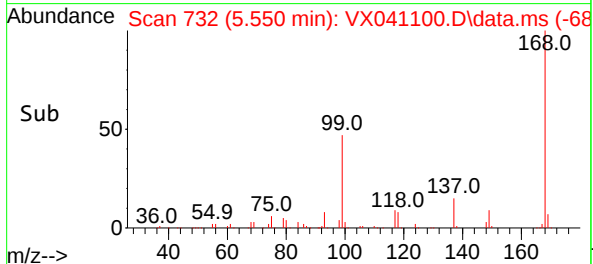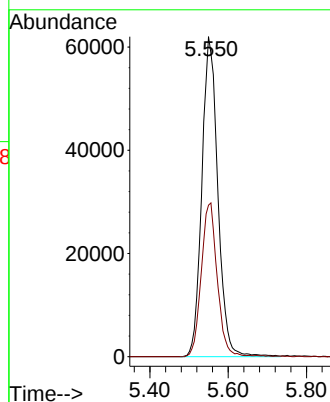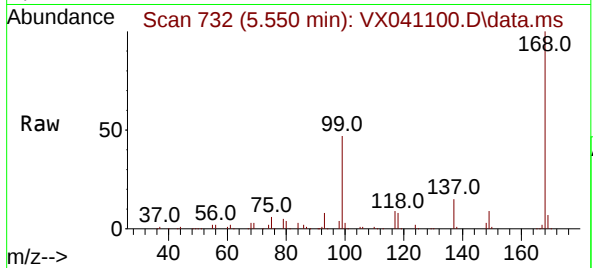

#33
1,2-Dichloroethane-d4
Concen: 50.952 ug/l
RT: 5.952 min Scan# 798
Delta R.T. -0.000 min
Lab File: VX041100.D
Acq: 16 Apr 2024 13:19

Tgt Ion: 65 Resp: 96893
Ion Ratio Lower Upper
65 100
67 50.3 0.0 100.2


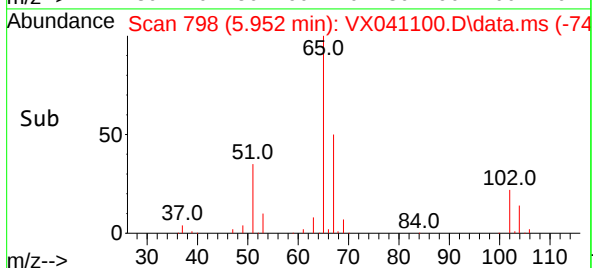
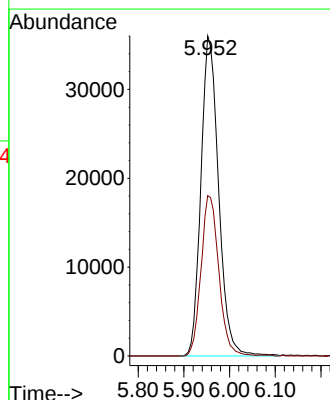
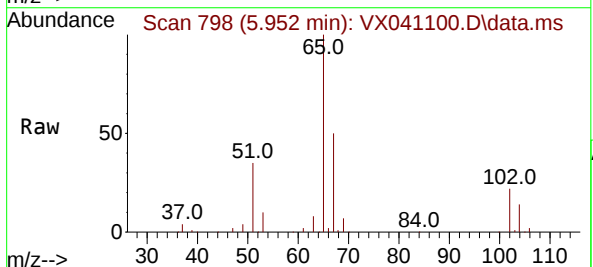




#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.763 min Scan# 911
Delta R.T. -0.000 min
Lab File: VX041100.D
Acq: 16 Apr 2024 13:19




Instrument :
MSVOA_X
ClientSampleId :
VX0416WBL01


Tgt Ion:114 Resp: 265995
Ion Ratio Lower Upper
114 100
63 18.7 0.0 45.0
88 14.8 0.0 36.6

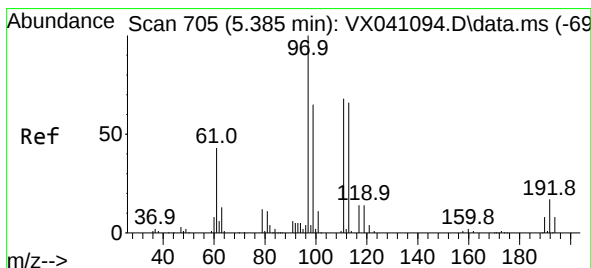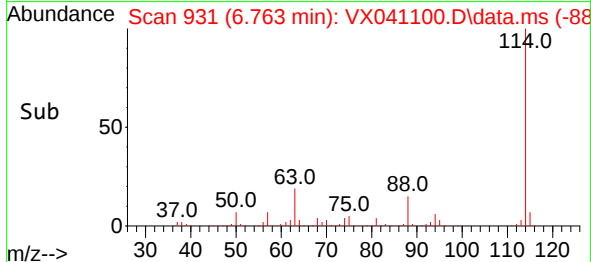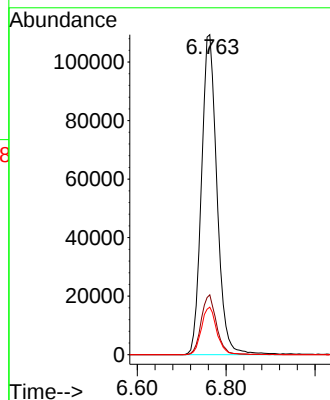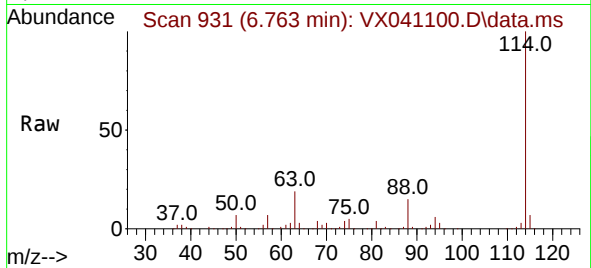

#35
Dibromofluoromethane
Concen: 48.104 ug/l
RT: 5.385 min Scan# 705
Delta R.T. -0.000 min
Lab File: VX041100.D
Acq: 16 Apr 2024 13:19

Tgt Ion:113 Resp: 85476
Ion Ratio Lower Upper
113 100
111 102.2 82.9 124.3
192 25.5 13.3 19.9#


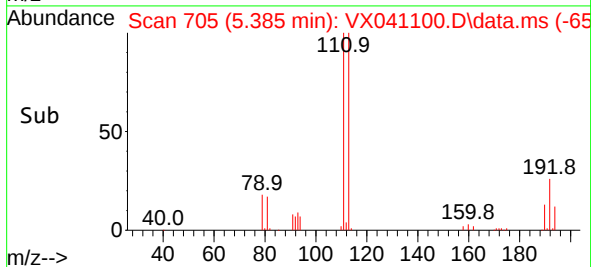
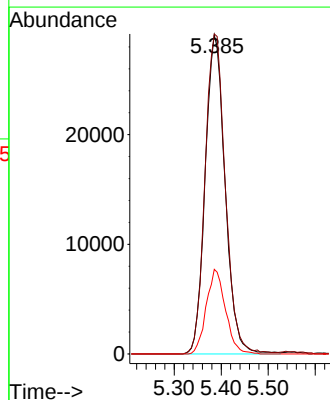
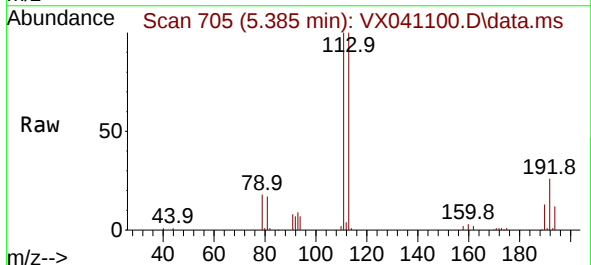


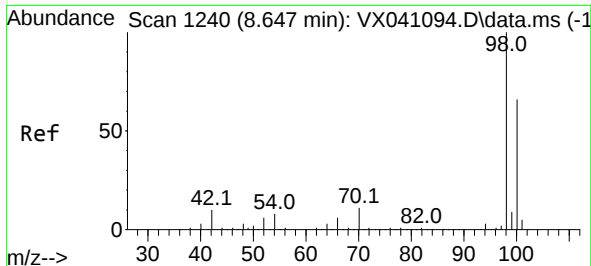

#50
Toluene-d8
Concen: 49.911 ug/l
RT: 8.647 min Scan# 11
Delta R.T. -0.000 min
Lab File: VX041100.D
Acq: 16 Apr 2024 13:19




Instrument :
MSVOA_X
ClientSampleId :
VX0416WBL01


Tgt Ion: 98 Resp: 310643
Ion Ratio Lower Upper
98 100
100 66.7 53.1 79.7

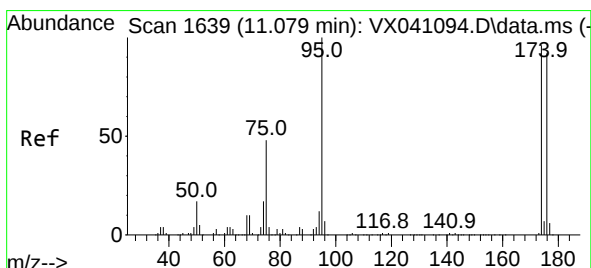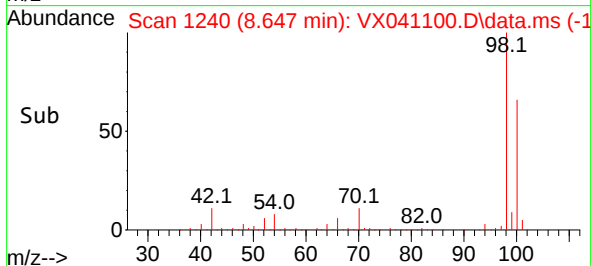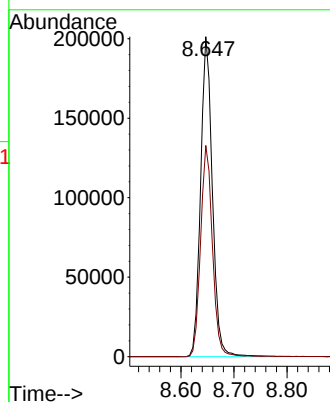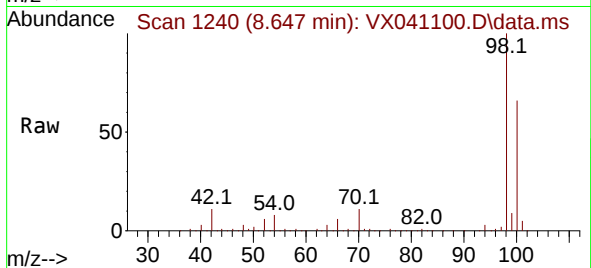

#62
4-Bromofluorobenzene
Concen: 49.786 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.000 min
Lab File: VX041100.D
Acq: 16 Apr 2024 13:19

Tgt Ion: 95 Resp: 117629
Ion Ratio Lower Upper
95 100
174 100.2 0.0 135.6
176 98.1 0.0 131.0


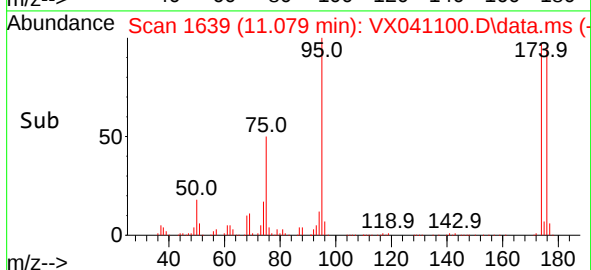
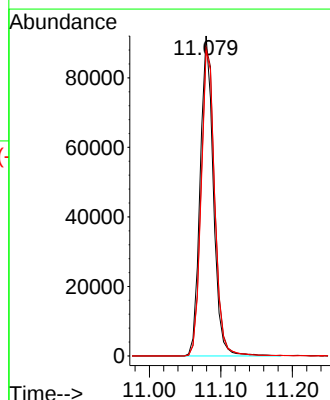
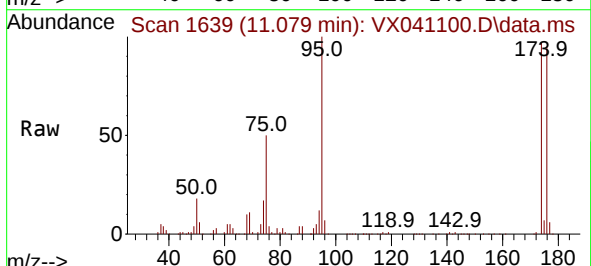


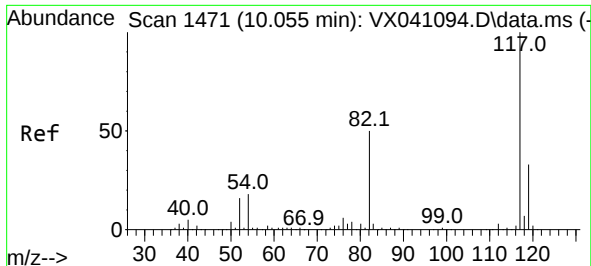

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. -0.000 min
Lab File: VX041100.D
Acq: 16 Apr 2024 13:19

Instrument :
MSVOA_X
ClientSampleId :
VX0416WBL01

Tgt Ion:117 Resp: 258252
Ion Ratio Lower Upper
117 100
82 50.2 46.2 69.4
119 33.2 25.5 38.3

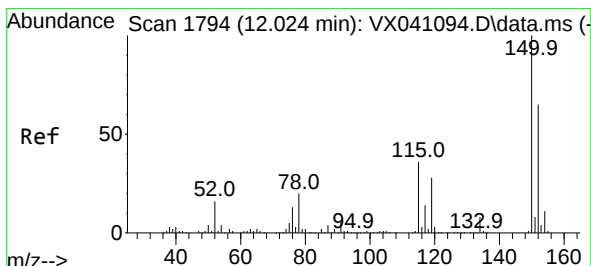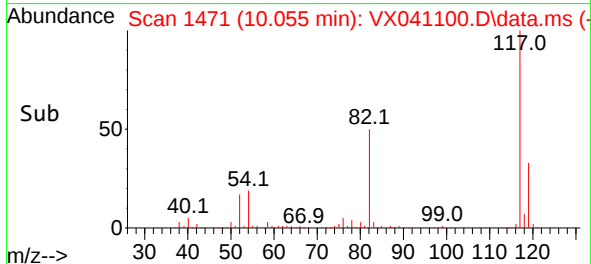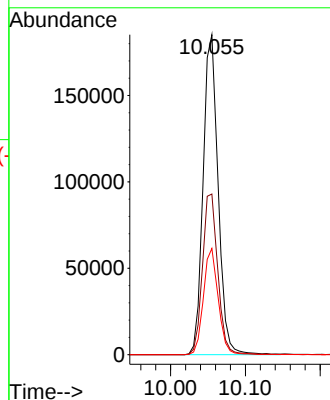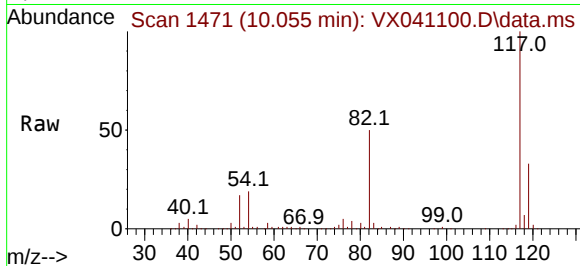

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. -0.000 min
Lab File: VX041100.D
Acq: 16 Apr 2024 13:19

Tgt Ion:152 Resp: 144124
Ion Ratio Lower Upper
152 100
115 53.8 43.3 129.9
150 157.0 0.0 345.0

