

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041624\
 Data File : VX041104.D
 Acq On : 16 Apr 2024 14:56
 Operator : JC/MD
 Sample : P2076-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 240410075-02-VOA

Quant Time: Apr 17 02:11:11 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X041624W.M
 Quant Title : SW846 8260
 QLast Update : Wed Apr 17 02:04:44 2024
 Response via : Initial Calibration

Compound	R.T. QIon		Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.556	168	185223	50.000	ug/l	# 0.00
34) 1,4-Difluorobenzene	6.763	114	275360	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	270984	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	159870	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.952	65	100177	50.095	ug/l	0.00
Spiked Amount 50.000	Range 78 - 117		Recovery	= 100.180%		
35) Dibromofluoromethane	5.385	113	89023	48.396	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery	= 96.800%		
50) Toluene-d8	8.647	98	319259	49.551	ug/l	0.00
Spiked Amount 50.000	Range 92 - 112		Recovery	= 99.100%		
62) 4-Bromofluorobenzene	11.079	95	125753	51.415	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery	= 102.820%		
Target Compounds						
						Qvalue
2) Dichlorodifluoromethane	1.172	85	656	0.447	ug/l	76
4) Vinyl Chloride	1.374	62	794	0.424	ug/l #	86
6) Chloroethane	1.697	64	1242	1.005	ug/l #	88
8) Diethyl Ether	2.136	74	13198	11.450	ug/l	90
11) Tert butyl alcohol	2.953	59	107411	274.555	ug/l #	91
16) Acetone	2.380	43	11345	13.497	ug/l	96
17) Carbon Disulfide	2.514	76	1506	0.405	ug/l #	94
19) Methyl tert-butyl Ether	3.117	73	2947	0.583	ug/l #	79
25) 2-Butanone	4.568	43	7060	5.346	ug/l #	87
27) cis-1,2-Dichloroethene	4.495	96	1209	0.597	ug/l	89
29) Tetrahydrofuran	5.001	42	152633	174.577	ug/l	96
40) Benzene	6.043	78	12670	1.782	ug/l	99
44) Trichloroethene	7.123	130	1427	0.676	ug/l	72
49) 1,4-Dioxane	7.659	88	8844	187.752	ug/l #	92
52) Toluene	8.720	92	8588	1.851	ug/l	97
65) Chlorobenzene	10.079	112	50082	8.372	ug/l	98
67) Ethyl Benzene	10.195	91	38297	4.103	ug/l	98
68) m/p-Xylenes	10.299	106	19623	5.285	ug/l	91
69) o-Xylene	10.640	106	16837	4.659	ug/l	94
73) Isopropylbenzene	10.963	105	13007	1.379	ug/l	97
78) n-propylbenzene	11.305	91	5842	0.552	ug/l	100
79) 2-Chlorotoluene	11.366	91	5886	0.913	ug/l	94
80) 1,3,5-Trimethylbenzene	11.451	105	6559	0.835	ug/l	88
84) 1,2,4-Trimethylbenzene	11.750	105	26884	3.429	ug/l	91
85) sec-Butylbenzene	11.890	105	2565	0.255	ug/l #	67
86) p-Isopropyltoluene	12.012	119	8096	0.907	ug/l	95
88) 1,4-Dichlorobenzene	12.042	146	53322	9.681	ug/l	96
89) n-Butylbenzene	12.335	91	3143	0.415	ug/l #	64
91) 1,2-Dichlorobenzene	12.335	146	3976	0.767	ug/l	93
93) 1,2,4-Trichlorobenzene	13.591	180	1924	0.494	ug/l	94
94) Hexachlorobutadiene	13.725	225	413	0.222	ug/l	78
95) Naphthalene	13.774	128	91680	8.714	ug/l	100
96) 1,2,3-Trichlorobenzene	13.963	180	1322	0.342	ug/l	88


(#) = qualifier out of range (m) = manual integration (+) = signals summed


Instrument :
MSVOA_X
ClientSampleId :
240410075-02-VOA

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041624\
Data File : VX041104.D
Acq On : 16 Apr 2024 14:56
Operator : JC/MD
Sample : P2076-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
240410075-02-VOA

Quant Time: Apr 17 02:11:11 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X041624W.M
Quant Title : SW846 8260
QLast Update : Wed Apr 17 02:04:44 2024
Response via : Initial Calibration




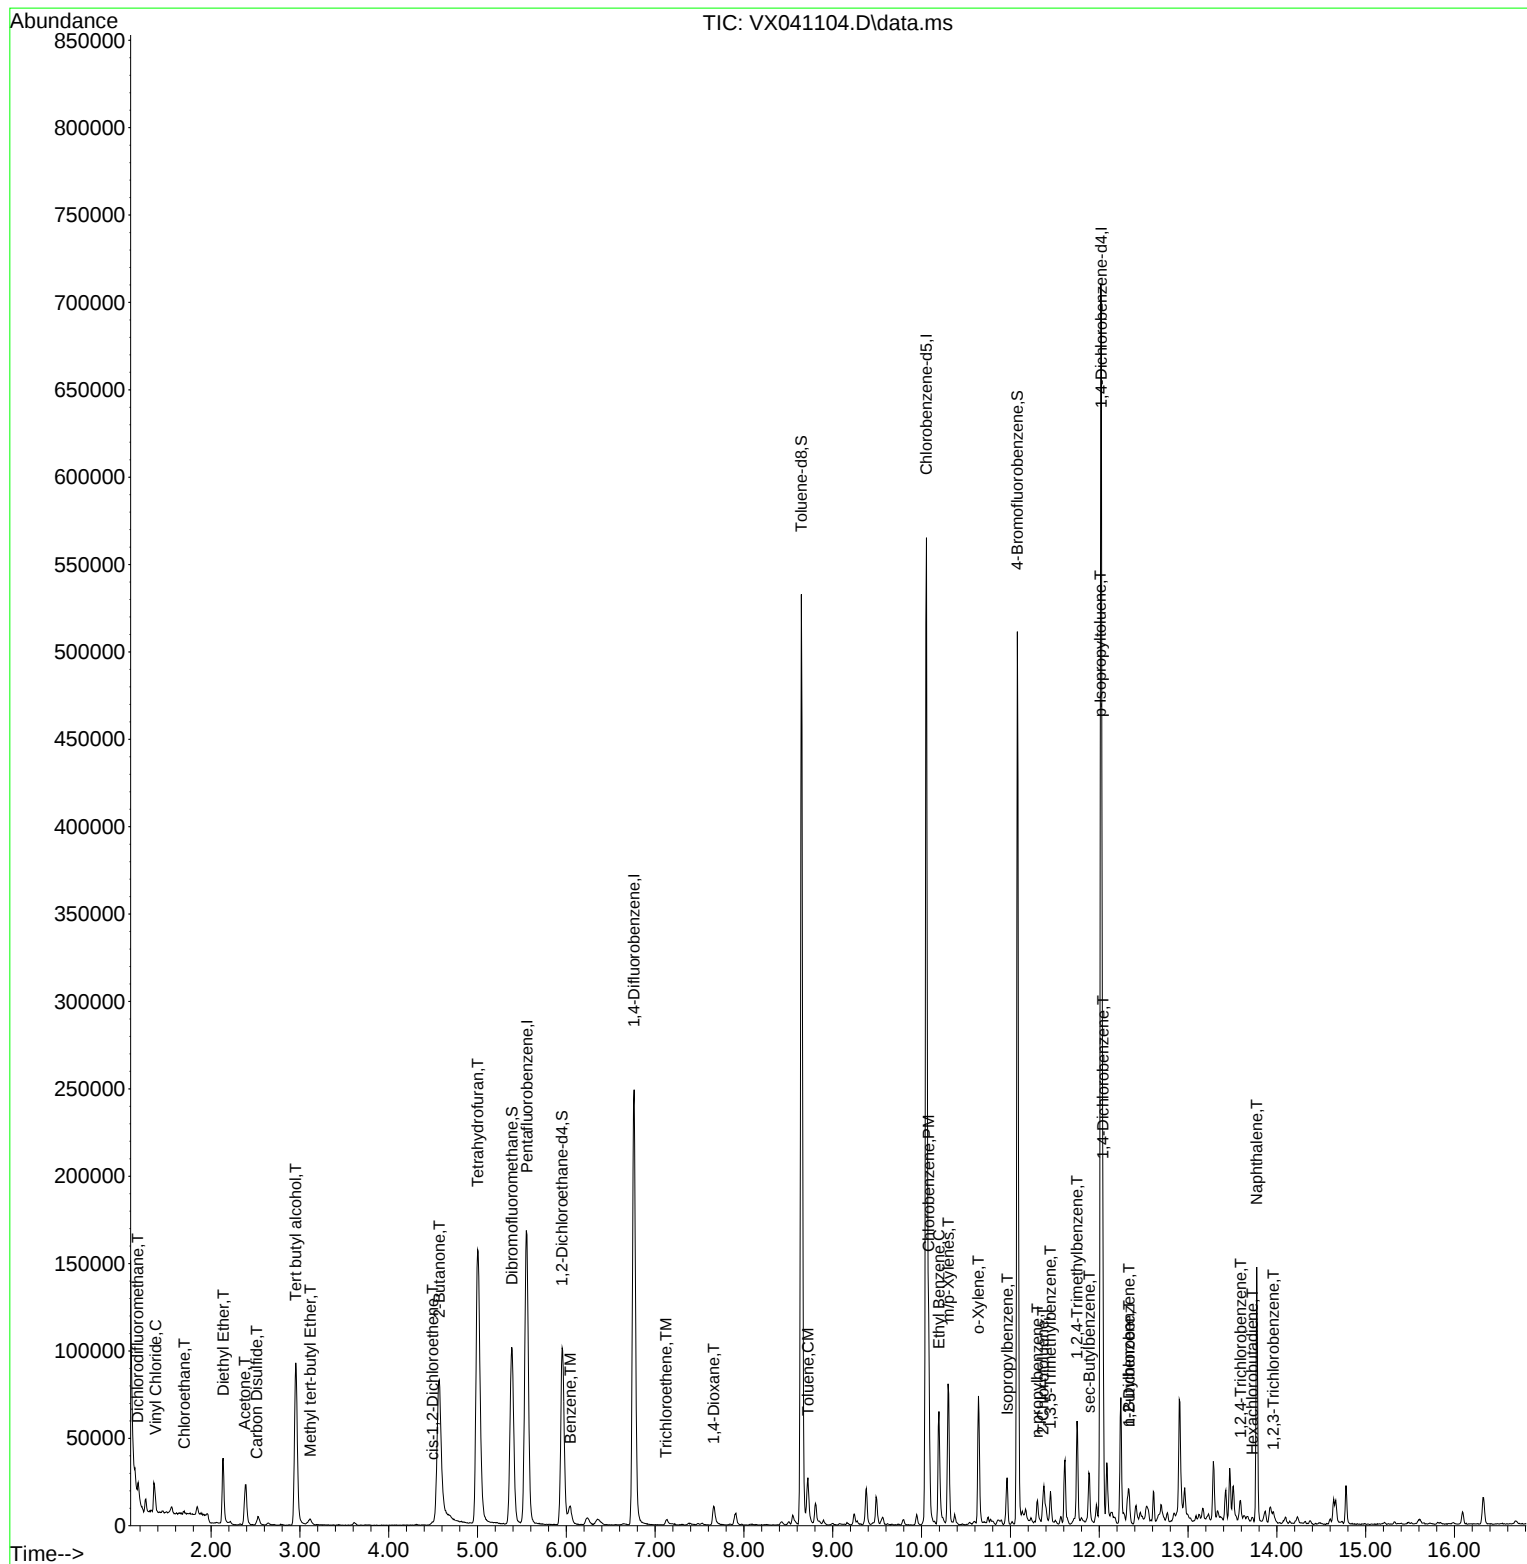




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.556 min Scan# 71
Delta R.T. 0.006 min
Lab File: VX041104.D
Acq: 16 Apr 2024 14:56




Instrument :
MSVOA_X
ClientSampleId :
240410075-02-VOA


Tgt Ion:168 Resp: 185223
Ion Ratio Lower Upper
168 100
99 46.9 56.6 85.0#

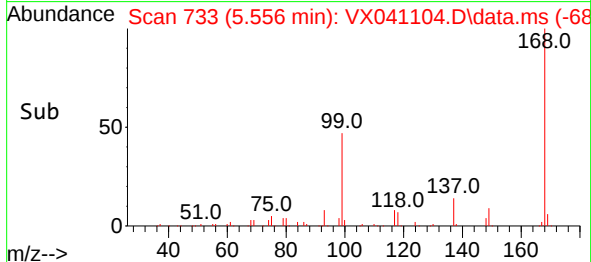

#2
Dichlorodifluoromethane
Concen: 0.447 ug/l
RT: 1.172 min Scan# 14
Delta R.T. 0.006 min
Lab File: VX041104.D
Acq: 16 Apr 2024 14:56

Tgt Ion: 85 Resp: 656
Ion Ratio Lower Upper
85 100
87 19.7 16.7 50.1


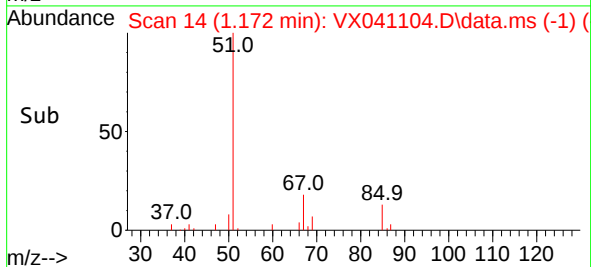

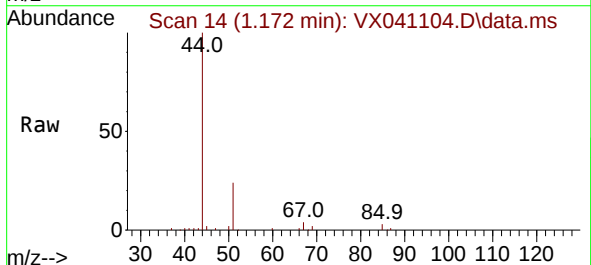


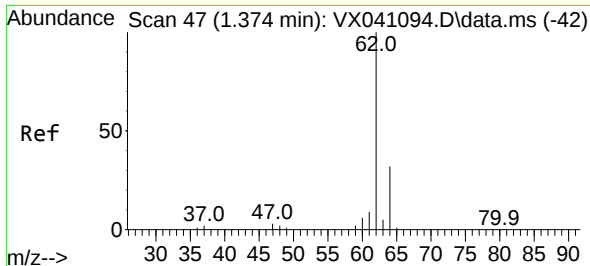

#4
Vinyl Chloride
Concen: 0.424 ug/l
RT: 1.374 min Scan# 41
Delta R.T. -0.000 min
Lab File: VX041104.D
Acq: 16 Apr 2024 14:56




Instrument :
MSVOA_X
ClientSampleId :
240410075-02-VOA


Tgt Ion: 62 Resp: 794
Ion Ratio Lower Upper
62 100
64 39.6 25.4 38.0#

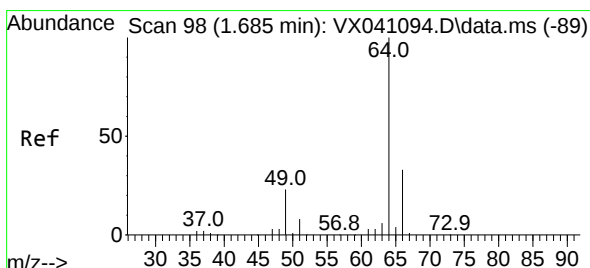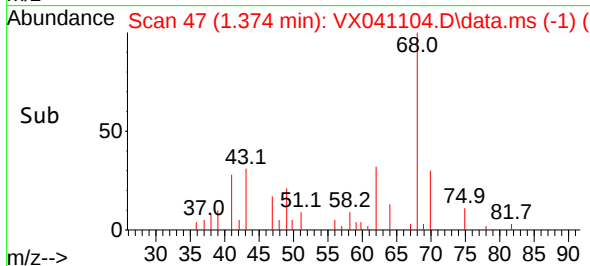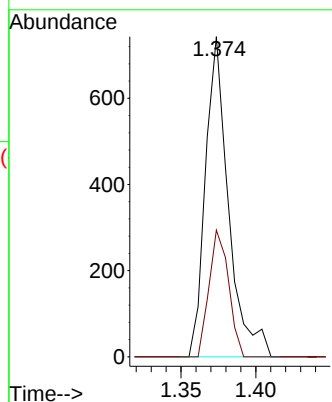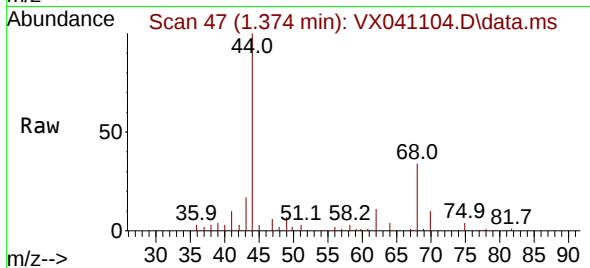

#6
Chloroethane
Concen: 1.005 ug/l
RT: 1.697 min Scan# 100
Delta R.T. 0.012 min
Lab File: VX041104.D
Acq: 16 Apr 2024 14:56

Tgt Ion: 64 Resp: 1242
Ion Ratio Lower Upper
64 100
66 24.6 25.1 37.7#


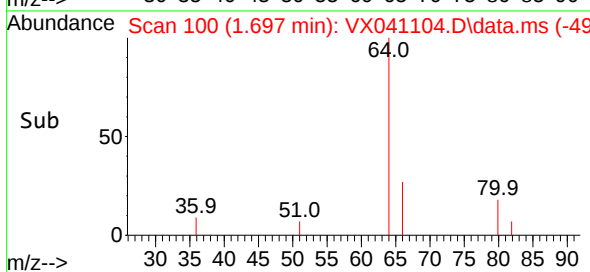
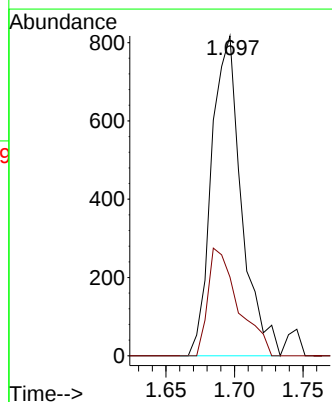
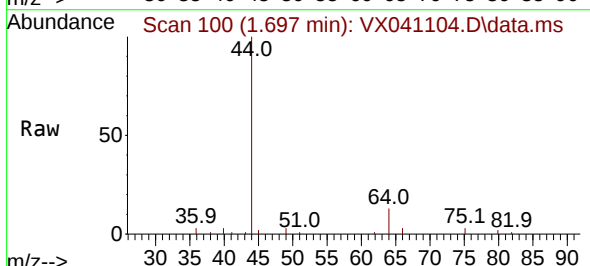




#8
Diethyl Ether
Concen: 11.450 ug/l
RT: 2.136 min Scan# 11
Delta R.T. -0.000 min
Lab File: VX041104.D
Acq: 16 Apr 2024 14:56




Instrument :
MSVOA_X
ClientSampleId :
240410075-02-VOA


Tgt Ion: 74 Resp: 13198
Ion Ratio Lower Upper
74 100
45 95.7 53.3 159.8

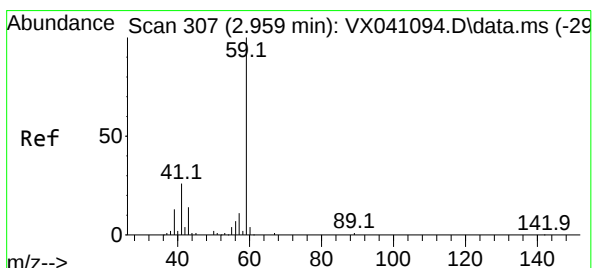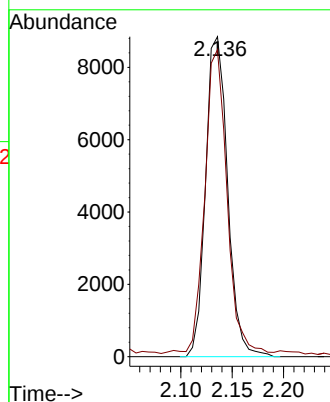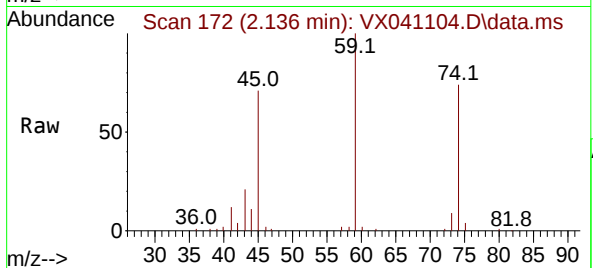

#11
Tert butyl alcohol
Concen: 274.555 ug/l
RT: 2.953 min Scan# 306
Delta R.T. -0.006 min
Lab File: VX041104.D
Acq: 16 Apr 2024 14:56

Tgt Ion: 59 Resp: 107411
Ion Ratio Lower Upper
59 100
57 10.7 6.0 9.0#


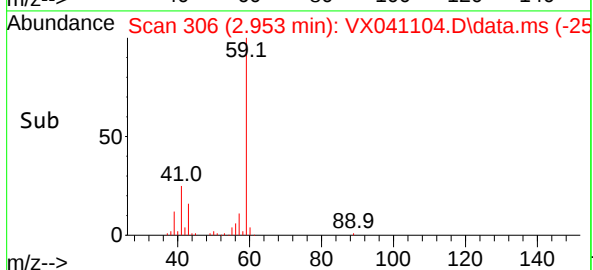






#16
Acetone
Concen: 13.497 ug/l
RT: 2.380 min Scan# 212
Delta R.T. -0.000 min
Lab File: VX041104.D
Acq: 16 Apr 2024 14:56




Instrument :
MSVOA_X
ClientSampleId :
240410075-02-VOA


Tgt Ion: 43 Resp: 11345
Ion Ratio Lower Upper
43 100
58 29.2 21.9 32.9

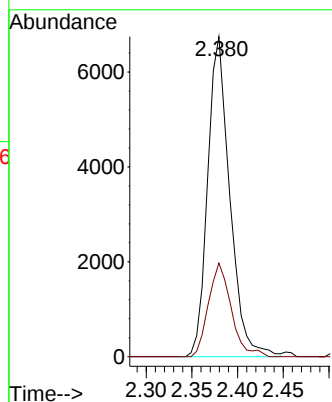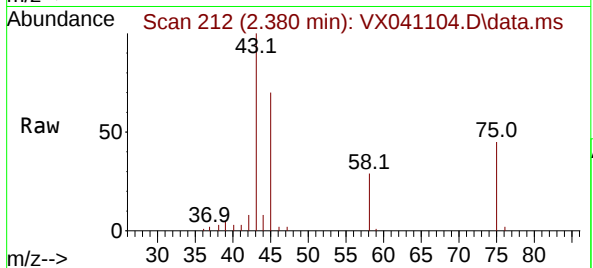

#17
Carbon Disulfide
Concen: 0.405 ug/l
RT: 2.514 min Scan# 234
Delta R.T. -0.000 min
Lab File: VX041104.D
Acq: 16 Apr 2024 14:56

Tgt Ion: 76 Resp: 1506
Ion Ratio Lower Upper
76 100
78 6.7 7.0 10.6#

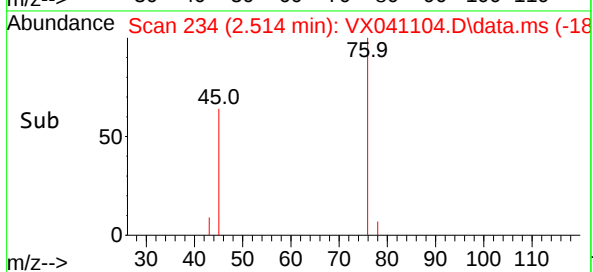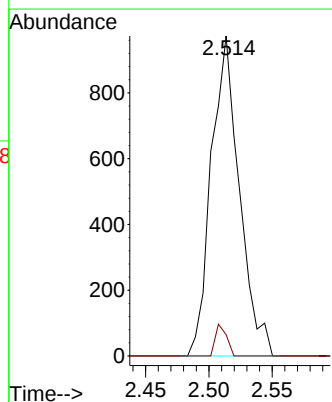



#19

Methyl tert-butyl Ether

Concen: 0.583 ug/l

RT: 3.117 min Scan# 31

Delta R.T. -0.000 min

Lab File: VX041104.D

Acq: 16 Apr 2024 14:56

Instrument :

MSVOA_X

ClientSampleId :





240410075-02-VOA

Tgt Ion: 73 Resp: 2947

Ion Ratio Lower Upper

73 100

57 31.8 17.3 25.9#

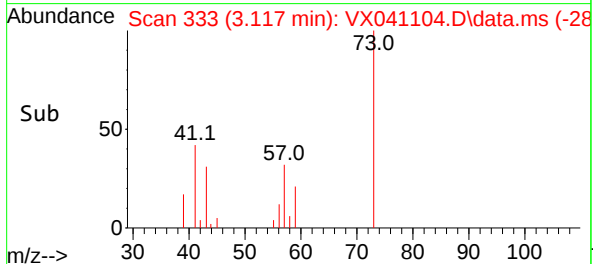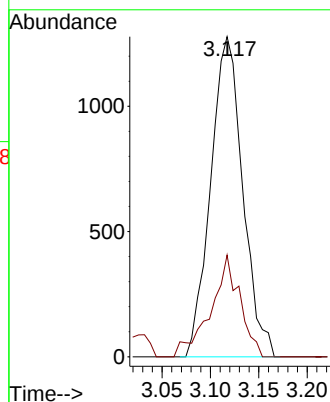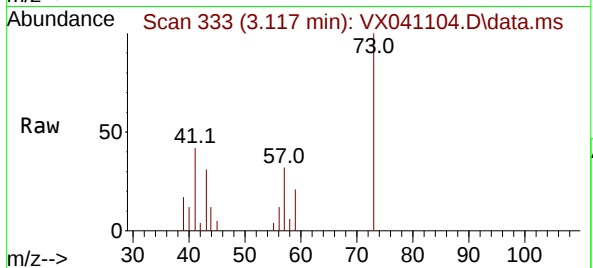

#25

2-Butanone

Concen: 5.346 ug/l

RT: 4.568 min Scan# 571

Delta R.T. 0.012 min

Lab File: VX041104.D




Acq: 16 Apr 2024 14:56


Tgt Ion: 43 Resp: 7060

Ion Ratio Lower Upper

43 100

72 18.1 19.4 29.2#

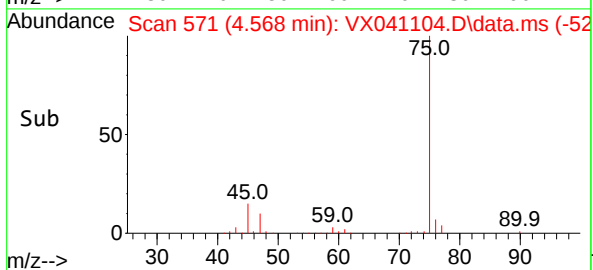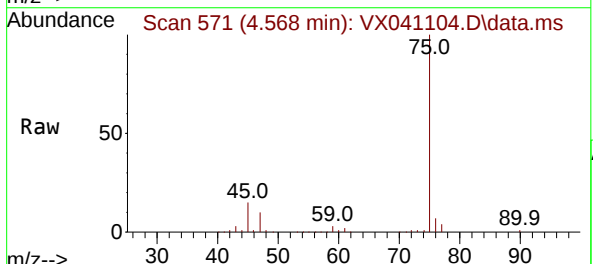



#27

cis-1,2-Dichloroethene

Concen: 0.597 ug/l

RT: 4.495 min Scan# 559

Delta R.T. 0.006 min

Lab File: VX041104.D


Acq: 16 Apr 2024 14:56

Instrument :

MSVOA_X

ClientSampleId :

240410075-02-VOA






Tgt Ion: 96 Resp: 1209

Ion Ratio Lower Upper

96 100

61 140.0 0.0 312.2

98 69.6 0.0 129.0

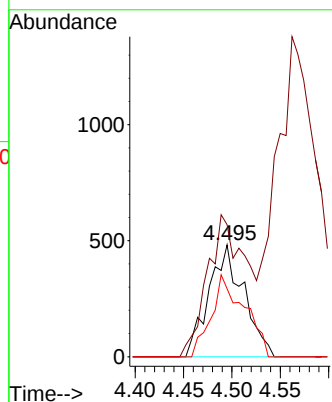

#29

Tetrahydrofuran

Concen: 174.577 ug/l

RT: 5.001 min Scan# 642

Delta R.T. -0.000 min

Lab File: VX041104.D

Acq: 16 Apr 2024 14:56




Tgt Ion: 42 Resp: 152633


Ion Ratio Lower Upper

42 100

72 45.4 34.2 51.4

71 42.7 32.2 48.2

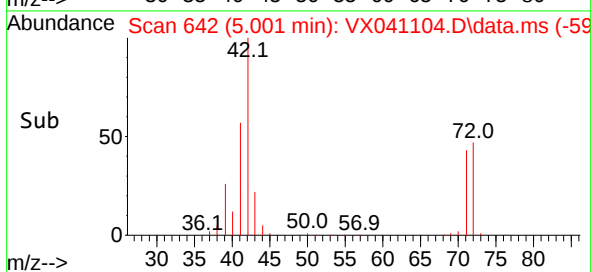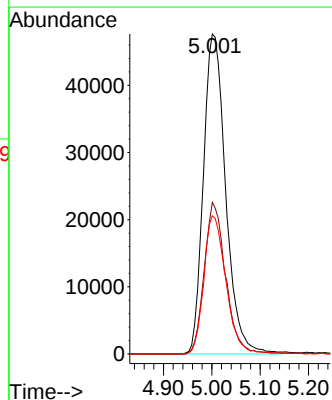



#33

1,2-Dichloroethane-d4

Concen: 50.095 ug/l

RT: 5.952 min Scan# 798

Delta R.T. -0.000 min

Lab File: VX041104.D

Acq: 16 Apr 2024 14:56

Instrument :

MSVOA_X

ClientSampleId :





240410075-02-VOA

Tgt Ion: 65 Resp: 100177

Ion Ratio Lower Upper

65 100

67 51.5 0.0 100.2

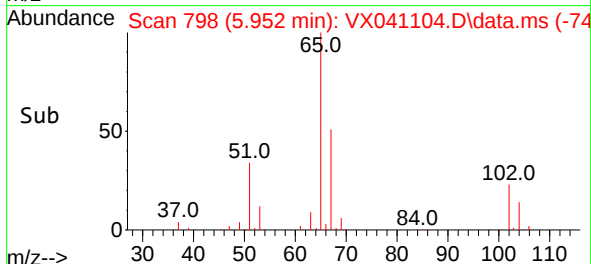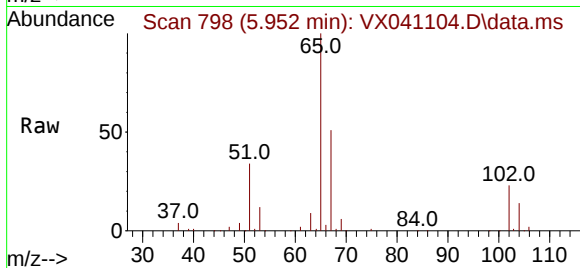

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.763 min Scan# 931

Delta R.T. -0.000 min

Lab File: VX041104.D

Acq: 16 Apr 2024 14:56




Tgt Ion: 114 Resp: 275360


Ion Ratio Lower Upper

114 100

63 18.5 0.0 45.0

88 15.0 0.0 36.6


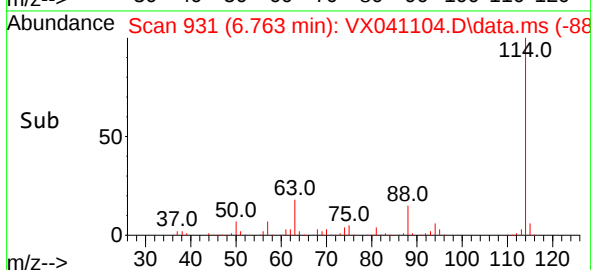

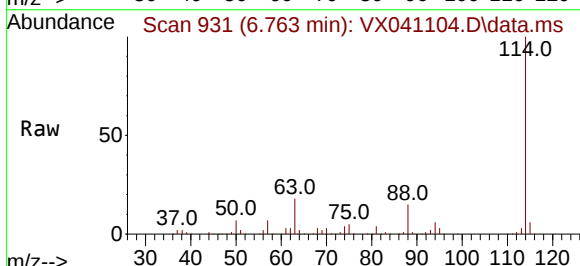




#35
Dibromofluoromethane
Concen: 48.396 ug/l
RT: 5.385 min Scan# 705
Delta R.T. -0.000 min
Lab File: VX041104.D
Acq: 16 Apr 2024 14:56




Instrument :
MSVOA_X
ClientSampleId :
240410075-02-VOA


Tgt Ion:113 Resp: 89023
Ion Ratio Lower Upper
113 100
111 101.2 82.9 124.3
192 26.0 13.3 19.9#

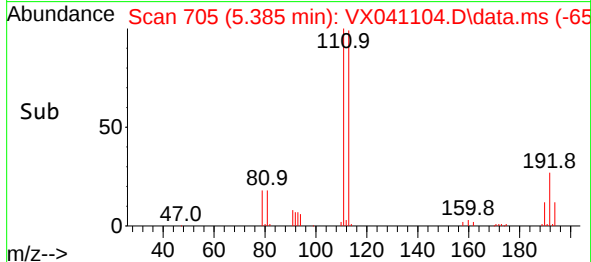

#40
Benzene
Concen: 1.782 ug/l
RT: 6.043 min Scan# 813
Delta R.T. 0.006 min
Lab File: VX041104.D
Acq: 16 Apr 2024 14:56

Tgt Ion: 78 Resp: 12670
Ion Ratio Lower Upper
78 100
77 23.5 19.3 28.9


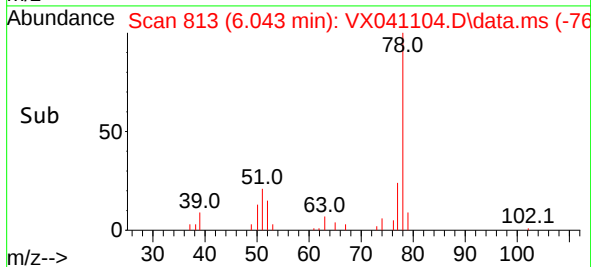

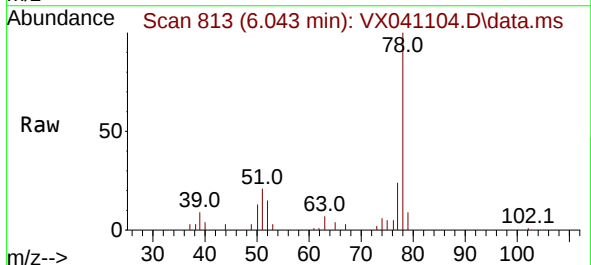




#44
Trichloroethene
Concen: 0.676 ug/l
RT: 7.123 min Scan# 990
Delta R.T. -0.000 min
Lab File: VX041104.D
Acq: 16 Apr 2024 14:56




Instrument :
MSVOA_X
ClientSampleId :
240410075-02-VOA


Tgt Ion:130 Resp: 1427
Ion Ratio Lower Upper
130 100
95 73.3 0.0 204.4

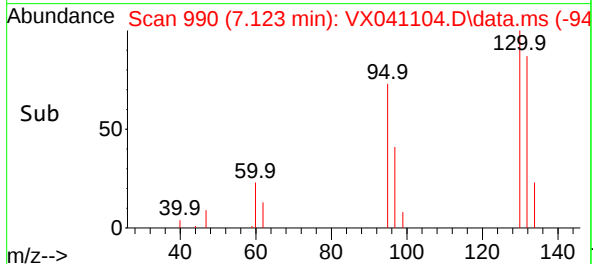

#49
1,4-Dioxane
Concen: 187.752 ug/l
RT: 7.659 min Scan# 1078
Delta R.T. -0.000 min
Lab File: VX041104.D
Acq: 16 Apr 2024 14:56

Tgt Ion: 88 Resp: 8844
Ion Ratio Lower Upper
88 100
43 29.0 0.0 0.0#
58 68.0 60.1 90.1


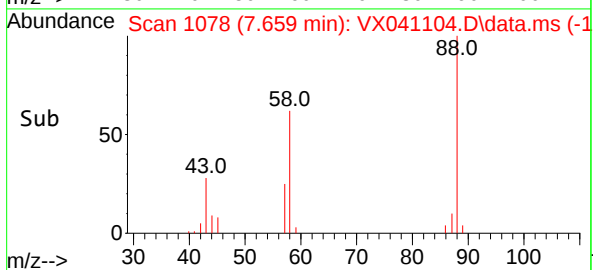

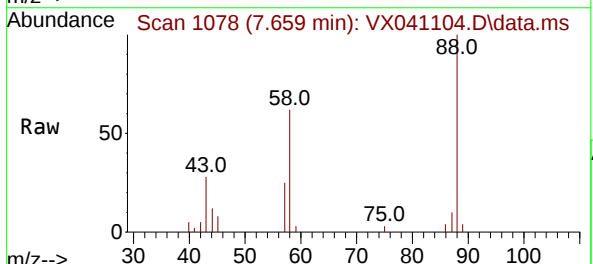




#50
Toluene-d8
Concen: 49.551 ug/l
RT: 8.647 min Scan# 11
Delta R.T. -0.000 min
Lab File: VX041104.D
Acq: 16 Apr 2024 14:56




Instrument :
MSVOA_X
ClientSampleId :
240410075-02-VOA


Tgt Ion: 98 Resp: 319259
Ion Ratio Lower Upper
98 100
100 66.8 53.1 79.7

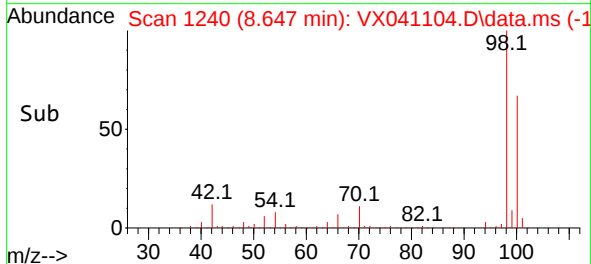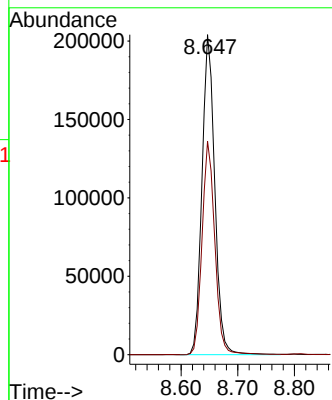

#52
Toluene
Concen: 1.851 ug/l
RT: 8.720 min Scan# 1252
Delta R.T. -0.000 min
Lab File: VX041104.D
Acq: 16 Apr 2024 14:56

Tgt Ion: 92 Resp: 8588
Ion Ratio Lower Upper
92 100
91 171.3 134.2 201.2


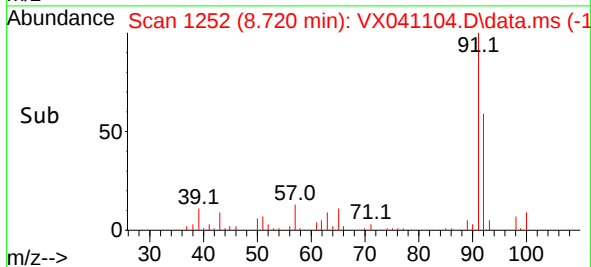
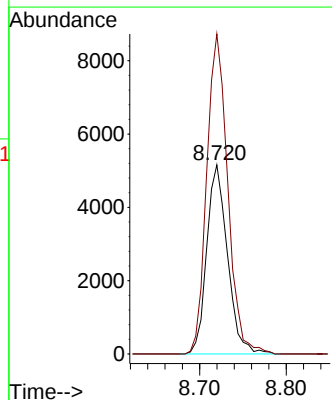
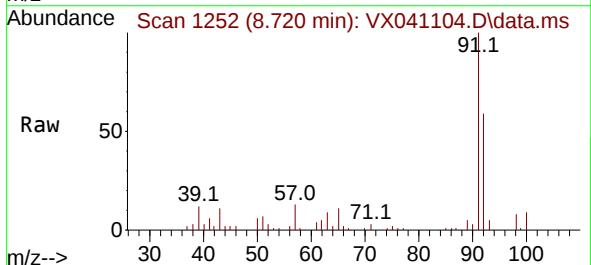




#62
4-Bromofluorobenzene
Concen: 51.415 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.000 min
Lab File: VX041104.D
Acq: 16 Apr 2024 14:56




Instrument :
MSVOA_X
ClientSampleId :
240410075-02-VOA


Tgt Ion: 95 Resp: 125753
Ion Ratio Lower Upper
95 100
174 100.4 0.0 135.6
176 96.8 0.0 131.0

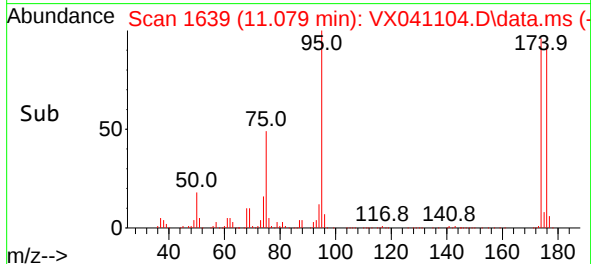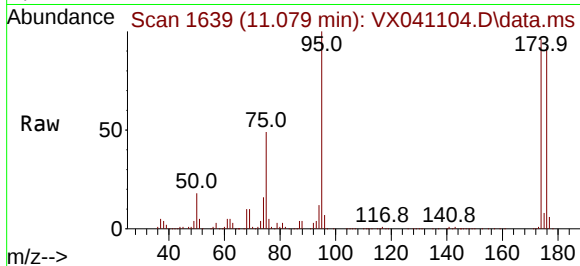

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. -0.000 min
Lab File: VX041104.D
Acq: 16 Apr 2024 14:56

Tgt Ion: 117 Resp: 270984
Ion Ratio Lower Upper
117 100
82 49.5 46.2 69.4
119 32.8 25.5 38.3


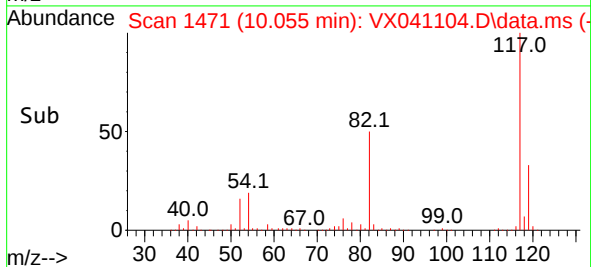

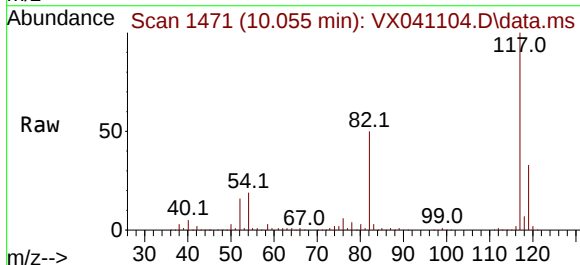




#65
Chlorobenzene
Concen: 8.372 ug/l
RT: 10.079 min Scan# 1475
Delta R.T. -0.000 min
Lab File: VX041104.D
Acq: 16 Apr 2024 14:56




Instrument :
MSVOA_X
ClientSampleId :
240410075-02-VOA


Tgt Ion:112 Resp: 50082
Ion Ratio Lower Upper
112 100
114 33.4 25.7 38.5

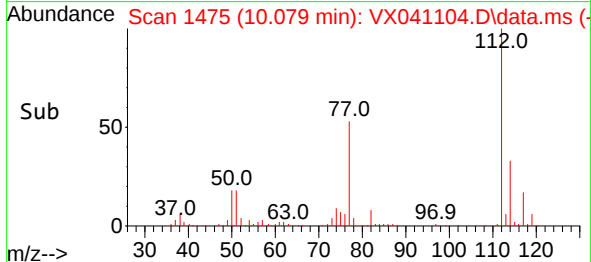

#67
Ethyl Benzene
Concen: 4.103 ug/l
RT: 10.195 min Scan# 1494
Delta R.T. -0.000 min
Lab File: VX041104.D
Acq: 16 Apr 2024 14:56

Tgt Ion: 91 Resp: 38297
Ion Ratio Lower Upper
91 100
106 32.4 24.9 37.3


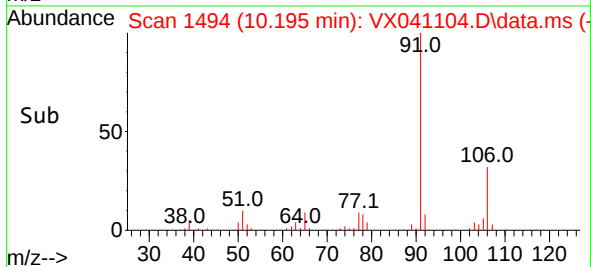

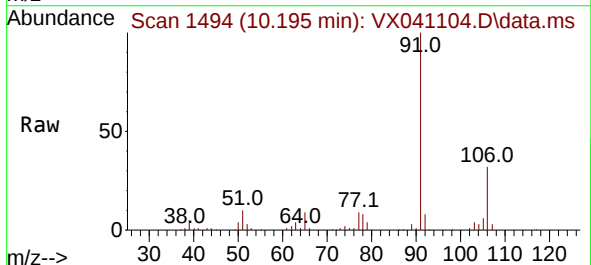




#68
m/p-Xylenes
Concen: 5.285 ug/l
RT: 10.299 min Scan# 1511
Delta R.T. -0.000 min
Lab File: VX041104.D
Acq: 16 Apr 2024 14:56




Instrument :
MSVOA_X
ClientSampleId :
240410075-02-VOA


Tgt Ion:106 Resp: 19623
Ion Ratio Lower Upper
106 100
91 193.4 165.5 248.3

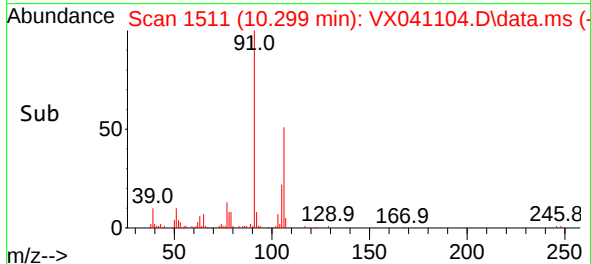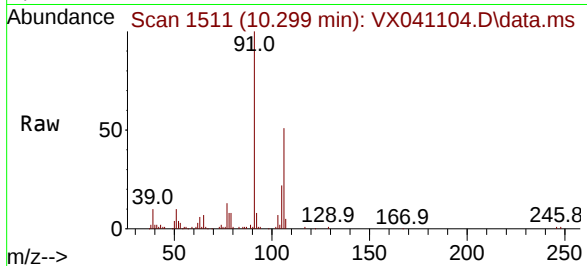

#69
o-Xylene
Concen: 4.659 ug/l
RT: 10.640 min Scan# 1567
Delta R.T. -0.000 min
Lab File: VX041104.D
Acq: 16 Apr 2024 14:56

Tgt Ion:106 Resp: 16837
Ion Ratio Lower Upper
106 100
91 208.1 108.9 326.8


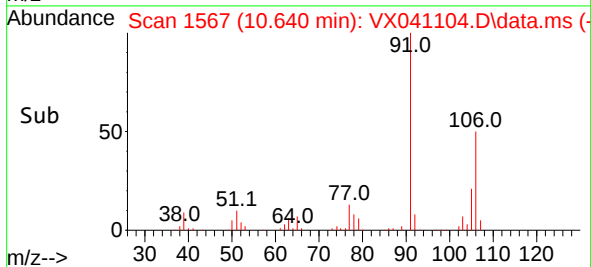

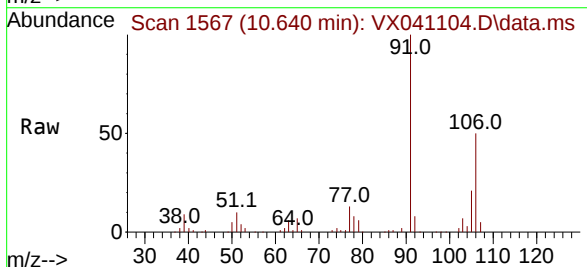




#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. -0.000 min
Lab File: VX041104.D
Acq: 16 Apr 2024 14:56




Instrument :
MSVOA_X
ClientSampleId :
240410075-02-VOA


Tgt Ion:152 Resp: 159870
Ion Ratio Lower Upper
152 100
115 52.6 43.3 129.9
150 159.5 0.0 345.0

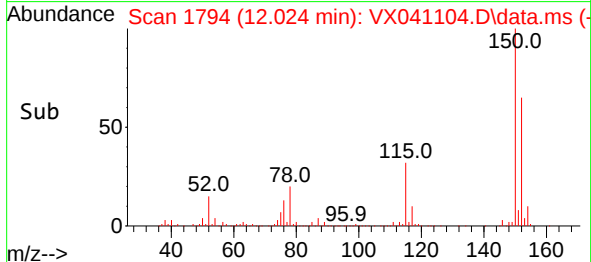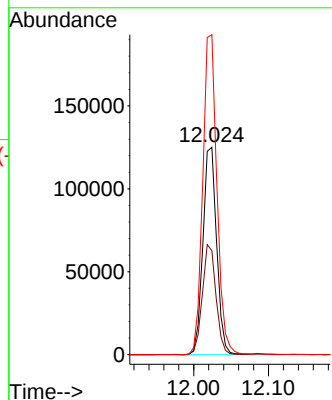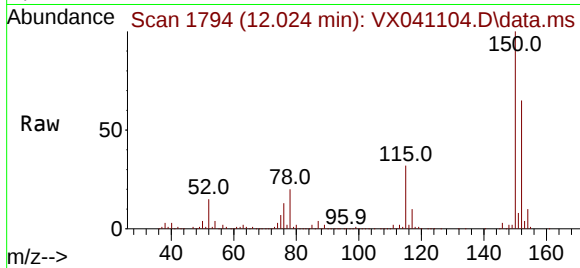

#73
Isopropylbenzene
Concen: 1.379 ug/l
RT: 10.963 min Scan# 1620
Delta R.T. -0.000 min
Lab File: VX041104.D
Acq: 16 Apr 2024 14:56

Tgt Ion:105 Resp: 13007
Ion Ratio Lower Upper
105 100
120 27.1 12.9 38.6


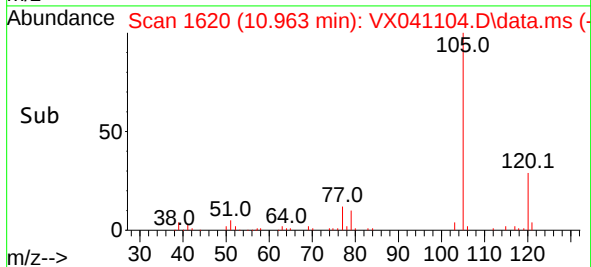
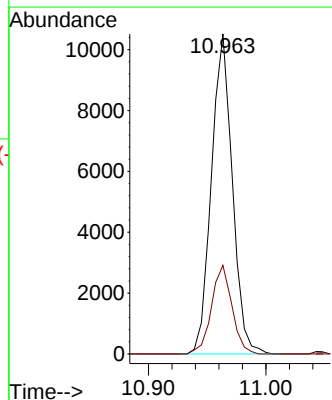
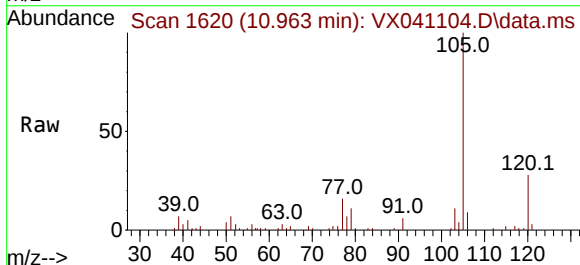


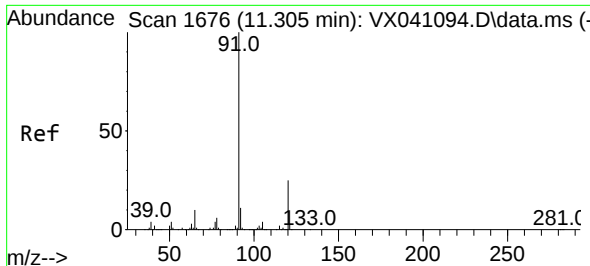

#78
n-propylbenzene
Concen: 0.552 ug/l
RT: 11.305 min Scan# 1676
Delta R.T. -0.000 min
Lab File: VX041104.D
Acq: 16 Apr 2024 14:56




Instrument :
MSVOA_X
ClientSampleId :
240410075-02-VOA


Tgt Ion: 91 Resp: 5842
Ion Ratio Lower Upper
91 100
120 23.1 11.5 34.4

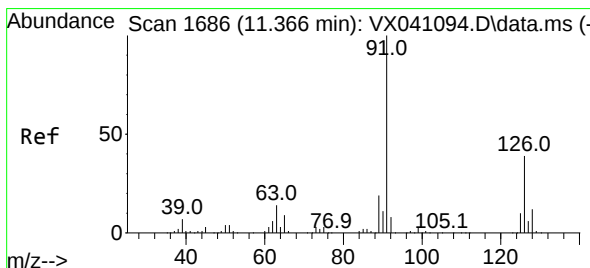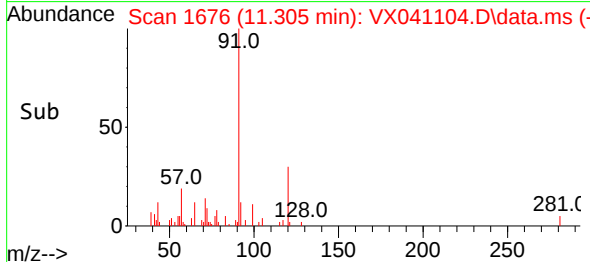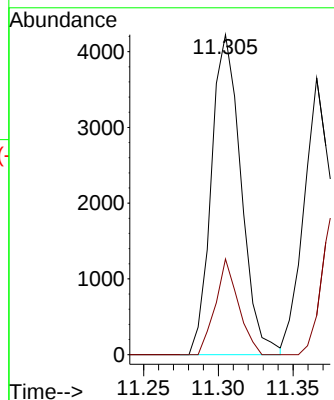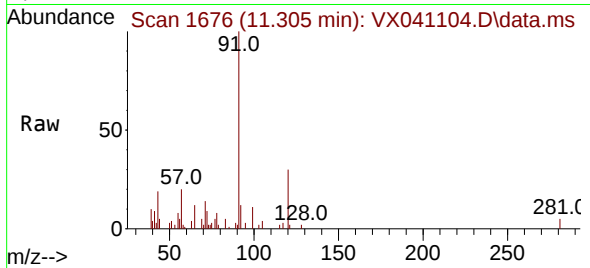

#79
2-Chlorotoluene
Concen: 0.913 ug/l
RT: 11.366 min Scan# 1686
Delta R.T. -0.000 min
Lab File: VX041104.D
Acq: 16 Apr 2024 14:56

Tgt Ion: 91 Resp: 5886
Ion Ratio Lower Upper
91 100
126 29.3 16.3 48.8


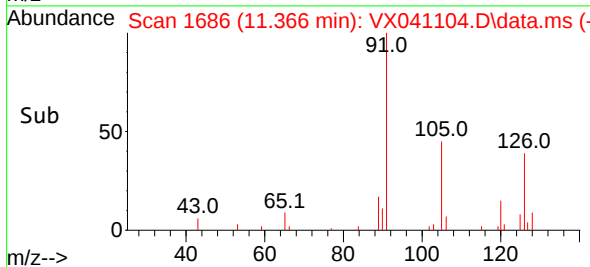
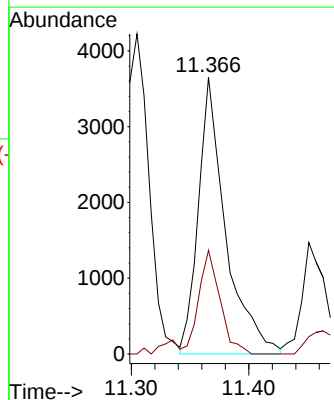
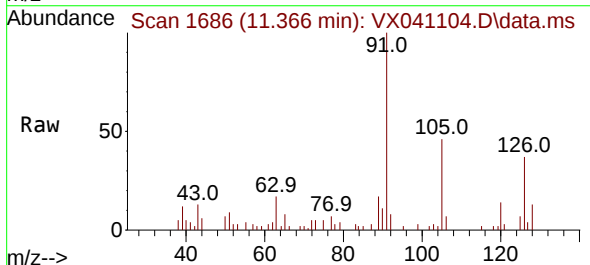




#80
 1,3,5-Trimethylbenzene
 Concen: 0.835 ug/l
 RT: 11.451 min Scan# 1700
 Delta R.T. -0.000 min
 Lab File: VX041104.D
 Acq: 16 Apr 2024 14:56




Instrument :
 MSVOA_X
 ClientSampleId :
 240410075-02-VOA


Tgt Ion:105 Resp: 6559
 Ion Ratio Lower Upper
 105 100
 120 56.0 24.1 72.3

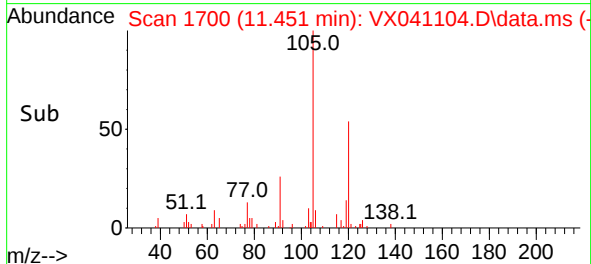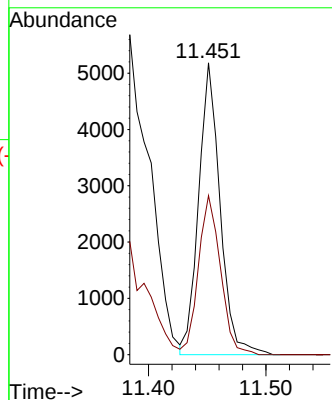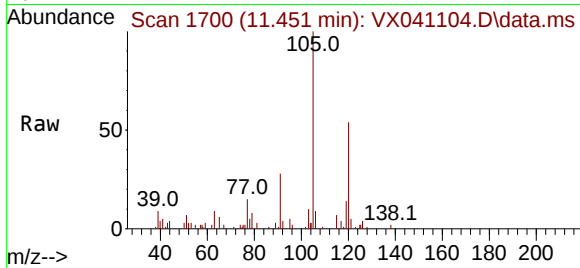

#84
 1,2,4-Trimethylbenzene
 Concen: 3.429 ug/l
 RT: 11.750 min Scan# 1749
 Delta R.T. -0.000 min
 Lab File: VX041104.D
 Acq: 16 Apr 2024 14:56

Tgt Ion:105 Resp: 26884
 Ion Ratio Lower Upper
 105 100
 120 48.0 21.2 63.6

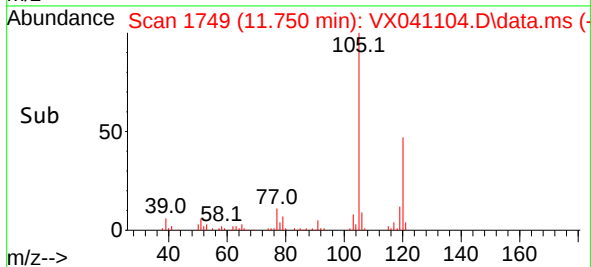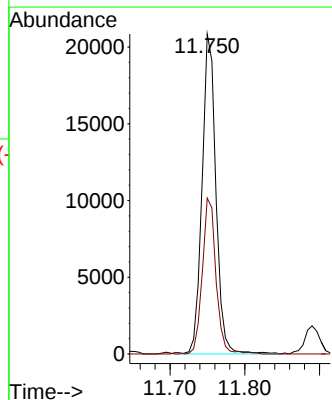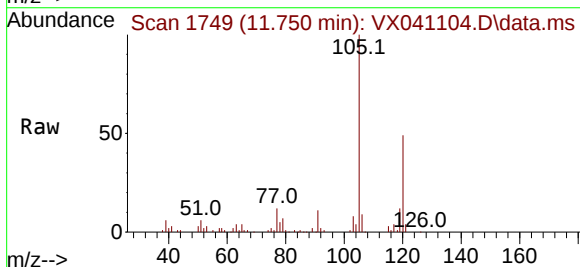

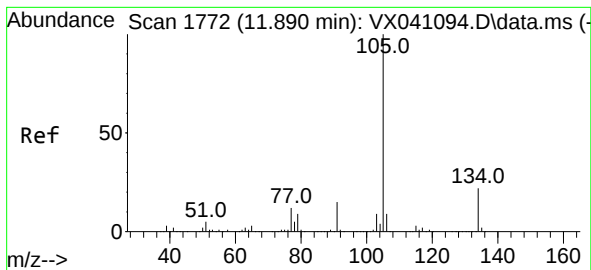

#85

sec-Butylbenzene

Concen: 0.255 ug/l

RT: 11.890 min Scan# 1772

Delta R.T. -0.000 min

Lab File: VX041104.D

Acq: 16 Apr 2024 14:56

Instrument :

MSVOA_X

ClientSampleId :





240410075-02-VOA

Tgt Ion:105 Resp: 2565

Ion Ratio Lower Upper

105 100

134 34.9 9.8 29.4#

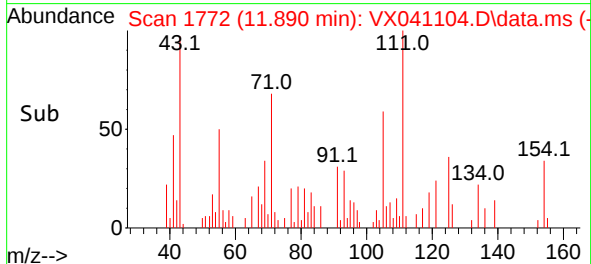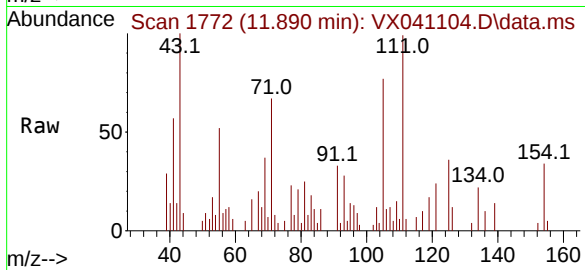

#86

p-Isopropyltoluene

Concen: 0.907 ug/l

RT: 12.012 min Scan# 1792

Delta R.T. 0.006 min

Lab File: VX041104.D

Acq: 16 Apr 2024 14:56




Tgt Ion:119 Resp: 8096


Ion Ratio Lower Upper

119 100

134 28.4 12.8 38.3

91 28.8 13.1 39.3

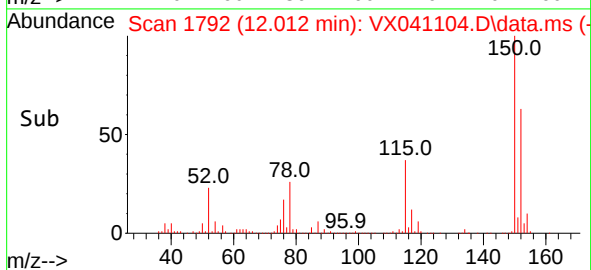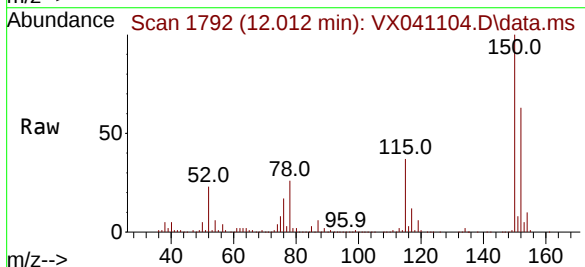



#88

1,4-Dichlorobenzene

Concen: 9.681 ug/l

RT: 12.042 min Scan# 11

Delta R.T. -0.000 min

Lab File: VX041104.D

Acq: 16 Apr 2024 14:56

Instrument :

MSVOA_X

ClientSampleId :

240410075-02-VOA





Tgt Ion:146 Resp: 53322

Ion Ratio Lower Upper

146 100

111 38.1 21.3 63.7

148 65.4 31.8 95.4

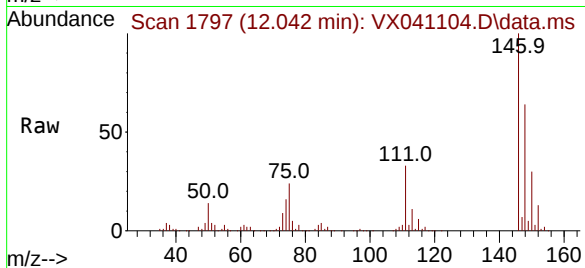

#89

n-Butylbenzene

Concen: 0.415 ug/l

RT: 12.335 min Scan# 1845

Delta R.T. 0.006 min

Lab File: VX041104.D

Acq: 16 Apr 2024 14:56




Tgt Ion: 91 Resp: 3143


Ion Ratio Lower Upper

91 100

92 44.3 27.4 82.0

134 66.9 12.6 37.8#

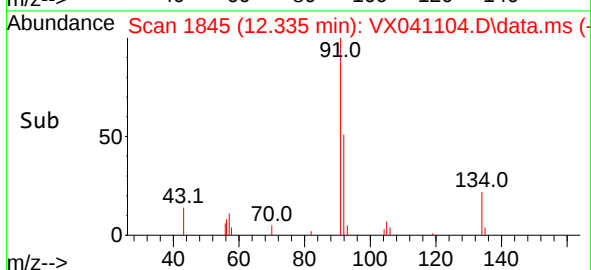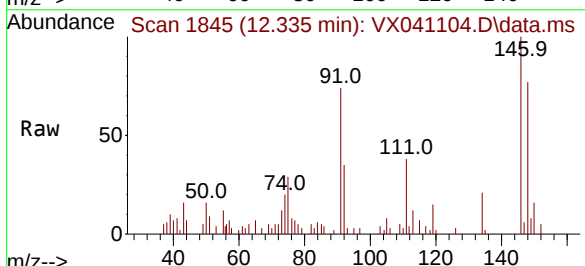



#91

1,2-Dichlorobenzene

Concen: 0.767 ug/l

RT: 12.335 min Scan# 11

Delta R.T. -0.000 min

Lab File: VX041104.D


Acq: 16 Apr 2024 14:56

Instrument :

MSVOA_X

ClientSampleId :

240410075-02-VOA

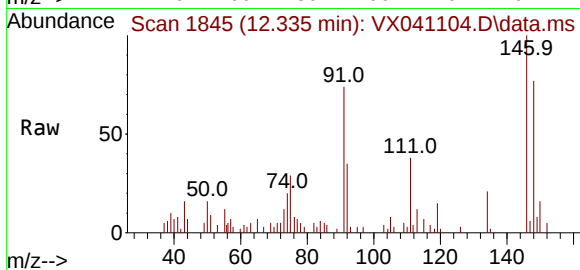




Tgt Ion:146 Resp: 3976

Ion Ratio Lower Upper

146 100

111 40.7 22.4 67.0

148 69.7 31.6 95.0

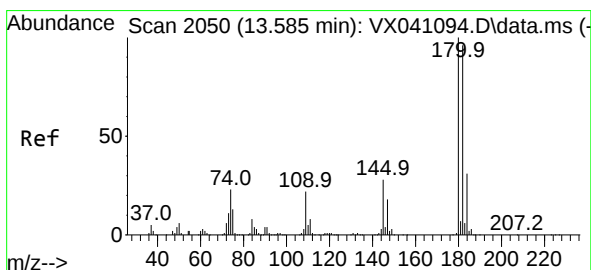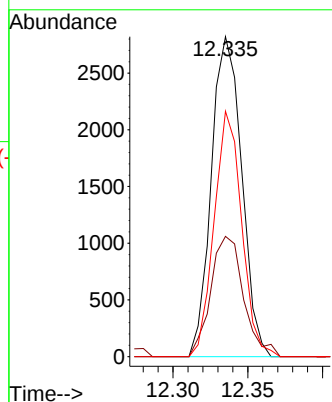

#93

1,2,4-Trichlorobenzene

Concen: 0.494 ug/l

RT: 13.591 min Scan# 2051

Delta R.T. 0.006 min

Lab File: VX041104.D

Acq: 16 Apr 2024 14:56




Tgt Ion:180 Resp: 1924


Ion Ratio Lower Upper

180 100

182 102.0 48.3 144.8

145 40.9 18.0 54.0


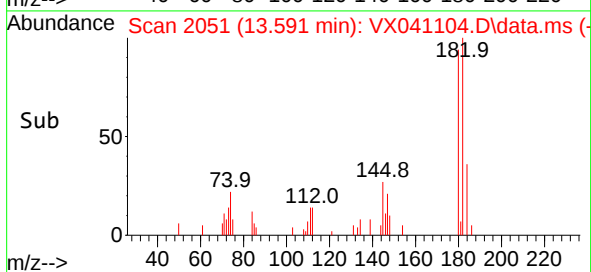
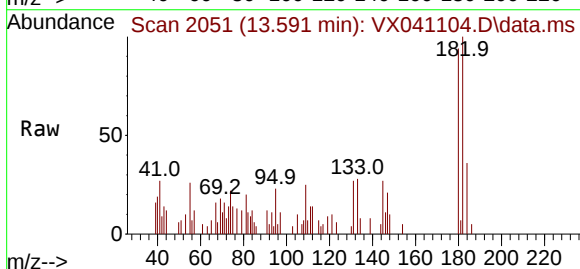
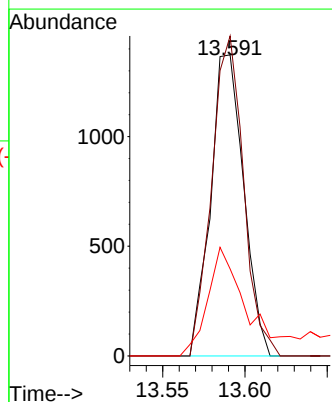




#94
Hexachlorobutadiene
Concen: 0.222 ug/l
RT: 13.725 min Scan# 2073
Delta R.T. -0.000 min
Lab File: VX041104.D
Acq: 16 Apr 2024 14:56




Instrument :
MSVOA_X
ClientSampleId :
240410075-02-VOA


Tgt Ion:	225	Resp:	413
Ion	Ratio	Lower	Upper
225	100		
223	85.5	31.1	93.2
227	76.8	32.5	97.5

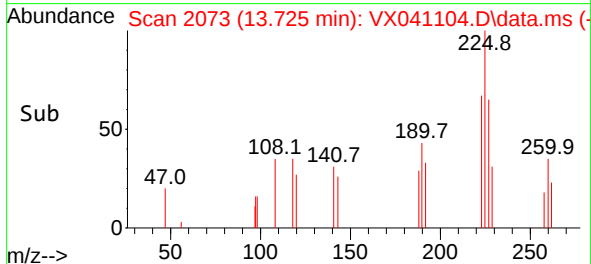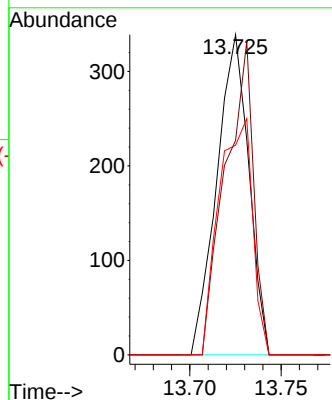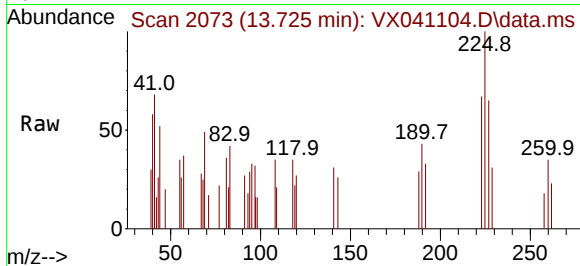

#95
Naphthalene
Concen: 8.714 ug/l
RT: 13.774 min Scan# 2081
Delta R.T. -0.000 min
Lab File: VX041104.D
Acq: 16 Apr 2024 14:56


Tgt Ion:	128	Resp:	91680
Ion	Ratio	Lower	Upper
128	100		
127	12.8	10.3	15.5
129	11.2	8.8	13.2

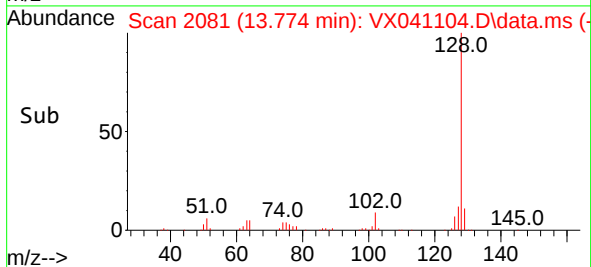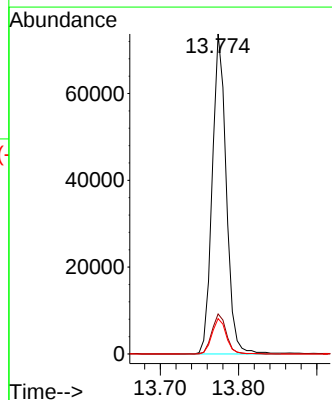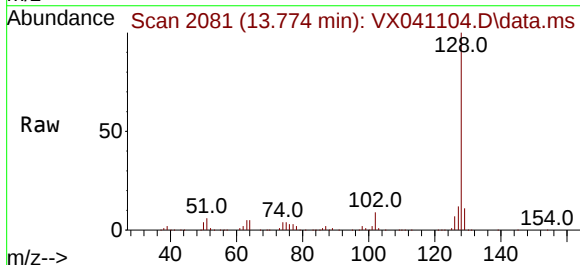



#96
 1,2,3-Trichlorobenzene
 Concen: 0.342 ug/l
 RT: 13.963 min Scan# 2112
 Delta R.T. 0.006 min
 Lab File: VX041104.D
 Acq: 16 Apr 2024 14:56

Instrument :
 MSVOA_X
 ClientSampleId :
 240410075-02-VOA

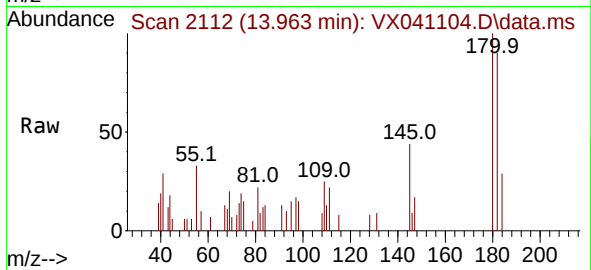

Tgt Ion:	180	Resp:	1322
Ion	Ratio	Lower	Upper
180	100		
182	101.2	46.9	140.6
145	49.2	17.8	53.5

