

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041625\
 Data File : VX045813.D
 Acq On : 16 Apr 2025 17:17
 Operator : JC/MD
 Sample : IBLK
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 IBLK

Quant Time: Apr 17 01:38:25 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X040225W.M
 Quant Title : SW846 8260
 QLast Update : Wed Apr 02 03:11:43 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.544	168	75481	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.757	114	150229	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.049	117	139284	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.018	152	61170	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.952	65	74217	53.767	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	107.540%
35) Dibromofluoromethane	5.379	113	53574	50.263	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	100.520%
50) Toluene-d8	8.647	98	185759	49.931	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	99.860%
62) 4-Bromofluorobenzene	11.079	95	70259	51.847	ug/l	0.00
Spiked Amount	50.000	Range	77 - 121	Recovery	=	103.700%


Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041625\
Data File : VX045813.D
Acq On : 16 Apr 2025 17:17
Operator : JC/MD
Sample : IBLK
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
IBLK

Quant Time: Apr 17 01:38:25 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X040225W.M
Quant Title : SW846 8260
QLast Update : Wed Apr 02 03:11:43 2025
Response via : Initial Calibration




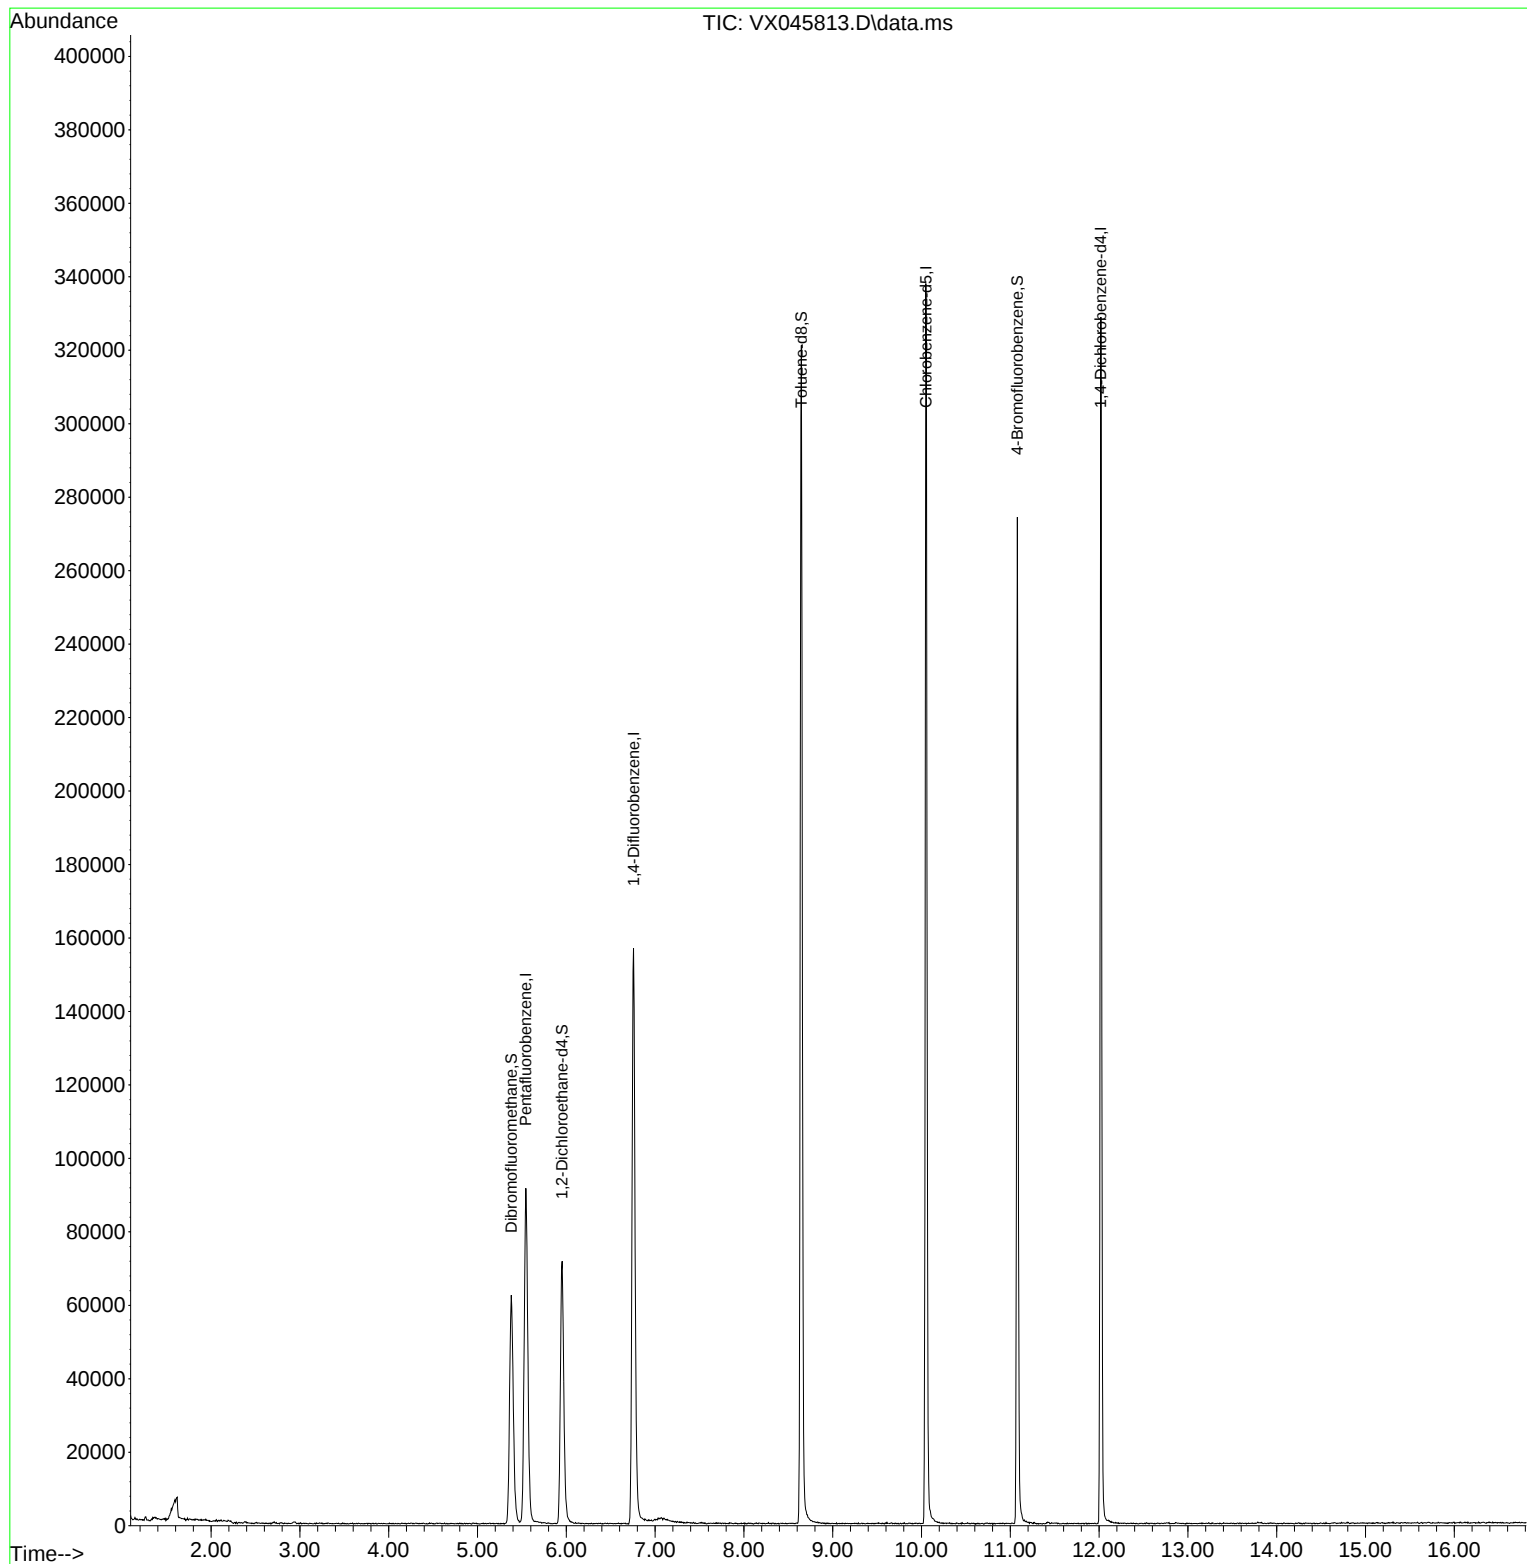




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.544 min Scan# 71
Delta R.T. -0.006 min
Lab File: VX045813.D
Acq: 16 Apr 2025 17:17




Instrument :
MSVOA_X
ClientSampleId :
IBLK

Tgt Ion:168 Resp: 75481
Ion Ratio Lower Upper
168 100
99 73.9 52.3 78.5

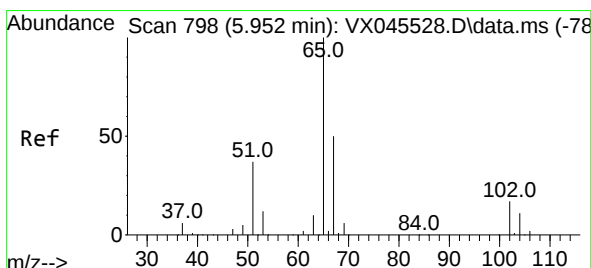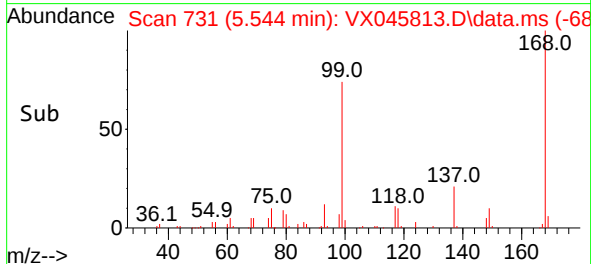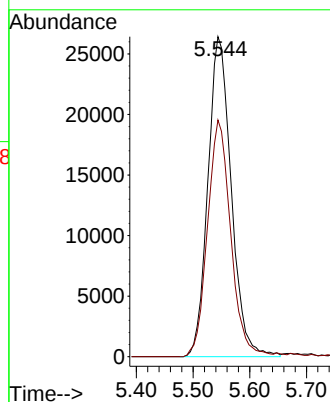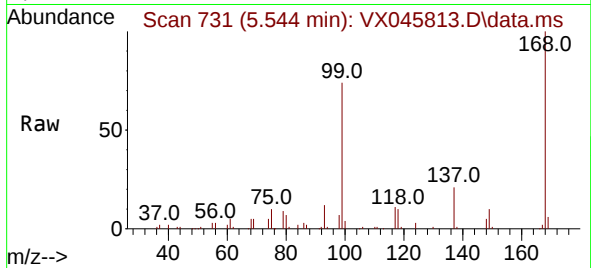

#33
1,2-Dichloroethane-d4
Concen: 53.767 ug/l
RT: 5.952 min Scan# 798
Delta R.T. 0.000 min
Lab File: VX045813.D
Acq: 16 Apr 2025 17:17

Tgt Ion: 65 Resp: 74217
Ion Ratio Lower Upper
65 100
67 48.4 0.0 99.0

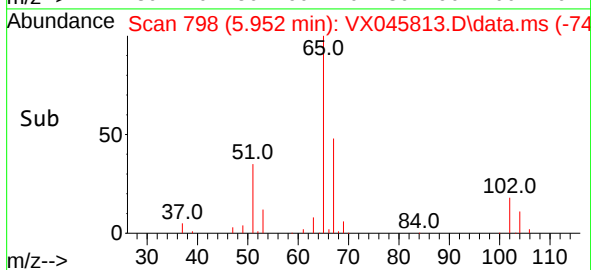
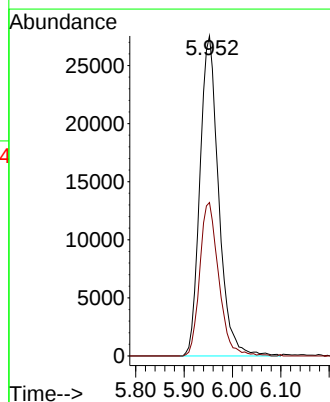
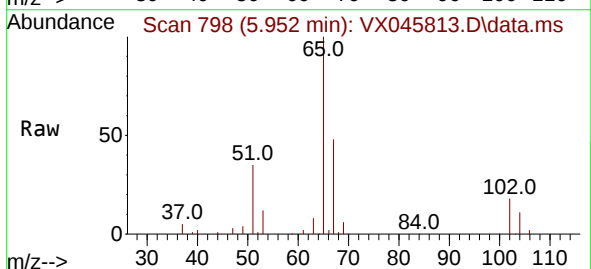




#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.757 min Scan# 91
Delta R.T. 0.000 min
Lab File: VX045813.D
Acq: 16 Apr 2025 17:17




Instrument :
MSVOA_X
ClientSampleId :
IBLK


Tgt Ion:114 Resp: 150229
Ion Ratio Lower Upper
114 100
63 22.7 0.0 46.8
88 16.7 0.0 35.4

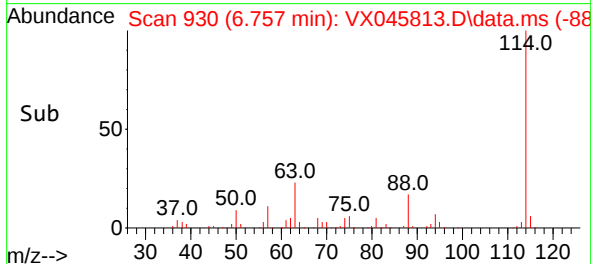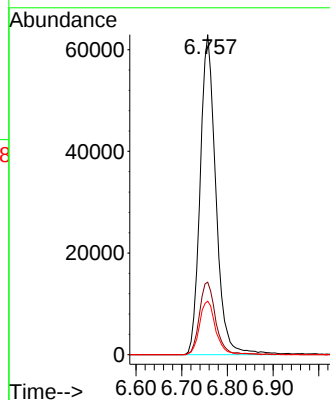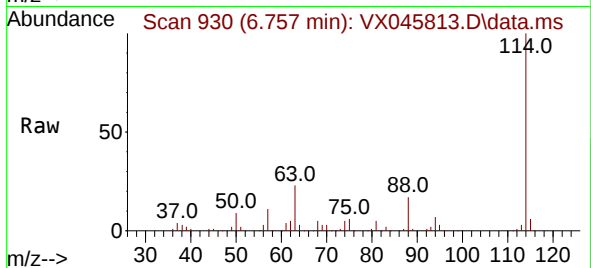

#35
Dibromofluoromethane
Concen: 50.263 ug/l
RT: 5.379 min Scan# 704
Delta R.T. 0.000 min
Lab File: VX045813.D
Acq: 16 Apr 2025 17:17

Tgt Ion:113 Resp: 53574
Ion Ratio Lower Upper
113 100
111 101.9 81.8 122.6
192 16.2 13.8 20.6


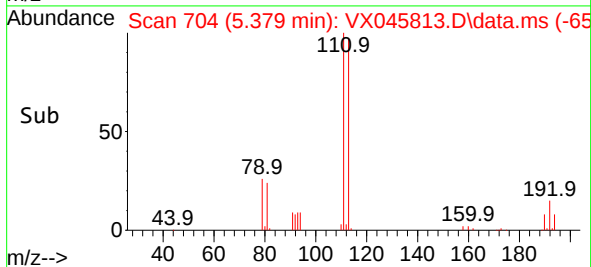
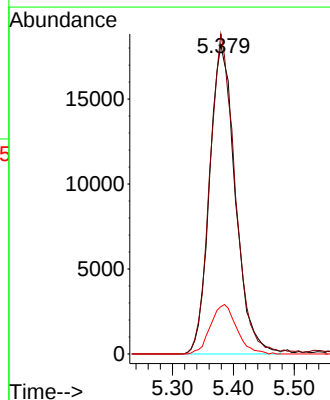
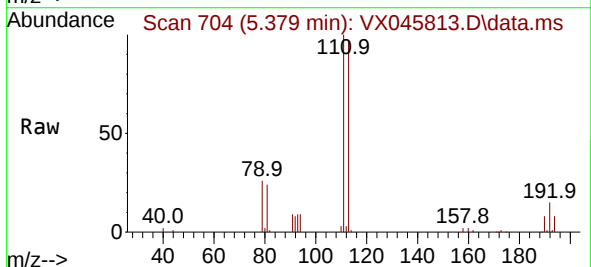


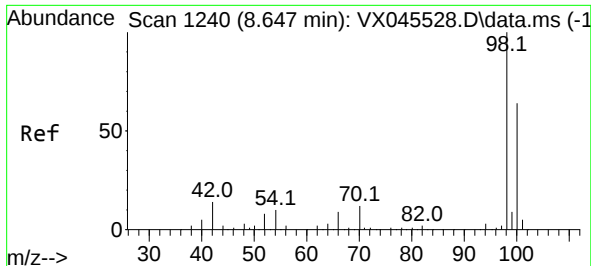

#50
Toluene-d8
Concen: 49.931 ug/l
RT: 8.647 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX045813.D
Acq: 16 Apr 2025 17:17




Instrument :
MSVOA_X
ClientSampleId :
IBLK


Tgt Ion: 98 Resp: 185759
Ion Ratio Lower Upper
98 100
100 64.5 52.2 78.4

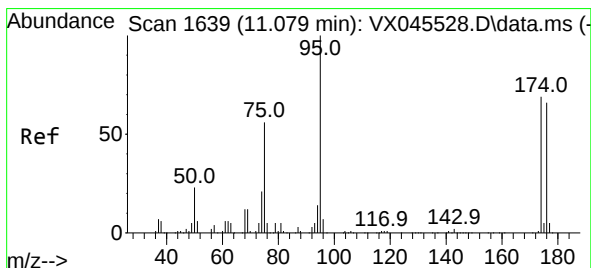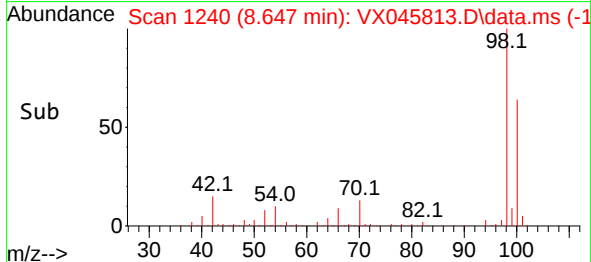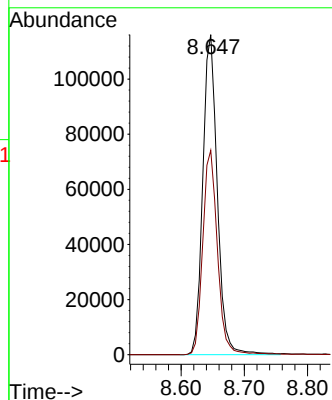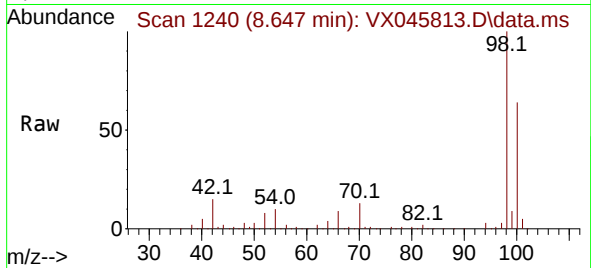

#62
4-Bromofluorobenzene
Concen: 51.847 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.000 min
Lab File: VX045813.D
Acq: 16 Apr 2025 17:17

Tgt Ion: 95 Resp: 70259
Ion Ratio Lower Upper
95 100
174 67.3 0.0 135.8
176 66.0 0.0 131.4

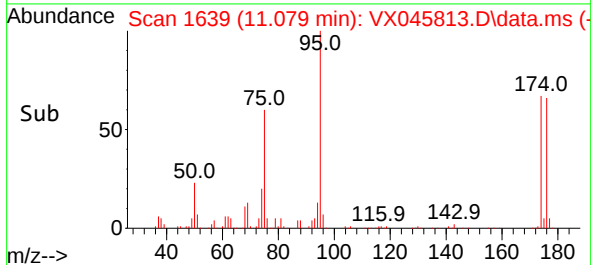
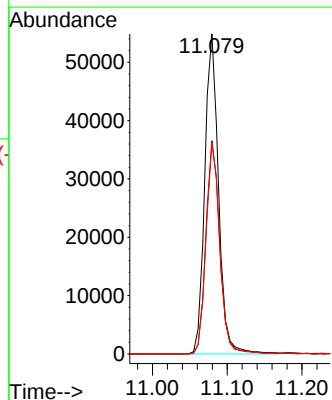
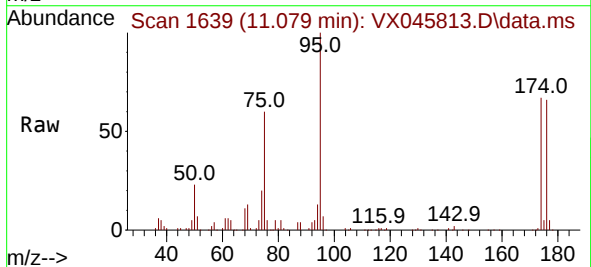


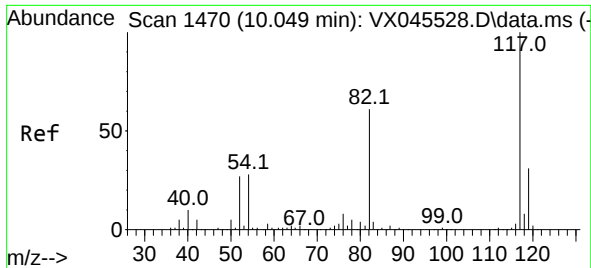

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.049 min Scan# 1470
Delta R.T. 0.000 min
Lab File: VX045813.D
Acq: 16 Apr 2025 17:17

Instrument :
MSVOA_X
ClientSampleId :
IBLK

Tgt Ion:117 Resp: 139284
Ion Ratio Lower Upper
117 100
82 62.6 49.2 73.8
119 31.1 25.1 37.7

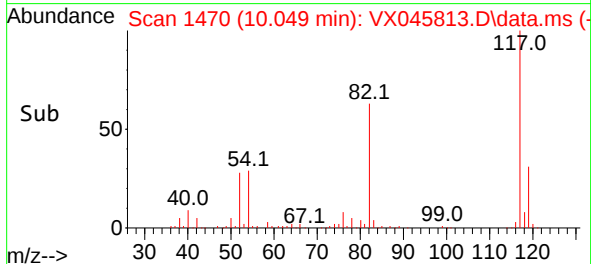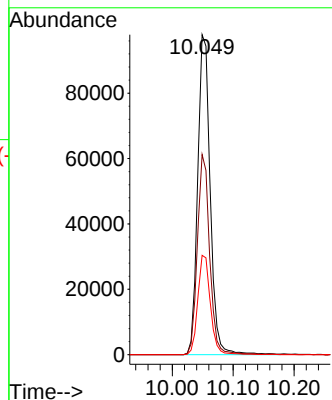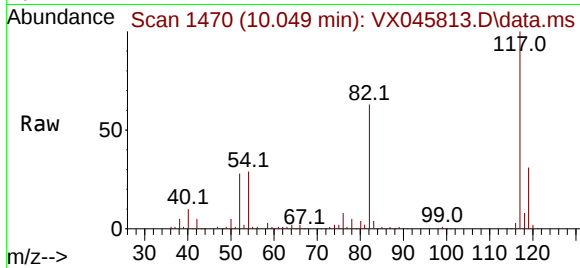

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.018 min Scan# 1793
Delta R.T. 0.000 min
Lab File: VX045813.D
Acq: 16 Apr 2025 17:17

Tgt Ion:152 Resp: 61170
Ion Ratio Lower Upper
152 100
115 62.8 46.9 140.7
150 155.0 0.0 349.4

