

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX041719\  
Data File : VX009025.D  
Acq On : 17 Apr 2019 19:17  
Operator : JC/SP  
Sample : K2449-03  
Misc : 5.0mL/MSVOA X/WATER  
ALS Vial : 23 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
SS042MW127-190415

## Integration Parameters: RTEINT.P

Integrator: RTE  
Smoothing : ON Filtering: 5  
Sampling : 1 Min Area: 3 % of largest Peak  
Start Thrs: 0.2 Max Peaks: 100  
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >  
Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA\_X\METHOD\82X041519W.M  
Title : SW846 8260

Signal : TIC

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 4.598       | 556           | 565         | 575          | rBV      | 9498           | 27729         | 2.05%           | 0.403%        |
| 2         | 5.501       | 699           | 713         | 727          | rBV      | 140970         | 407948        | 30.17%          | 5.931%        |
| 3         | 5.665       | 728           | 740         | 753          | rVB      | 260558         | 734818        | 54.34%          | 10.683%       |
| 4         | 6.061       | 794           | 805         | 819          | rBV      | 179611         | 469986        | 34.76%          | 6.833%        |
| 5         | 6.860       | 925           | 936         | 949          | rBV      | 419997         | 983195        | 72.71%          | 14.294%       |
| 6         | 7.214       | 986           | 994         | 1003         | rBV6     | 5773           | 14350         | 1.06%           | 0.209%        |
| 7         | 8.713       | 1231          | 1240        | 1255         | rBV      | 867656         | 1352166       | 100.00%         | 19.658%       |
| 8         | 9.335       | 1336          | 1342        | 1350         | rBV      | 49205          | 71943         | 5.32%           | 1.046%        |
| 9         | 10.110      | 1462          | 1469        | 1482         | rBV      | 809877         | 1090671       | 80.66%          | 15.857%       |
| 10        | 11.134      | 1630          | 1637        | 1651         | rBV      | 610371         | 802710        | 59.36%          | 11.670%       |
| 11        | 12.079      | 1784          | 1792        | 1803         | rBV      | 720728         | 922797        | 68.25%          | 13.416%       |


Sum of corrected areas: 6878313

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX041719\  
Data File : VX009025.D  
Acq On : 17 Apr 2019 19:17  
Operator : JC/SP  
Sample : K2449-03  
Misc : 5.0mL/MSVOA X/WATER  
ALS Vial : 23 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
SS042MW127-190415

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA\_X\METHOD\82X041519W.M  
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

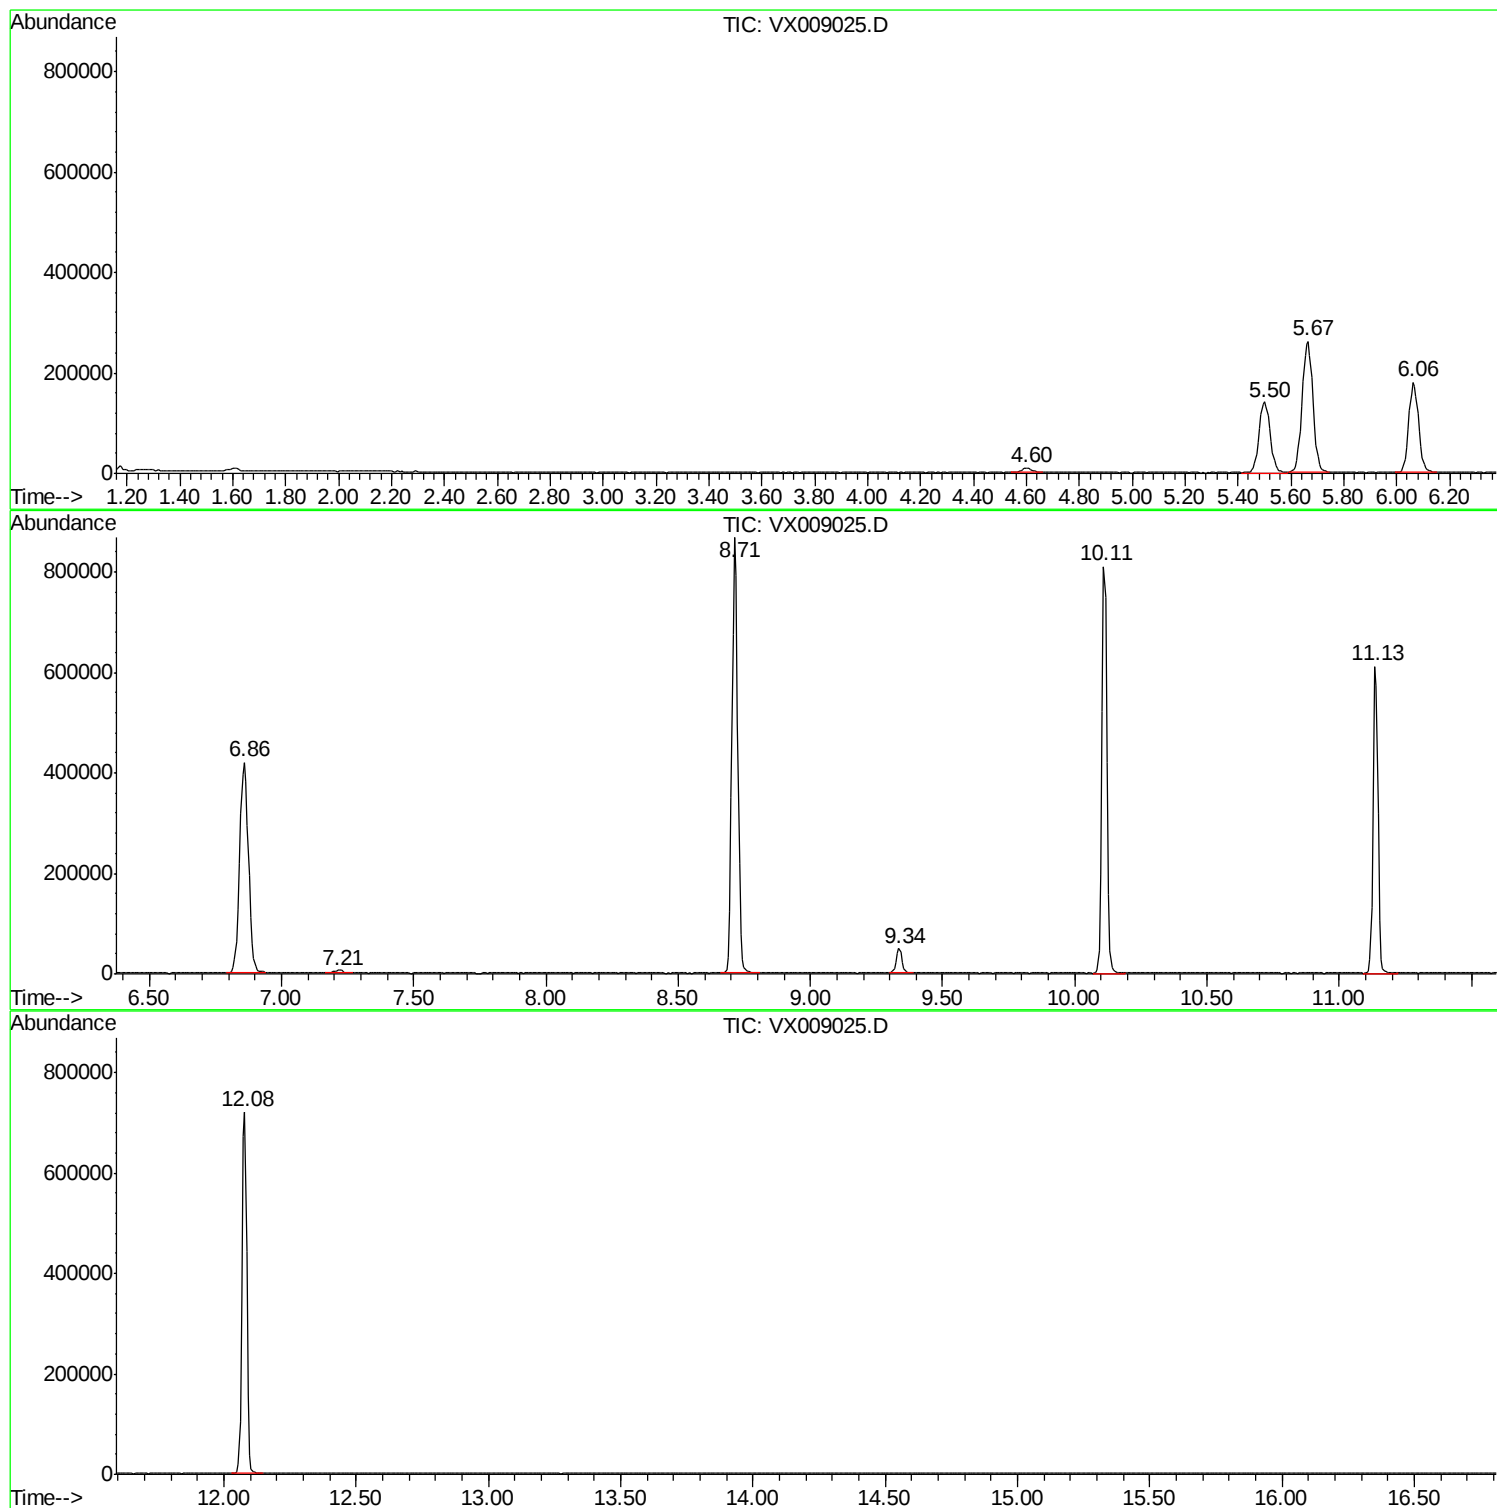

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA\_X\DATA\VX041719\  
Data File : VX009025.D  
Acq On : 17 Apr 2019 19:17  
Operator : JC/SP  
Sample : K2449-03  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 23 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
SS042MW127-190415

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA\_X\METHOD\82X041519W.M  
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA\_X\DATA\VX041719\  
Data File : VX009025.D  
Acq On : 17 Apr 2019 19:17  
Operator : JC/SP  
Sample : K2449-03  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 23 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
SS042MW127-190415

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA\_X\METHOD\82X041519W.M  
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | ---Internal Standard--- |
|------------------|----|---------|-------|----------|-------------------------|
|                  |    |         |       |          | # RT Resp Conc          |