

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041724\
 Data File : VX041137.D
 Acq On : 17 Apr 2024 19:57
 Operator : JC/MD
 Sample : P2037-10
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :

Quant Time: Apr 18 02:24:43 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041724WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Apr 18 02:15:13 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.763	114	281017	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	252426	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	116346	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.368	65	92962	46.231	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	92.460%
7) Chloroethane-d5	1.648	69	45931	45.900	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	91.800%
11) 1,1-Dichloroethene-d2	2.288	65	40324	46.808	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	93.620%
21) 2-Butanone-d5	4.471	46	128484	111.929	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	111.930%
24) Chloroform-d	5.056	84	174846	47.241	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	94.480%
26) 1,2-Dichloroethane-d4	5.952	65	116271	49.436	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	98.880%
32) Benzene-d6	5.970	84	368629	50.698	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	101.400%
36) 1,2-Dichloropropane-d6	7.305	67	106968	50.824	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	101.640%
41) Toluene-d8	8.647	98	328126	48.106	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	96.220%
43) trans-1,3-Dichloroprop...	8.952	79	43266	45.953	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	91.900%
47) 2-Hexanone-d5	9.390	63	88879	104.014	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	104.010%
56) 1,1,2,2-Tetrachloroeth...	11.195	84	153455	49.975	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	99.940%
66) 1,2-Dichlorobenzene-d4	12.323	152	132704	53.038	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	106.080%
Target Compounds						
					Qvalue	
13) Acetone	2.392	43	7192	7.811	ug/L	98
61) 1,2,3-Trichloropropane	12.018	75	11071	5.772	ug/L #	63


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041724\
Data File : VX041137.D
Acq On : 17 Apr 2024 19:57
Operator : JC/MD
Sample : P2037-10
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :

Quant Time: Apr 18 02:24:43 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041724WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Apr 18 02:15:13 2024
Response via : Initial Calibration

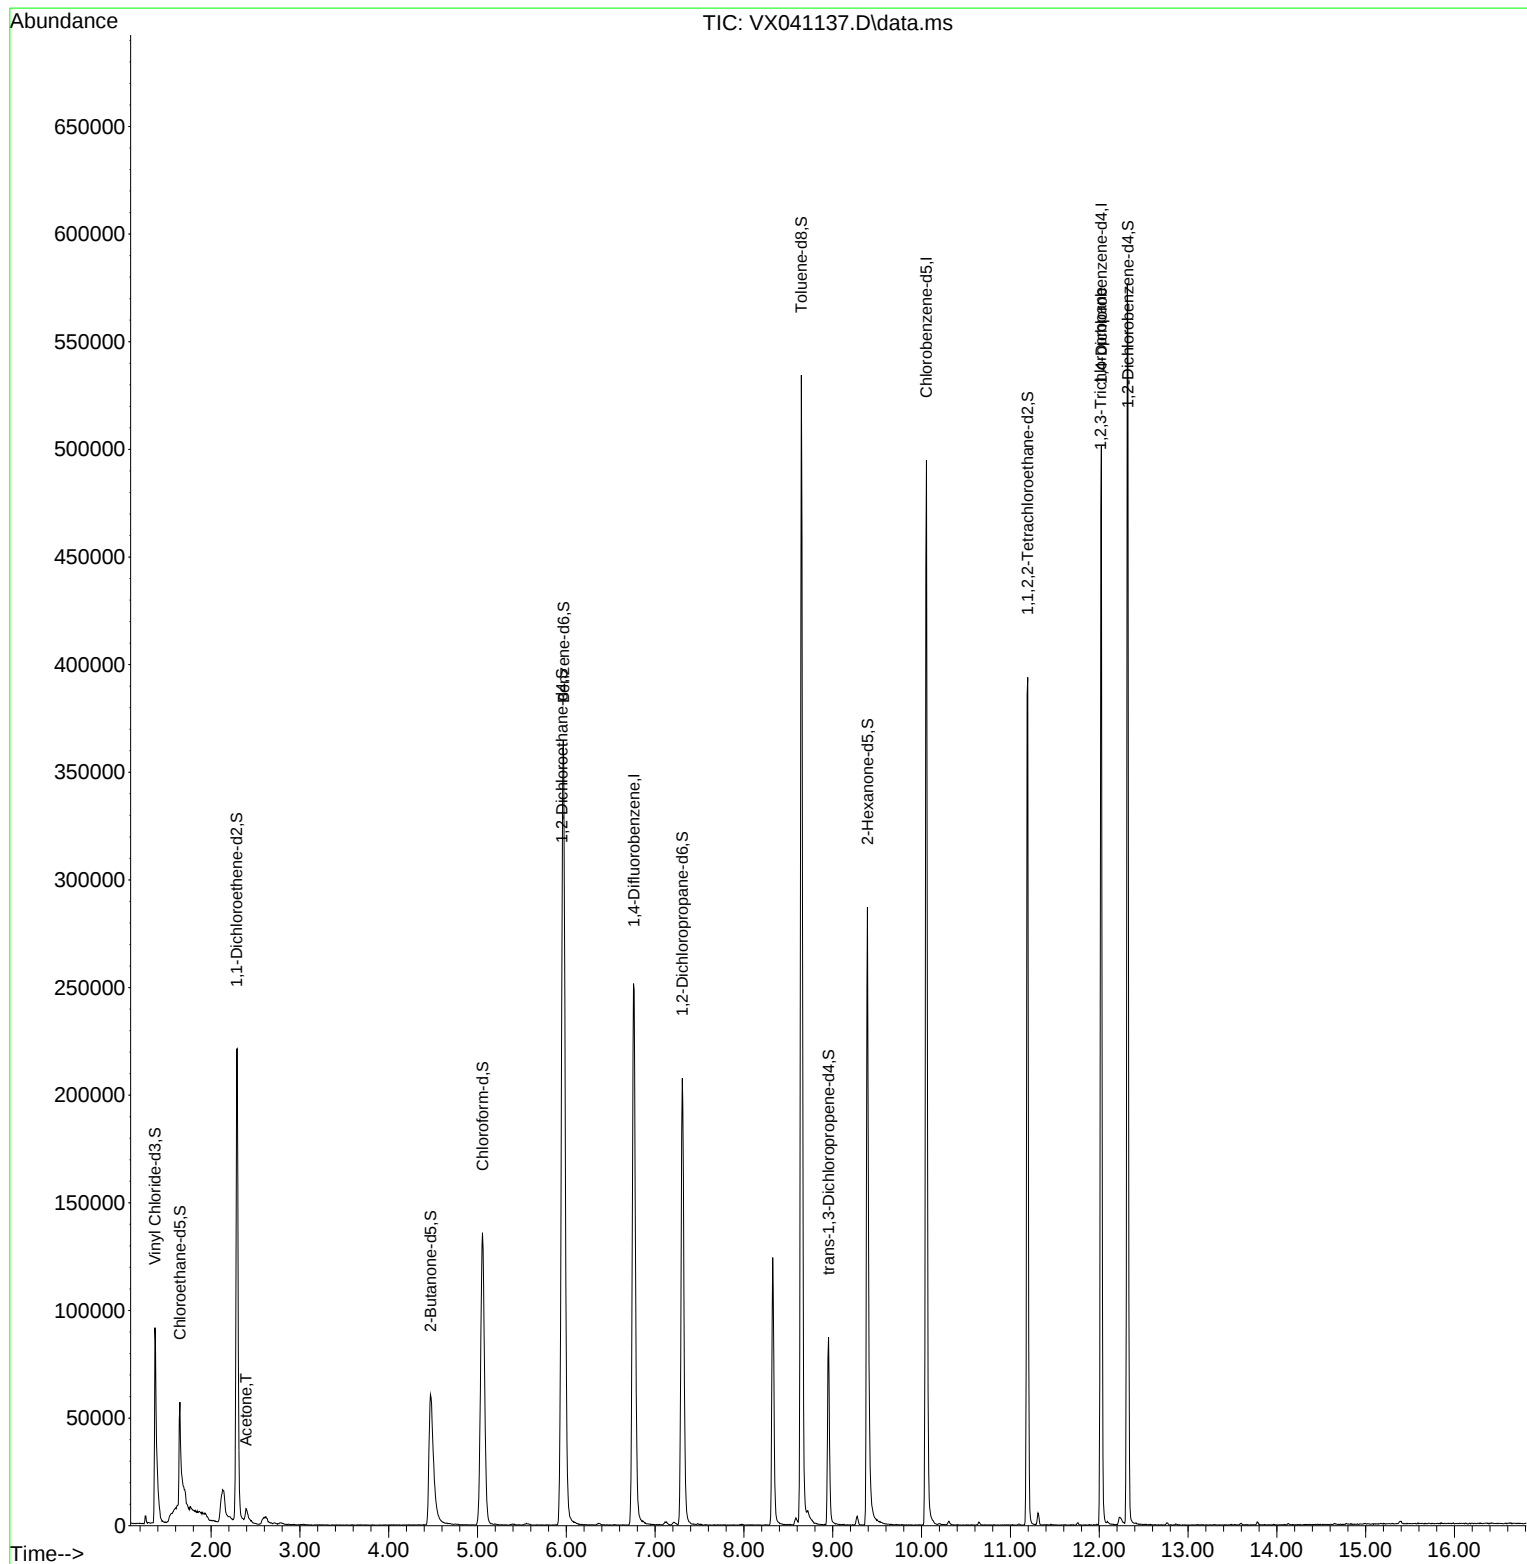

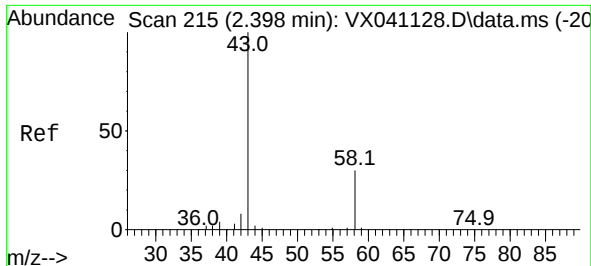

#13

Acetone

Concen: 7.811 ug/L

RT: 2.392 min Scan# 215

Delta R.T. -0.006 min

Lab File: VX041137.D

Acq: 17 Apr 2024 19:57

Instrument :

MSVOA_X





ClientSampleId :

Tgt Ion: 43 Resp: 7192

Ion Ratio Lower Upper

43 100

58 29.8 0.0 62.4

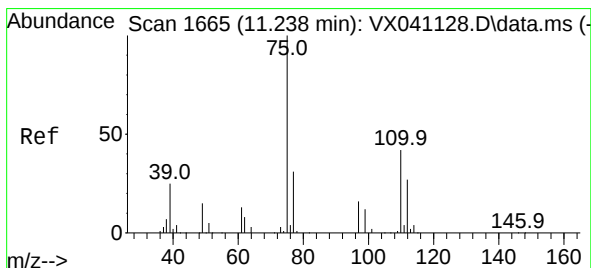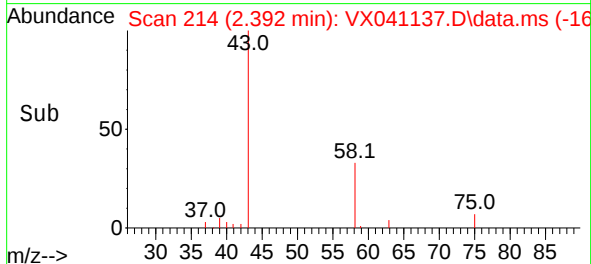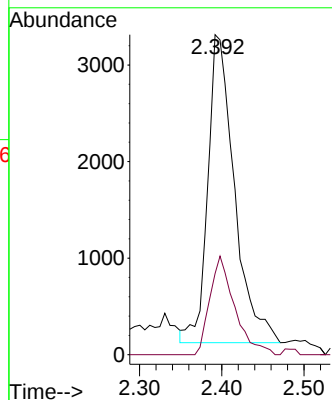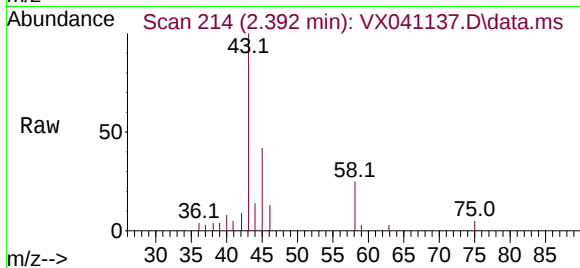

#61

1,2,3-Trichloropropane

Concen: 5.772 ug/L

RT: 12.018 min Scan# 1793

Delta R.T. 0.780 min

Lab File: VX041137.D

Acq: 17 Apr 2024 19:57

Tgt Ion: 75 Resp: 11071

Ion Ratio Lower Upper

75 100

77 33.1 25.5 38.3

110 3.1 35.0 52.6#

