

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041724\
 Data File : VX041141.D
 Acq On : 17 Apr 2024 21:29
 Operator : JC/MD
 Sample : P2078-20
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :

Quant Time: Apr 18 02:25:37 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041724WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Apr 18 02:15:13 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.757	114	275411	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	247274	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	113163	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.367	65	94023	47.710	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	95.420%		
7) Chloroethane-d5	1.648	69	44657	45.535	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	91.080%		
11) 1,1-Dichloroethene-d2	2.294	65	40440	47.898	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	95.800%		
21) 2-Butanone-d5	4.464	46	120911	107.476	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	107.480%		
24) Chloroform-d	5.056	84	172931	47.675	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	95.340%		
26) 1,2-Dichloroethane-d4	5.952	65	115086	49.928	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	99.860%		
32) Benzene-d6	5.970	84	363932	51.095	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	102.200%		
36) 1,2-Dichloropropane-d6	7.305	67	105726	51.281	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	102.560%		
41) Toluene-d8	8.647	98	324623	48.584	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	97.160%		
43) trans-1,3-Dichloroprop...	8.951	79	40547	43.962	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	87.920%		
47) 2-Hexanone-d5	9.390	63	85895	102.617	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	102.620%		
56) 1,1,2,2-Tetrachloroeth...	11.189	84	147706	49.105	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	98.200%		
66) 1,2-Dichlorobenzene-d4	12.323	152	131595	54.074	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	108.140%		
Target Compounds						
					Qvalue	
61) 1,2,3-Trichloropropane	12.024	75	10625	5.695	ug/L #	62


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041724\
Data File : VX041141.D
Acq On : 17 Apr 2024 21:29
Operator : JC/MD
Sample : P2078-20
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :

Quant Time: Apr 18 02:25:37 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041724WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Apr 18 02:15:13 2024
Response via : Initial Calibration

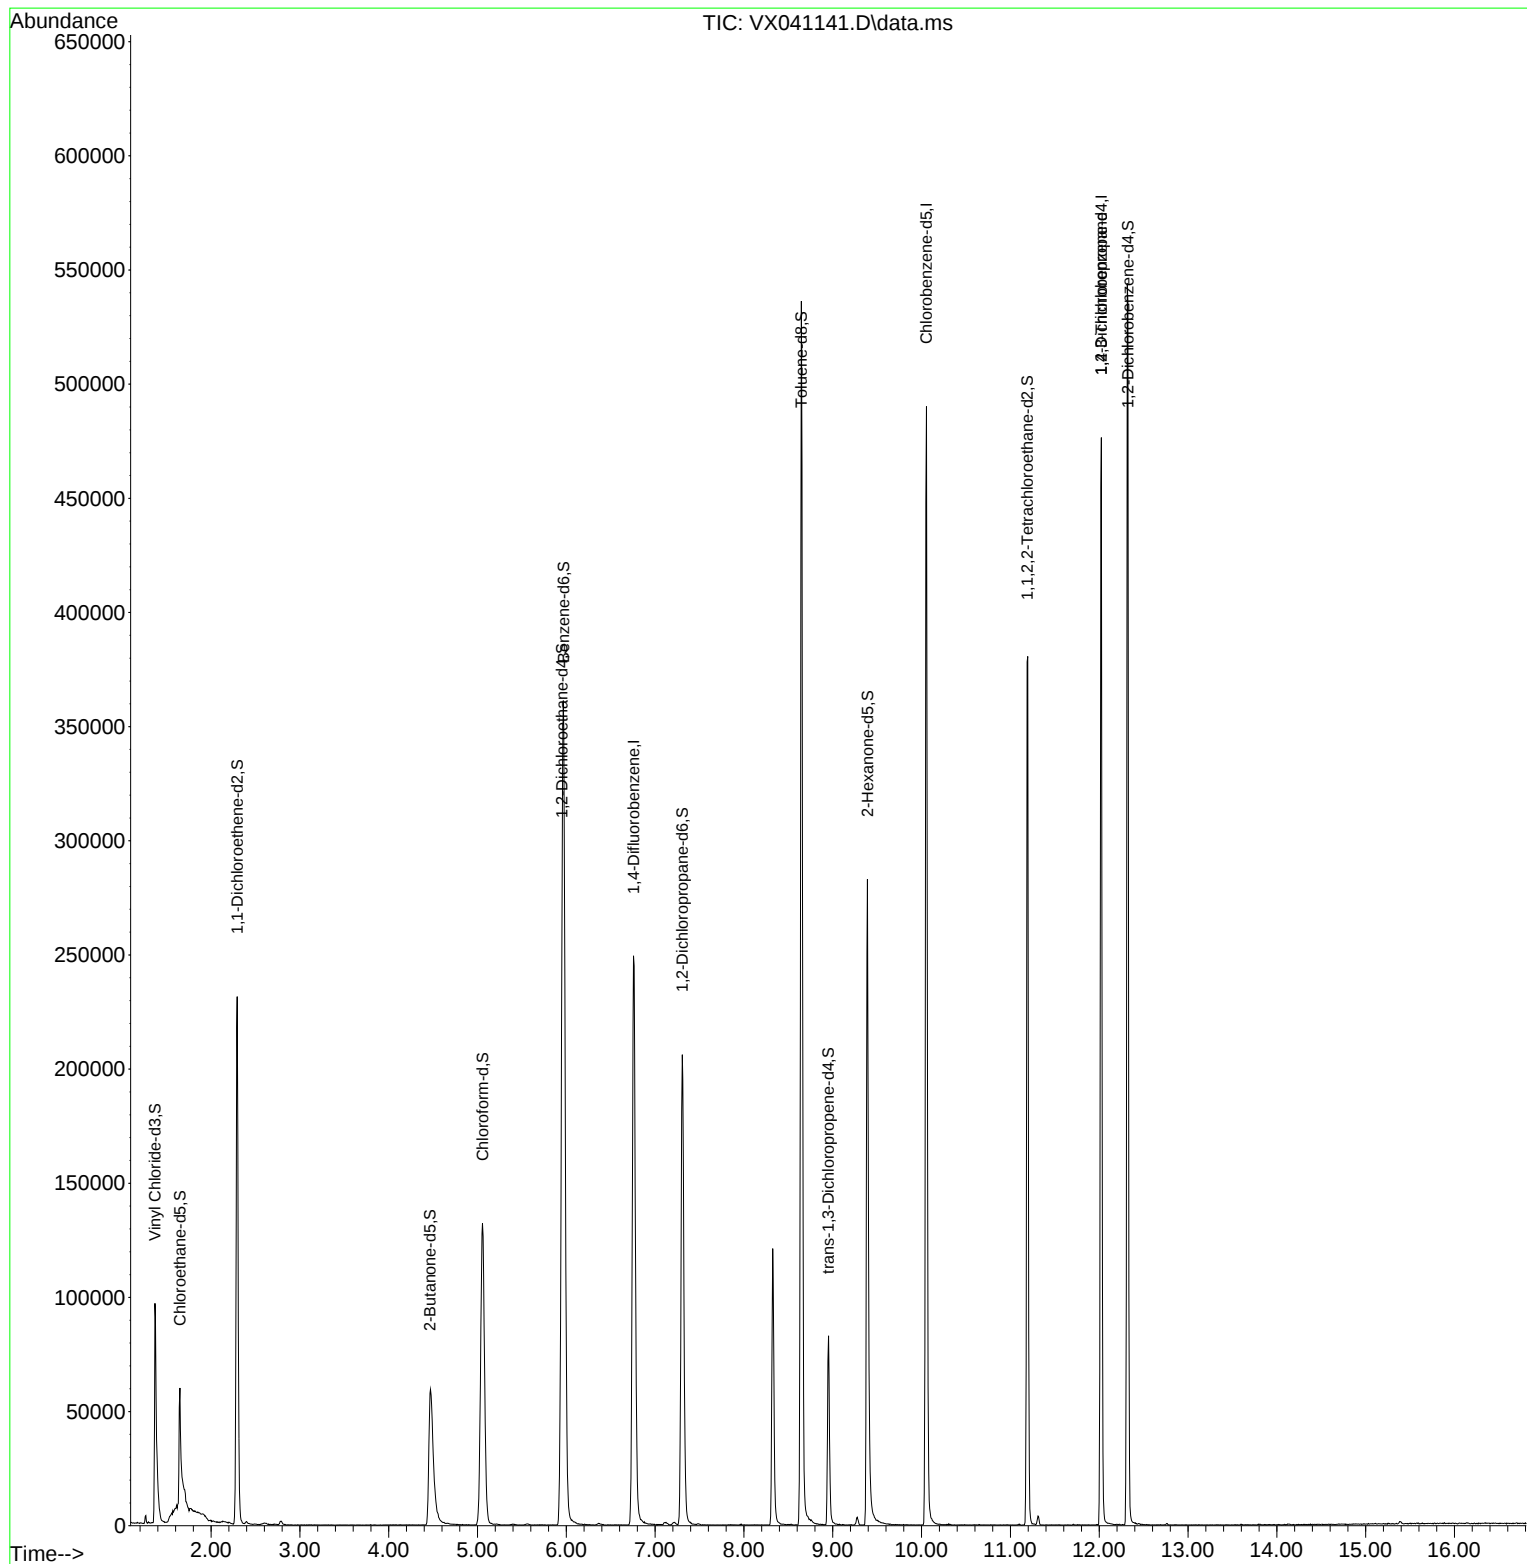

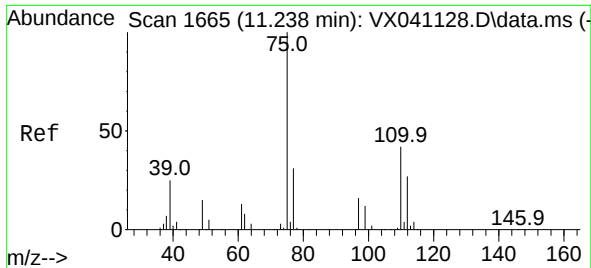

#61

1,2,3-Trichloropropane

Concen: 5.695 ug/L

RT: 12.024 min Scan# 11

Delta R.T. 0.786 min


Lab File: VX041141.D

Acq: 17 Apr 2024 21:29

Instrument :

MSVOA_X

ClientSampleId :

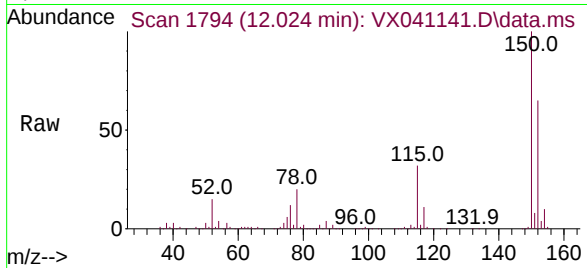

Tgt Ion: 75 Resp: 10625

Ion Ratio Lower Upper

75 100

77 33.6 25.5 38.3

110 2.7 35.0 52.6#

