

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041724\
 Data File : VX041149.D
 Acq On : 18 Apr 2024 00:32
 Operator : JC/MD
 Sample : P2039-04
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :

Quant Time: Apr 18 02:27:48 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041724WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Apr 18 02:15:13 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.757	114	273776	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	244447	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	111555	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.368	65	96433	49.226	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	98.460%
7) Chloroethane-d5	1.648	69	47416	48.637	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	97.280%
11) 1,1-Dichloroethene-d2	2.294	65	41464	49.404	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	98.800%
21) 2-Butanone-d5	4.465	46	135235	120.927	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	120.930%
24) Chloroform-d	5.056	84	177335	49.181	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	98.360%
26) 1,2-Dichloroethane-d4	5.952	65	116896	51.016	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	102.040%
32) Benzene-d6	5.970	84	375214	53.288	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	106.580%
36) 1,2-Dichloropropane-d6	7.306	67	108744	53.355	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	106.700%
41) Toluene-d8	8.647	98	336960	51.014	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	102.020%
43) trans-1,3-Dichloroprop...	8.952	79	43009	47.171	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	94.340%
47) 2-Hexanone-d5	9.391	63	93478	112.967	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	112.970%
56) 1,1,2,2-Tetrachloroeth...	11.189	84	156283	52.557	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	105.120%
66) 1,2-Dichlorobenzene-d4	12.323	152	134254	55.962	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	111.920%
Target Compounds						
39) cis-1,3-Dichloropropene	8.324	75	3120	1.239	ug/L	Qvalue # 66


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041724\
Data File : VX041149.D
Acq On : 18 Apr 2024 00:32
Operator : JC/MD
Sample : P2039-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :

Quant Time: Apr 18 02:27:48 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041724WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Apr 18 02:15:13 2024
Response via : Initial Calibration

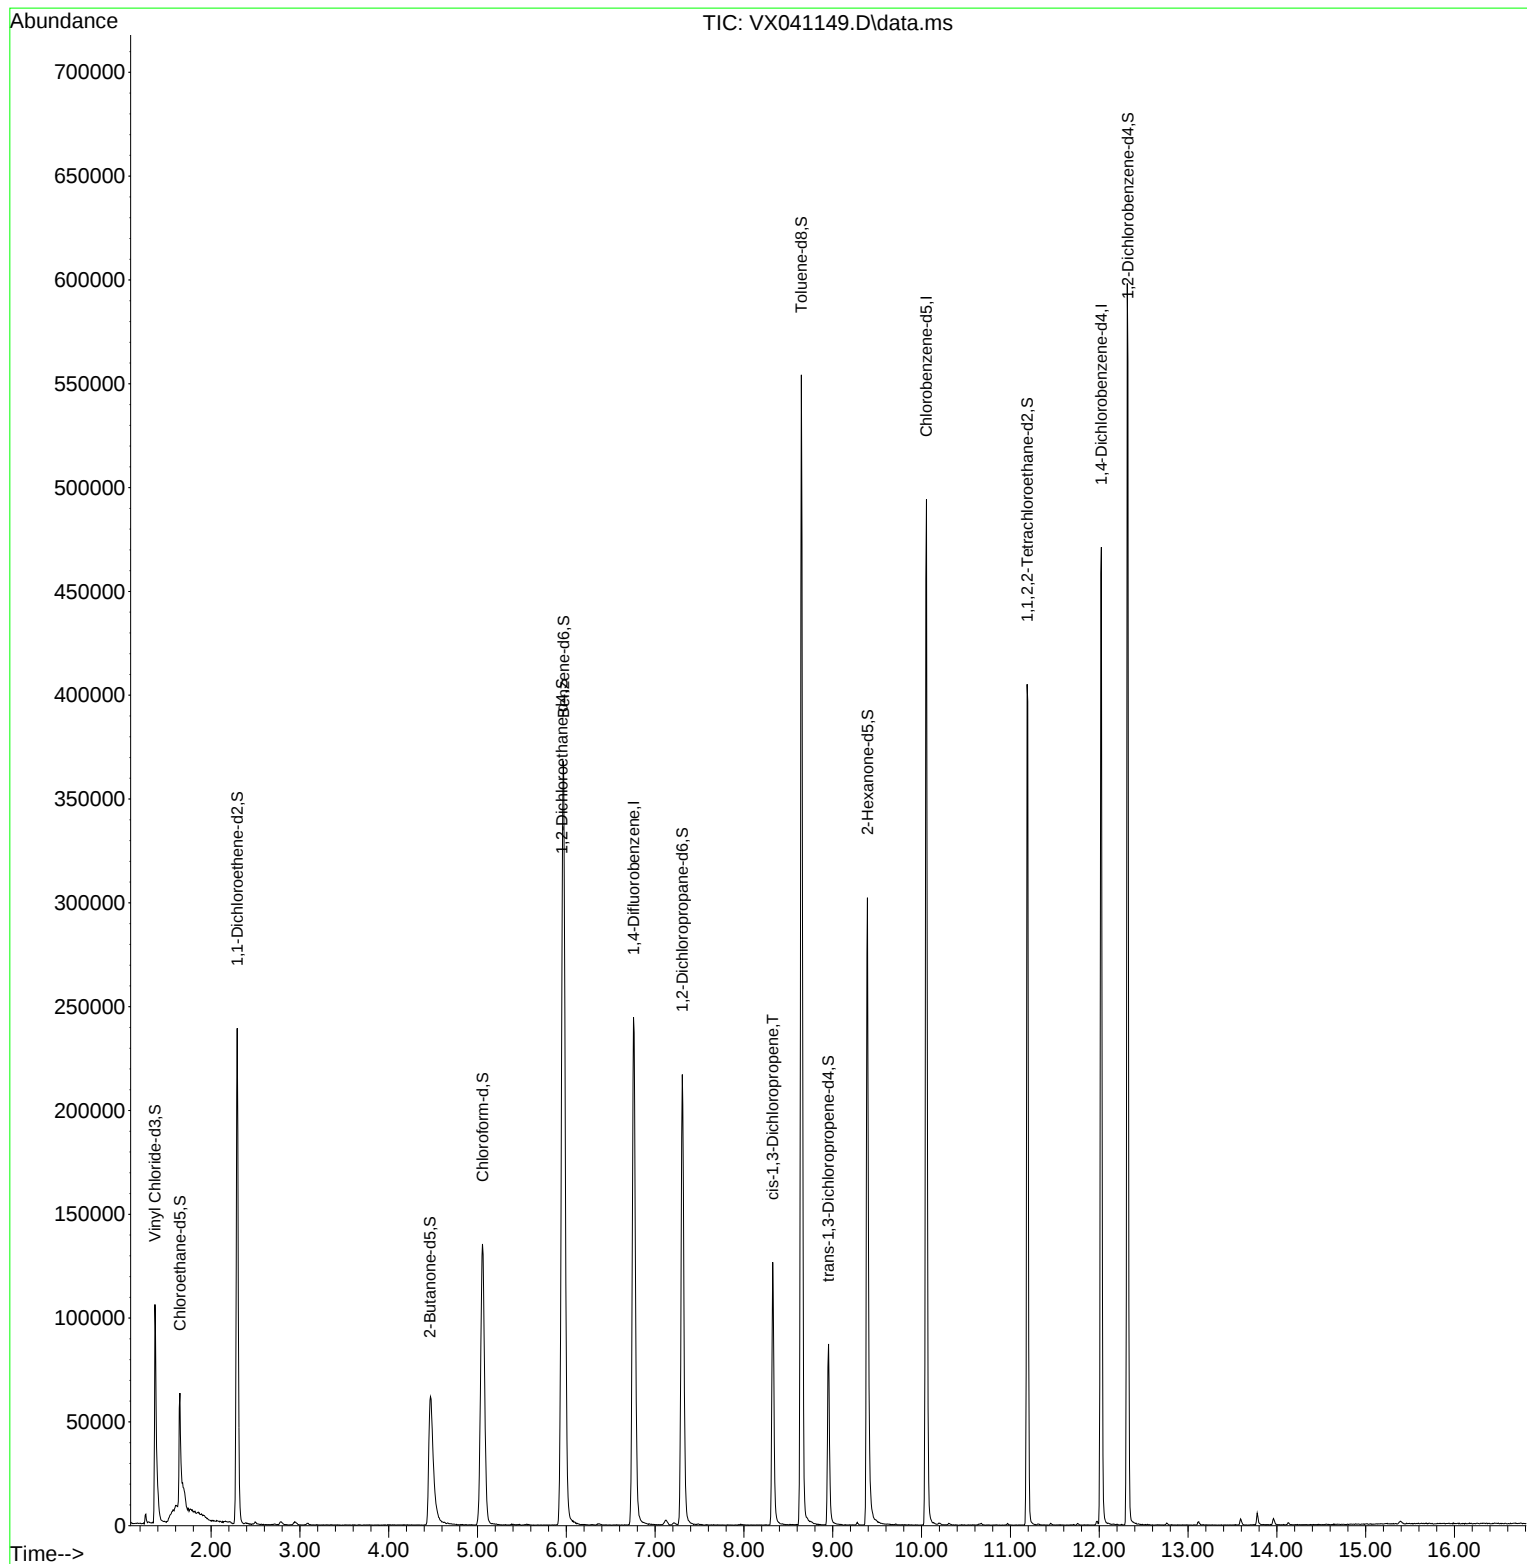

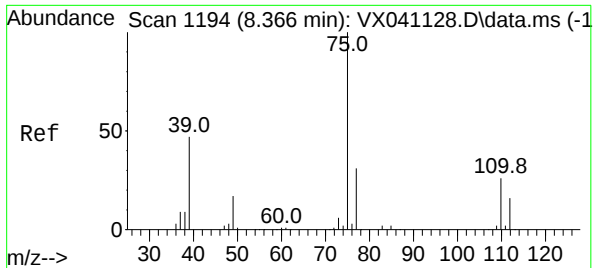

#39
 cis-1,3-Dichloropropene
 Concen: 1.239 ug/L
 RT: 8.324 min Scan# 11
 Delta R.T. -0.043 min
 Lab File: VX041149.D
 Acq: 18 Apr 2024 00:32

Instrument :
 MSVOA_X
 ClientSampleId :

Tgt Ion: 75 Resp: 3120
 Ion Ratio Lower Upper
 75 100
 77 49.6 21.6 40.0#

