

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041724\
 Data File : VX041137.D
 Acq On : 17 Apr 2024 19:57
 Operator : JC/MD
 Sample : P2037-10
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E1D00

Quant Time: Apr 18 02:24:43 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041724WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Apr 18 02:15:13 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.763	114	281017	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	252426	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	116346	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.368	65	92962	46.231	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	92.460%		
7) Chloroethane-d5	1.648	69	45931	45.900	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	91.800%		
11) 1,1-Dichloroethene-d2	2.288	65	40324	46.808	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	93.620%		
21) 2-Butanone-d5	4.471	46	128484	111.929	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	111.930%		
24) Chloroform-d	5.056	84	174846	47.241	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	94.480%		
26) 1,2-Dichloroethane-d4	5.952	65	116271	49.436	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	98.880%		
32) Benzene-d6	5.970	84	368629	50.698	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	101.400%		
36) 1,2-Dichloropropane-d6	7.305	67	106968	50.824	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	101.640%		
41) Toluene-d8	8.647	98	328126	48.106	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	96.220%		
43) trans-1,3-Dichloroprop...	8.952	79	43266	45.953	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	91.900%		
47) 2-Hexanone-d5	9.390	63	88879	104.014	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	104.010%		
56) 1,1,2,2-Tetrachloroeth...	11.195	84	153455	49.975	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	99.940%		
66) 1,2-Dichlorobenzene-d4	12.323	152	132704	53.038	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	106.080%		
Target Compounds					Qvalue	
13) Acetone	2.392	43	7192	7.811	ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041724\
Data File : VX041137.D
Acq On : 17 Apr 2024 19:57
Operator : JC/MD
Sample : P2037-10
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E1D00

Quant Time: Apr 18 02:24:43 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041724WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Apr 18 02:15:13 2024
Response via : Initial Calibration

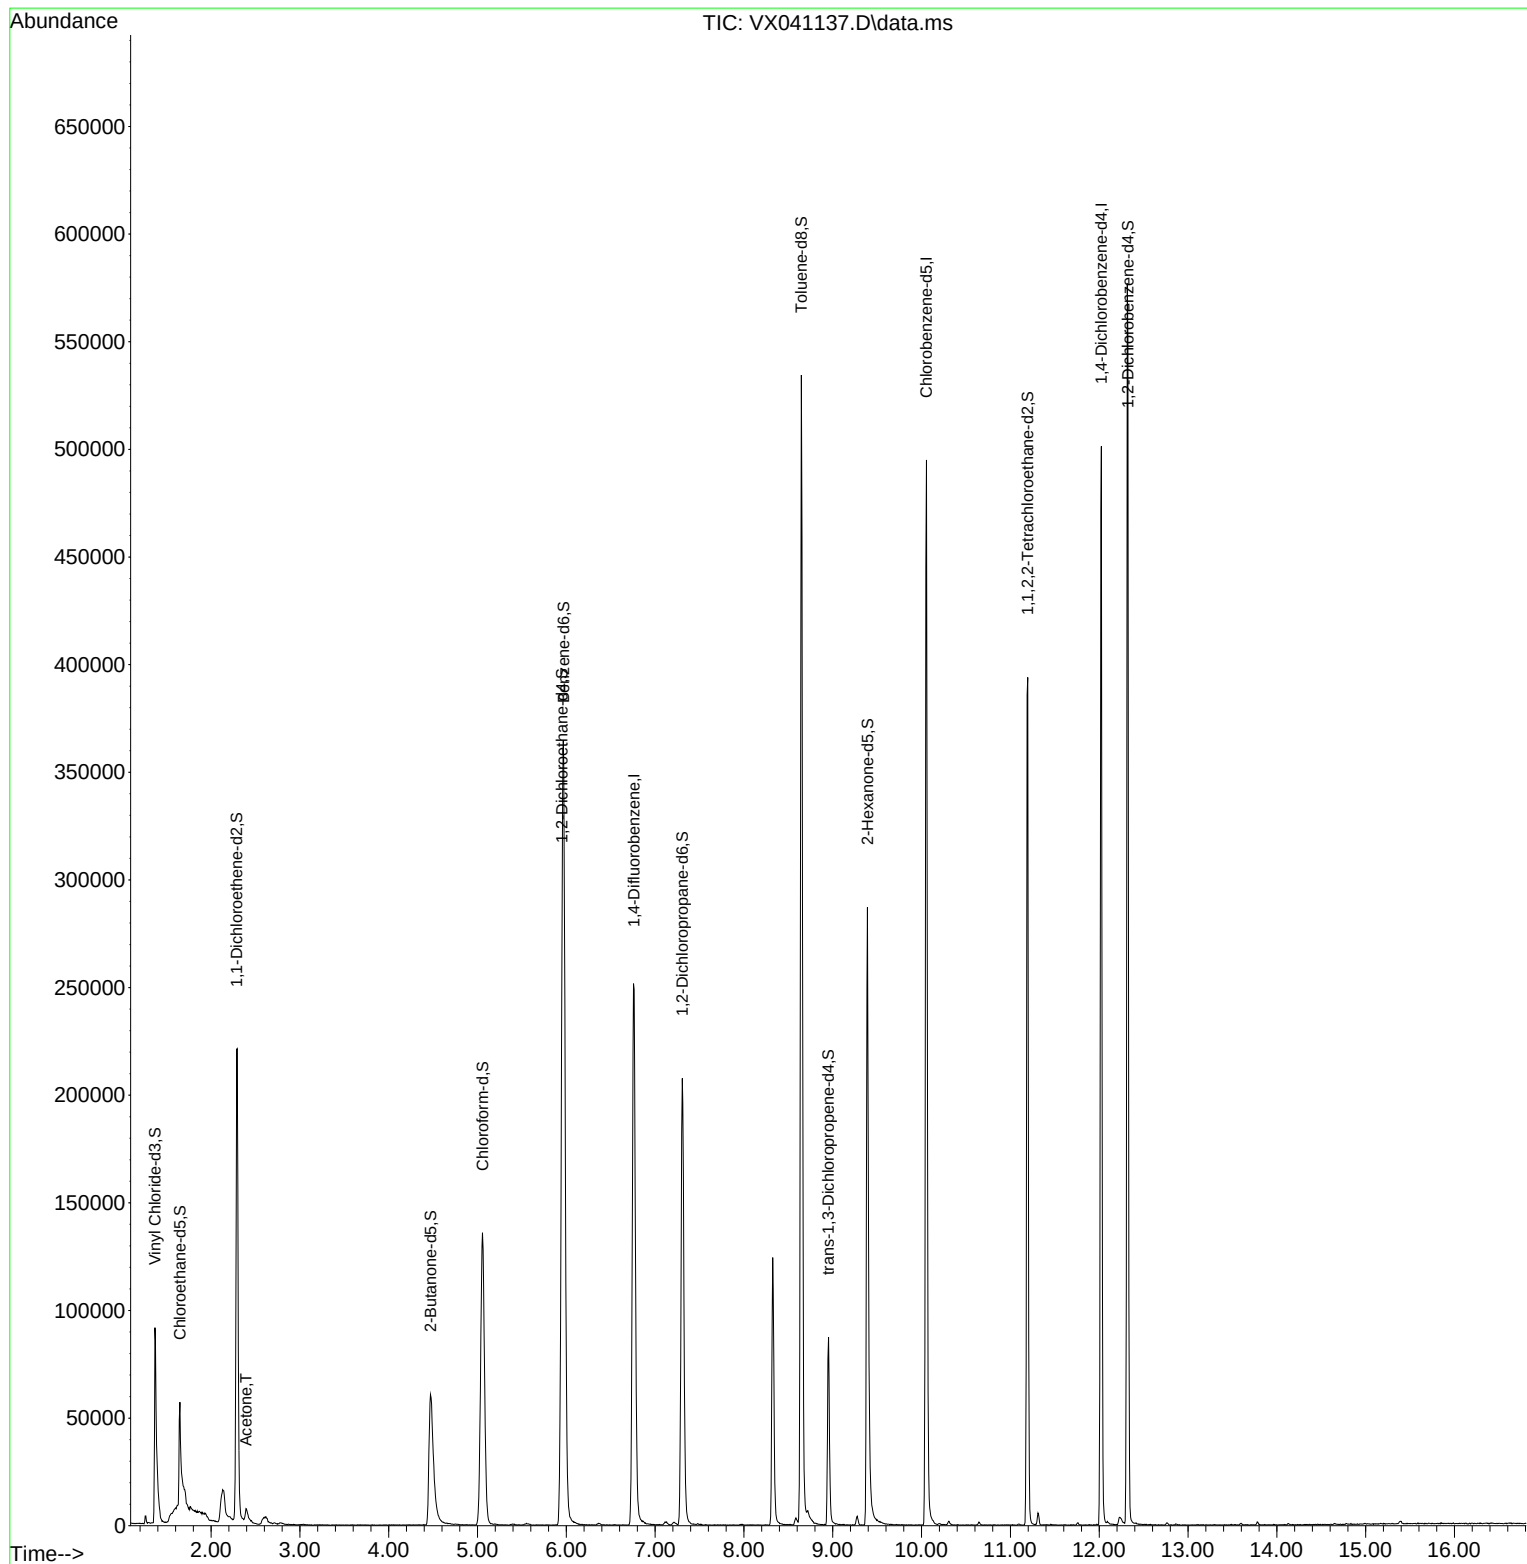

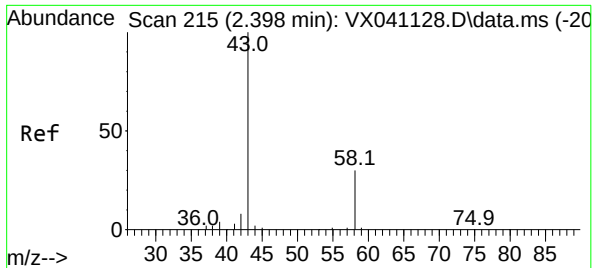

#13
 Acetone
 Concen: 7.811 ug/L
 RT: 2.392 min Scan# 21
 Delta R.T. -0.006 min
 Lab File: VX041137.D
 Acq: 17 Apr 2024 19:57

Instrument :
 MSVOA_X
 ClientSampleId :
 E1D00

Tgt Ion: 43 Resp: 7192
 Ion Ratio Lower Upper
 43 100
 58 29.8 0.0 62.4

