

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041724\
 Data File : VX041138.D
 Acq On : 17 Apr 2024 20:20
 Operator : JC/MD
 Sample : P2037-11
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E1D12

Quant Time: Apr 18 02:24:54 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041724WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Apr 18 02:15:13 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.763	114	288372	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	257350	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	121380	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.368	65	94354	45.726	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	91.460%		
7) Chloroethane-d5	1.648	69	47102	45.870	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	91.740%		
11) 1,1-Dichloroethene-d2	2.294	65	40894	46.259	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	92.520%		
21) 2-Butanone-d5	4.471	46	129193	109.677	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	109.680%		
24) Chloroform-d	5.056	84	175639	46.245	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	92.480%		
26) 1,2-Dichloroethane-d4	5.952	65	115506	47.858	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	95.720%		
32) Benzene-d6	5.970	84	370542	49.986	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	99.980%		
36) 1,2-Dichloropropane-d6	7.306	67	107962	50.315	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	100.640%		
41) Toluene-d8	8.647	98	330467	47.522	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	95.040%		
43) trans-1,3-Dichloroprop...	8.952	79	42957	44.752	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	89.500%		
47) 2-Hexanone-d5	9.391	63	88233	101.283	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	101.280%		
56) 1,1,2,2-Tetrachloroeth...	11.195	84	154760	49.435	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	98.880%		
66) 1,2-Dichlorobenzene-d4	12.317	152	135667	51.973	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	103.940%		
Target Compounds					Qvalue	
13) Acetone	2.398	43	6056	6.410	ug/L	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041724\
Data File : VX041138.D
Acq On : 17 Apr 2024 20:20
Operator : JC/MD
Sample : P2037-11
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E1D12

Quant Time: Apr 18 02:24:54 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041724WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Apr 18 02:15:13 2024
Response via : Initial Calibration

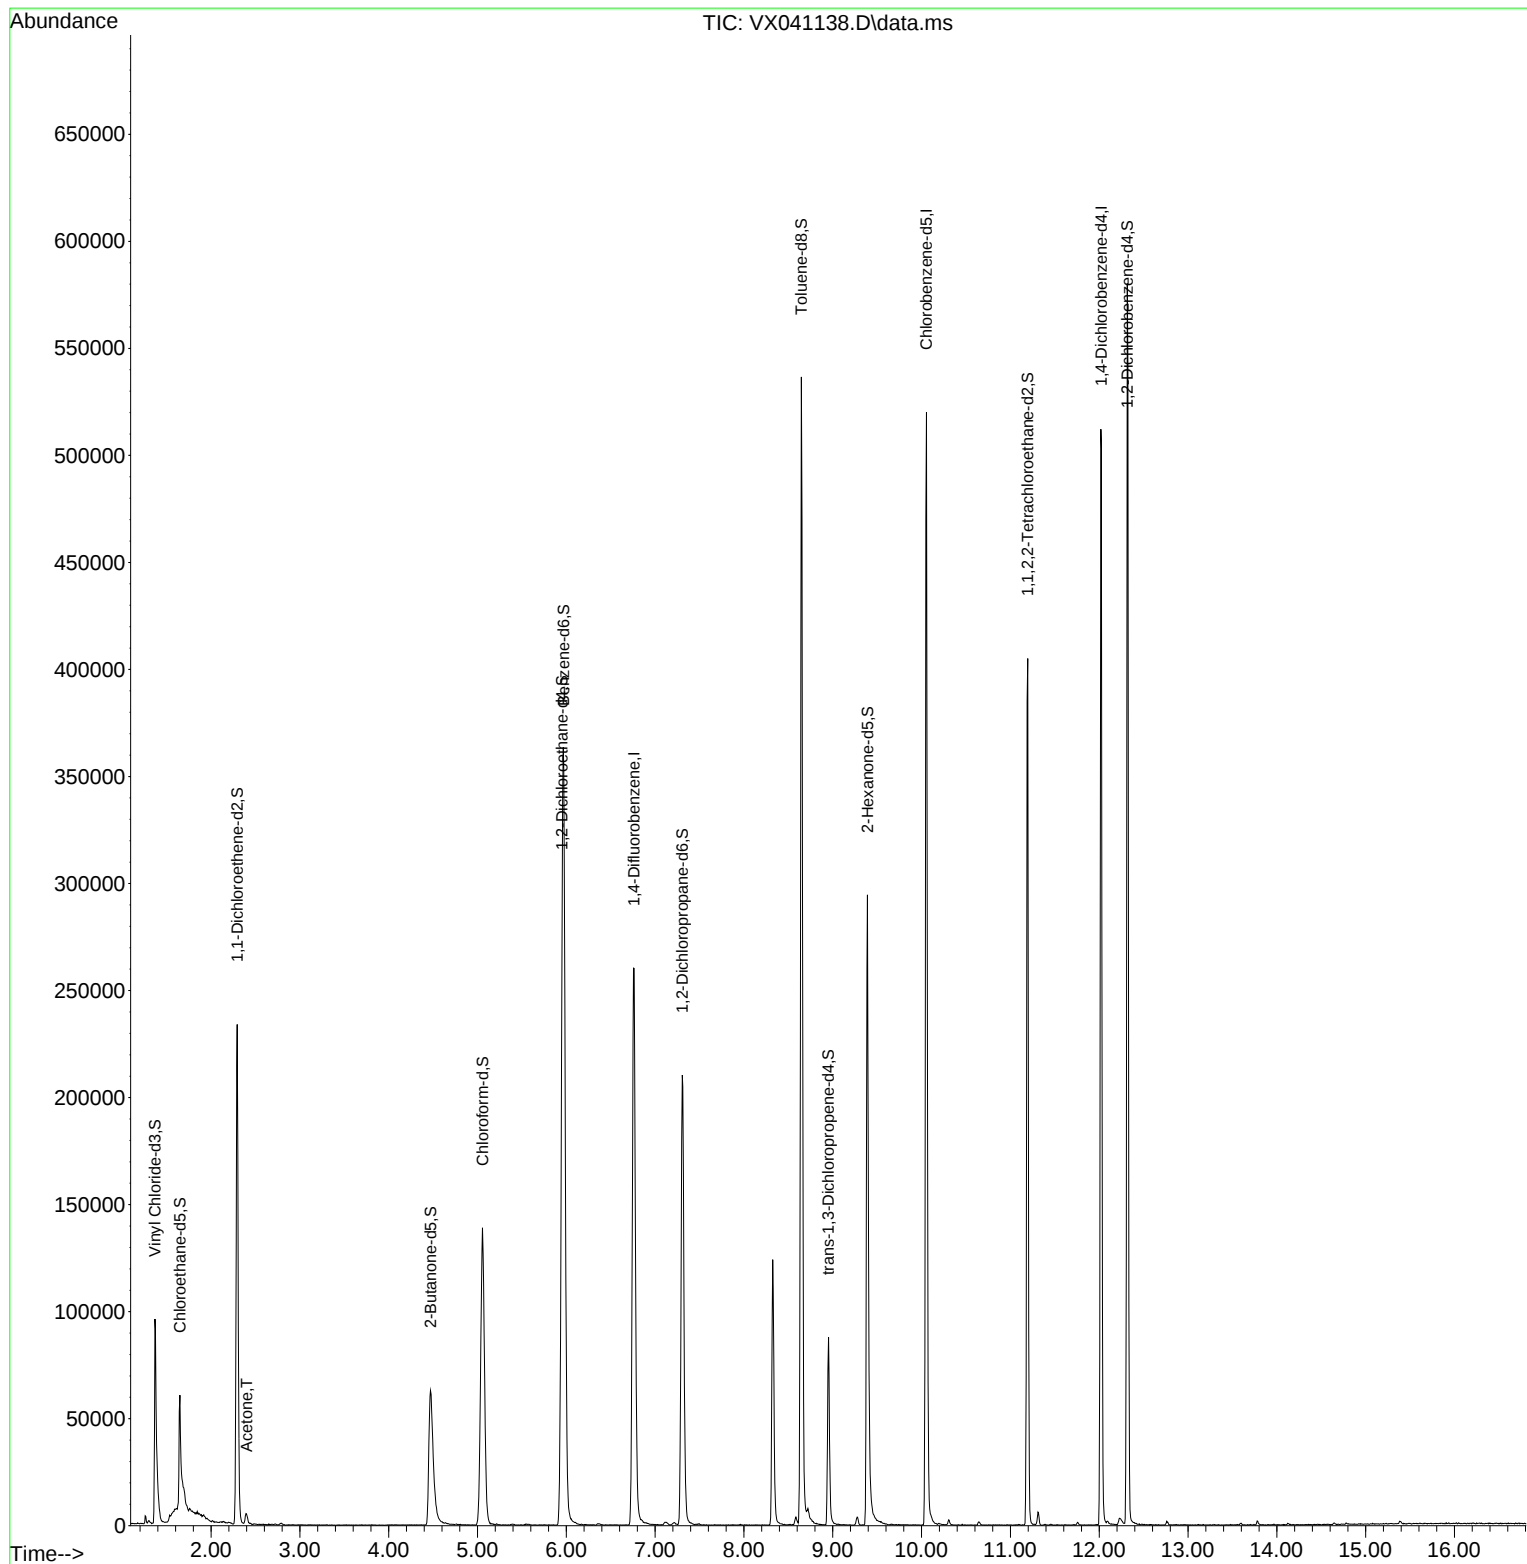

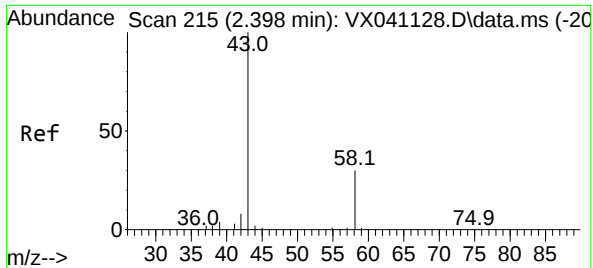

#13
 Acetone
 Concen: 6.410 ug/L
 RT: 2.398 min Scan# 21
 Delta R.T. 0.000 min
 Lab File: VX041138.D
 Acq: 17 Apr 2024 20:20

Instrument :
 MSVOA_X
 ClientSampleId :
 E1D12

Tgt Ion: 43 Resp: 6056
 Ion Ratio Lower Upper
 43 100
 58 31.1 0.0 62.4

