

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041724\
 Data File : VX041130.D
 Acq On : 17 Apr 2024 17:16
 Operator : JC/MD
 Sample : P2101-09
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 COAL3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041724WMA.M

Title : VOC Analysis

Signal : TIC: VX041130.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.258	26	28	32	rBV2	3385	3289	0.32%	0.042%
2	1.368	43	46	59	rBV	104549	151829	14.69%	1.937%
3	1.648	88	92	108	rVB	57633	99571	9.63%	1.270%
4	2.294	192	198	209	rVB	231619	353117	34.16%	4.504%
5	2.501	228	232	236	rVB2	1506	2379	0.23%	0.030%
6	2.788	274	279	286	rBV3	896	1678	0.16%	0.021%
7	2.861	289	291	292	rBV	238	152	0.01%	0.002%
8	2.947	302	305	307	rBV3	285	324	0.03%	0.004%
9	3.075	322	326	327	rVB2	161	192	0.02%	0.002%
10	3.093	327	329	330	rBV	278	186	0.02%	0.002%
11	3.251	353	355	357	rBV2	138	170	0.02%	0.002%
12	3.404	378	380	383	rVV	187	184	0.02%	0.002%
13	3.440	383	386	388	rVB2	130	137	0.01%	0.002%
14	3.556	402	405	408	rBV2	106	161	0.02%	0.002%
15	3.794	442	444	446	rVV	162	145	0.01%	0.002%
16	3.879	455	458	461	rBV	159	153	0.01%	0.002%
17	3.983	471	475	476	rBV	158	201	0.02%	0.003%
18	4.087	490	492	495	rBV2	118	142	0.01%	0.002%
19	4.172	505	506	509	rBV2	155	146	0.01%	0.002%
20	4.300	524	527	529	rVB2	202	214	0.02%	0.003%
21	4.318	529	530	532	rBV	191	136	0.01%	0.002%
22	4.471	546	555	578	rBV	63838	223832	21.65%	2.855%
23	4.855	616	618	620	rVB	312	241	0.02%	0.003%
24	5.056	639	651	669	rBV	132728	410316	39.69%	5.233%
25	5.288	686	689	692	rBV	174	283	0.03%	0.004%
26	5.397	701	707	711	rVV3	424	935	0.09%	0.012%
27	5.458	715	717	718	rVV2	221	141	0.01%	0.002%
28	5.727	759	761	764	rVB	164	148	0.01%	0.002%
29	5.763	764	767	770	rBV	126	177	0.02%	0.002%
30	5.964	788	800	821	rBV2	352632	1033674	100.00%	13.184%
31	6.361	861	865	874	rVB4	716	1558	0.15%	0.020%
32	6.489	882	886	889	rBV2	139	200	0.02%	0.003%
33	6.665	912	915	916	rVB	234	176	0.02%	0.002%
34	6.757	921	930	954	rBV	259068	634983	61.43%	8.099%
35	7.116	983	989	996	rVB5	1393	3517	0.34%	0.045%
36	7.208	999	1004	1012	rBV3	987	2281	0.22%	0.029%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041724\
 Data File : VX041130.D
 Acq On : 17 Apr 2024 17:16
 Operator : JC/MD
 Sample : P2101-09
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 COAL3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041724WMA.M
 Title : VOC Analysis

37	7.305	1012	1020	1043	rVV	205122	454013	43.92%	5.791%
38	7.696	1082	1084	1087	rVB2	147	167	0.02%	0.002%
39	7.769	1094	1096	1098	rVV2	204	160	0.02%	0.002%
40	7.952	1124	1126	1128	rBV2	310	364	0.04%	0.005%
41	8.324	1181	1187	1200	rBV	129368	210160	20.33%	2.680%
42	8.488	1210	1214	1215	rBV3	286	381	0.04%	0.005%
43	8.647	1234	1240	1255	rBV	538267	845995	81.84%	10.790%
44	8.952	1284	1290	1302	rBV	88331	135916	13.15%	1.734%
45	9.061	1306	1308	1309	rBV2	377	280	0.03%	0.004%
46	9.183	1326	1328	1331	rBV2	196	234	0.02%	0.003%
47	9.275	1338	1343	1348	rBV2	6477	9890	0.96%	0.126%
48	9.390	1356	1362	1378	rBV	297815	486300	47.05%	6.203%
49	9.647	1402	1404	1405	rVB	257	171	0.02%	0.002%
50	9.744	1419	1420	1422	rVB	212	136	0.01%	0.002%
51	9.787	1425	1427	1430	rBV	237	168	0.02%	0.002%
52	9.848	1435	1437	1439	rBV	275	164	0.02%	0.002%
53	9.884	1441	1443	1444	rBV2	221	174	0.02%	0.002%
54	10.000	1457	1462	1465	rBV	166	253	0.02%	0.003%
55	10.055	1465	1471	1488	rBV	527091	732395	70.85%	9.341%
56	10.305	1509	1512	1517	rVB2	619	843	0.08%	0.011%
57	10.348	1517	1519	1521	rVB	223	140	0.01%	0.002%
58	10.427	1531	1532	1536	rVV3	218	190	0.02%	0.002%
59	10.488	1539	1542	1544	rBV2	166	169	0.02%	0.002%
60	10.646	1565	1568	1571	rBV4	410	703	0.07%	0.009%
61	10.677	1571	1573	1577	rVB4	352	338	0.03%	0.004%
62	10.835	1598	1599	1603	rBV2	168	220	0.02%	0.003%
63	10.963	1619	1620	1622	rVV2	263	222	0.02%	0.003%
64	11.091	1638	1641	1647	rBV3	589	774	0.07%	0.010%
65	11.195	1652	1658	1667	rBV	402775	533607	51.62%	6.806%
66	11.317	1672	1678	1685	rVB	9685	14256	1.38%	0.182%
67	11.415	1692	1694	1696	rBV	164	158	0.02%	0.002%
68	11.451	1698	1700	1704	rVB2	315	474	0.05%	0.006%
69	11.591	1720	1723	1725	rBV2	113	147	0.01%	0.002%
70	11.707	1740	1742	1745	rBV	130	189	0.02%	0.002%
71	11.756	1747	1750	1753	rVB2	445	470	0.05%	0.006%
72	11.896	1770	1773	1774	rBV2	155	164	0.02%	0.002%
73	11.939	1778	1780	1783	rBV2	342	344	0.03%	0.004%
74	11.975	1783	1786	1788	rBV2	750	781	0.08%	0.010%
75	12.018	1788	1793	1804	rBV	522277	691749	66.92%	8.823%
76	12.231	1824	1828	1832	rBV6	1368	2780	0.27%	0.035%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041724\
 Data File : VX041130.D
 Acq On : 17 Apr 2024 17:16
 Operator : JC/MD
 Sample : P2101-09
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 COAL3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM041724WMA.M
 Title : VOC Analysis

77	12.317	1837	1842	1853	rBV	594744	771693	74.66%	9.843%
78	12.762	1907	1915	1922	rBV	2523	3347	0.32%	0.043%
79	12.829	1924	1926	1928	rBV	215	142	0.01%	0.002%
80	12.865	1928	1932	1935	rBV3	1027	1538	0.15%	0.020%
81	12.981	1949	1951	1955	rVB	140	173	0.02%	0.002%
82	13.030	1958	1959	1963	rVV2	172	147	0.01%	0.002%
83	13.122	1970	1974	1979	rVB4	508	856	0.08%	0.011%
84	13.371	2011	2015	2016	rVB2	165	207	0.02%	0.003%
85	13.390	2016	2018	2023	rVB	167	235	0.02%	0.003%
86	13.597	2048	2052	2057	rVB3	907	1294	0.13%	0.017%
87	13.676	2062	2065	2066	rBV	145	161	0.02%	0.002%
88	13.786	2079	2083	2090	rVB2	893	1576	0.15%	0.020%
89	13.859	2092	2095	2099	rBV2	205	282	0.03%	0.004%
90	13.908	2102	2103	2105	rBV	235	189	0.02%	0.002%
91	13.963	2108	2112	2116	rVB3	897	1035	0.10%	0.013%
92	14.018	2119	2121	2122	rBV	249	178	0.02%	0.002%
93	14.042	2123	2125	2129	rVB2	221	229	0.02%	0.003%
94	14.097	2129	2134	2136	rBV2	245	383	0.04%	0.005%
95	14.134	2136	2140	2143	rBV2	704	926	0.09%	0.012%
96	14.231	2155	2156	2157	rBV	286	141	0.01%	0.002%
97	14.609	2216	2218	2220	rBV3	282	273	0.03%	0.003%
98	14.780	2244	2246	2248	rBV2	360	214	0.02%	0.003%
99	15.194	2313	2314	2316	rBV2	418	324	0.03%	0.004%
100	15.389	2341	2346	2350	rBV3	1016	1783	0.17%	0.023%




Sum of corrected areas: 7840333

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041724\
Data File : VX041130.D
Acq On : 17 Apr 2024 17:16
Operator : JC/MD
Sample : P2101-09
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
COAL3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041724WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

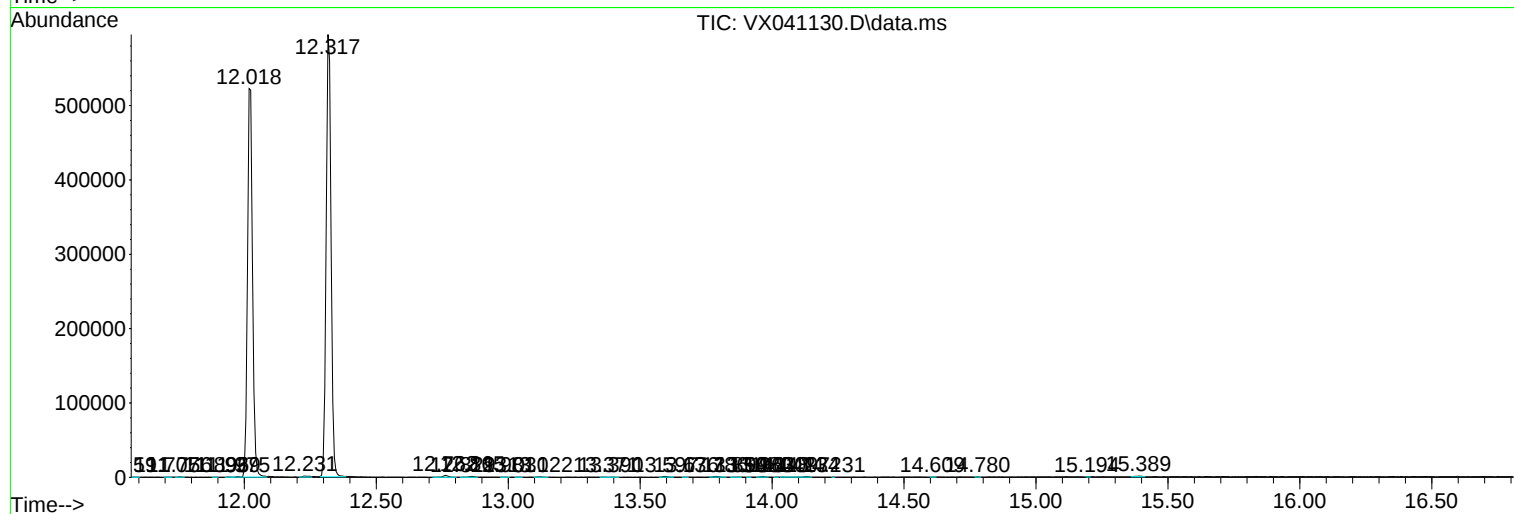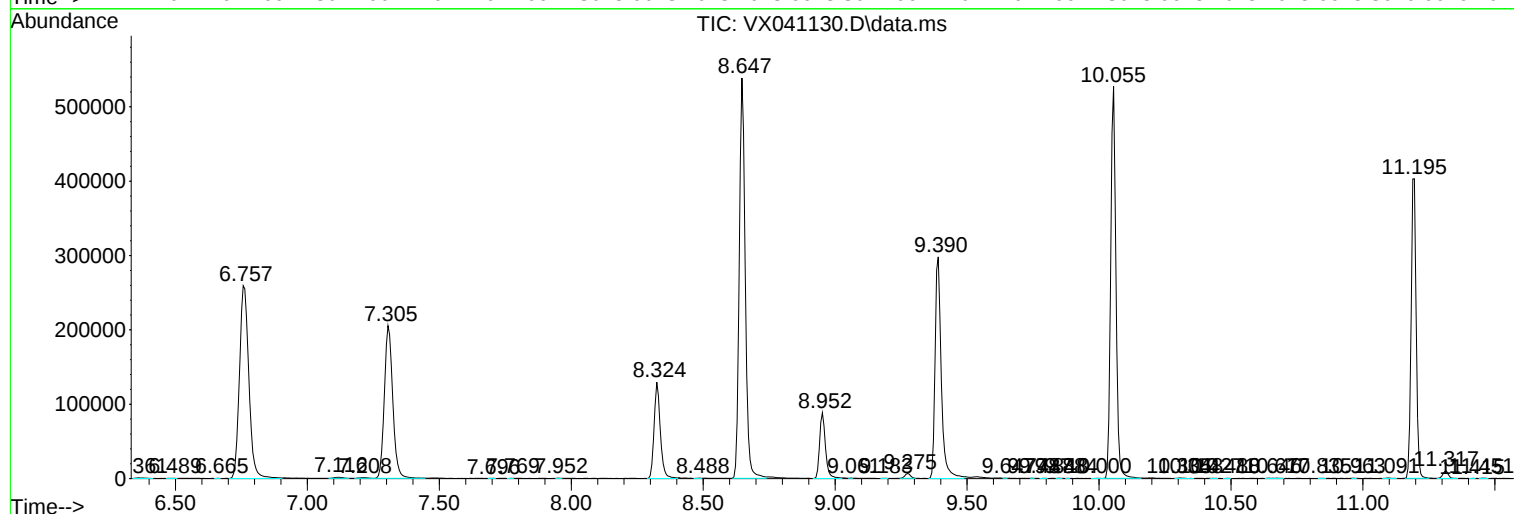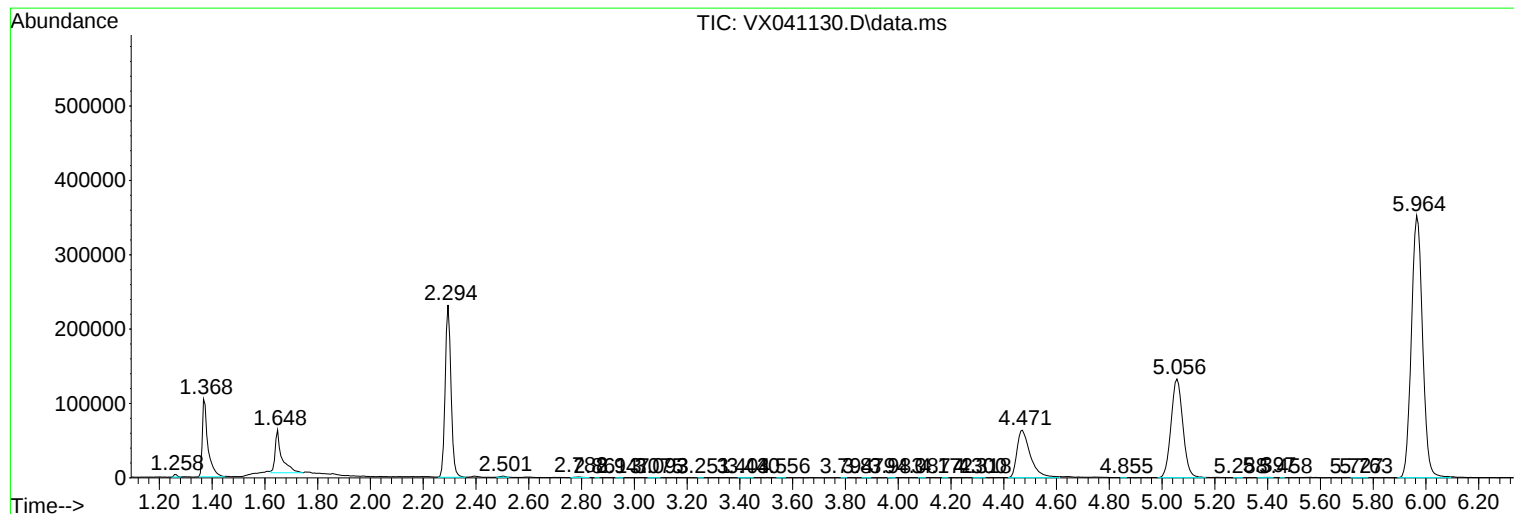

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041724\
Data File : VX041130.D
Acq On : 17 Apr 2024 17:16
Operator : JC/MD
Sample : P2101-09
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0AL3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM041724WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041724\
Data File : VX041130.D
Acq On : 17 Apr 2024 17:16
Operator : JC/MD
Sample : P2101-09
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0AL3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041724WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
