

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041724\
 Data File : VX041132.D
 Acq On : 17 Apr 2024 18:02
 Operator : JC/MD
 Sample : P2101-14
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041724WMA.M
 Title : VOC Analysis

Signal : TIC: VX041132.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.258	26	28	32	rBV2	3709	3731	0.35%	0.048%
2	1.368	43	46	62	rBV	106023	153657	14.53%	1.959%
3	1.648	88	92	109	rVB	58492	102175	9.66%	1.303%
4	2.294	192	198	210	rBV	237408	366745	34.69%	4.676%
5	2.703	263	265	267	rBV	294	206	0.02%	0.003%
6	2.788	274	279	284	rBV3	1363	2276	0.22%	0.029%
7	2.965	306	308	309	rBV	185	111	0.01%	0.001%
8	3.062	321	324	325	rVV	255	227	0.02%	0.003%
9	3.081	325	327	328	rVB2	269	151	0.01%	0.002%
10	3.160	338	340	343	rVB	153	118	0.01%	0.002%
11	3.270	356	358	359	rBV	124	131	0.01%	0.002%
12	3.367	371	374	376	rBV2	166	204	0.02%	0.003%
13	3.459	388	389	392	rVB2	154	122	0.01%	0.002%
14	3.495	393	395	398	rVB2	125	118	0.01%	0.002%
15	3.532	398	401	405	rVB2	194	295	0.03%	0.004%
16	3.642	417	419	421	rBV	106	127	0.01%	0.002%
17	3.684	423	426	427	rBV2	126	114	0.01%	0.001%
18	3.782	441	442	443	rBV	212	127	0.01%	0.002%
19	3.940	466	468	471	rBV2	99	152	0.01%	0.002%
20	4.081	489	491	495	rVV2	151	169	0.02%	0.002%
21	4.209	510	512	515	rBV2	173	222	0.02%	0.003%
22	4.471	544	555	579	rBV	65182	225654	21.34%	2.877%
23	4.824	611	613	614	rVB	229	119	0.01%	0.002%
24	4.891	622	624	626	rBV	187	178	0.02%	0.002%
25	4.940	630	632	633	rBV2	170	125	0.01%	0.002%
26	5.056	639	651	666	rBV	138608	414241	39.18%	5.281%
27	5.391	698	706	713	rVB3	593	1399	0.13%	0.018%
28	5.452	713	716	717	rBV	179	132	0.01%	0.002%
29	5.483	719	721	724	rVB2	192	155	0.01%	0.002%
30	5.702	755	757	761	rVB2	180	158	0.01%	0.002%
31	5.964	788	800	817	rBV2	360488	1057315	100.00%	13.480%
32	6.300	853	855	859	rVB2	203	213	0.02%	0.003%
33	6.361	861	865	870	rVV4	601	1061	0.10%	0.014%
34	6.476	881	884	887	rBV	154	212	0.02%	0.003%
35	6.544	892	895	896	rBV3	140	132	0.01%	0.002%
36	6.672	915	916	919	rVB	215	144	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041724\
 Data File : VX041132.D
 Acq On : 17 Apr 2024 18:02
 Operator : JC/MD
 Sample : P2101-14
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041724WMA.M
 Title : VOC Analysis

37	6.757	919	930	956	rBV	256511	634635	60.02%	8.091%
38	7.074	980	982	983	rVB	242	139	0.01%	0.002%
39	7.111	983	988	996	rBV7	1576	4221	0.40%	0.054%
40	7.208	1000	1004	1011	rVB3	925	1930	0.18%	0.025%
41	7.306	1011	1020	1038	rBV	207245	464246	43.91%	5.919%
42	7.891	1114	1116	1118	rBV	126	140	0.01%	0.002%
43	7.964	1124	1128	1130	rBV3	345	479	0.05%	0.006%
44	8.324	1181	1187	1199	rBV	128715	212351	20.08%	2.707%
45	8.647	1234	1240	1253	rBV	546660	853748	80.75%	10.885%
46	8.952	1285	1290	1303	rBV	88909	137323	12.99%	1.751%
47	9.128	1317	1319	1323	rBV	168	130	0.01%	0.002%
48	9.275	1338	1343	1349	rVB	4533	6689	0.63%	0.085%
49	9.391	1356	1362	1377	rBV	297781	486280	45.99%	6.200%
50	9.647	1402	1404	1407	rVB2	435	338	0.03%	0.004%
51	9.811	1429	1431	1433	rBV2	202	214	0.02%	0.003%
52	9.854	1433	1438	1439	rVV2	215	288	0.03%	0.004%
53	9.872	1439	1441	1444	rVV2	162	162	0.02%	0.002%
54	9.994	1459	1461	1465	rBV2	119	112	0.01%	0.001%
55	10.055	1465	1471	1485	rBV	519850	718477	67.95%	9.160%
56	10.317	1508	1514	1517	rBV2	515	766	0.07%	0.010%
57	10.433	1530	1533	1535	rBV	159	196	0.02%	0.002%
58	10.567	1553	1555	1556	rBV	156	116	0.01%	0.001%
59	10.585	1556	1558	1560	rVV2	117	118	0.01%	0.002%
60	10.921	1611	1613	1617	rVB2	293	290	0.03%	0.004%
61	10.970	1617	1621	1624	rVB3	372	556	0.05%	0.007%
62	10.994	1624	1625	1627	rBV	150	110	0.01%	0.001%
63	11.098	1640	1642	1646	rVB3	372	318	0.03%	0.004%
64	11.189	1652	1657	1673	rBV	403275	539650	51.04%	6.880%
65	11.311	1673	1677	1682	rVB	5809	7852	0.74%	0.100%
66	11.463	1698	1702	1704	rBV3	273	414	0.04%	0.005%
67	11.500	1707	1708	1711	rBV2	121	109	0.01%	0.001%
68	11.573	1717	1720	1722	rVB2	233	214	0.02%	0.003%
69	11.628	1728	1729	1733	rBV2	125	127	0.01%	0.002%
70	11.713	1739	1743	1745	rBV2	214	252	0.02%	0.003%
71	11.756	1747	1750	1753	rBV2	358	554	0.05%	0.007%
72	11.817	1759	1760	1762	rBV	203	147	0.01%	0.002%
73	11.915	1774	1776	1777	rBV2	145	115	0.01%	0.001%
74	11.975	1783	1786	1788	rBV2	709	671	0.06%	0.009%
75	12.024	1788	1794	1807	rBV	505095	661212	62.54%	8.430%
76	12.238	1826	1829	1831	rVB2	136	160	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041724\
 Data File : VX041132.D
 Acq On : 17 Apr 2024 18:02
 Operator : JC/MD
 Sample : P2101-14
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041724WMA.M
 Title : VOC Analysis

77	12.262	1831	1833	1835	rVB2	164	136	0.01%	0.002%
78	12.280	1835	1836	1837	rBV	176	128	0.01%	0.002%
79	12.317	1837	1842	1858	rBV	603466	767930	72.63%	9.790%
80	12.585	1884	1886	1887	rBV	185	180	0.02%	0.002%
81	12.646	1894	1896	1900	rBV2	192	259	0.02%	0.003%
82	12.695	1903	1904	1905	rBV	186	126	0.01%	0.002%
83	12.762	1910	1915	1920	rVV2	1216	1656	0.16%	0.021%
84	12.866	1929	1932	1934	rVB2	160	195	0.02%	0.002%
85	12.908	1937	1939	1941	rBV	156	110	0.01%	0.001%
86	13.189	1983	1985	1987	rBV2	135	130	0.01%	0.002%
87	13.359	2010	2013	2014	rBV	171	153	0.01%	0.002%
88	13.439	2025	2026	2028	rBV2	144	107	0.01%	0.001%
89	13.469	2029	2031	2032	rVB2	255	144	0.01%	0.002%
90	13.481	2032	2033	2037	rBV2	87	110	0.01%	0.001%
91	13.695	2066	2068	2069	rVB2	225	132	0.01%	0.002%
92	13.792	2080	2084	2091	rVB2	453	893	0.08%	0.011%
93	13.847	2091	2093	2094	rBV	151	149	0.01%	0.002%
94	13.884	2097	2099	2102	rBV	161	214	0.02%	0.003%
95	13.926	2104	2106	2109	rBV3	208	258	0.02%	0.003%
96	14.128	2135	2139	2144	rVB2	737	1204	0.11%	0.015%
97	14.207	2151	2152	2155	rBV	257	157	0.01%	0.002%
98	14.469	2193	2195	2198	rBV	165	185	0.02%	0.002%
99	15.383	2343	2345	2346	rBV2	696	545	0.05%	0.007%
100	15.999	2444	2446	2447	rBV2	441	281	0.03%	0.004%




Sum of corrected areas: 7843647

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041724\
Data File : VX041132.D
Acq On : 17 Apr 2024 18:02
Operator : JC/MD
Sample : P2101-14
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041724WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

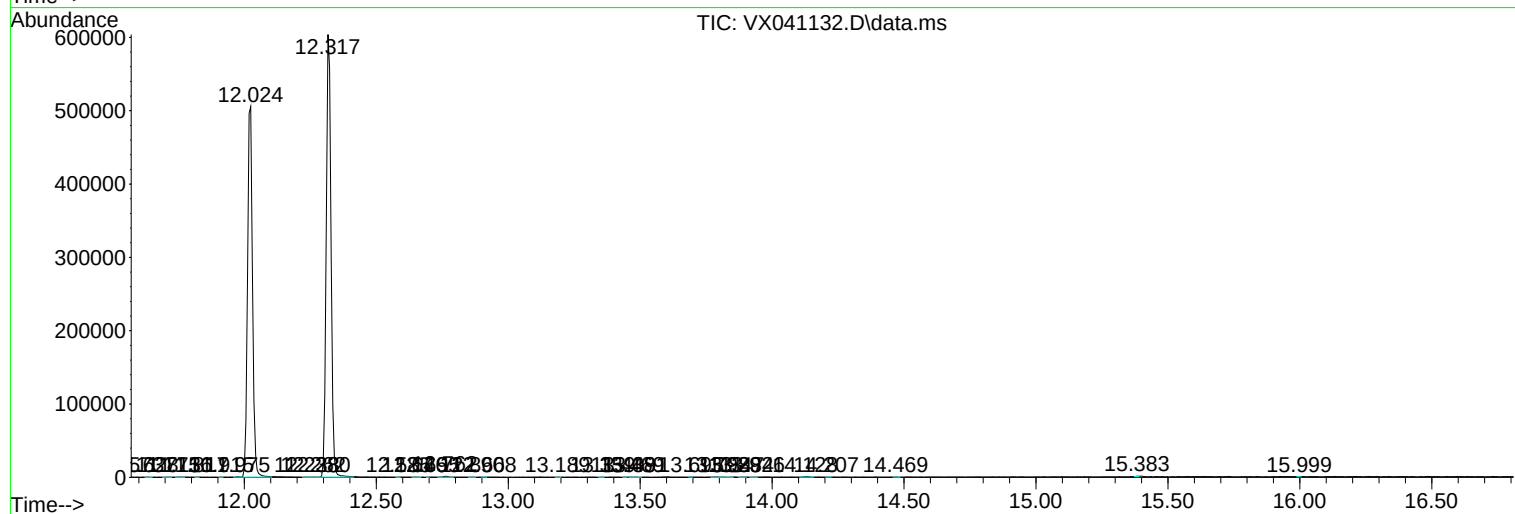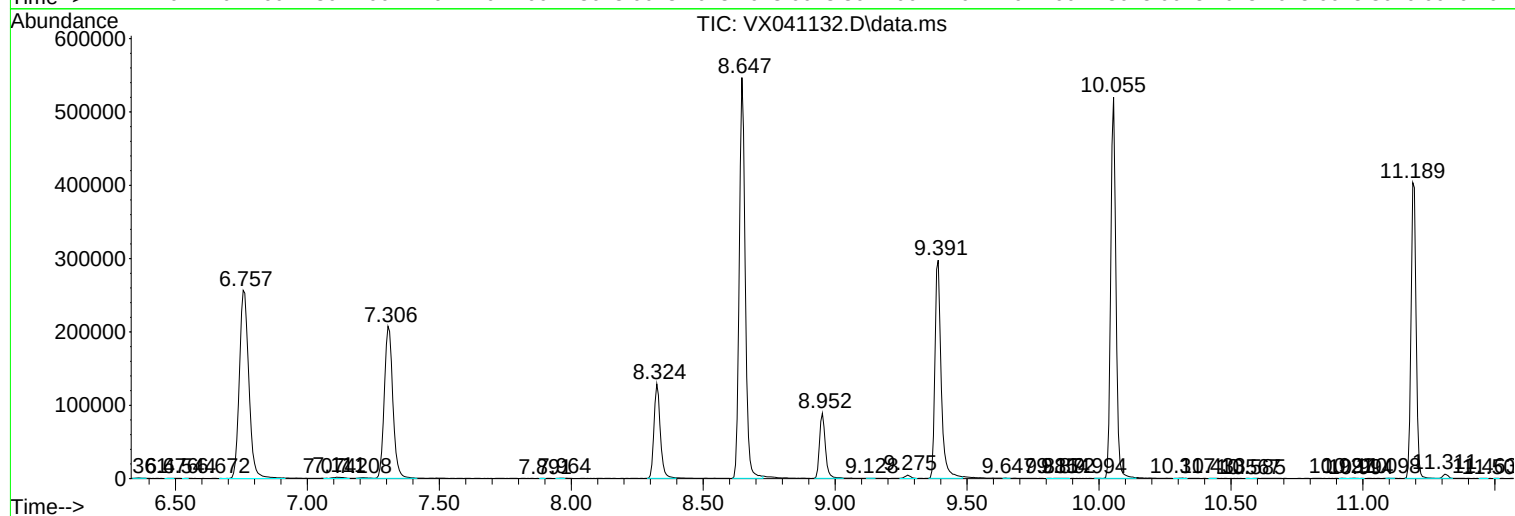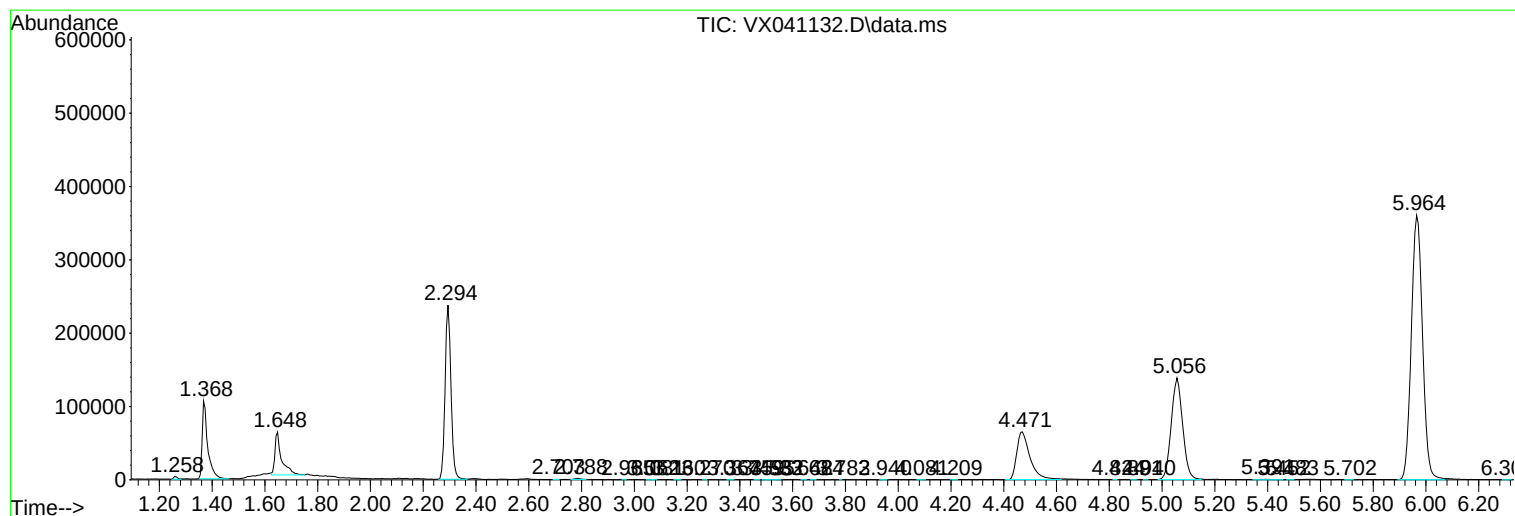

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041724\
Data File : VX041132.D
Acq On : 17 Apr 2024 18:02
Operator : JC/MD
Sample : P2101-14
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM041724WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041724\
Data File : VX041132.D
Acq On : 17 Apr 2024 18:02
Operator : JC/MD
Sample : P2101-14
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041724WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc