
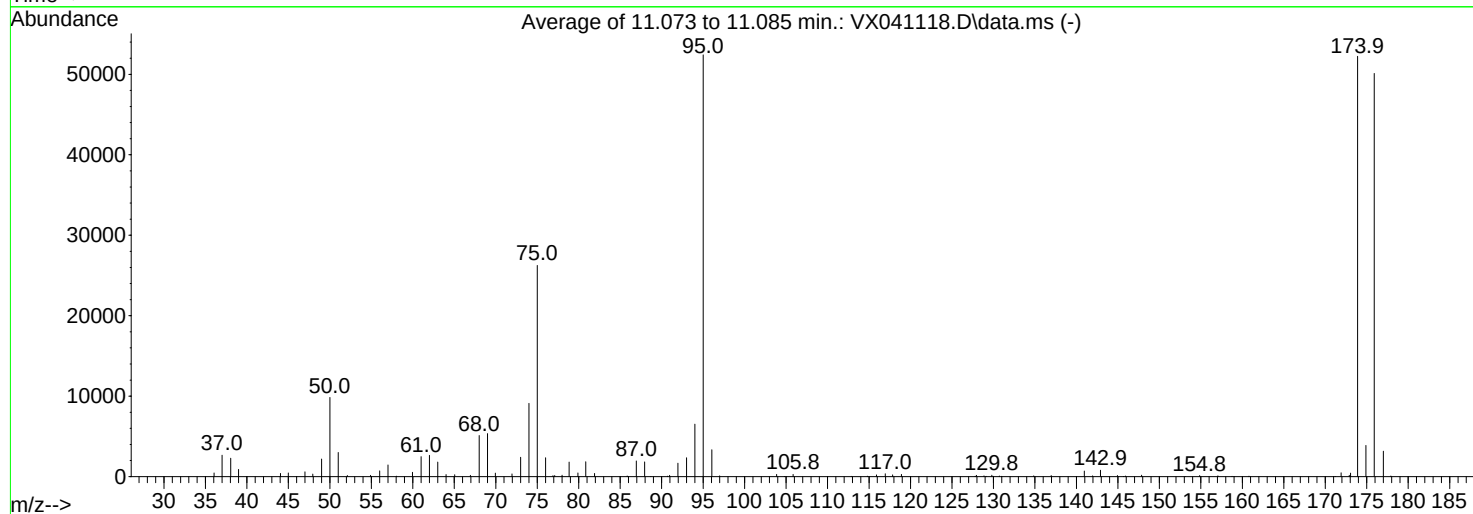


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041724\
Data File : VX041118.D
Acq On : 17 Apr 2024 08:26
Operator : JC/MD
Sample : BFB673
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB673

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM041724WMA.M
Title : VOC Analysis
Last Update : Thu Apr 18 02:15:13 2024

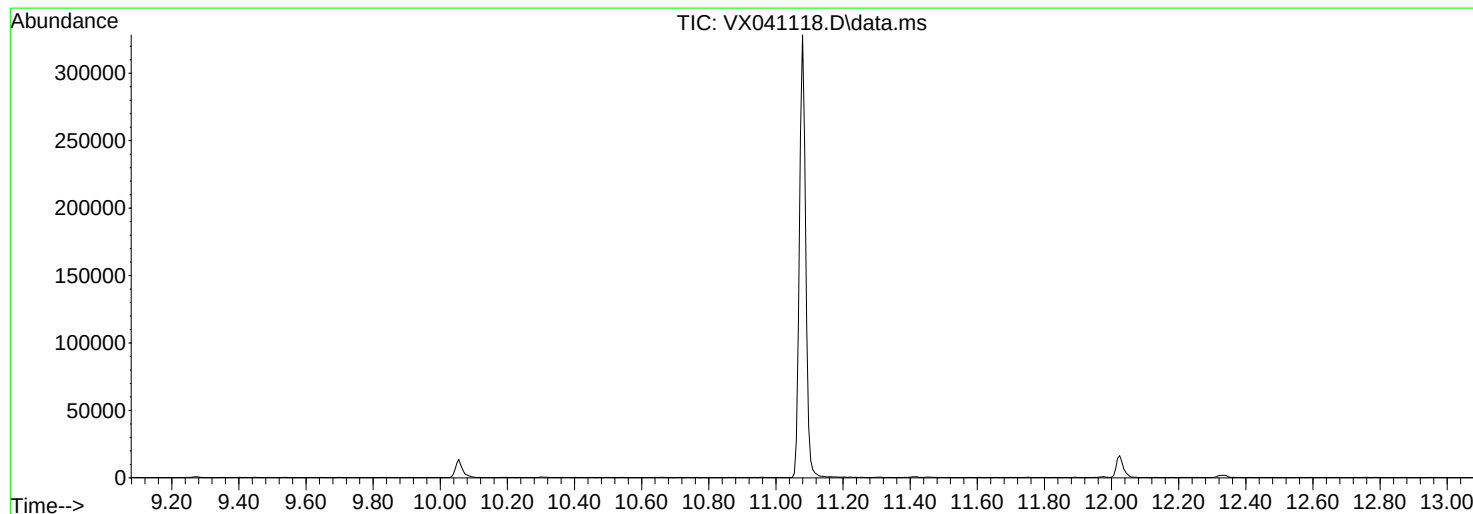

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1633

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.8	9843	PASS
75	95	30	80	50.1	26256	PASS
95	95	100	100	100.0	52421	PASS
96	95	5	9	6.4	3333	PASS
173	174	0.00	2	0.8	432	PASS
174	95	50	120	99.6	52232	PASS
175	174	5	9	7.4	3879	PASS
176	174	95	101	95.9	50115	PASS
177	176	5	9	6.3	3171	PASS

Scan 1633 (11.043 min): VX041118.D\data.ms
BFB673

m/z	Abundance
40.10	175.0
44.10	89.0

Instrument :
MSVOA_X
ClientSampleId :
BFB673

m/z	Abundance
36.10	442.0
37.00	2861.0
38.00	2381.0
39.00	957.0
40.10	135.0
44.10	420.0
45.00	505.0
46.00	64.0
47.00	652.0
48.00	292.0
49.00	2335.0
50.00	10492.0
51.00	2900.0
52.10	78.0
54.90	179.0
56.00	668.0
57.00	1509.0
58.00	63.0
59.90	522.0
61.00	2493.0
62.00	2685.0
63.00	2024.0
64.00	298.0
65.10	166.0
66.90	147.0
68.00	5103.0
69.00	5509.0
69.90	439.0
71.90	395.0
73.00	2312.0
74.00	9040.0
75.00	25504.0
76.00	2388.0
76.90	340.0
78.00	201.0
79.00	1729.0
79.90	463.0
80.90	1814.0
81.90	336.0
85.80	77.0
86.90	1970.0
88.00	1937.0
90.70	161.0
92.00	1503.0
93.00	2164.0
94.00	6440.0
95.00	50504.0
96.00	3816.0
97.20	77.0
103.80	326.0
104.80	58.0
105.90	346.0
115.90	264.0
116.90	345.0
117.90	219.0
118.80	304.0
127.80	163.0
129.00	129.0
129.80	132.0
130.00	135.0
131.00	108.0
135.00	61.0
137.00	96.0
141.00	560.0
142.10	58.0
142.90	742.0
145.00	95.0
145.70	69.0
147.80	131.0
154.90	108.0
157.10	83.0
158.70	52.0
160.80	65.0
171.90	493.0
172.90	462.0
173.90	42736.0
174.90	3259.0
175.90	40656.0
177.00	2655.0
178.00	73.0

Instrument :
MSVOA_X
ClientSampleId :
BFB673

m/z	Abundance
36.00	501.0
37.00	3179.0
38.10	2686.0
39.00	1029.0
40.00	260.0
44.00	598.0
45.00	503.0
47.00	664.0
48.00	365.0
49.00	2657.0
50.00	11310.0
51.00	3740.0
52.10	226.0
54.90	189.0
56.00	912.0
57.00	1762.0
58.10	105.0
60.00	663.0
61.00	3094.0
62.00	3274.0
63.00	1876.0
64.00	309.0
65.00	294.0
67.00	190.0
68.00	6152.0
69.00	6278.0
70.00	567.0
72.00	341.0
73.00	2903.0
74.00	10676.0
75.00	31544.0
76.00	2785.0
77.10	262.0
78.00	208.0
78.80	2204.0
79.90	537.0
80.90	2211.0
81.90	470.0
85.80	99.0
87.00	2221.0
87.90	2099.0
90.90	316.0
91.90	2012.0
93.00	2845.0
94.00	7485.0
95.00	61888.0
96.00	3552.0
97.00	138.0
103.90	298.0
105.00	69.0
105.80	248.0
112.90	60.0
114.80	74.0
115.90	259.0
116.90	417.0
117.80	265.0
118.90	325.0
128.00	254.0
128.80	100.0
129.80	225.0
130.70	146.0
134.80	169.0
136.90	137.0
140.90	899.0
141.90	117.0
142.90	886.0
145.00	150.0
145.90	149.0
147.90	204.0
154.90	181.0
157.00	86.0
159.00	89.0
160.80	53.0
171.00	83.0
171.90	506.0
173.10	687.0
173.90	62176.0
174.90	4561.0
175.90	60104.0
177.00	4075.0
177.90	97.0

Instrument :
MSVOA_X
ClientSampleId :
BFB673

m/z	Abundance
36.00	440.0
37.10	1973.0
38.00	1811.0
39.00	678.0
39.90	191.0
44.00	452.0
45.00	347.0
47.00	477.0
47.90	295.0
49.00	1581.0
50.00	7728.0
51.00	2378.0
52.00	59.0
52.10	55.0
54.90	122.0
56.00	570.0
57.00	1071.0
59.90	419.0
61.00	1867.0
62.10	1978.0
63.00	1522.0
64.10	157.0
65.00	278.0
66.90	157.0
68.00	4092.0
69.00	4242.0
70.00	322.0
72.00	275.0
73.00	1978.0
74.00	7612.0
75.00	21720.0
76.00	1894.0
77.10	181.0
78.00	132.0
78.80	1481.0
79.90	401.0
80.80	1499.0
81.90	413.0
85.90	66.0
86.90	1645.0
87.90	1440.0
88.70	74.0
91.00	181.0
92.00	1480.0
93.00	2004.0
94.00	5646.0
95.00	44872.0
96.10	2631.0
96.90	90.0
103.80	223.0
105.90	257.0
112.80	54.0
114.80	87.0
115.90	119.0
117.00	332.0
117.90	201.0
119.00	209.0
127.90	250.0
128.70	85.0
129.10	97.0
129.80	208.0
130.70	78.0
134.90	81.0
136.90	160.0
141.00	653.0
141.90	100.0
142.90	735.0
144.90	147.0
145.90	95.0
147.90	210.0
153.10	64.0
154.80	136.0
157.00	140.0
158.80	74.0
160.80	63.0
171.20	92.0
171.90	447.0
173.00	608.0
173.90	51784.0
174.90	3816.0
175.90	49584.0
177.00	2784.0
177.80	90.0

Instrument :
MSVOA_X
ClientSampleId :
BFB673