

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041725\
 Data File : VX045831.D
 Acq On : 17 Apr 2025 16:19
 Operator : JC/MD
 Sample : Q1824-04DL 1000X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 285DL

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X040225W.M
 Title : SW846 8260

Signal : TIC: VX045831.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.379	693	704	720	rBV2	56511	169792	33.97%	3.111%
2	5.543	721	731	746	rVB	84136	241340	48.28%	4.422%
3	5.952	788	798	808	rBV	65822	178749	35.76%	3.275%
4	6.757	921	930	944	rBV	148114	360087	72.03%	6.598%
5	8.647	1233	1240	1246	rBV	311993	499885	100.00%	9.160%
6	8.714	1246	1251	1268	rVB	191142	313765	62.77%	5.749%
7	10.049	1465	1470	1487	rBV	323455	454804	90.98%	8.334%
8	10.195	1489	1494	1505	rVV	44315	64290	12.86%	1.178%
9	10.299	1505	1511	1528	rVB	206974	292225	58.46%	5.355%
10	10.640	1561	1567	1578	rBV	124318	164204	32.85%	3.009%
11	10.963	1614	1620	1627	rVB	6829	9830	1.97%	0.180%
12	11.079	1634	1639	1652	rBV	266644	346259	69.27%	6.345%
13	11.305	1671	1676	1683	rBV	27836	35987	7.20%	0.659%
14	11.378	1683	1688	1696	rVV	129155	219264	43.86%	4.018%
15	11.451	1696	1700	1711	rVB	70098	92186	18.44%	1.689%
16	11.609	1720	1726	1736	rBV	59207	78570	15.72%	1.440%
17	11.750	1744	1749	1761	rBV	303029	369102	73.84%	6.763%
18	11.890	1769	1772	1778	rVB2	4297	5563	1.11%	0.102%
19	11.969	1778	1785	1788	rBV	9558	11797	2.36%	0.216%
20	12.018	1788	1793	1800	rVV	324241	402212	80.46%	7.370%
21	12.085	1800	1804	1811	rVB	92051	113360	22.68%	2.077%
22	12.244	1825	1830	1832	rBV	53743	72663	14.54%	1.331%
23	12.268	1832	1834	1838	rVV	31536	35069	7.02%	0.643%
24	12.317	1838	1842	1850	rVV3	47545	73145	14.63%	1.340%
25	12.402	1852	1856	1862	rVB5	3929	5946	1.19%	0.109%
26	12.463	1862	1866	1873	rVB	15040	18829	3.77%	0.345%
27	12.530	1873	1877	1879	rBV	28938	38686	7.74%	0.709%
28	12.554	1879	1881	1886	rVV	28238	29691	5.94%	0.544%
29	12.609	1886	1890	1894	rVV	40834	55098	11.02%	1.010%
30	12.640	1894	1895	1899	rVB	9045	8908	1.78%	0.163%
31	12.695	1899	1904	1914	rBV3	25423	45050	9.01%	0.825%
32	12.847	1924	1929	1934	rBV2	13178	16869	3.37%	0.309%
33	12.920	1934	1941	1944	rBV	28340	34276	6.86%	0.628%
34	12.963	1944	1948	1954	rVB	41527	52022	10.41%	0.953%
35	13.024	1954	1958	1960	rBV2	4846	6399	1.28%	0.117%
36	13.164	1977	1981	1986	rVB	28452	38311	7.66%	0.702%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041725\
Data File : VX045831.D
Acq On : 17 Apr 2025 16:19
Operator : JC/MD
Sample : Q1824-04DL 1000X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
285DL

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X040225W.M
Title : SW846 8260

37	13.249	1992	1995	1997	rBV3	5121	6683	1.34%	0.122%
38	13.292	1997	2002	2012	rVB2	67182	96192	19.24%	1.763%
39	13.420	2019	2023	2031	rVB	33354	42216	8.45%	0.774%
40	13.505	2033	2037	2040	rBV5	6254	8961	1.79%	0.164%
41	13.542	2040	2043	2046	rVV	13391	17388	3.48%	0.319%
42	13.585	2046	2050	2055	rVV3	14681	28892	5.78%	0.529%
43	13.664	2055	2063	2069	rVB3	14239	31672	6.34%	0.580%
44	13.774	2075	2081	2088	rBV	23319	33390	6.68%	0.612%
45	13.853	2090	2094	2100	rVB2	12567	16752	3.35%	0.307%
46	13.926	2100	2106	2110	rBV2	13804	21641	4.33%	0.397%
47	13.969	2110	2113	2117	rVB2	5418	6440	1.29%	0.118%
48	14.072	2126	2130	2138	rVB2	11490	15739	3.15%	0.288%
49	14.225	2147	2155	2167	rBV	30771	58040	11.61%	1.063%
50	14.371	2174	2179	2183	rVV2	9867	12358	2.47%	0.226%
51	14.481	2192	2197	2202	rBV2	19379	28002	5.60%	0.513%
52	14.639	2214	2223	2226	rBV2	18464	37066	7.41%	0.679%
53	14.670	2226	2228	2233	rVB3	6664	8107	1.62%	0.149%
54	14.780	2242	2246	2249	rBV	7070	9395	1.88%	0.172%
55	15.182	2306	2312	2315	rBV2	7616	11790	2.36%	0.216%
56	15.481	2357	2361	2366	rBV5	3693	7526	1.51%	0.138%
57	15.609	2378	2382	2387	rBV6	3548	5039	1.01%	0.092%


Sum of corrected areas: 5457522

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041725\
Data File : VX045831.D
Acq On : 17 Apr 2025 16:19
Operator : JC/MD
Sample : Q1824-04DL 1000X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
285DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X040225W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

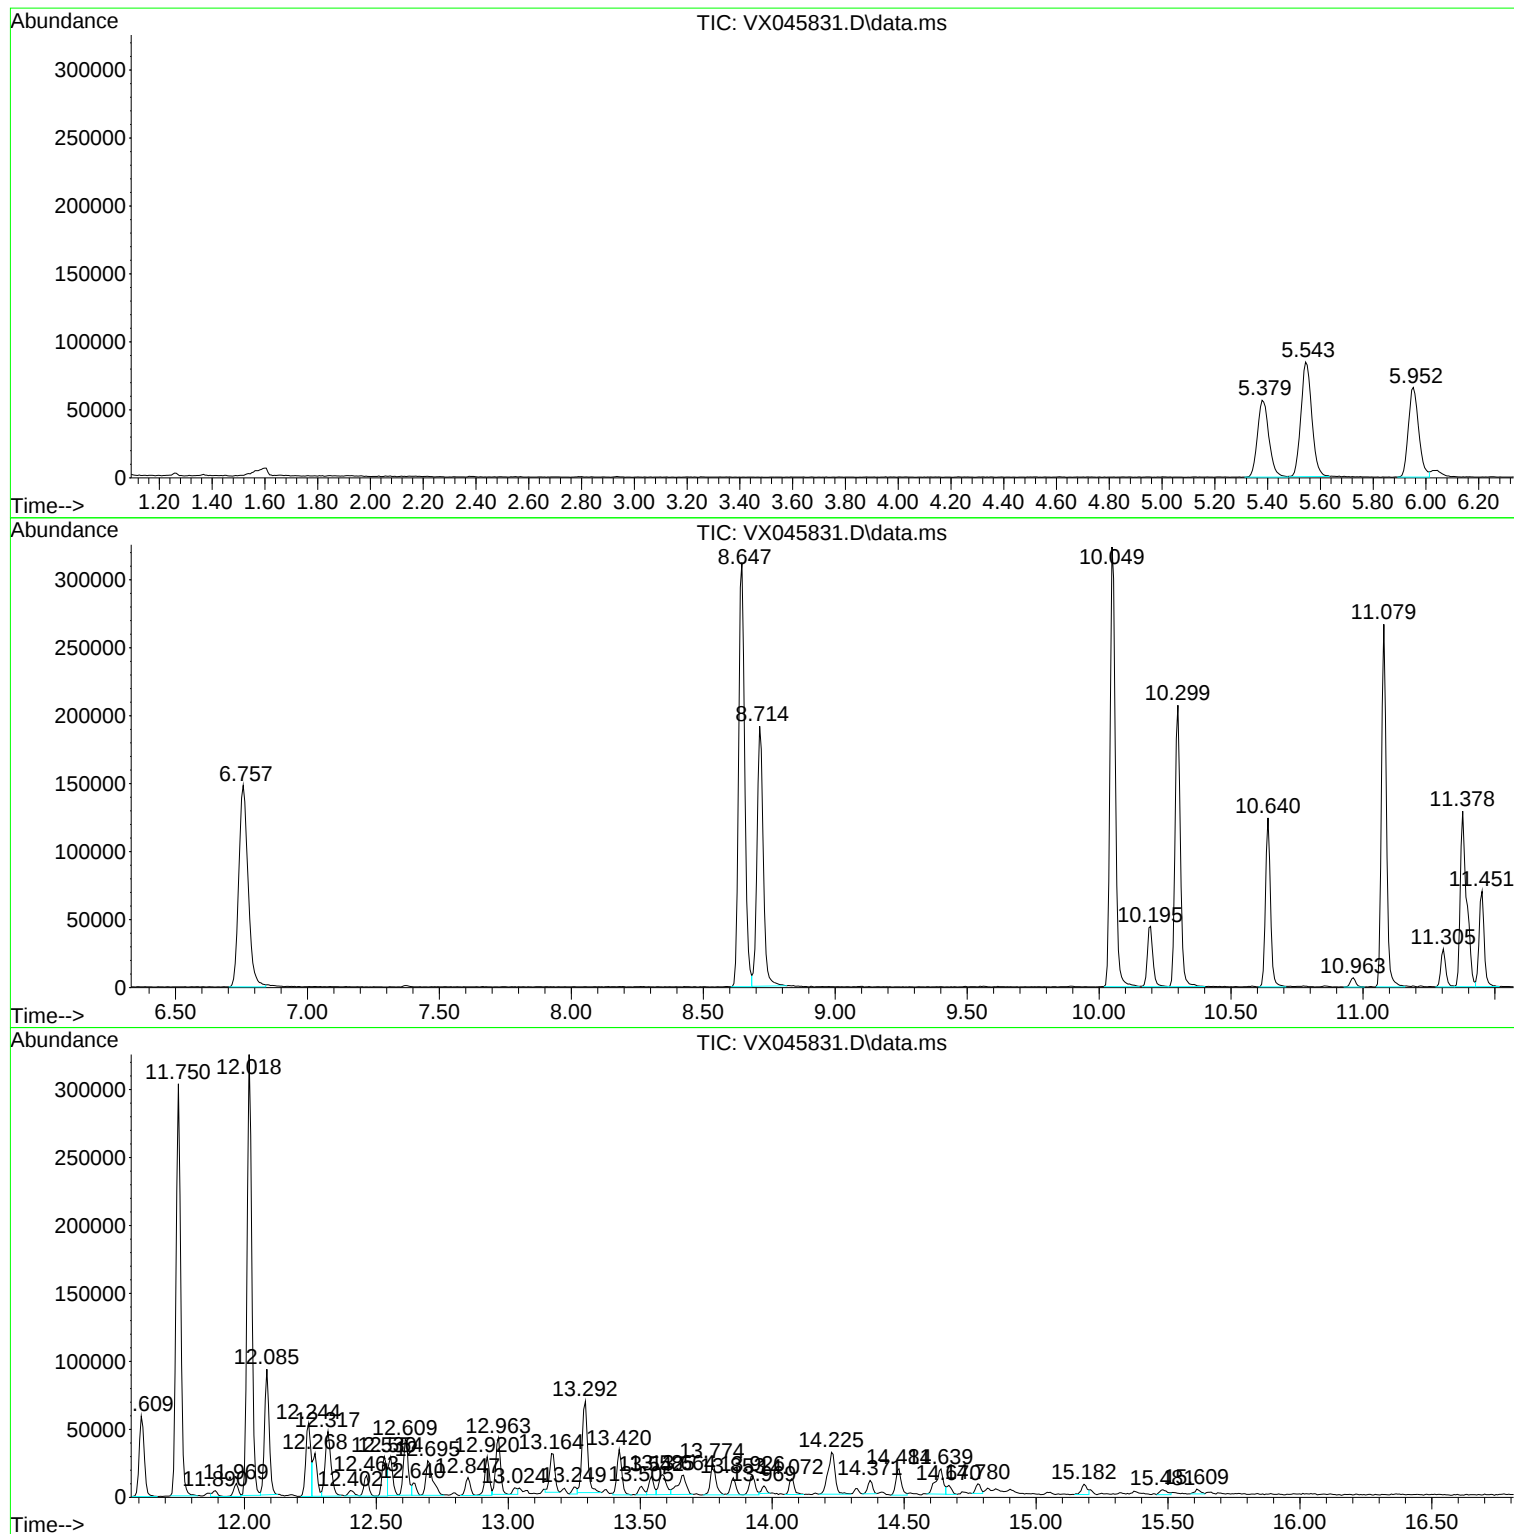

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041725\
Data File : VX045831.D
Acq On : 17 Apr 2025 16:19
Operator : JC/MD
Sample : Q1824-04DL 1000X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
285DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X040225W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041725\
Data File : VX045831.D
Acq On : 17 Apr 2025 16:19
Operator : JC/MD
Sample : Q1824-04DL 1000X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
285DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X040225W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc