

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX041725\  
Data File : VX045838.D  
Acq On : 17 Apr 2025 18:56  
Operator : JC/MD  
Sample : IBLK  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 23 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
IBLK

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X040225W.M

Title : SW846 8260

Signal : TIC: VX045838.D\data.ms

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 1.246       | 22            | 26          | 33           | rBV2     | 4708           | 9111          | 1.74%           | 0.326%        |
| 2         | 1.575       | 67            | 80          | 81           | rBV5     | 5121           | 12883         | 2.47%           | 0.461%        |
| 3         | 5.379       | 694           | 704         | 721          | rBV2     | 61769          | 181397        | 34.73%          | 6.495%        |
| 4         | 5.544       | 721           | 731         | 746          | rVV      | 87231          | 255912        | 49.00%          | 9.163%        |
| 5         | 5.952       | 785           | 798         | 811          | rBV      | 70025          | 188780        | 36.15%          | 6.759%        |
| 6         | 6.757       | 921           | 930         | 948          | rBV      | 154993         | 380476        | 72.85%          | 13.623%       |
| 7         | 8.647       | 1233          | 1240        | 1255         | rBV      | 322785         | 522281        | 100.00%         | 18.701%       |
| 8         | 10.049      | 1465          | 1470        | 1484         | rBV      | 335707         | 468487        | 89.70%          | 16.775%       |
| 9         | 11.079      | 1634          | 1639        | 1653         | rBV      | 269676         | 349506        | 66.92%          | 12.514%       |
| 10        | 12.018      | 1788          | 1793        | 1806         | rBV      | 322772         | 404717        | 77.49%          | 14.491%       |
| 11        | 14.189      | 2144          | 2149        | 2158         | rBV2     | 9985           | 19287         | 3.69%           | 0.691%        |




Sum of corrected areas: 2792837

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX041725\  
Data File : VX045838.D  
Acq On : 17 Apr 2025 18:56  
Operator : JC/MD  
Sample : IBLK  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 23 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
IBLK

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X040225W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

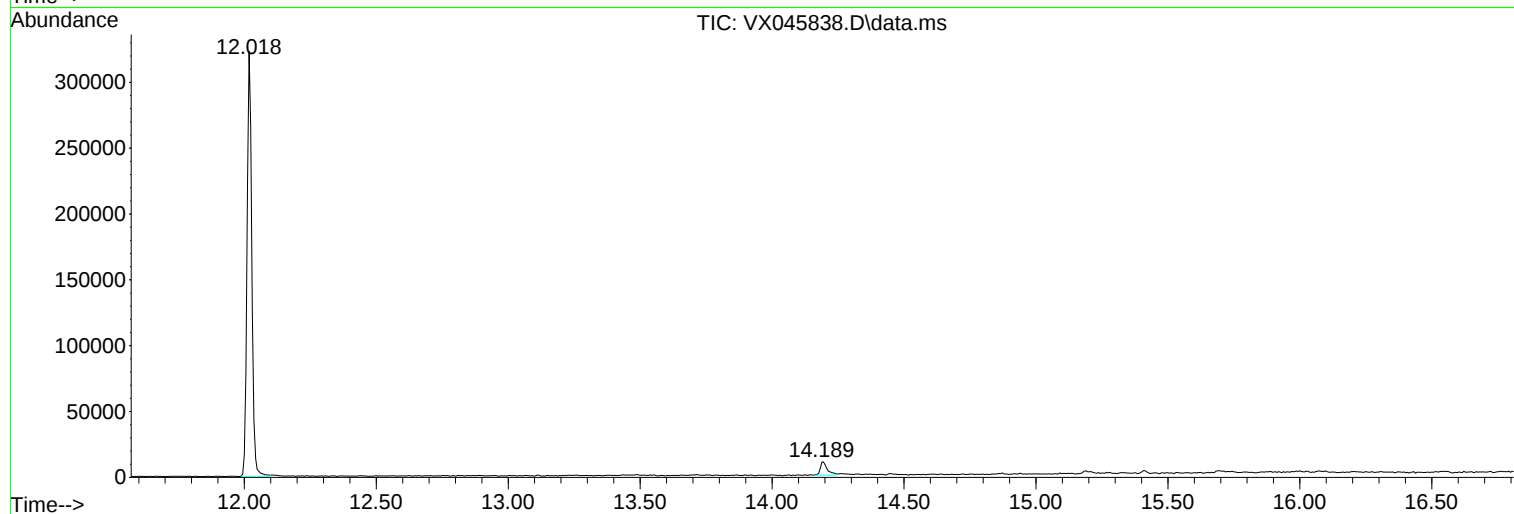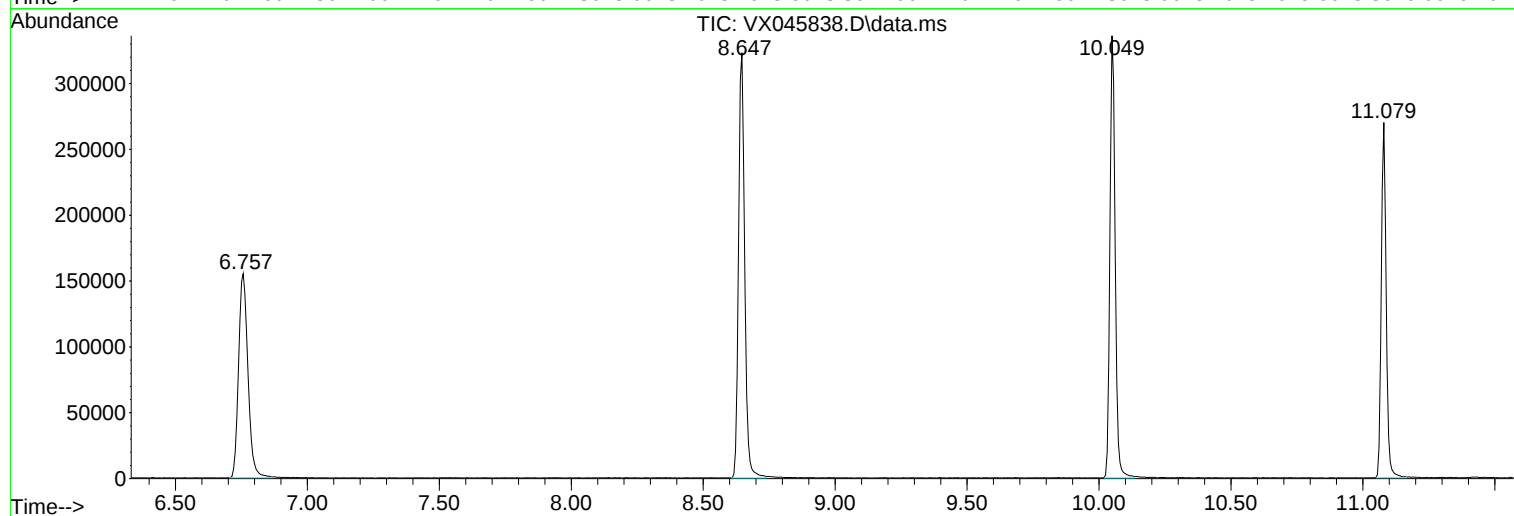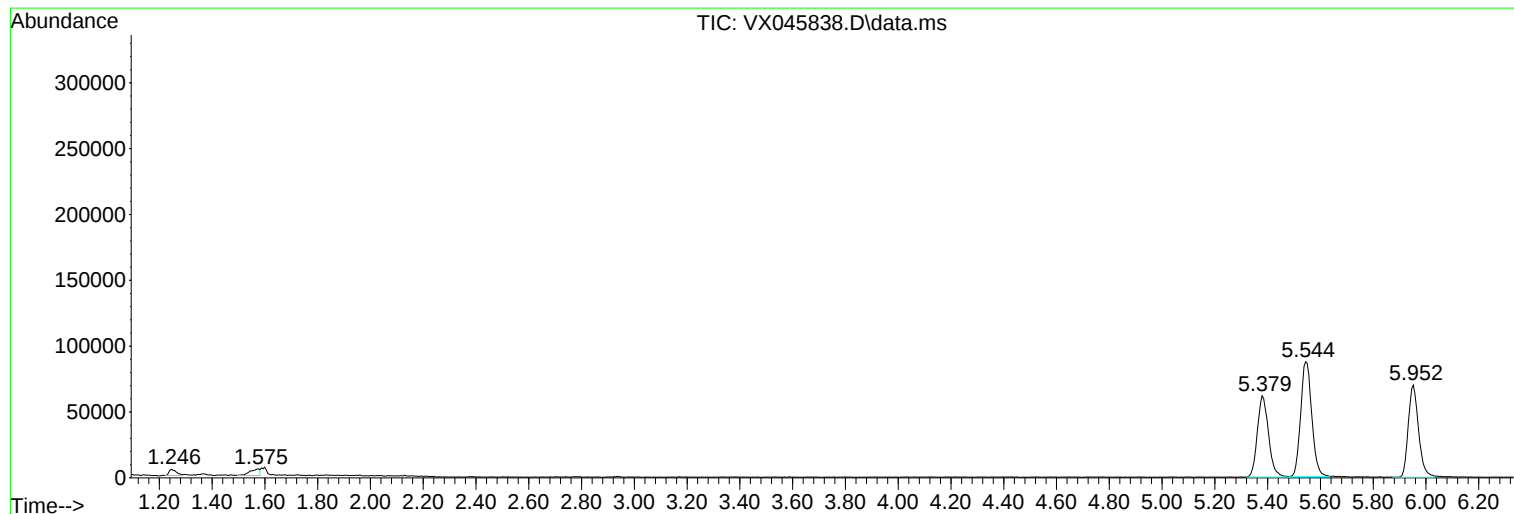

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX041725\  
Data File : VX045838.D  
Acq On : 17 Apr 2025 18:56  
Operator : JC/MD  
Sample : IBLK  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 23 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
IBLK

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X040225W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX041725\  
Data File : VX045838.D  
Acq On : 17 Apr 2025 18:56  
Operator : JC/MD  
Sample : IBLK  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 23 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
IBLK

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X040225W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | --Internal Standard-- |    |      |      |
|------------------|----|---------|-------|----------|-----------------------|----|------|------|
|                  |    |         |       |          | #                     | RT | Resp | Conc |