


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX041819\
Data File : VX009030.D
Acq On : 18 Apr 2019 09:12
Operator : JC/SP
Sample : BFB
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X041519W.M
Title : SW846 8260
Last Update : Wed Apr 17 06:47:58 2019

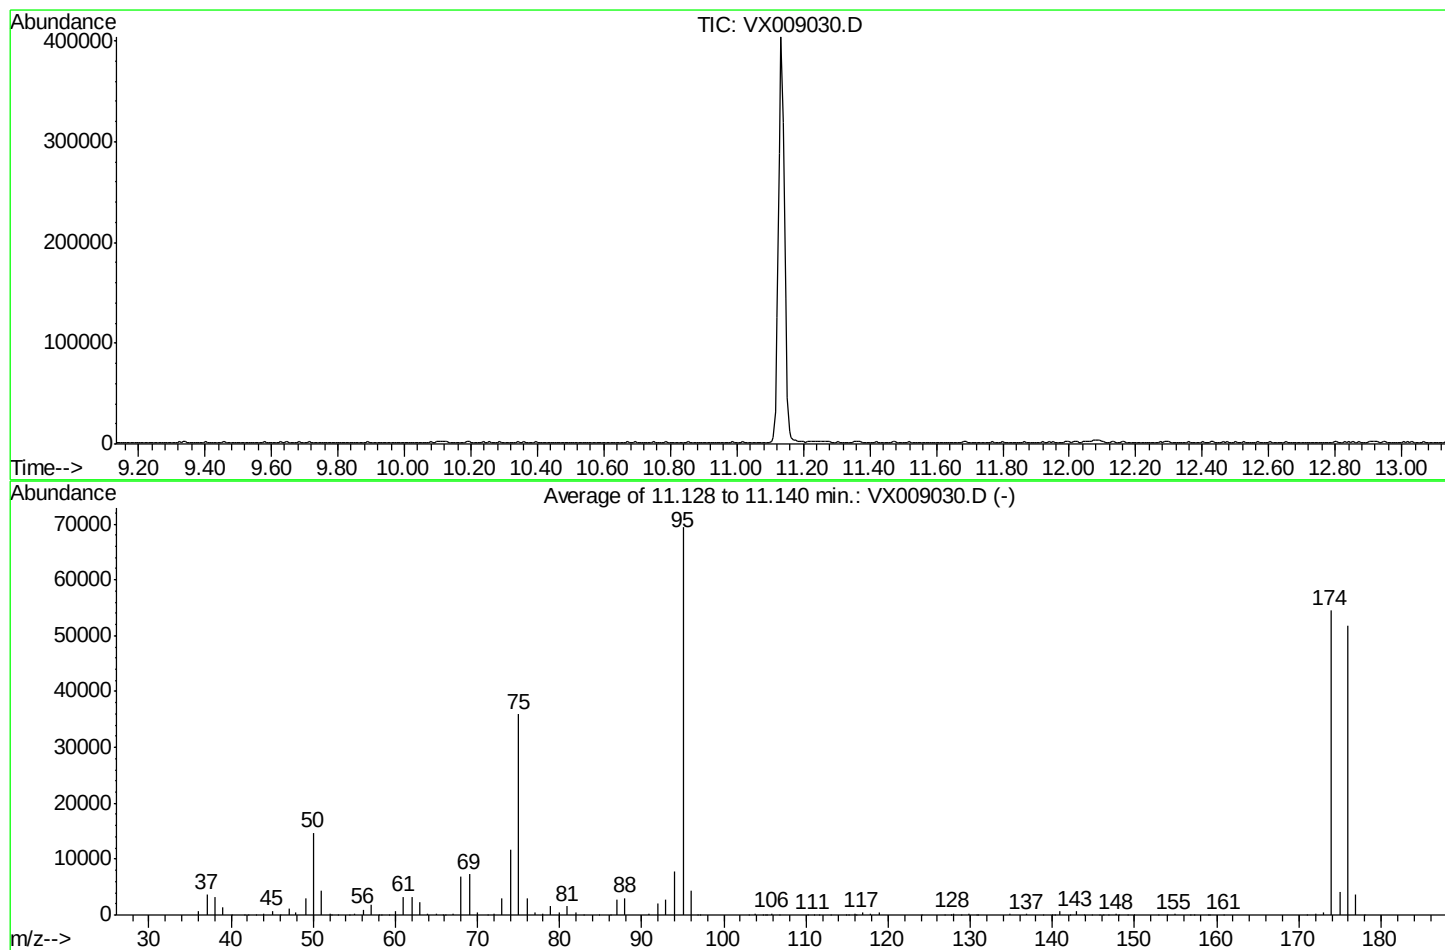

AutoFind: Scans 1636, 1637, 1638; Background Corrected with Scan 1629

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.3	14759	PASS
75	95	30	60	51.7	35872	PASS
95	95	100	100	100.0	69400	PASS
96	95	5	9	6.4	4422	PASS
173	174	0.00	2	1.1	575	PASS
174	95	50	100	78.6	54514	PASS
175	174	5	9	7.5	4102	PASS
176	174	95	101	95.2	51893	PASS
177	176	5	9	7.0	3627	PASS