

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041823\
 Data File : VX035123.D
 Acq On : 18 Apr 2023 15:15
 Operator : JC/MD
 Sample : VX0418WBL02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK622

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M
 Title : VOC Analysis

Signal : TIC: VX035123.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.264	26	29	31	rBV2	2518	2669	0.14%	0.019%
2	1.367	42	46	62	rBV	217048	261580	13.58%	1.838%
3	1.672	91	96	109	rBV	143861	223845	11.62%	1.573%
4	2.306	193	200	211	rBV	429669	692448	35.94%	4.865%
5	2.508	229	233	240	rVB	5038	8256	0.43%	0.058%
6	2.617	249	251	252	rBV2	391	376	0.02%	0.003%
7	2.678	259	261	262	rVV	430	327	0.02%	0.002%
8	2.703	262	265	271	rVV5	1929	3155	0.16%	0.022%
9	2.788	274	279	287	rVB3	8676	16343	0.85%	0.115%
10	2.898	296	297	301	rVB	460	296	0.02%	0.002%
11	2.995	310	313	316	rBV2	286	391	0.02%	0.003%
12	3.093	323	329	330	rBV2	4836	6919	0.36%	0.049%
13	3.446	386	387	391	rVB2	499	367	0.02%	0.003%
14	3.611	409	414	425	rVB5	2274	5376	0.28%	0.038%
15	3.684	425	426	428	rBV	357	334	0.02%	0.002%
16	3.977	470	474	476	rBV	318	481	0.02%	0.003%
17	4.117	494	497	498	rBV2	292	294	0.02%	0.002%
18	4.184	505	508	510	rBV2	283	331	0.02%	0.002%
19	4.202	510	511	514	rVB	363	240	0.01%	0.002%
20	4.233	514	516	517	rBV2	294	263	0.01%	0.002%
21	4.465	545	554	571	rBV	119492	368560	19.13%	2.590%
22	4.690	589	591	592	rVB2	555	333	0.02%	0.002%
23	4.727	592	597	599	rBV3	328	589	0.03%	0.004%
24	4.897	618	625	634	rVB5	1770	4787	0.25%	0.034%
25	5.056	639	651	671	rVV	230045	728854	37.83%	5.121%
26	5.385	698	705	710	rBV5	3340	8106	0.42%	0.057%
27	5.550	727	732	738	rBV3	4051	9410	0.49%	0.066%
28	5.751	761	765	766	rBV3	187	237	0.01%	0.002%
29	5.964	784	800	819	rBV2	648957	1926664	100.00%	13.538%
30	6.214	839	841	844	rBV2	466	362	0.02%	0.003%
31	6.361	863	865	868	rVB	337	302	0.02%	0.002%
32	6.452	878	880	883	rBV3	348	406	0.02%	0.003%
33	6.549	892	896	897	rBV2	309	321	0.02%	0.002%
34	6.757	917	930	948	rVV	475199	1138914	59.11%	8.003%
35	7.123	982	990	1000	rVB5	7968	21298	1.11%	0.150%
36	7.305	1011	1020	1029	rBV	397369	857167	44.49%	6.023%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041823\
 Data File : VX035123.D
 Acq On : 18 Apr 2023 15:15
 Operator : JC/MD
 Sample : VX0418WBL02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK622

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M
 Title : VOC Analysis

37	7.622	1068	1072	1073	rVV2	236	260	0.01%	0.002%
38	7.653	1074	1077	1080	rVB2	273	348	0.02%	0.002%
39	7.830	1100	1106	1111	rVB4	1927	3846	0.20%	0.027%
40	7.939	1121	1124	1128	rBV3	845	1632	0.08%	0.011%
41	8.324	1180	1187	1206	rBV	249166	415402	21.56%	2.919%
42	8.445	1206	1207	1210	rVB2	758	553	0.03%	0.004%
43	8.574	1224	1228	1233	rBV	4979	8462	0.44%	0.059%
44	8.647	1233	1240	1249	rBV	1015846	1574445	81.72%	11.063%
45	8.952	1284	1290	1305	rBV	168929	264972	13.75%	1.862%
46	9.159	1319	1324	1330	rVB4	4520	7445	0.39%	0.052%
47	9.275	1338	1343	1350	rVB3	6446	10602	0.55%	0.074%
48	9.384	1356	1361	1380	rBV	526922	803940	41.73%	5.649%
49	9.610	1394	1398	1404	rVB3	2433	4624	0.24%	0.032%
50	9.653	1404	1405	1406	rBV	497	259	0.01%	0.002%
51	9.793	1426	1428	1431	rVB3	409	363	0.02%	0.003%
52	9.951	1451	1454	1456	rVB3	343	322	0.02%	0.002%
53	9.988	1458	1460	1463	rBV2	325	399	0.02%	0.003%
54	10.055	1465	1471	1488	rBV	923795	1276070	66.23%	8.966%
55	10.195	1490	1494	1501	rVB	11015	14903	0.77%	0.105%
56	10.305	1507	1512	1519	rVB	9802	14417	0.75%	0.101%
57	10.579	1555	1557	1560	rBV3	372	296	0.02%	0.002%
58	10.646	1563	1568	1577	rVV3	13557	28136	1.46%	0.198%
59	10.732	1580	1582	1584	rVB2	453	315	0.02%	0.002%
60	10.762	1584	1587	1588	rBV2	422	333	0.02%	0.002%
61	10.805	1589	1594	1598	rBV3	1650	2057	0.11%	0.014%
62	10.963	1615	1620	1627	rVB	13134	17312	0.90%	0.122%
63	11.018	1627	1629	1633	rVB	353	372	0.02%	0.003%
64	11.061	1633	1636	1637	rBV	432	357	0.02%	0.003%
65	11.085	1638	1640	1643	rVB2	545	585	0.03%	0.004%
66	11.189	1652	1657	1664	rBV	614541	826739	42.91%	5.809%
67	11.384	1687	1689	1690	rVB2	426	275	0.01%	0.002%
68	11.402	1690	1692	1696	rBV2	306	354	0.02%	0.002%
69	11.451	1696	1700	1705	rBV	17087	21609	1.12%	0.152%
70	11.549	1713	1716	1719	rBV3	285	464	0.02%	0.003%
71	11.634	1728	1730	1735	rBV5	570	724	0.04%	0.005%
72	11.683	1735	1738	1740	rVV2	747	817	0.04%	0.006%
73	11.713	1740	1743	1745	rVV3	857	945	0.05%	0.007%
74	11.750	1745	1749	1757	rVB	14014	19328	1.00%	0.136%
75	11.829	1761	1762	1767	rVB2	436	496	0.03%	0.003%
76	11.878	1767	1770	1771	rBV2	384	324	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041823\
 Data File : VX035123.D
 Acq On : 18 Apr 2023 15:15
 Operator : JC/MD
 Sample : VX0418WBL02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK622

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM041823WMA.M
 Title : VOC Analysis

77	11.969	1781	1785	1788	rBV2	11313	13599	0.71%	0.096%
78	12.024	1788	1794	1804	rVB	874843	1172051	60.83%	8.235%
79	12.317	1837	1842	1856	rBV	948977	1264960	65.66%	8.888%
80	12.555	1877	1881	1885	rVB2	337	560	0.03%	0.004%
81	12.591	1885	1887	1890	rVB	299	364	0.02%	0.003%
82	12.622	1890	1892	1893	rBV2	334	296	0.02%	0.002%
83	12.762	1912	1915	1919	rVB3	820	948	0.05%	0.007%
84	12.945	1940	1945	1951	rBV5	1746	2574	0.13%	0.018%
85	13.061	1962	1964	1965	rBV	234	231	0.01%	0.002%
86	13.115	1968	1973	1982	rVV	33084	43623	2.26%	0.307%
87	13.323	2005	2007	2008	rVB2	403	284	0.01%	0.002%
88	13.591	2046	2051	2058	rBV	26232	33524	1.74%	0.236%
89	13.676	2061	2065	2066	rBV	266	280	0.01%	0.002%
90	13.780	2074	2082	2090	rBV	15669	22073	1.15%	0.155%
91	13.932	2104	2107	2108	rBV2	462	434	0.02%	0.003%
92	13.963	2108	2112	2121	rVV	25181	33016	1.71%	0.232%
93	14.127	2136	2139	2142	rBV4	708	982	0.05%	0.007%
94	14.237	2154	2157	2159	rBV4	288	310	0.02%	0.002%
95	14.304	2166	2168	2172	rVB2	374	257	0.01%	0.002%
96	14.810	2249	2251	2254	rBV3	450	667	0.03%	0.005%
97	15.078	2294	2295	2297	rBV3	462	408	0.02%	0.003%
98	15.213	2314	2317	2321	rVB6	2638	3324	0.17%	0.023%
99	15.493	2360	2363	2367	rVB3	4654	5716	0.30%	0.040%
100	16.377	2503	2508	2513	rBV4	8916	15785	0.82%	0.111%




Sum of corrected areas: 14231969

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041823\
Data File : VX035123.D
Acq On : 18 Apr 2023 15:15
Operator : JC/MD
Sample : VX0418WBL02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK622

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

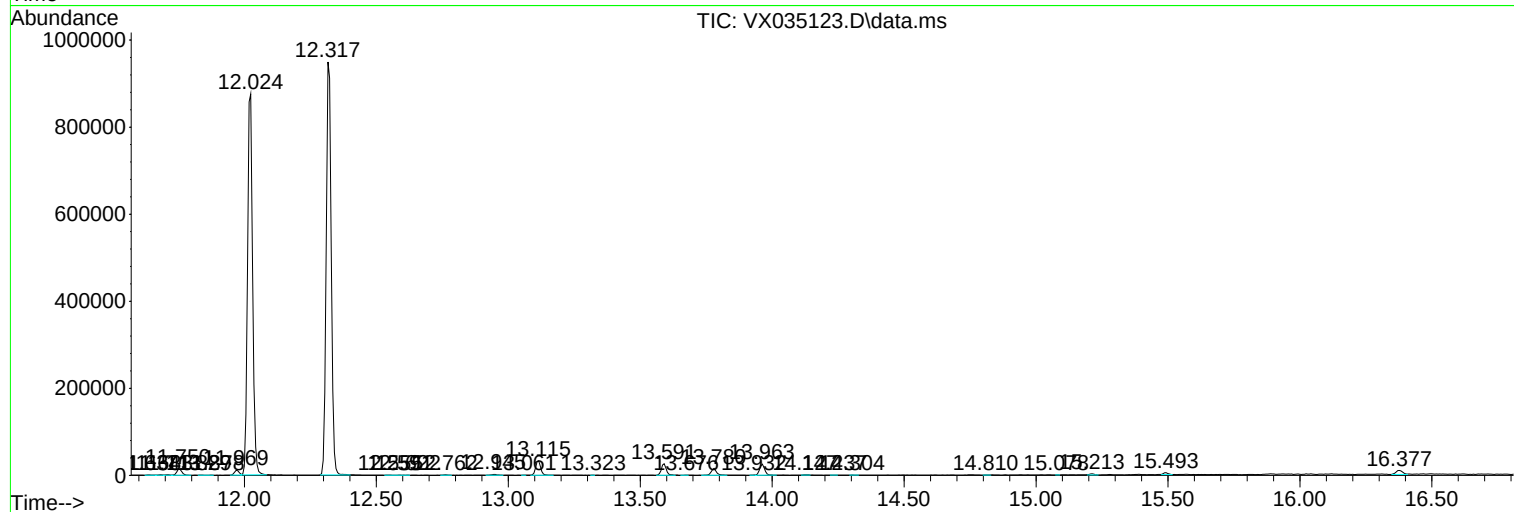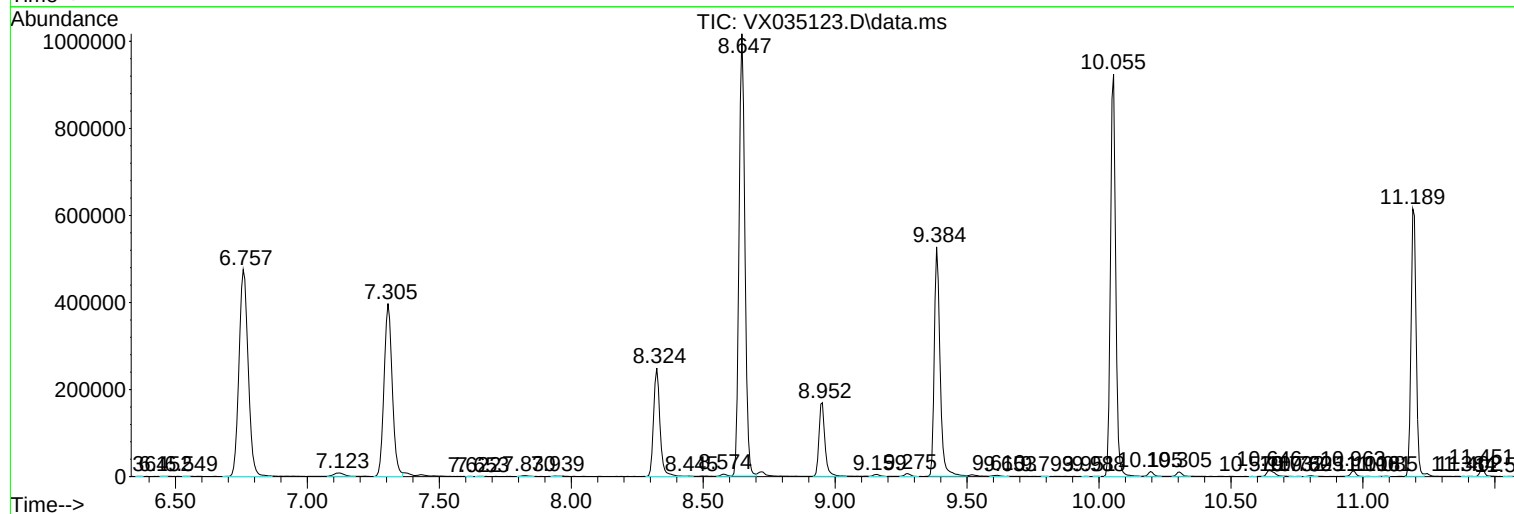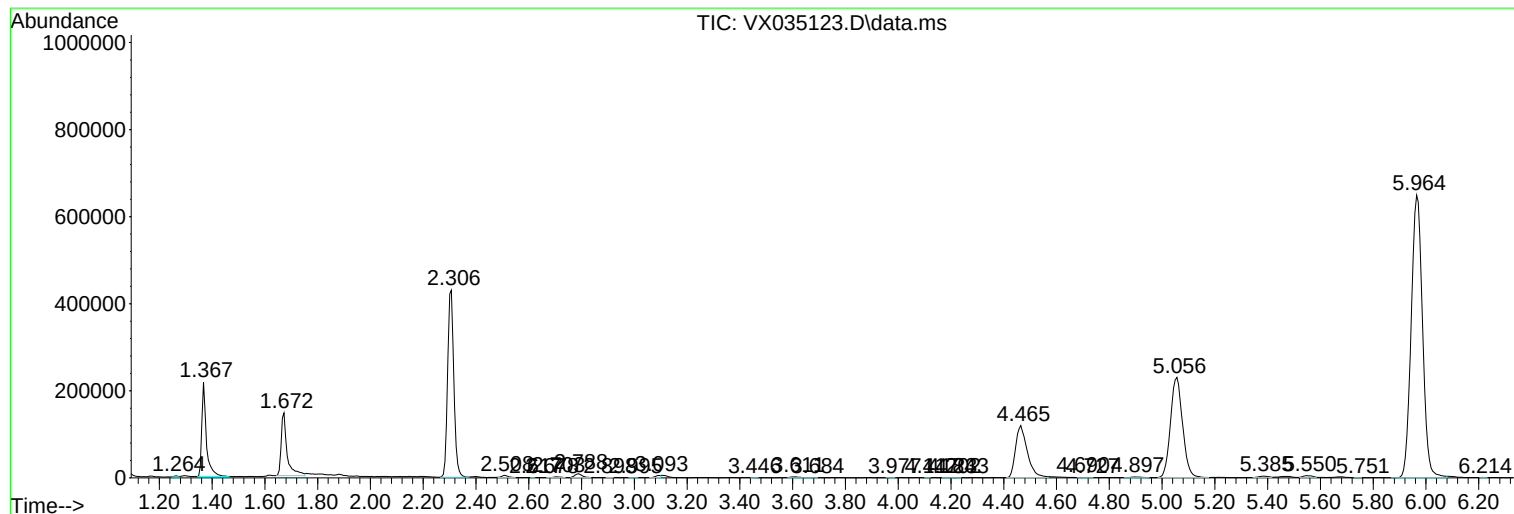

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041823\
Data File : VX035123.D
Acq On : 18 Apr 2023 15:15
Operator : JC/MD
Sample : VX0418WBL02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK622

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM041823WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041823\
Data File : VX035123.D
Acq On : 18 Apr 2023 15:15
Operator : JC/MD
Sample : VX0418WBL02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK622

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------