

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041823\
 Data File : VX035124.D
 Acq On : 18 Apr 2023 15:42
 Operator : JC/MD
 Sample : 02333-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 COMF6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M
 Title : VOC Analysis

Signal : TIC: VX035124.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.264	26	29	31	rBV2	2301	2547	0.17%	0.022%
2	1.368	42	46	57	rBV	178820	194612	13.10%	1.652%
3	1.672	91	96	115	rBV	129528	178138	11.99%	1.512%
4	2.306	194	200	209	rBV	341754	526087	35.41%	4.466%
5	2.508	229	233	240	rVB2	2538	4679	0.31%	0.040%
6	2.562	240	242	246	rBV3	304	363	0.02%	0.003%
7	2.666	257	259	263	rVB2	475	521	0.04%	0.004%
8	2.709	263	266	274	rVV2	465	866	0.06%	0.007%
9	2.788	274	279	285	rVB3	2156	2910	0.20%	0.025%
10	3.099	325	330	337	rVV4	893	1920	0.13%	0.016%
11	3.148	337	338	341	rVV2	320	304	0.02%	0.003%
12	3.245	351	354	355	rVB2	292	209	0.01%	0.002%
13	3.312	364	365	370	rVB3	308	331	0.02%	0.003%
14	3.422	381	383	386	rBV	309	362	0.02%	0.003%
15	3.495	393	395	399	rBV2	312	363	0.02%	0.003%
16	3.593	410	411	414	rVV2	297	253	0.02%	0.002%
17	3.696	421	428	432	rVB3	260	624	0.04%	0.005%
18	3.733	432	434	435	rBV	236	220	0.01%	0.002%
19	3.788	441	443	445	rVB2	293	245	0.02%	0.002%
20	3.873	455	457	460	rBV3	336	328	0.02%	0.003%
21	3.995	476	477	480	rVB	479	287	0.02%	0.002%
22	4.032	480	483	486	rBV2	343	446	0.03%	0.004%
23	4.178	502	507	510	rBV2	339	575	0.04%	0.005%
24	4.465	545	554	571	rBV	86222	272644	18.35%	2.315%
25	4.769	603	604	606	rVB	448	269	0.02%	0.002%
26	4.794	606	608	609	rBV	407	311	0.02%	0.003%
27	4.940	630	632	637	rBV2	248	376	0.03%	0.003%
28	5.056	637	651	670	rBV	182322	593089	39.92%	5.035%
29	5.367	698	702	703	rBV3	636	741	0.05%	0.006%
30	5.470	718	719	722	rVV2	385	389	0.03%	0.003%
31	5.519	724	727	728	rVV2	759	706	0.05%	0.006%
32	5.562	728	734	742	rVV4	3000	7452	0.50%	0.063%
33	5.635	744	746	748	rVB2	339	256	0.02%	0.002%
34	5.653	748	749	752	rBV2	290	290	0.02%	0.002%
35	5.830	776	778	780	rBV2	287	292	0.02%	0.002%
36	5.964	786	800	820	rBV2	492568	1485824	100.00%	12.614%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041823\
 Data File : VX035124.D
 Acq On : 18 Apr 2023 15:42
 Operator : JC/MD
 Sample : 02333-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 COMF6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M
 Title : VOC Analysis

37	6.446	877	879	882	rVB2	292	272	0.02%	0.002%
38	6.482	882	885	887	rBV2	470	478	0.03%	0.004%
39	6.543	891	895	897	rBV3	379	564	0.04%	0.005%
40	6.757	920	930	951	rBV	525627	1247128	83.94%	10.588%
41	7.190	999	1001	1003	rBV	296	341	0.02%	0.003%
42	7.306	1011	1020	1038	rBV	300449	665916	44.82%	5.653%
43	7.452	1043	1044	1045	rBV	537	273	0.02%	0.002%
44	7.555	1060	1061	1064	rBV	340	456	0.03%	0.004%
45	7.610	1068	1070	1072	rVV2	451	306	0.02%	0.003%
46	7.702	1084	1085	1088	rVB2	340	244	0.02%	0.002%
47	7.732	1088	1090	1091	rBV2	268	260	0.02%	0.002%
48	7.854	1104	1110	1112	rBV2	1256	1467	0.10%	0.012%
49	7.940	1121	1124	1125	rBV3	470	600	0.04%	0.005%
50	8.049	1140	1142	1145	rVB2	382	321	0.02%	0.003%
51	8.159	1156	1160	1161	rBV2	242	266	0.02%	0.002%
52	8.202	1166	1167	1170	rVB2	259	224	0.02%	0.002%
53	8.324	1180	1187	1206	rBV	169585	284841	19.17%	2.418%
54	8.500	1213	1216	1220	rBV3	511	671	0.05%	0.006%
55	8.647	1233	1240	1260	rBV	783924	1219631	82.08%	10.354%
56	8.952	1284	1290	1301	rBV	116871	178479	12.01%	1.515%
57	9.116	1314	1317	1320	rBV2	327	287	0.02%	0.002%
58	9.275	1340	1343	1349	rVB4	2626	3467	0.23%	0.029%
59	9.384	1356	1361	1377	rBV	402003	594712	40.03%	5.049%
60	9.610	1396	1398	1403	rVB3	670	850	0.06%	0.007%
61	9.781	1424	1426	1428	rBV2	496	447	0.03%	0.004%
62	10.055	1465	1471	1489	rBV	1000008	1381712	92.99%	11.730%
63	10.305	1510	1512	1517	rVB3	967	1226	0.08%	0.010%
64	10.372	1521	1523	1524	rBV2	401	372	0.03%	0.003%
65	10.585	1554	1558	1561	rBV2	262	306	0.02%	0.003%
66	10.652	1565	1569	1570	rBV2	916	907	0.06%	0.008%
67	10.774	1587	1589	1593	rBV2	205	289	0.02%	0.002%
68	10.969	1617	1621	1626	rVB3	1173	1525	0.10%	0.013%
69	11.085	1635	1640	1648	rBV3	570	1369	0.09%	0.012%
70	11.189	1652	1657	1673	rVV	466688	620936	41.79%	5.272%
71	11.311	1673	1677	1683	rVB3	1974	2951	0.20%	0.025%
72	11.366	1683	1686	1689	rBV2	398	445	0.03%	0.004%
73	11.457	1697	1701	1708	rVB4	1256	1956	0.13%	0.017%
74	11.579	1719	1721	1723	rBV	228	223	0.02%	0.002%
75	11.604	1723	1725	1731	rVB2	373	614	0.04%	0.005%
76	11.677	1733	1737	1740	rVB3	474	641	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041823\
 Data File : VX035124.D
 Acq On : 18 Apr 2023 15:42
 Operator : JC/MD
 Sample : 02333-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 COMF6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M
 Title : VOC Analysis

77	11.707	1740	1742	1744	rBV2	506	519	0.03%	0.004%
78	11.756	1747	1750	1752	rBV4	914	1019	0.07%	0.009%
79	11.811	1757	1759	1760	rBV2	627	469	0.03%	0.004%
80	11.933	1777	1779	1782	rVV3	1081	981	0.07%	0.008%
81	11.969	1782	1785	1788	rVV3	1660	2104	0.14%	0.018%
82	12.024	1788	1794	1806	rBV	967048	1263943	85.07%	10.731%
83	12.219	1822	1826	1831	rBV2	9077	13774	0.93%	0.117%
84	12.317	1837	1842	1856	rVB	743058	958237	64.49%	8.135%
85	12.542	1876	1879	1880	rBV2	448	606	0.04%	0.005%
86	12.585	1883	1886	1888	rBV2	698	786	0.05%	0.007%
87	12.768	1910	1916	1917	rBV3	813	1222	0.08%	0.010%
88	12.853	1927	1930	1936	rVB4	4141	5815	0.39%	0.049%
89	13.115	1969	1973	1979	rBV3	6686	8903	0.60%	0.076%
90	13.250	1992	1995	1996	rBV3	645	790	0.05%	0.007%
91	13.353	2011	2012	2014	rBV2	408	355	0.02%	0.003%
92	13.445	2023	2027	2028	rBV3	775	957	0.06%	0.008%
93	13.591	2047	2051	2055	rVB2	4603	6135	0.41%	0.052%
94	13.737	2073	2075	2077	rVV3	783	875	0.06%	0.007%
95	13.780	2078	2082	2087	rVB	3545	4686	0.32%	0.040%
96	13.963	2107	2112	2116	rBV5	4915	6674	0.45%	0.057%
97	14.024	2119	2122	2125	rBV3	432	709	0.05%	0.006%
98	14.493	2197	2199	2201	rVB3	591	454	0.03%	0.004%
99	14.682	2229	2230	2232	rBV	565	293	0.02%	0.002%
100	15.127	2301	2303	2305	rBV2	717	758	0.05%	0.006%


Sum of corrected areas: 11778866

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041823\
Data File : VX035124.D
Acq On : 18 Apr 2023 15:42
Operator : JC/MD
Sample : 02333-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
COMF6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

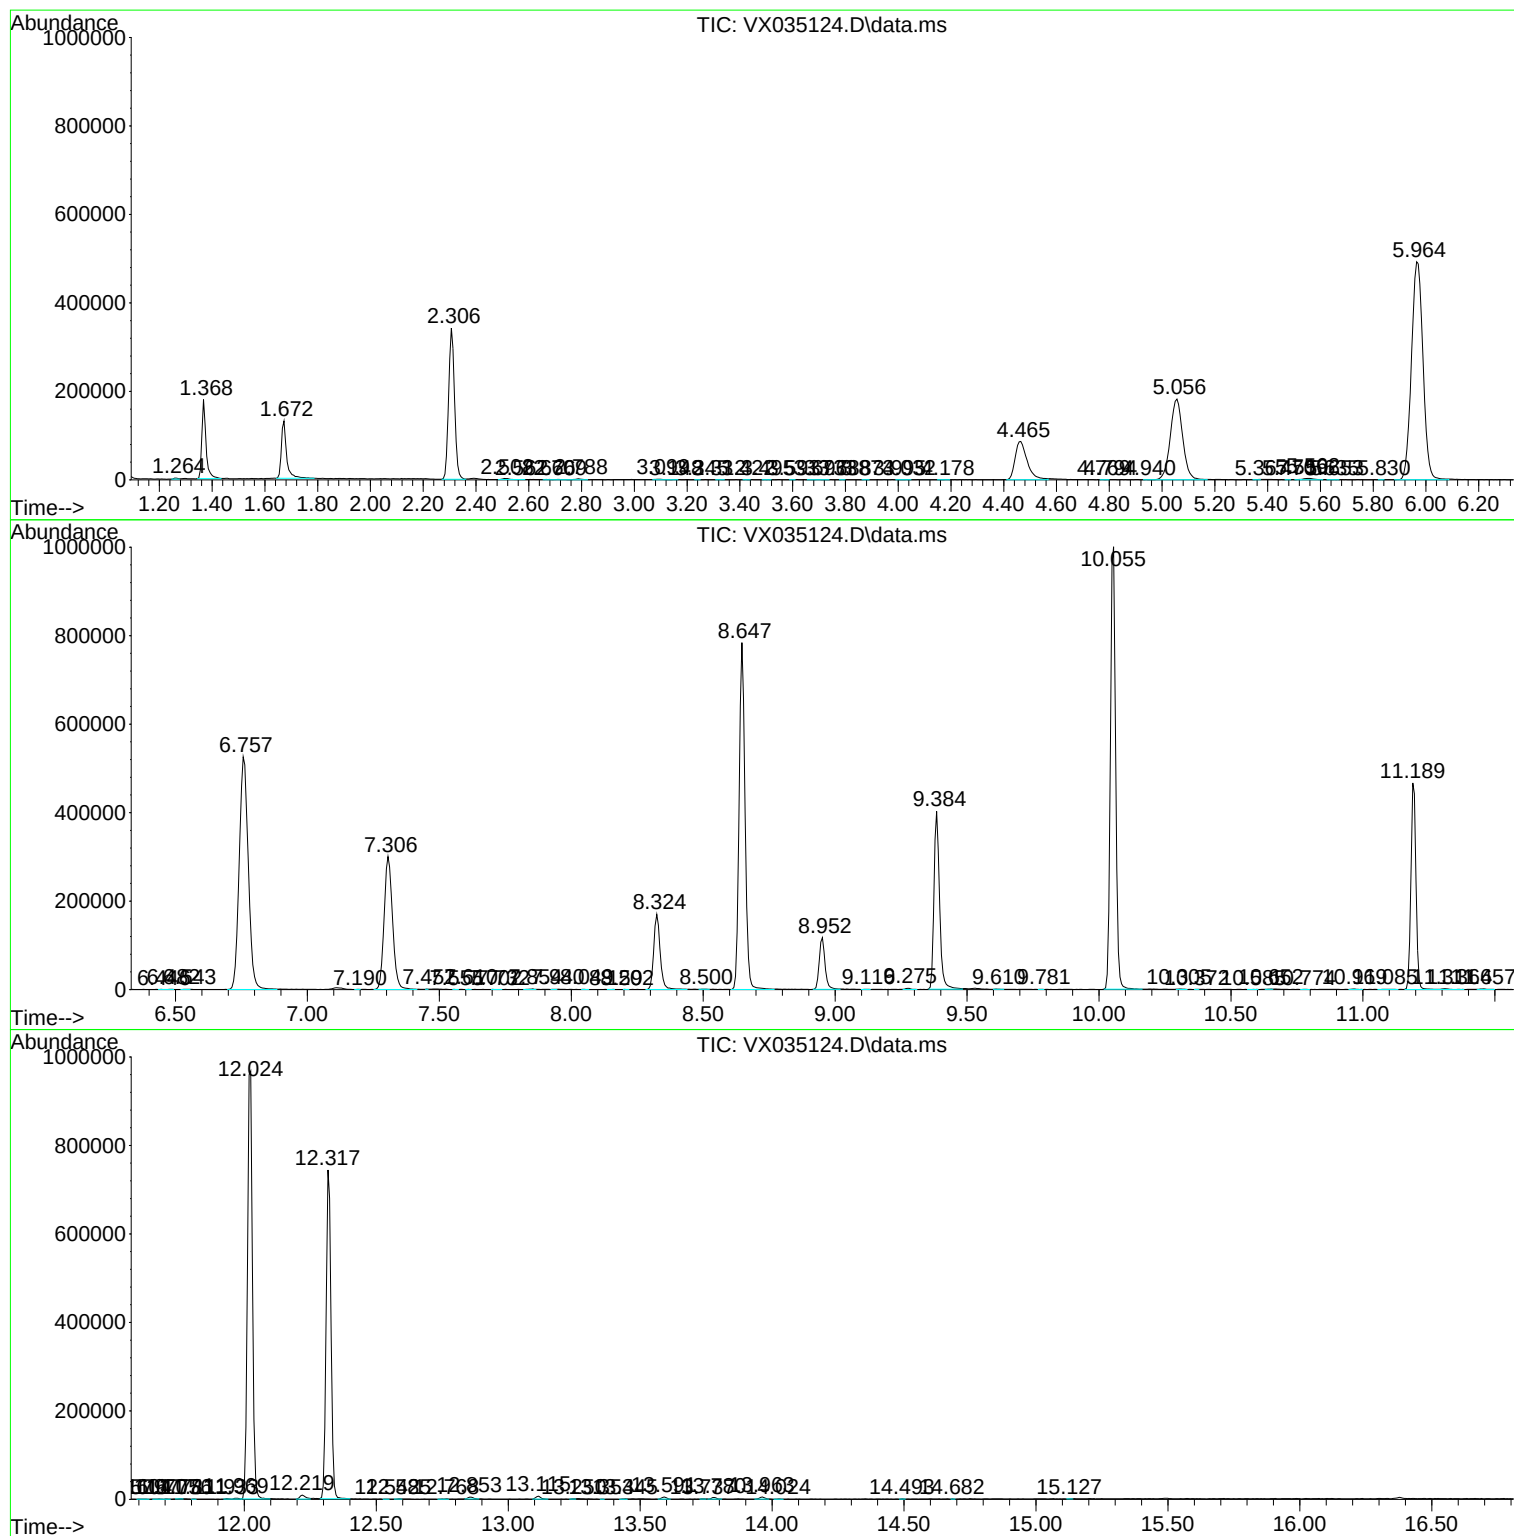

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041823\
Data File : VX035124.D
Acq On : 18 Apr 2023 15:42
Operator : JC/MD
Sample : 02333-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
COMF6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM041823WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041823\
Data File : VX035124.D
Acq On : 18 Apr 2023 15:42
Operator : JC/MD
Sample : 02333-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
COMF6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------