

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041823\
 Data File : VX035125.D
 Acq On : 18 Apr 2023 16:05
 Operator : JC/MD
 Sample : 02378-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 COMJ4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M
 Title : VOC Analysis

Signal : TIC: VX035125.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.264	26	29	31	rBV3	2524	2708	0.18%	0.023%
2	1.367	42	46	56	rBV	184372	196155	13.36%	1.699%
3	1.672	91	96	108	rBV	127595	176527	12.03%	1.529%
4	2.306	194	200	210	rBV	336341	521591	35.53%	4.518%
5	2.508	229	233	239	rVB2	2135	3708	0.25%	0.032%
6	2.605	246	249	250	rBV2	405	353	0.02%	0.003%
7	2.751	270	273	274	rBV3	266	316	0.02%	0.003%
8	2.788	274	279	285	rVV5	1496	3178	0.22%	0.028%
9	2.989	311	312	315	rBV2	306	314	0.02%	0.003%
10	3.087	325	328	329	rBV	766	770	0.05%	0.007%
11	3.257	354	356	357	rVB	402	210	0.01%	0.002%
12	3.312	364	365	368	rVB3	254	224	0.02%	0.002%
13	3.404	379	380	383	rBV	377	268	0.02%	0.002%
14	3.879	457	458	461	rVB	304	212	0.01%	0.002%
15	3.916	461	464	466	rBV	231	234	0.02%	0.002%
16	3.952	469	470	474	rVB	386	229	0.02%	0.002%
17	3.989	474	476	479	rVB2	273	249	0.02%	0.002%
18	4.080	489	491	493	rVB2	271	237	0.02%	0.002%
19	4.099	493	494	497	rBV2	192	226	0.02%	0.002%
20	4.385	538	541	542	rBV	257	257	0.02%	0.002%
21	4.464	545	554	569	rBV	89440	271089	18.47%	2.348%
22	4.830	612	614	616	rVV2	543	471	0.03%	0.004%
23	4.861	618	619	624	rVV2	491	362	0.02%	0.003%
24	5.056	637	651	668	rBV	184882	590348	40.22%	5.113%
25	5.300	690	691	693	rBV	272	219	0.01%	0.002%
26	5.391	699	706	710	rBV4	1039	2578	0.18%	0.022%
27	5.464	715	718	723	rVV5	495	1038	0.07%	0.009%
28	5.550	727	732	743	rVB4	2705	7337	0.50%	0.064%
29	5.726	755	761	765	rBV2	317	673	0.05%	0.006%
30	5.836	777	779	782	rVB	253	224	0.02%	0.002%
31	5.970	788	801	817	rBV2	487788	1467929	100.00%	12.714%
32	6.220	840	842	843	rBV	282	213	0.01%	0.002%
33	6.367	863	866	869	rVV2	396	472	0.03%	0.004%
34	6.397	869	871	874	rVV2	188	264	0.02%	0.002%
35	6.440	876	878	881	rBV2	192	289	0.02%	0.003%
36	6.543	893	895	897	rVV	318	265	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041823\
 Data File : VX035125.D
 Acq On : 18 Apr 2023 16:05
 Operator : JC/MD
 Sample : 02378-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 COMJ4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M
 Title : VOC Analysis

37	6.647	911	912	915	rVB2	558	342	0.02%	0.003%
38	6.763	921	931	953	rBV	496962	1196303	81.50%	10.361%
39	7.019	971	973	974	rVB	428	210	0.01%	0.002%
40	7.037	974	976	981	rBV2	357	412	0.03%	0.004%
41	7.110	981	988	995	rBV5	4002	9847	0.67%	0.085%
42	7.305	1011	1020	1039	rBV	293459	657532	44.79%	5.695%
43	7.726	1087	1089	1094	rVB2	170	271	0.02%	0.002%
44	7.763	1094	1095	1098	rBV2	244	223	0.02%	0.002%
45	7.793	1098	1100	1103	rVB	402	231	0.02%	0.002%
46	7.848	1103	1109	1115	rBV4	910	1766	0.12%	0.015%
47	8.000	1132	1134	1137	rVB3	212	204	0.01%	0.002%
48	8.171	1157	1162	1163	rBV2	177	228	0.02%	0.002%
49	8.196	1163	1166	1168	rBV	206	220	0.01%	0.002%
50	8.324	1181	1187	1203	rBV	168088	278608	18.98%	2.413%
51	8.586	1226	1230	1231	rBV2	482	534	0.04%	0.005%
52	8.647	1234	1240	1262	rVV	758178	1209400	82.39%	10.475%
53	8.951	1284	1290	1304	rVV	115749	174862	11.91%	1.514%
54	9.275	1335	1343	1349	rBV	4546	6873	0.47%	0.060%
55	9.384	1356	1361	1375	rBV	406996	599630	40.85%	5.193%
56	9.604	1396	1397	1400	rVB3	469	445	0.03%	0.004%
57	9.756	1420	1422	1424	rVB2	422	270	0.02%	0.002%
58	9.781	1424	1426	1429	rBV2	358	338	0.02%	0.003%
59	9.872	1438	1441	1444	rBV	284	472	0.03%	0.004%
60	9.945	1449	1453	1457	rVB2	387	618	0.04%	0.005%
61	10.055	1465	1471	1487	rVV	979410	1333172	90.82%	11.547%
62	10.238	1500	1501	1508	rVB3	570	798	0.05%	0.007%
63	10.402	1526	1528	1532	rBV2	342	494	0.03%	0.004%
64	10.433	1532	1533	1537	rVV3	372	417	0.03%	0.004%
65	10.488	1540	1542	1546	rVB2	446	309	0.02%	0.003%
66	10.610	1559	1562	1564	rBV2	205	293	0.02%	0.003%
67	10.652	1565	1569	1575	rBV5	752	1560	0.11%	0.014%
68	10.860	1600	1603	1606	rBV2	464	477	0.03%	0.004%
69	10.915	1609	1612	1615	rBV3	389	405	0.03%	0.004%
70	10.963	1615	1620	1625	rBV4	1099	1586	0.11%	0.014%
71	11.189	1652	1657	1670	rBV	461043	614819	41.88%	5.325%
72	11.317	1673	1678	1682	rBV3	2589	3778	0.26%	0.033%
73	11.457	1697	1701	1703	rVV3	899	1369	0.09%	0.012%
74	11.616	1725	1727	1728	rBV	347	220	0.01%	0.002%
75	11.671	1734	1736	1737	rBV	301	262	0.02%	0.002%
76	11.756	1748	1750	1757	rVB4	967	1604	0.11%	0.014%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041823\
 Data File : VX035125.D
 Acq On : 18 Apr 2023 16:05
 Operator : JC/MD
 Sample : 02378-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 COMJ4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M
 Title : VOC Analysis

77	11.847	1764	1765	1767	rBV2	407	429	0.03%	0.004%
78	11.933	1776	1779	1783	rBV3	605	637	0.04%	0.006%
79	11.975	1783	1786	1788	rBV3	1188	1420	0.10%	0.012%
80	12.018	1788	1793	1803	rBV	907079	1205040	82.09%	10.437%
81	12.219	1822	1826	1833	rBV2	7927	13259	0.90%	0.115%
82	12.317	1837	1842	1855	rVB	723428	947050	64.52%	8.202%
83	12.463	1864	1866	1869	rVB3	649	455	0.03%	0.004%
84	12.542	1877	1879	1882	rVB2	392	342	0.02%	0.003%
85	12.597	1884	1888	1889	rBV	873	880	0.06%	0.008%
86	12.768	1912	1916	1918	rBV3	817	1026	0.07%	0.009%
87	12.817	1922	1924	1926	rBV2	446	420	0.03%	0.004%
88	12.853	1927	1930	1936	rVB4	4679	6094	0.42%	0.053%
89	13.012	1955	1956	1959	rVB	371	227	0.02%	0.002%
90	13.036	1959	1960	1963	rBV2	321	351	0.02%	0.003%
91	13.115	1969	1973	1977	rVB3	2868	3448	0.23%	0.030%
92	13.560	2044	2046	2047	rBV	379	225	0.02%	0.002%
93	13.585	2047	2050	2055	rVV4	2417	3137	0.21%	0.027%
94	13.780	2079	2082	2087	rVB	2050	2730	0.19%	0.024%
95	13.963	2109	2112	2115	rVB4	1652	2091	0.14%	0.018%
96	14.170	2144	2146	2149	rBV3	711	657	0.04%	0.006%
97	14.286	2163	2165	2169	rBV	404	580	0.04%	0.005%
98	14.828	2253	2254	2257	rVB2	598	334	0.02%	0.003%
99	14.920	2267	2269	2272	rBV3	583	469	0.03%	0.004%
100	16.090	2458	2461	2466	rBV4	853	1516	0.10%	0.013%




Sum of corrected areas: 11545956

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041823\
Data File : VX035125.D
Acq On : 18 Apr 2023 16:05
Operator : JC/MD
Sample : 02378-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
COMJ4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

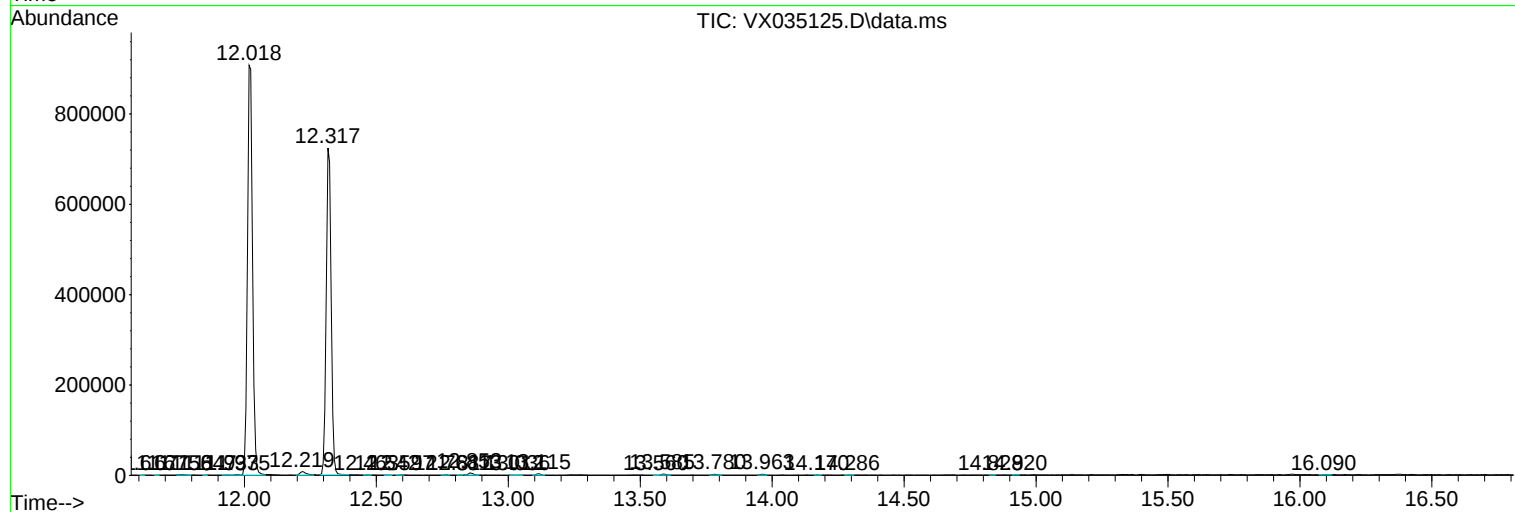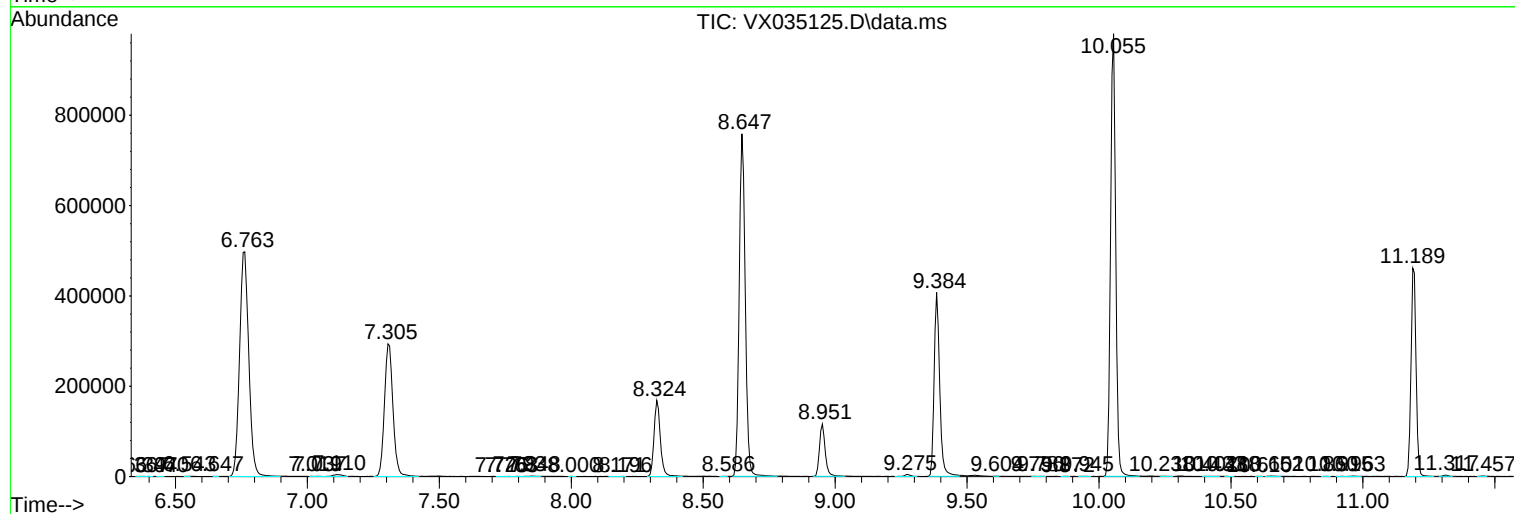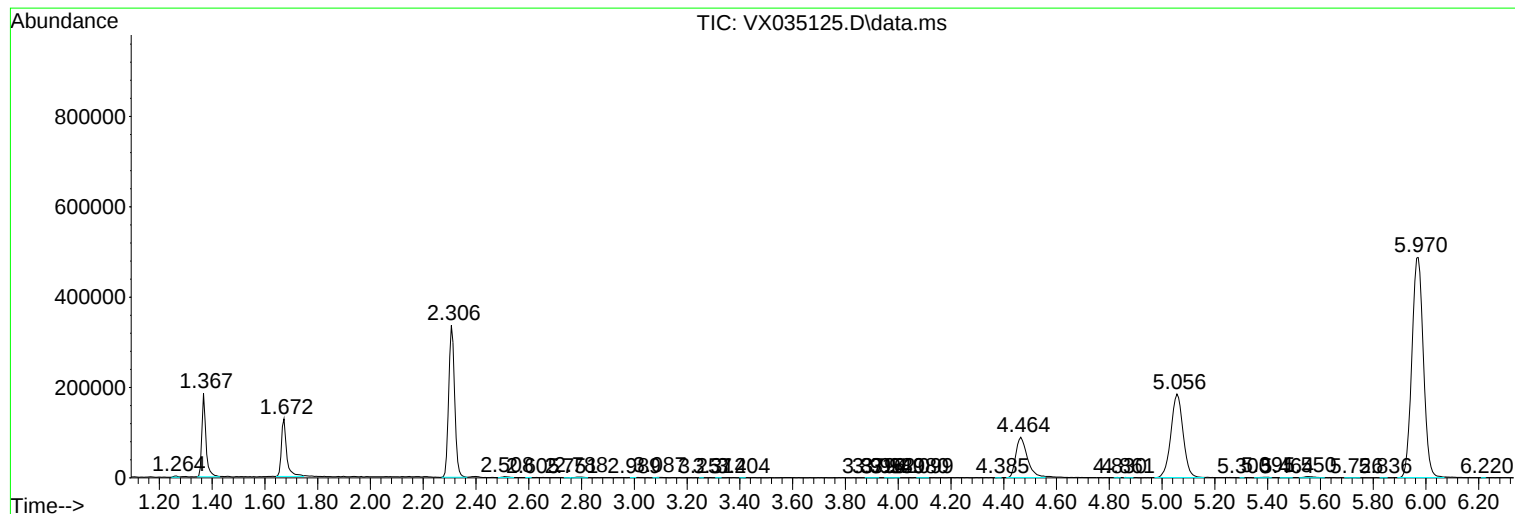

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041823\
Data File : VX035125.D
Acq On : 18 Apr 2023 16:05
Operator : JC/MD
Sample : 02378-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
COMJ4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM041823WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041823\
Data File : VX035125.D
Acq On : 18 Apr 2023 16:05
Operator : JC/MD
Sample : 02378-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
COMJ4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc